

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021524\
 Data File : PD081374.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2024 10:31
 Operator : AR\AJ
 Sample : P1300-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6Z6MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 21:46:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.794	30062605	52729556	21.989	21.509
27)	SA Decachlor...	9.114	7.933	47412216	64761058	24.574	26.106
Target Compounds							
2)	A alpha-BHC	4.022	3.296	126.7E6	206.3E6	54.244	53.654
3)	MA gamma-BHC...	4.356	3.625	121.0E6	187.8E6	52.375	51.855
4)	MA Heptachlor	4.948	3.966	127.9E6	184.3E6	52.161	51.958
5)	MB Aldrin	5.293	4.246	121.6E6	176.7E6	51.432	52.173
6)	B beta-BHC	4.550	3.920	50190671	77784251	48.296	46.035
7)	B delta-BHC	4.799	4.151	125.1E6	191.3E6	52.804	51.088
8)	B Heptachlo...	5.719	4.748	111.8E6	165.8E6	49.348	51.681
9)	A Endosulfan I	6.106	5.118	105.3E6	155.5E6	50.017	51.949
10)	B trans-Chl...	5.975	4.997	108.3E6	164.9E6	49.450	52.852
11)	B cis-Chlor...	6.055	5.062	111.3E6	166.3E6	49.420	51.915
12)	B 4,4'-DDE	6.226	5.250	215.0E6	319.9E6	100.135	108.198
13)	MA Dieldrin	6.382	5.382	228.0E6	344.8E6	102.696	104.986
14)	MA Endrin	6.612	5.657	186.5E6	307.2E6	99.397	106.929
15)	B Endosulfa...	6.830	5.950	193.9E6	299.7E6	100.418	106.184
16)	A 4,4'-DDD	6.744	5.804	168.2E6	270.0E6	101.260	107.127
17)	MA 4,4'-DDT	7.058	6.055	186.7E6	278.7E6	107.442	107.938
18)	B Endrin al...	6.961	6.129	141.3E6	215.0E6	94.606	99.221
19)	B Endosulfa...	7.195	6.352	186.7E6	282.4E6	101.974	105.270
20)	A Methoxychlor	7.533	6.630	470.0E6	655.0E6	512.390	490.274
21)	B Endrin ke...	7.682	6.859	203.2E6	324.1E6	105.097	108.074

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021524\
Data File : PD081374.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2024 10:31
Operator : AR\AJ
Sample : P1300-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 21:46:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

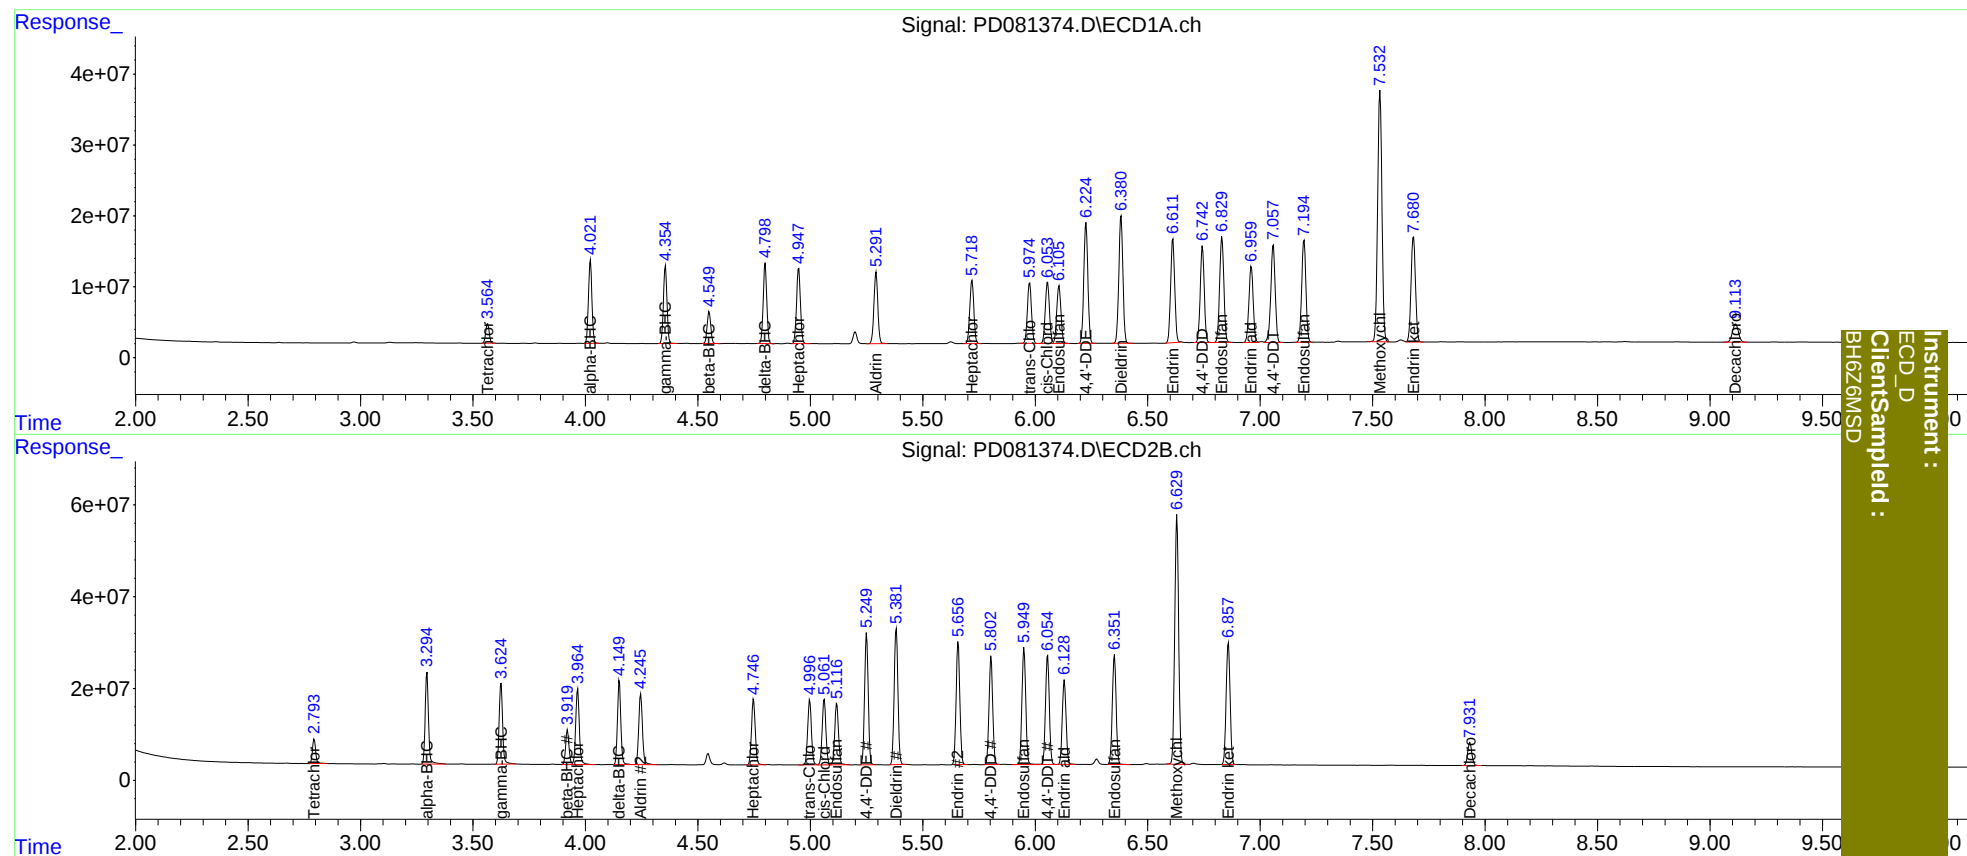

Instrument :
ECD_D
ClientSampled :
BH6Z6MSD