

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021524\
 Data File : PD081391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2024 14:17
 Operator : AR\AJ
 Sample : P1286-14MSD
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6S5MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/15/2024
 Supervised By :Ankita Jodhani 02/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 21:50:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.794	22708284	42845337	16.610	17.477
27)	SA Decachlor...	9.111	7.931	35178536	46396573	18.233	18.703
Target Compounds							
2)	A alpha-BHC	4.022	3.296	119.8E6	193.5E6	51.280	50.315
3)	MA gamma-BHC...	4.354	3.625	113.5E6	179.9E6	49.107m	49.675
4)	MA Heptachlor	4.948	3.966	118.7E6	177.9E6	48.381	50.155
5)	MB Aldrin	5.291	4.246	111.3E6	167.8E6	47.071	49.528
6)	B beta-BHC	4.550	3.920	44755275	74175256	43.066	43.899
7)	B delta-BHC	4.799	4.151	117.2E6	181.3E6	49.481	48.415
8)	B Heptachlo...	5.718	4.747	100.0E6	152.2E6	44.159	47.438
9)	A Endosulfan I	6.104	5.117	95447381	142.0E6	45.330	47.429
10)	B trans-Chl...	5.973	4.997	97818711	156.2E6	44.679m	50.069
11)	B cis-Chlor...	6.054	5.062	99894808	155.2E6	44.353	48.448
12)	B 4,4'-DDE	6.225	5.250	195.1E6	296.4E6	90.883	100.243
13)	MA Dieldrin	6.380	5.382	210.6E6	318.7E6	94.839	97.017
14)	MA Endrin	6.611	5.657	175.6E6	291.1E6	93.543	101.322
15)	B Endosulfa...	6.829	5.950	176.1E6	275.7E6	91.236	97.686
16)	A 4,4'-DDD	6.742	5.803	154.7E6	248.2E6	93.153	98.501
17)	MA 4,4'-DDT	7.057	6.054	166.8E6	254.9E6	96.000	98.709
18)	B Endrin al...	6.959	6.128	124.6E6	189.8E6	83.434	87.582
19)	B Endosulfa...	7.193	6.351	165.7E6	256.5E6	90.508	95.610
20)	A Methoxychlor	7.531	6.629	438.5E6	625.6E6	478.082	468.270
21)	B Endrin ke...	7.680	6.857	187.4E6	290.6E6	96.932	96.914

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021524\
Data File : PD081391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2024 14:17
Operator : AR\AJ
Sample : P1286-14MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 21:50:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

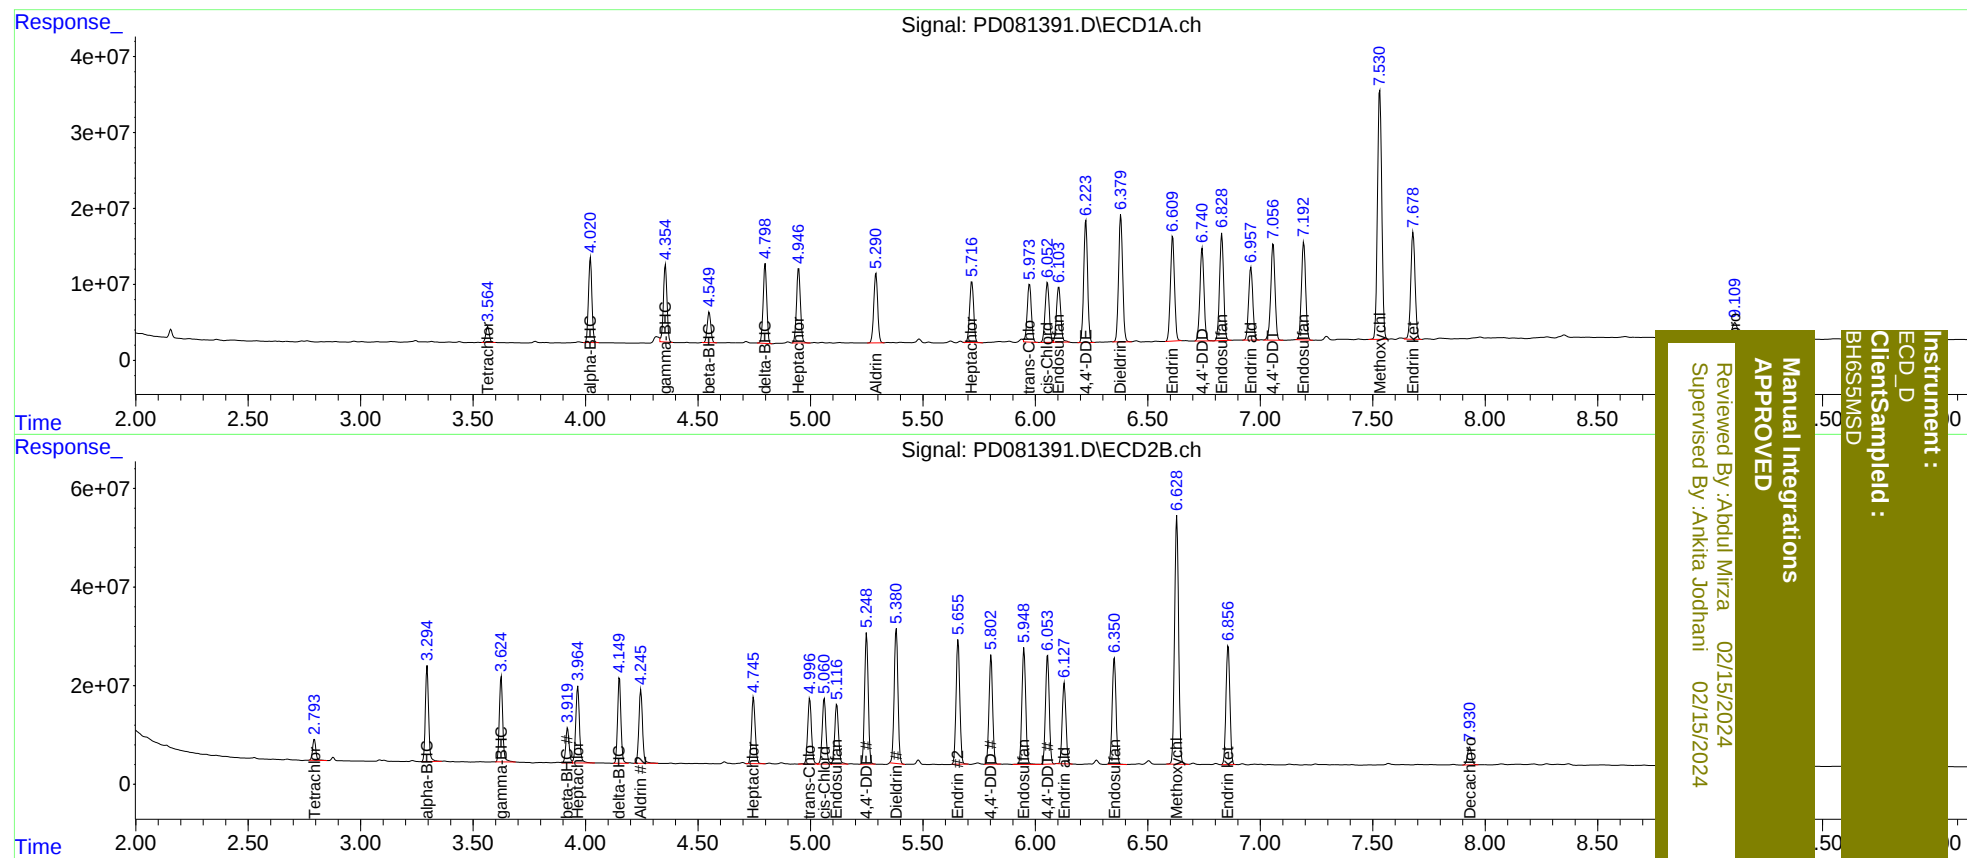

Instrument :
ECD_D
Client Sampled :
BH65MSD

Manual Integrations
APPROVED

Reviewed By : Abdul Miza 02/15/2024
Supervised By : Ankita Jodhani 02/15/2024