

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021524\
 Data File : PD081407.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2024 19:03
 Operator : AR\AJ
 Sample : P1286-20
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6S8

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/15/2024
 Supervised By :Ankita Jodhani 02/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 06:21:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.566	2.795	16417455	31870545	12.009	13.000
2) SA Decachlor...	9.107	7.932	42935224	47735240	22.254m	19.243
Target Compounds						
7) B delta-BHC	4.795	4.144	4677212	9906068	1.975	2.645 #
9) A Endosulfan I	6.135	5.145	17431882	49723000	8.279m	16.607 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021524\
Data File : PD081407.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2024 19:03
Operator : AR\AJ
Sample : P1286-20
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 06:21:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

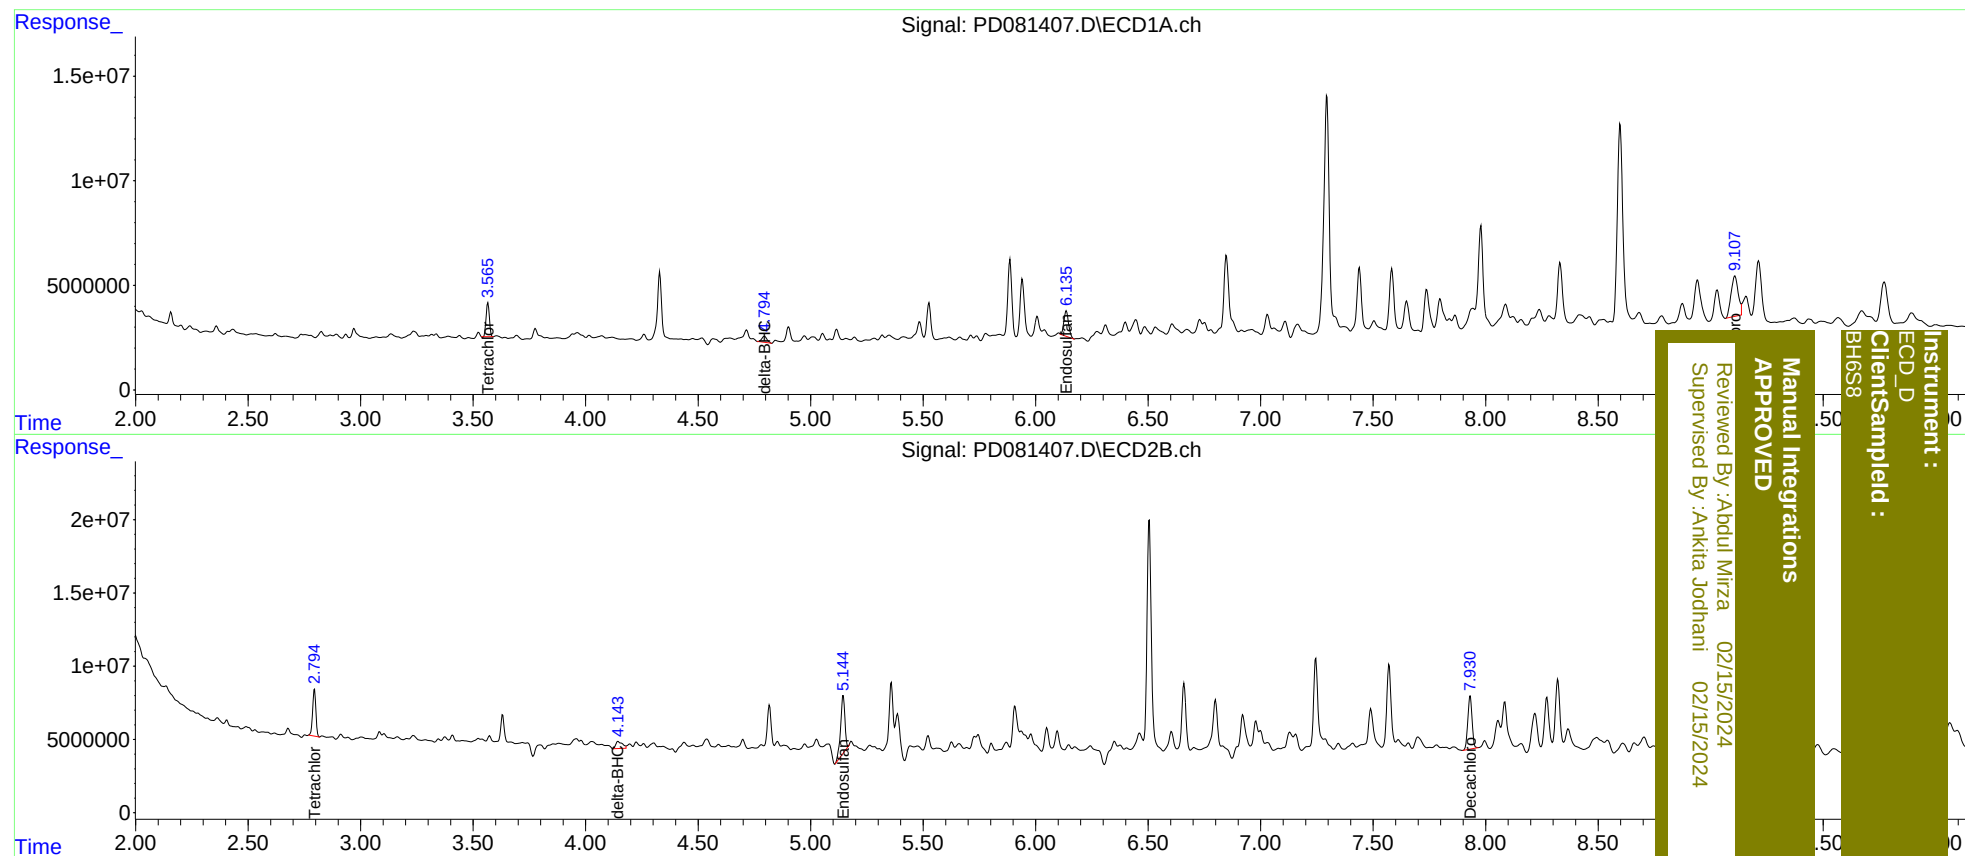

Reviewed By: Abdul Mirza 02/15/2024
Supervised By: Ankita Jodhani 02/15/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BH6S8