

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021524\
 Data File : PD081425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2024 23:03
 Operator : AR\AJ
 Sample : P1370-02MS
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA7MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 06:25:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.795	27825237	51824430	20.353	21.139
2)	SA Decachlor...	9.111	7.931	36465386	49104693	18.900	19.795
Target Compounds							
2)	A alpha-BHC	4.022	3.296	131.3E6	216.8E6	56.209	56.382
3)	MA gamma-BHC...	4.355	3.625	120.6E6	191.9E6	52.191	52.983
4)	MA Heptachlor	4.947	3.966	117.1E6	172.8E6	47.740	48.714
5)	MB Aldrin	5.291	4.246	111.9E6	167.1E6	47.340	49.327
6)	B beta-BHC	4.550	3.920	51602438	81224899	49.655	48.071
7)	B delta-BHC	4.799	4.151	129.3E6	200.7E6	54.603	53.608
8)	B Heptachlo...	5.718	4.748	109.0E6	163.9E6	48.146	51.096
9)	A Endosulfan I	6.104	5.117	103.0E6	153.1E6	48.916	51.145
10)	B trans-Chl...	5.974	4.997	100.1E6	153.9E6	45.711	49.331
11)	B cis-Chlor...	6.053	5.061	102.1E6	154.4E6	45.323	48.197
12)	B 4,4'-DDE	6.224	5.250	191.8E6	288.5E6	89.354	97.560
13)	MA Dieldrin	6.380	5.382	222.7E6	339.0E6	100.284	103.199
14)	MA Endrin	6.611	5.657	172.5E6	282.3E6	91.908	98.256
15)	B Endosulfa...	6.829	5.950	196.2E6	303.3E6	101.629	107.444
16)	A 4,4'-DDD	6.742	5.803	160.3E6	257.3E6	96.537	102.111
17)	MA 4,4'-DDT	7.057	6.054	163.4E6	243.8E6	94.068	94.424
18)	B Endrin al...	6.958	6.129	149.2E6	226.3E6	99.876	104.414
19)	B Endosulfa...	7.193	6.351	190.5E6	286.0E6	104.028	106.598
20)	A Methoxychlor	7.531	6.629	439.9E6	618.3E6	479.522	462.747
21)	B Endrin ke...	7.680	6.857	217.0E6	336.5E6	112.198	112.209

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021524\
Data File : PD081425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2024 23:03
Operator : AR\AJ
Sample : P1370-02MS
Misc :
ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 06:25:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

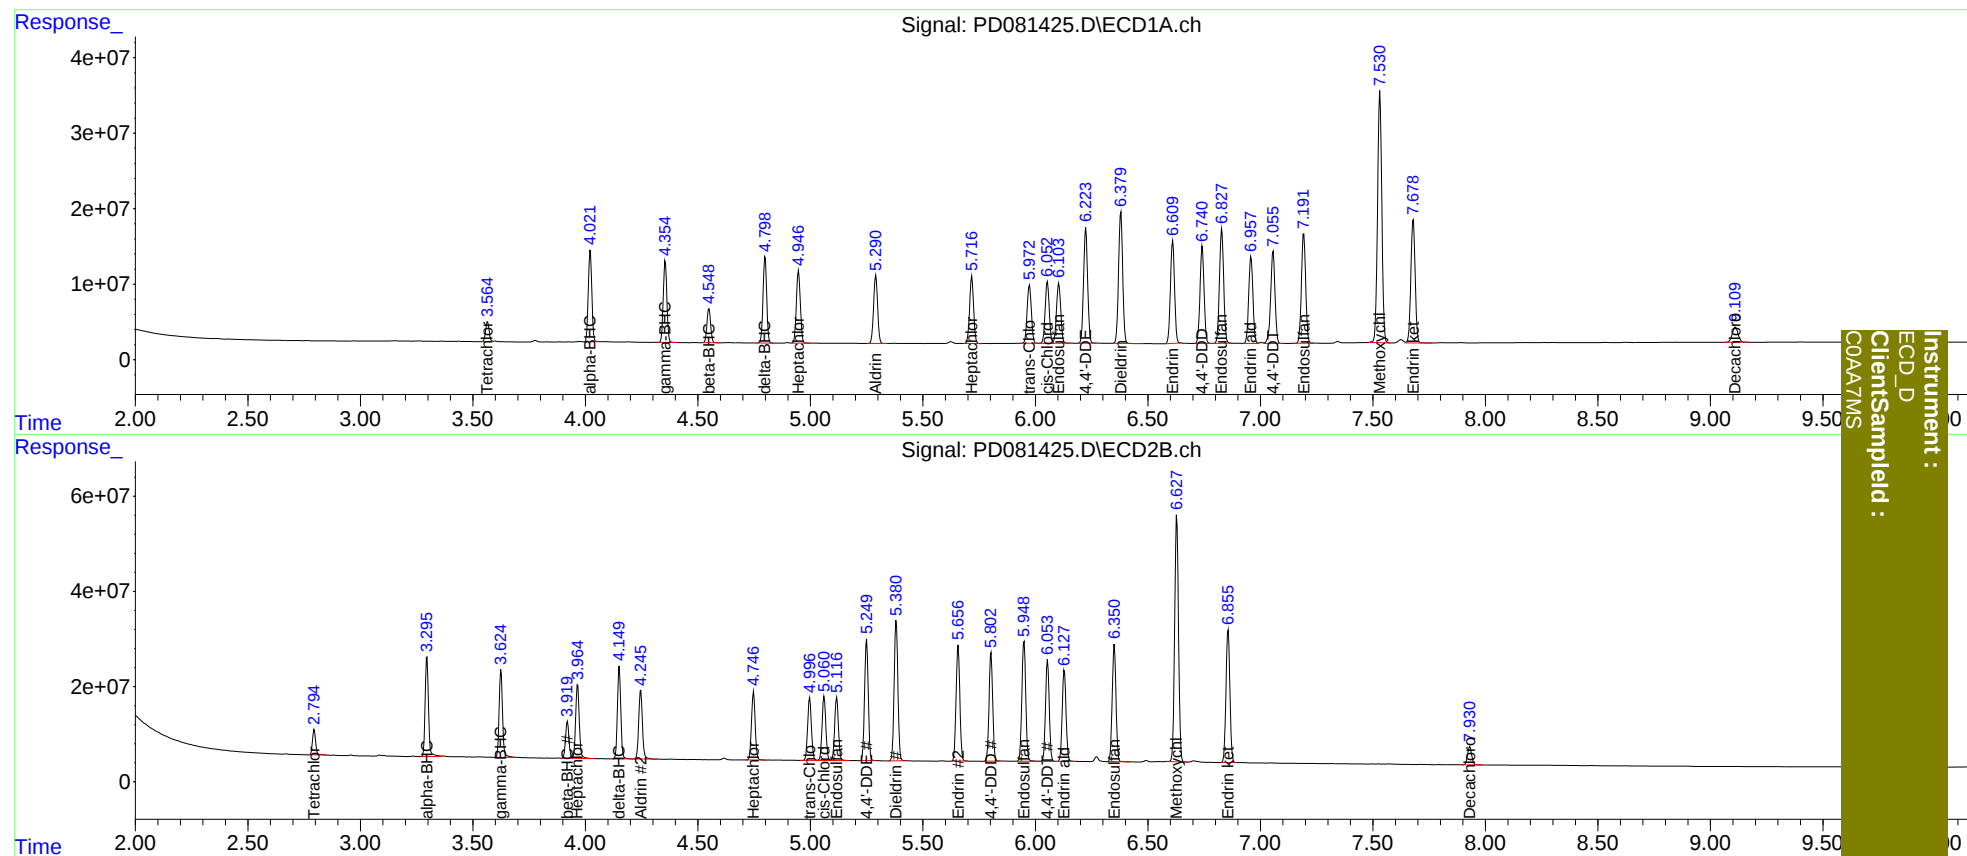

Instrument :
ECD_D
ClientSampled :
COAATMS