

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021624\
 Data File : PD081450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2024 15:47
 Operator : AR\AJ
 Sample : P1349-06MS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6X3MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/16/2024
 Supervised By :Ankita Jodhani 02/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 01:24:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.794	27751567	51539780	20.299	21.023
27)	SA Decachlor...	9.112	7.931	43397776	60307091	22.493	24.311m
Target Compounds							
2)	A alpha-BHC	4.022	3.296	124.3E6	209.2E6	53.223	54.407
3)	MA gamma-BHC...	4.355	3.625	117.2E6	190.8E6	50.747	52.682
4)	MA Heptachlor	4.948	3.966	126.1E6	189.3E6	51.405	53.373
5)	MB Aldrin	5.291	4.246	121.6E6	183.9E6	51.427	54.280
6)	B beta-BHC	4.550	3.920	53070673	81856052	51.068	48.444
7)	B delta-BHC	4.799	4.151	125.2E6	199.0E6	52.867	53.133
8)	B Heptachlo...	5.718	4.747	113.7E6	168.5E6	50.196	52.506
9)	A Endosulfan I	6.105	5.117	107.7E6	157.6E6	51.138	52.651
10)	B trans-Chl...	5.974	4.998	109.6E6	165.7E6	50.075	53.101
11)	B cis-Chlor...	6.054	5.062	114.5E6	169.9E6	50.850	53.036
12)	B 4,4'-DDE	6.225	5.250	213.7E6	322.0E6	99.548	108.907
13)	MA Dieldrin	6.380	5.382	217.8E6	346.5E6	98.072	105.508
14)	MA Endrin	6.610	5.657	191.8E6	307.1E6	102.224	106.893
15)	B Endosulfa...	6.829	5.950	199.0E6	297.6E6	103.077	105.442
16)	A 4,4'-DDD	6.742	5.804	177.3E6	265.9E6	106.758	105.498
17)	MA 4,4'-DDT	7.056	6.055	187.4E6	277.3E6	107.883	107.389
18)	B Endrin al...	6.959	6.129	134.3E6	198.5E6	89.881	91.589
19)	B Endosulfa...	7.193	6.351	188.9E6	282.2E6	103.198	105.179
20)	A Methoxychlor	7.532	6.630	455.1E6	652.2E6	496.151	488.145
21)	B Endrin ke...	7.680	6.858	205.8E6	321.2E6	106.430	107.112

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021624\
Data File : PD081450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2024 15:47
Operator : AR\AJ
Sample : P1349-06MS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 01:24:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

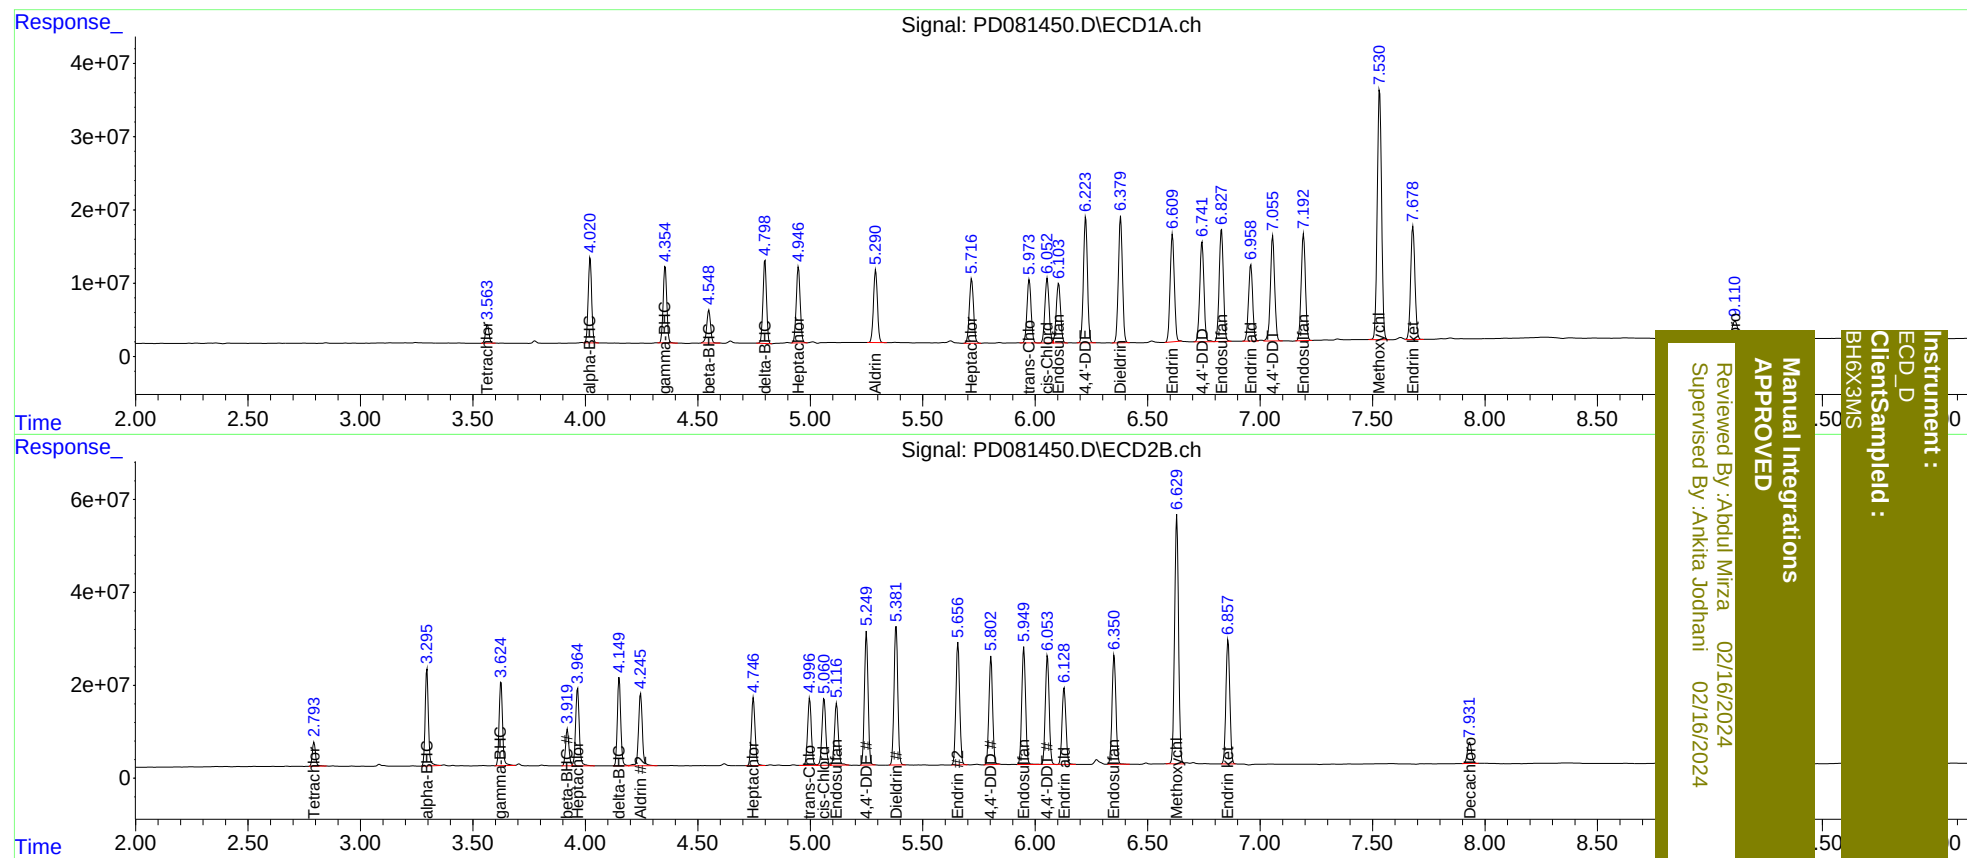

Instrument :
ECD_D
ClientSampled :
BH6X3MS

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/16/2024
Supervised By :Ankita Jodhani 02/16/2024