

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021720\
 Data File : PD057335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2020 10:44
 Operator : AJ\MA
 Sample : L1424-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5B07

Manual Integrations
 APPROVED

mohammad
 2/24/2020 2:50:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 05:32:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 11 04:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.284	3.959	12723732	30702060	15.317	16.475
27)	SA Decachlor...	7.953	8.993	25086164	48011543	24.181	21.238m
Target Compounds							
12)	B 4,4'-DDE	5.391	6.280	8368337	13385609	7.568m	5.230m#
16)	A 4,4'-DDD	5.901	6.770	9230248	23837718	13.324m	11.562m
17)	MA 4,4'-DDT	6.136	7.070	6781573	19916505	10.422m	10.490

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021720\
Data File : PD057335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2020 10:44
Operator : AJ\MA
Sample : L1424-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 05:32:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 11 04:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

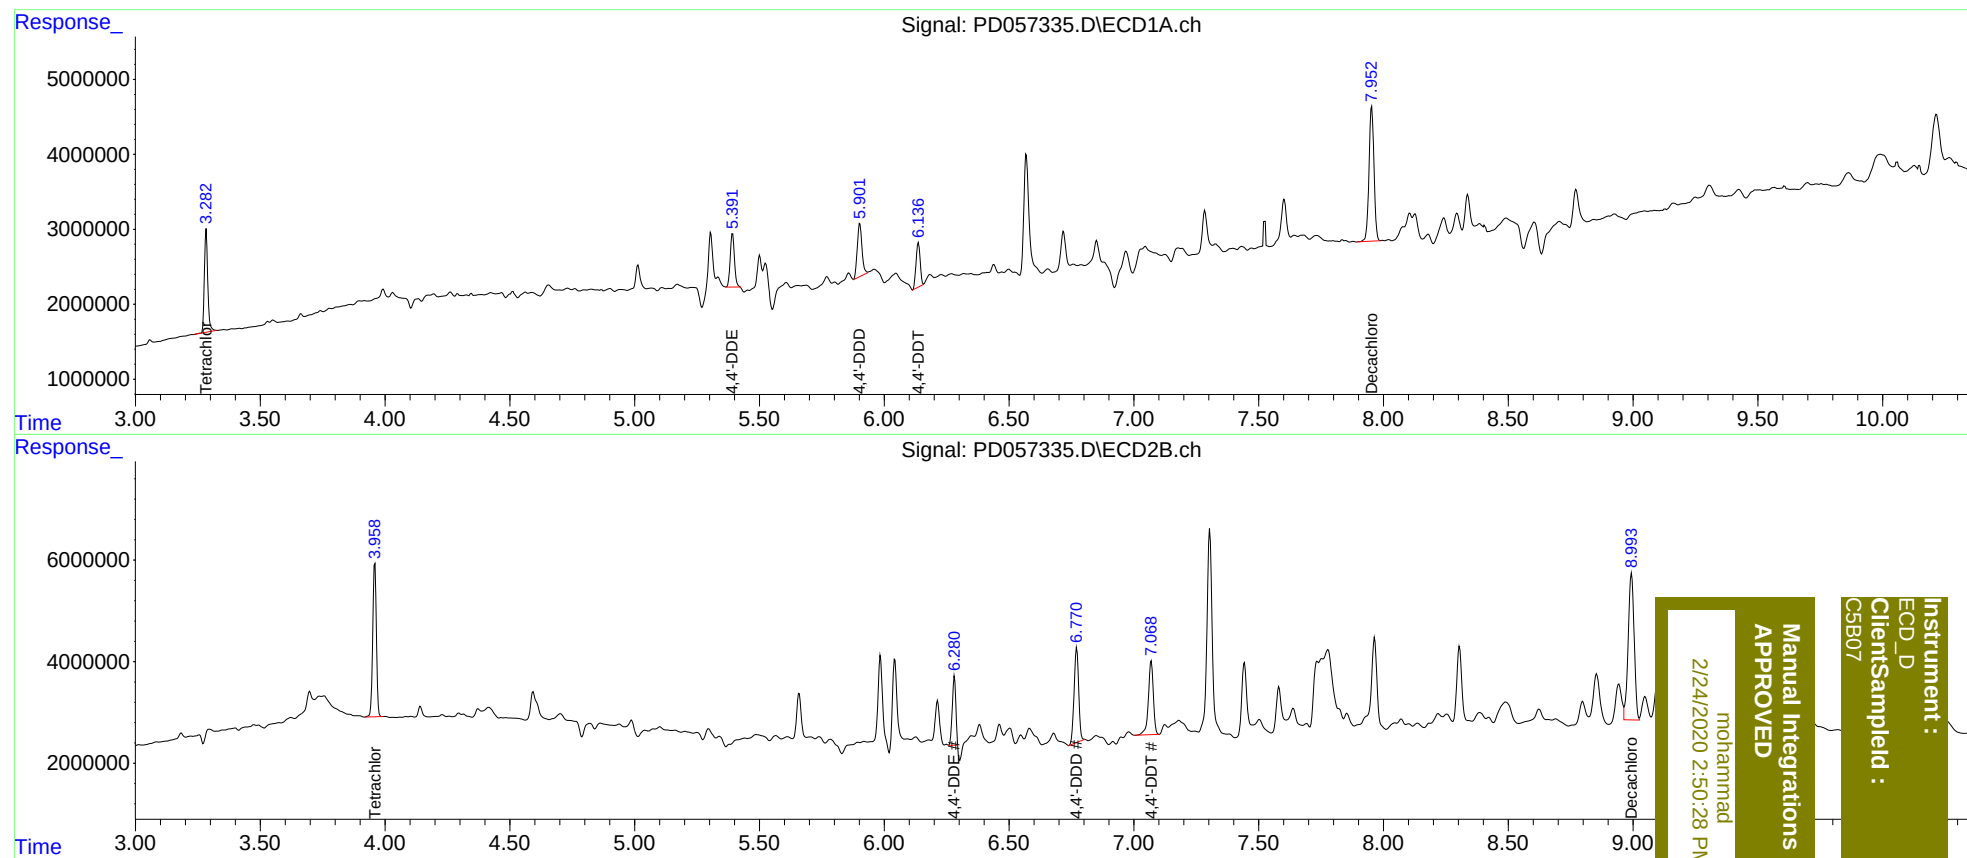

Manual Integrations
APPROVED

mohammad
2/24/2020 2:50:28 PM

Instrument :
ECD_D
ClientSampled :
C5B07