

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021820\
 Data File : PD057369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2020 16:30
 Operator : AJ\MA
 Sample : PCP-STD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCP-STD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 02:26:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 11 04:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA gamma-BHC...	0.000	4.591f	0	26177.2E6	N.D.	9239.046
--------------------	-------	--------	---	-----------	------	----------


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021820\
Data File : PD057369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2020 16:30
Operator : AJ\MA
Sample : PCP-STD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCP-STD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 02:26:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021020CLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 11 04:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

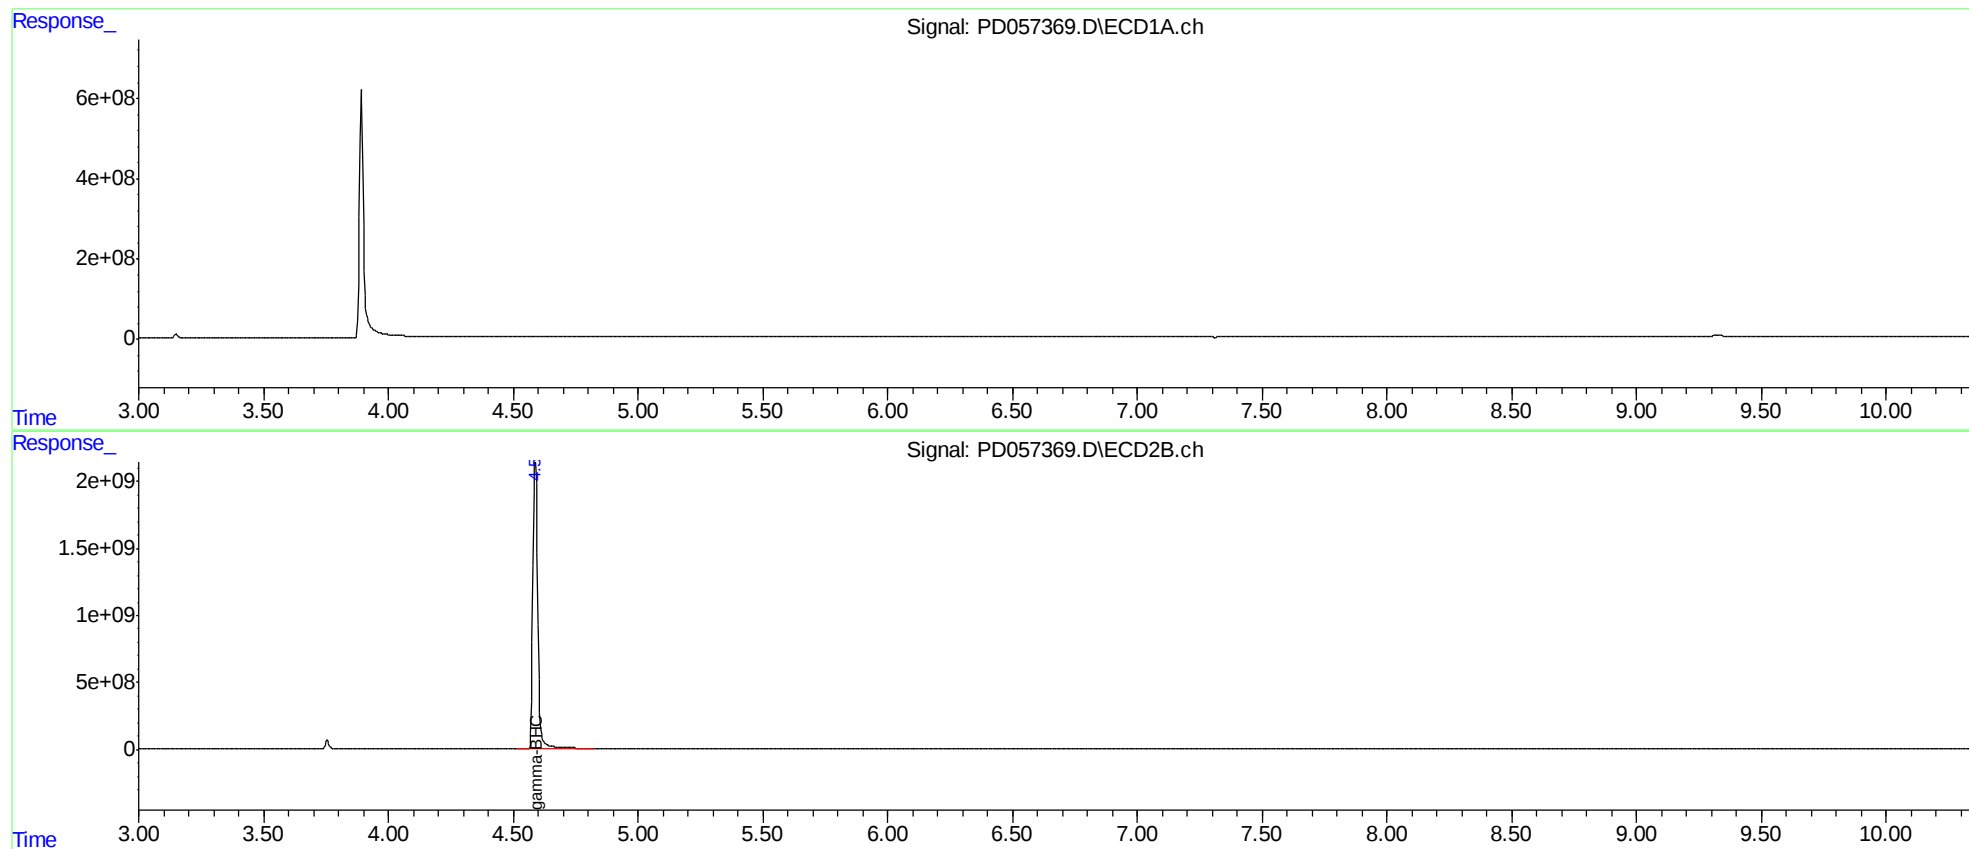


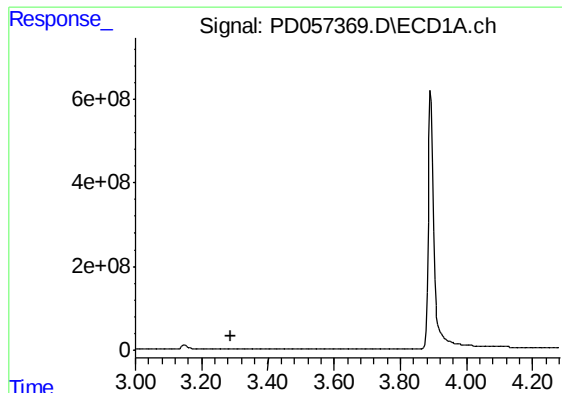

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PCP-STD

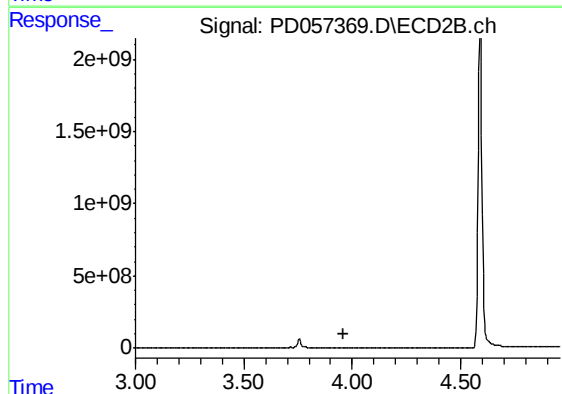


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.961 min
Response: 0
Conc: N.D.

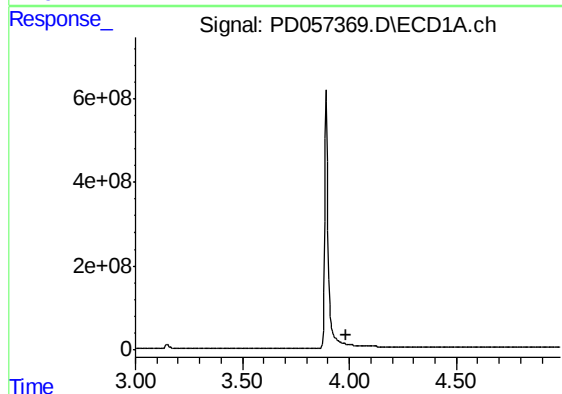


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.987 min
Response: 0
Conc: N.D.

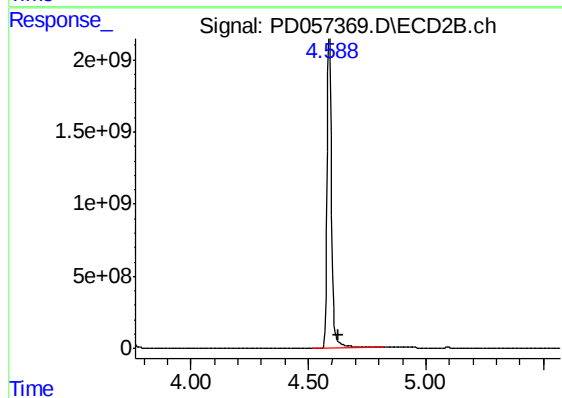

#3 gamma-BHC (Lindane)


R.T.: 4.591 min
Delta R.T.: -0.039 min
Response: 26177173821
Conc: 9239.05 ng/ml

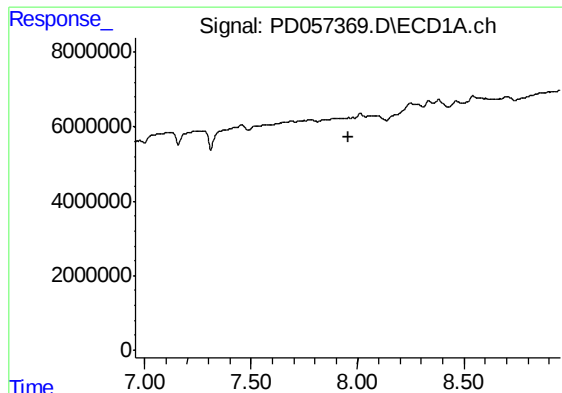

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PCP-STD

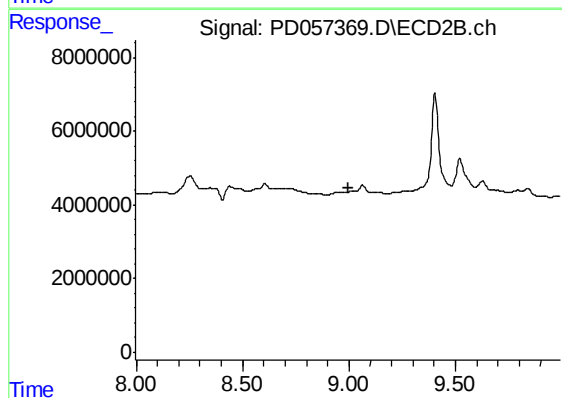

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.996 min
Response: 0
Conc: N.D.