

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021822\
 Data File : PD068088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2022 13:32
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 15:00:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 18 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	4.179	7596997	55686016	5.537	5.819
27)	SA Decachlor...	8.221	9.378	12951616	48117834	10.753	10.474
Target Compounds							
2)	A alpha-BHC	3.891	4.575	9644286	73805611	5.081	5.590
3)	MA gamma-BHC...	4.175	4.866	9445452	67711044	5.231	5.568
4)	MA Heptachlor	4.476	5.393	8963077	56770584	5.408	5.545
9)	A Endosulfan I	5.508	6.458	8480648	49643990	5.400	5.472
13)	MA Dieldrin	5.752	6.716	17417809	100.9E6	10.196	10.968
14)	MA Endrin	6.010	6.937	13786836	70910640	10.281	10.801
16)	A 4,4'-DDD	6.139	7.047	13702015	72050648	10.159	10.599
17)	MA 4,4'-DDT	6.380	7.351	10703250	49793770	9.437	9.969
20)	A Methoxychlor	6.932	7.803	31479639	115.2E6	49.783	51.643


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021822\
Data File : PD068088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2022 13:32
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 15:00:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 18 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

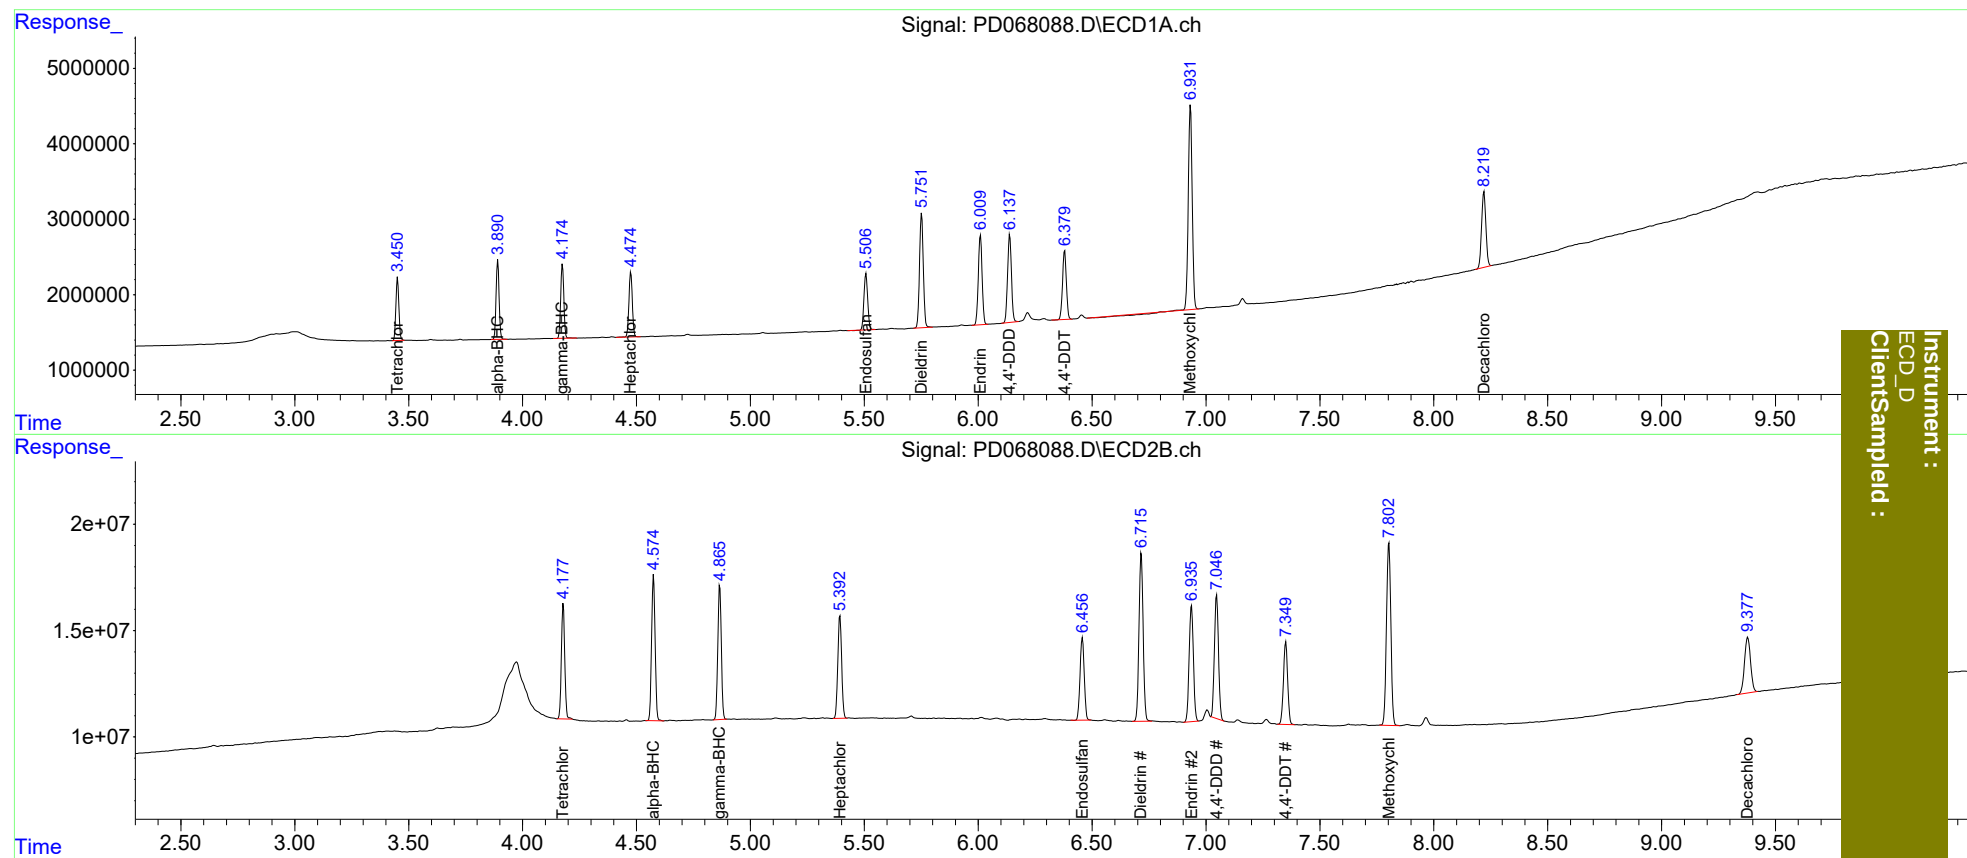


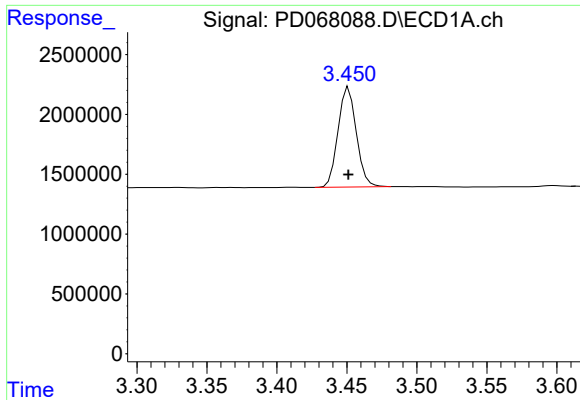

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 7596997
Conc: 5.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

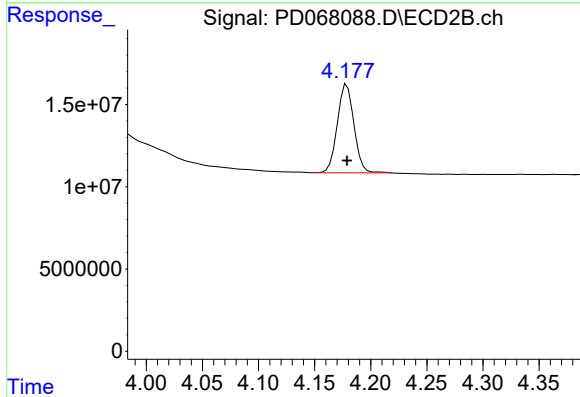


#1 Tetrachloro-m-xylene

R.T.: 4.179 min
Delta R.T.: 0.000 min
Response: 55686016
Conc: 5.82 ng/ml

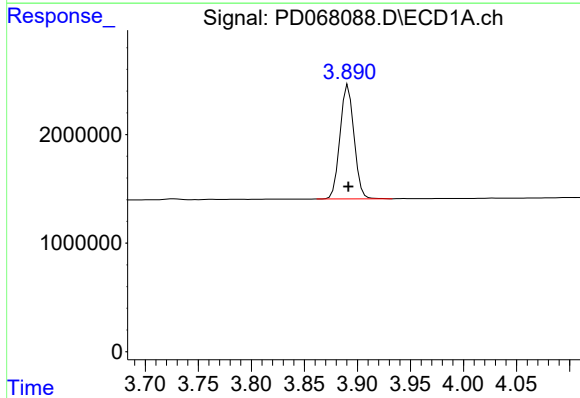


#2 alpha-BHC

R.T.: 3.891 min
Delta R.T.: 0.000 min
Response: 9644286
Conc: 5.08 ng/ml

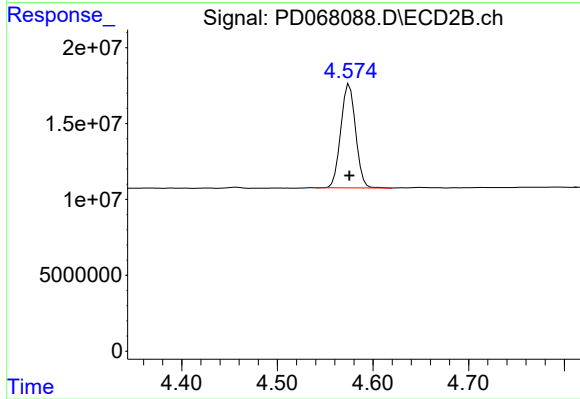

#2 alpha-BHC


R.T.: 4.575 min
Delta R.T.: 0.000 min
Response: 73805611
Conc: 5.59 ng/ml

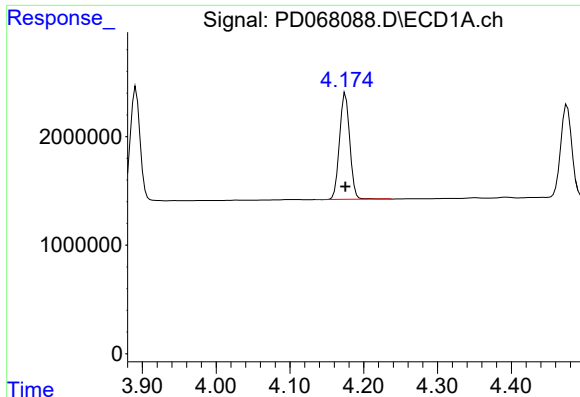

#3 gamma-BHC (Lindane)


R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 9445452
Conc: 5.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

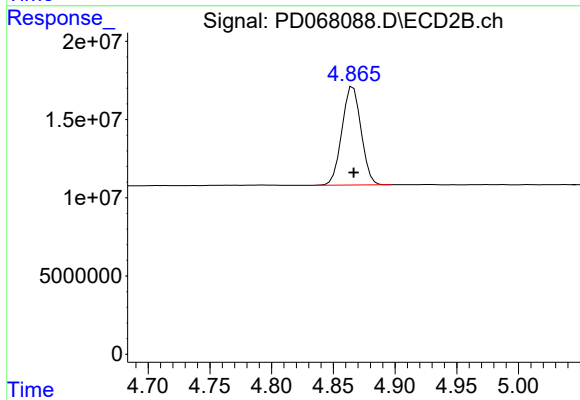


#3 gamma-BHC (Lindane)

R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 67711044
Conc: 5.57 ng/ml

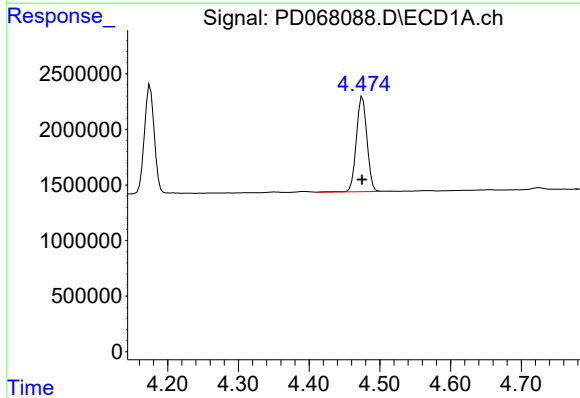


#4 Heptachlor

R.T.: 4.476 min
Delta R.T.: 0.000 min
Response: 8963077
Conc: 5.41 ng/ml

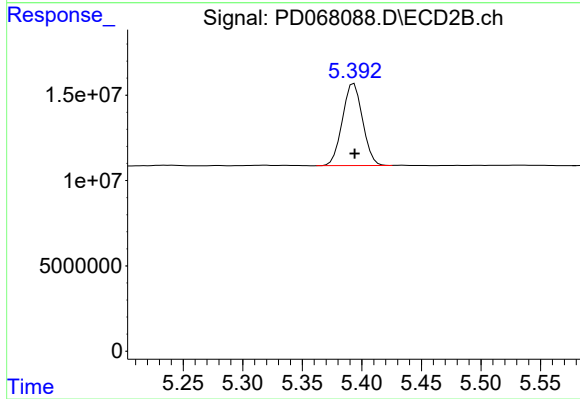

#4 Heptachlor


R.T.: 5.393 min
Delta R.T.: 0.000 min
Response: 56770584
Conc: 5.54 ng/ml

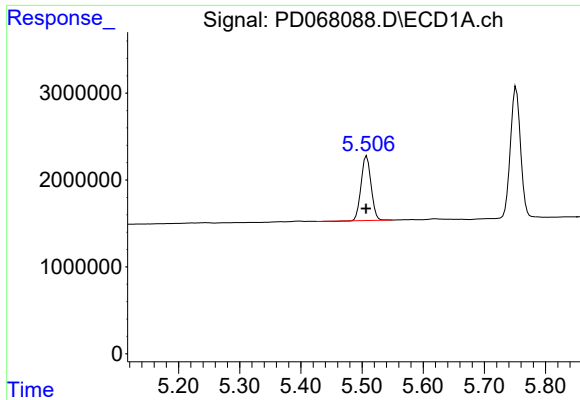

#9 Endosulfan I


R.T.: 5.508 min
Delta R.T.: 0.000 min
Response: 8480648
Conc: 5.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

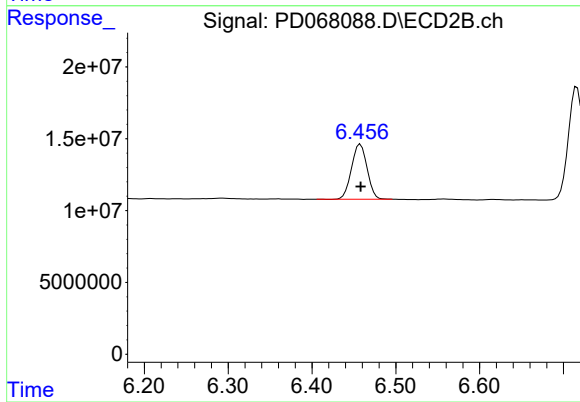


#9 Endosulfan I

R.T.: 6.458 min
Delta R.T.: 0.000 min
Response: 49643990
Conc: 5.47 ng/ml

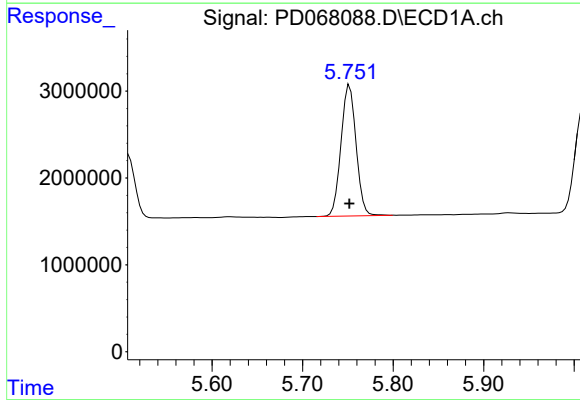


#13 Dieldrin

R.T.: 5.752 min
Delta R.T.: 0.000 min
Response: 17417809
Conc: 10.20 ng/ml

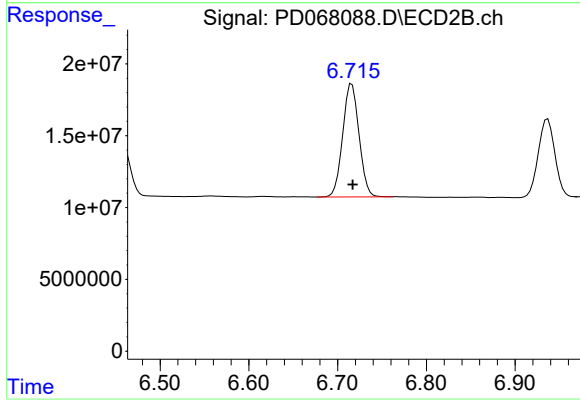

#13 Dieldrin


R.T.: 6.716 min
Delta R.T.: 0.000 min
Response: 100924888
Conc: 10.97 ng/ml

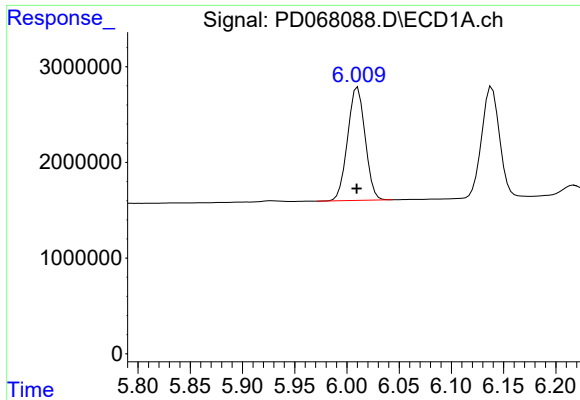

#14 Endrin


R.T.: 6.010 min
Delta R.T.: 0.001 min
Response: 13786836
Conc: 10.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

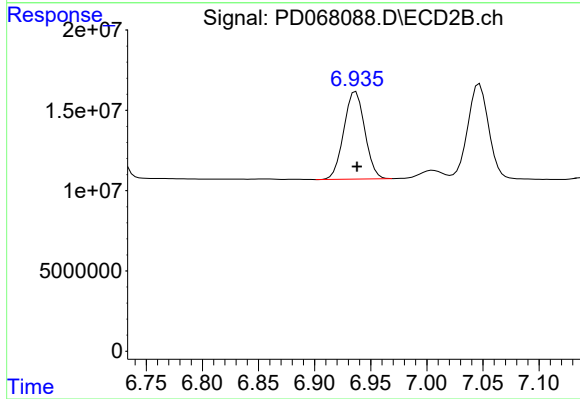


#14 Endrin

R.T.: 6.937 min
Delta R.T.: 0.000 min
Response: 70910640
Conc: 10.80 ng/ml

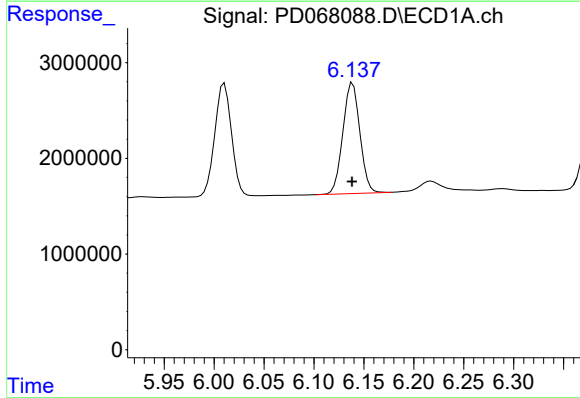


#16 4,4'-DDD

R.T.: 6.139 min
Delta R.T.: 0.000 min
Response: 13702015
Conc: 10.16 ng/ml

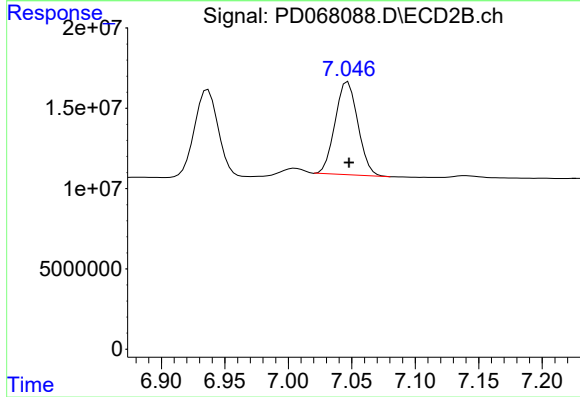

#16 4,4'-DDD


R.T.: 7.047 min
Delta R.T.: 0.000 min
Response: 72050648
Conc: 10.60 ng/ml

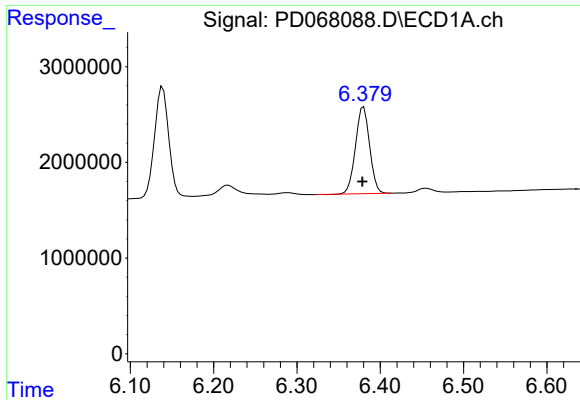

#17 4,4'-DDT


R.T.: 6.380 min
Delta R.T.: 0.001 min
Response: 10703250
Conc: 9.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

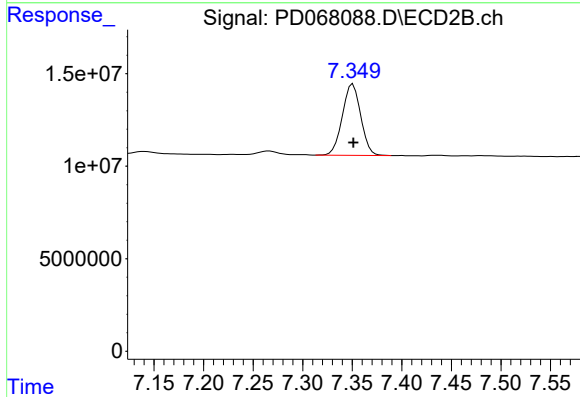


#17 4,4'-DDT

R.T.: 7.351 min
Delta R.T.: 0.000 min
Response: 49793770
Conc: 9.97 ng/ml

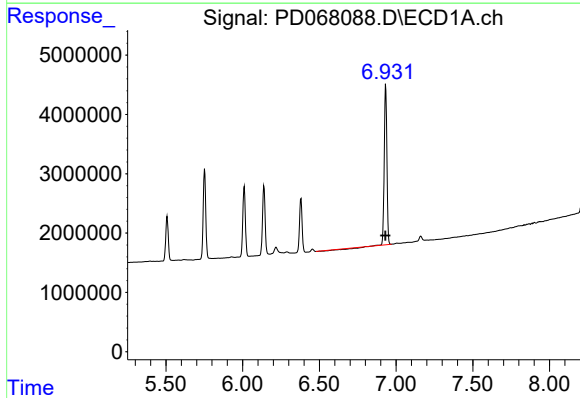


#20 Methoxychlor

R.T.: 6.932 min
Delta R.T.: 0.001 min
Response: 31479639
Conc: 49.78 ng/ml

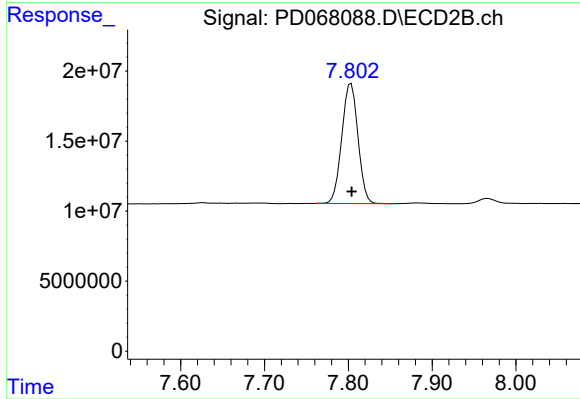

#20 Methoxychlor


R.T.: 7.803 min
Delta R.T.: 0.000 min
Response: 115166391
Conc: 51.64 ng/ml

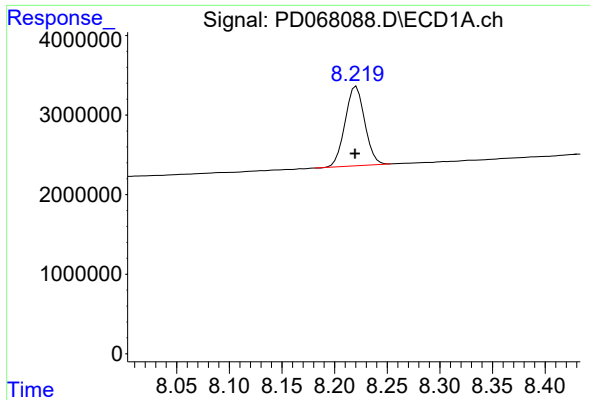

#27 Decachlorobiphenyl

R.T.: 8.221 min
Delta R.T.: 0.001 min
Response: 12951616
Conc: 10.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

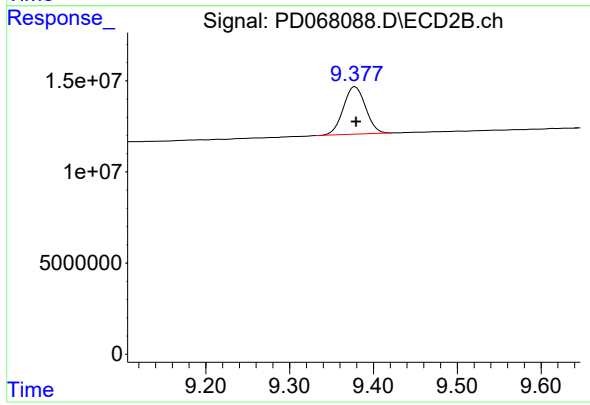

#27 Decachlorobiphenyl

R.T.: 9.378 min
Delta R.T.: 0.000 min
Response: 48117834
Conc: 10.47 ng/ml