

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021822\
 Data File : PD068090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2022 14:01
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 15:00:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 18 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	4.179	14664749	107.2E6	10.688	11.208
27)	SA Decachlor...	8.220	9.381	25328703	96750327	21.029	21.059
Target Compounds							
2)	A alpha-BHC	3.892	4.576	19429398	144.1E6	10.235	10.915
3)	MA gamma-BHC...	4.175	4.867	18729390	133.9E6	10.372	11.011
4)	MA Heptachlor	4.475	5.394	17238374	110.1E6	10.401	10.751
9)	A Endosulfan I	5.508	6.458	16777204	98617564	10.682	10.869
13)	MA Dieldrin	5.752	6.717	35362003	198.7E6	20.700	21.599
14)	MA Endrin	6.010	6.938	27300261	138.9E6	20.357	21.158
16)	A 4,4'-DDD	6.138	7.048	27906778	144.1E6	20.690	21.192
17)	MA 4,4'-DDT	6.379	7.351	22247420	100.9E6	19.616	20.191
20)	A Methoxychlor	6.932	7.804	65276524	229.4E6	103.232	102.869


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021822\
Data File : PD068090.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2022 14:01
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 15:00:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 18 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

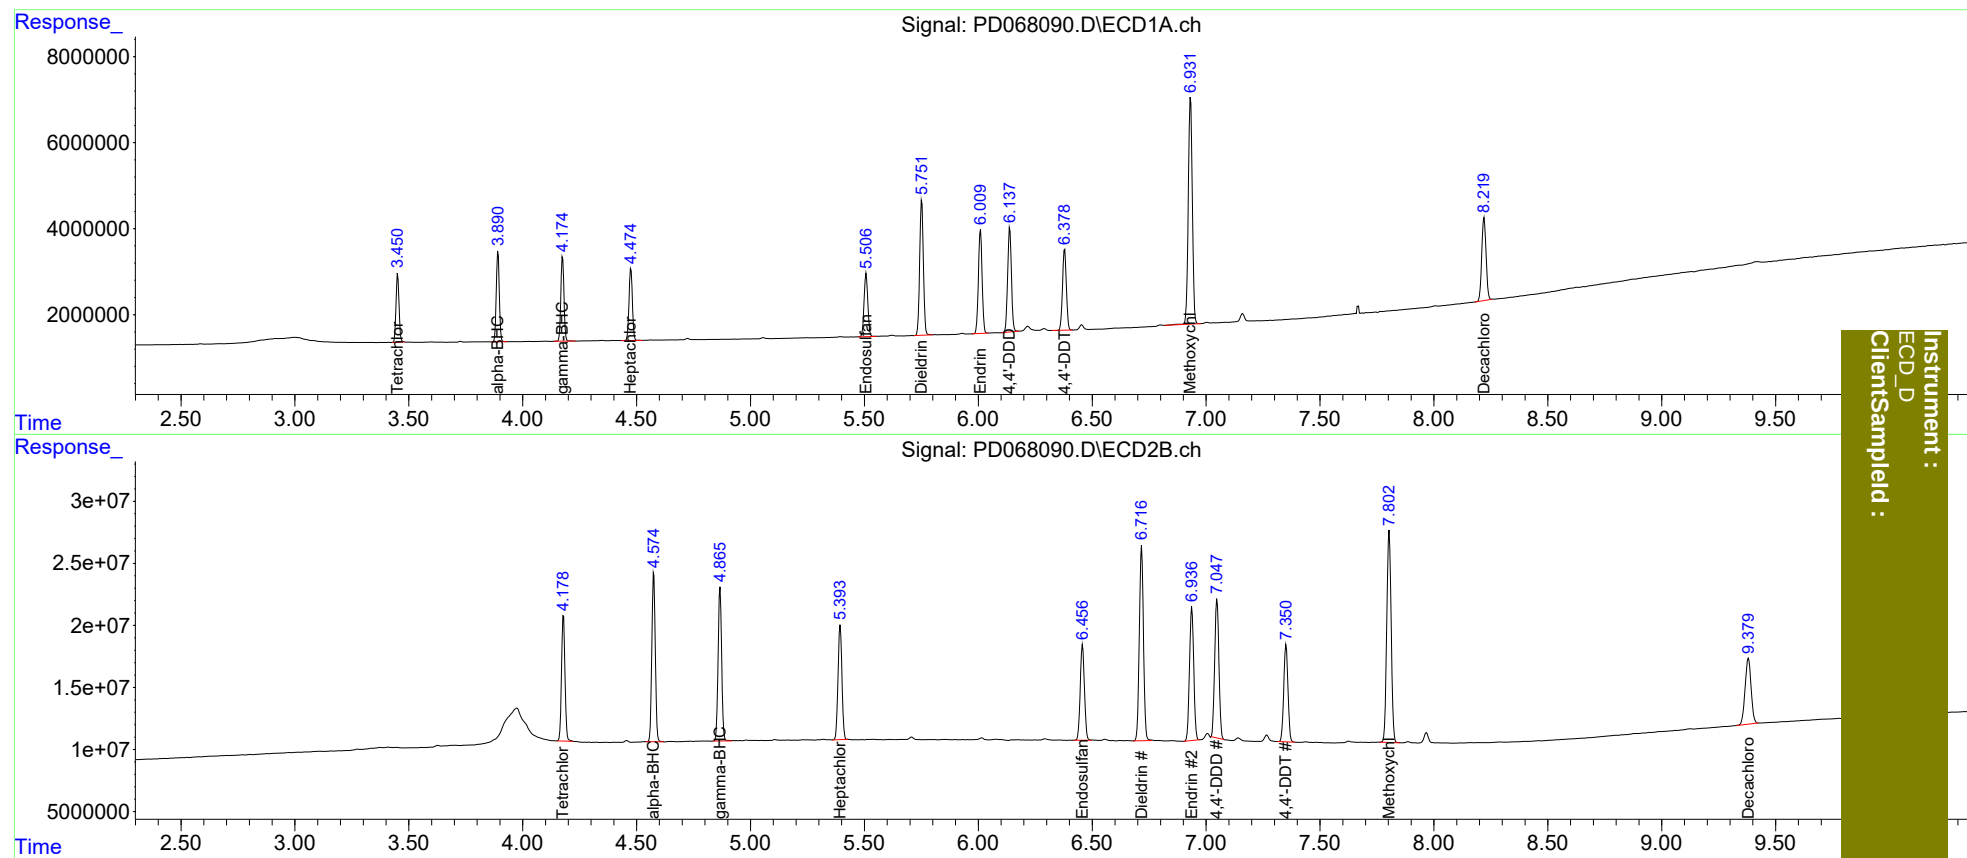


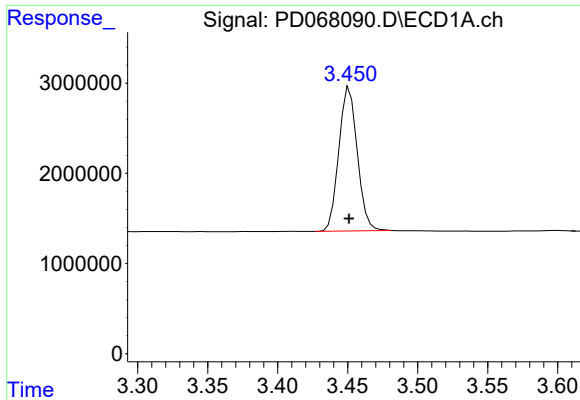

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 14664749
Conc: 10.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

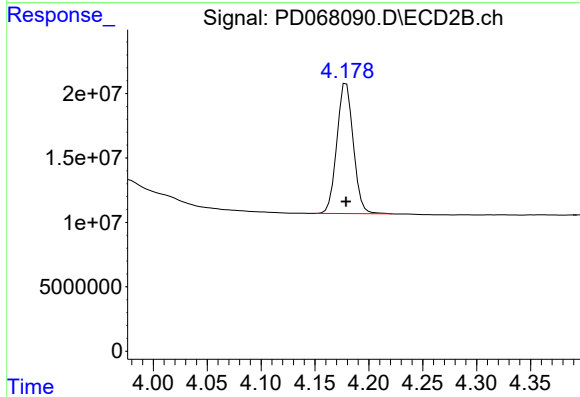


#1 Tetrachloro-m-xylene

R.T.: 4.179 min
Delta R.T.: 0.000 min
Response: 107247854
Conc: 11.21 ng/ml

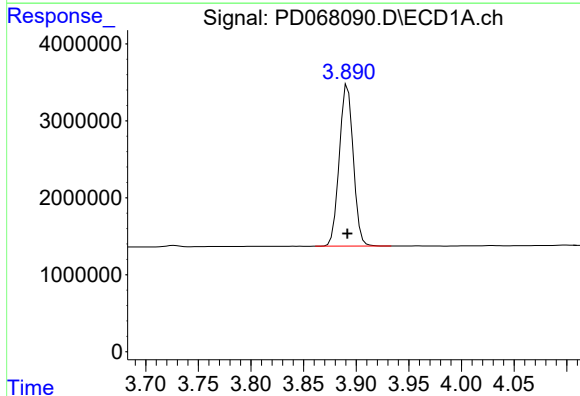


#2 alpha-BHC

R.T.: 3.892 min
Delta R.T.: 0.000 min
Response: 19429398
Conc: 10.24 ng/ml

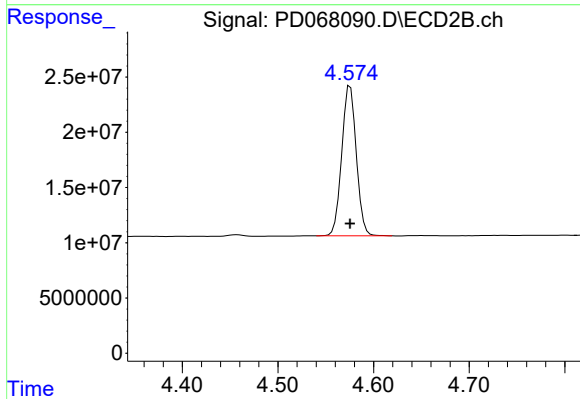

#2 alpha-BHC


R.T.: 4.576 min
Delta R.T.: 0.000 min
Response: 144103215
Conc: 10.92 ng/ml

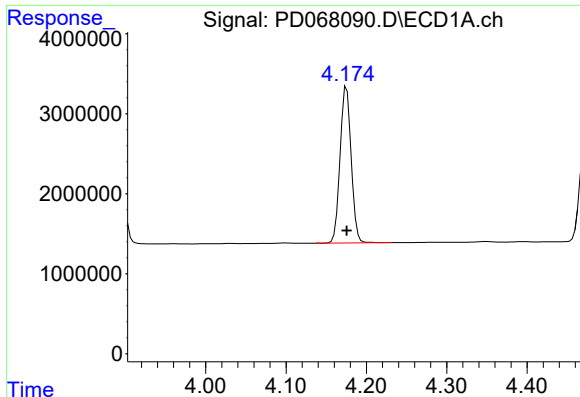

#3 gamma-BHC (Lindane)


R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 18729390
Conc: 10.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

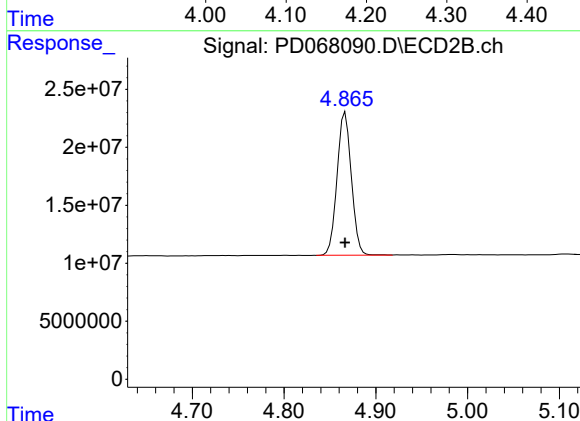


#3 gamma-BHC (Lindane)

R.T.: 4.867 min
Delta R.T.: 0.000 min
Response: 133900410
Conc: 11.01 ng/ml

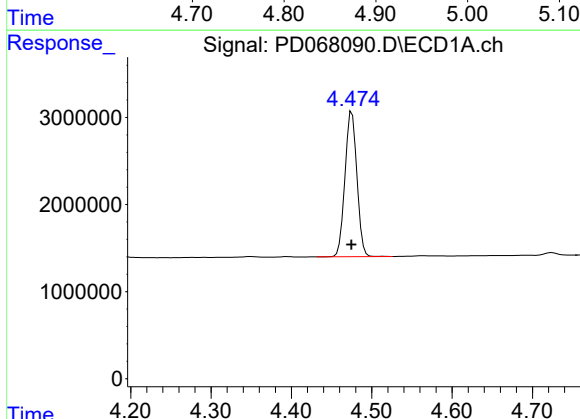


#4 Heptachlor

R.T.: 4.475 min
Delta R.T.: 0.000 min
Response: 17238374
Conc: 10.40 ng/ml

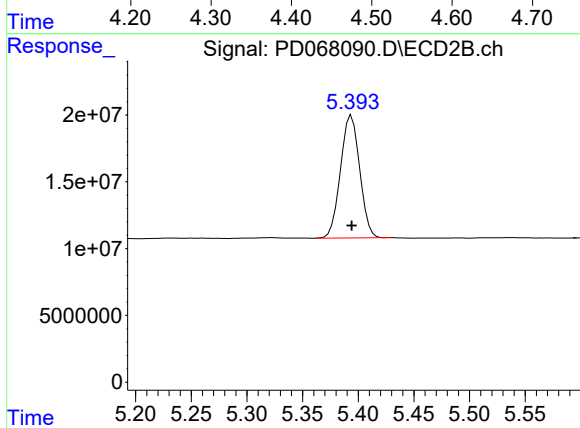

#4 Heptachlor


R.T.: 5.394 min
Delta R.T.: 0.000 min
Response: 110078487
Conc: 10.75 ng/ml

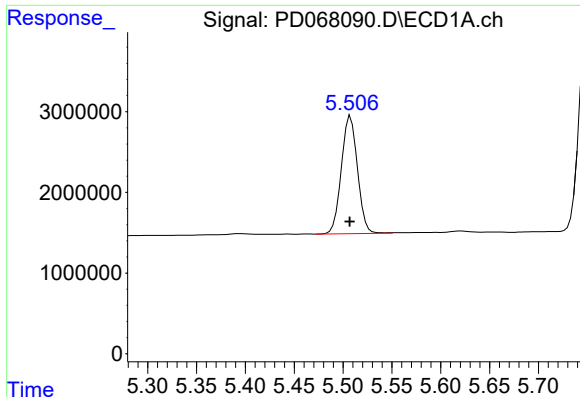

#9 Endosulfan I


R.T.: 5.508 min
Delta R.T.: 0.000 min
Response: 16777204
Conc: 10.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

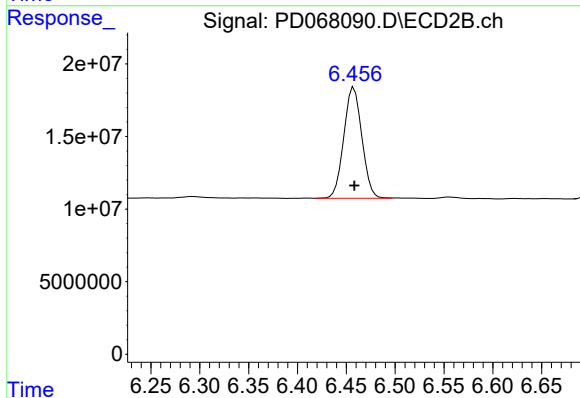


#9 Endosulfan I

R.T.: 6.458 min
Delta R.T.: 0.000 min
Response: 98617564
Conc: 10.87 ng/ml

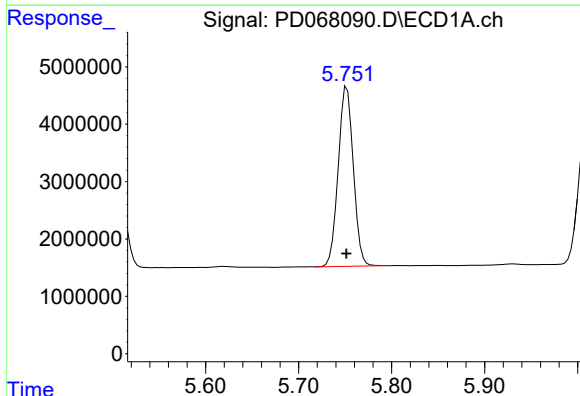


#13 Dieldrin

R.T.: 5.752 min
Delta R.T.: 0.000 min
Response: 35362003
Conc: 20.70 ng/ml

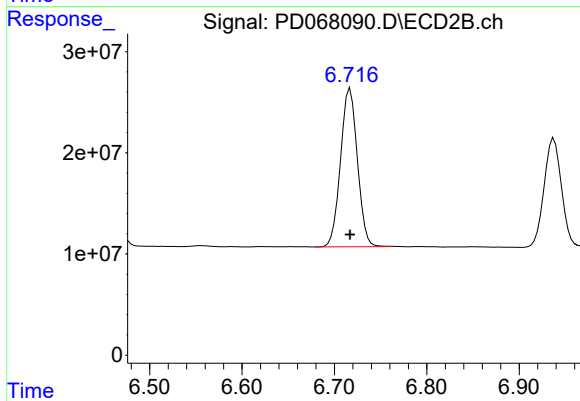

#13 Dieldrin


R.T.: 6.717 min
Delta R.T.: 0.000 min
Response: 198745263
Conc: 21.60 ng/ml

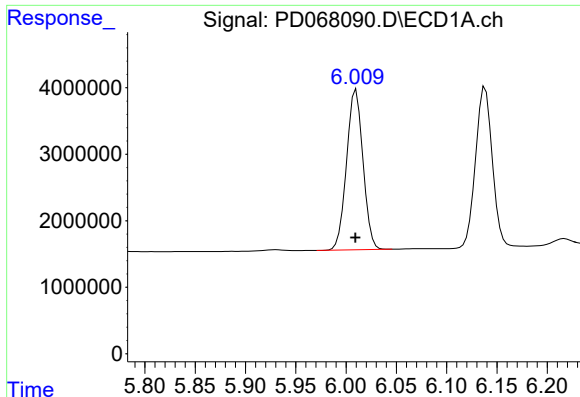

#14 Endrin


R.T.: 6.010 min
Delta R.T.: 0.000 min
Response: 27300261
Conc: 20.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

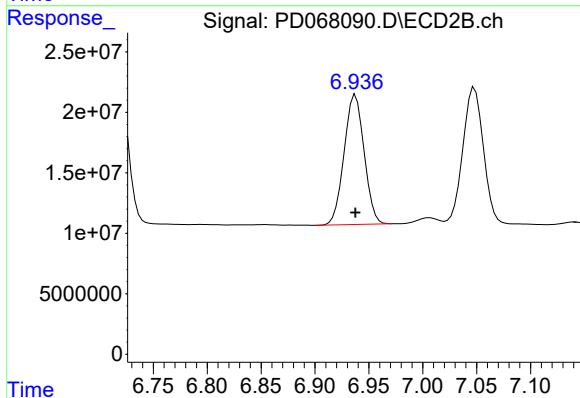


#14 Endrin

R.T.: 6.938 min
Delta R.T.: 0.000 min
Response: 138906423
Conc: 21.16 ng/ml

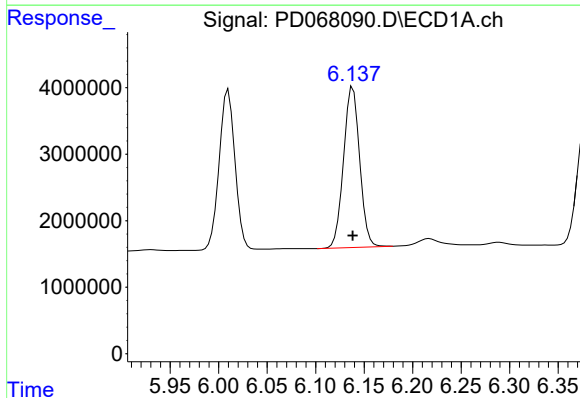


#16 4,4'-DDD

R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 27906778
Conc: 20.69 ng/ml

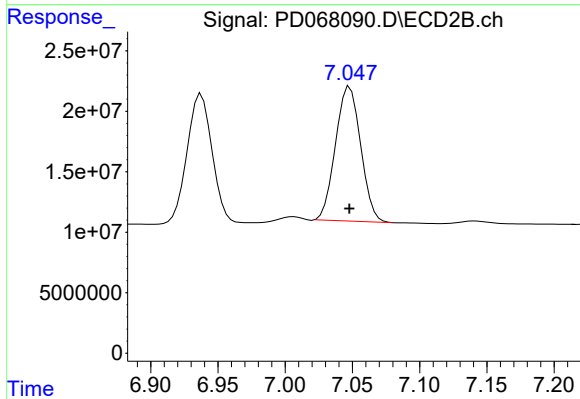

#16 4,4'-DDD


R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 144062379
Conc: 21.19 ng/ml

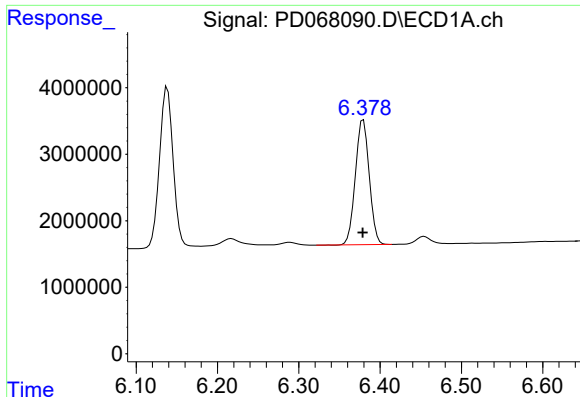

#17 4,4'-DDT


R.T.: 6.379 min
Delta R.T.: 0.000 min
Response: 22247420
Conc: 19.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

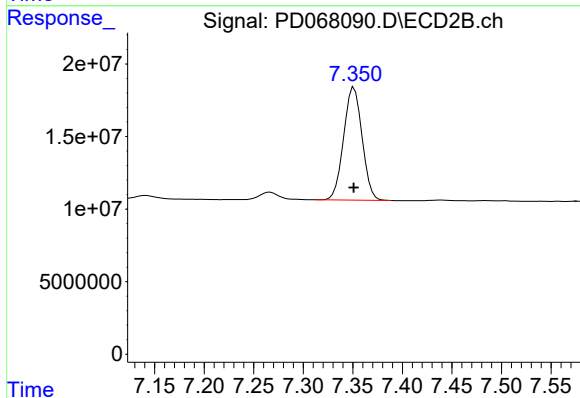


#17 4,4'-DDT

R.T.: 7.351 min
Delta R.T.: 0.000 min
Response: 100850677
Conc: 20.19 ng/ml

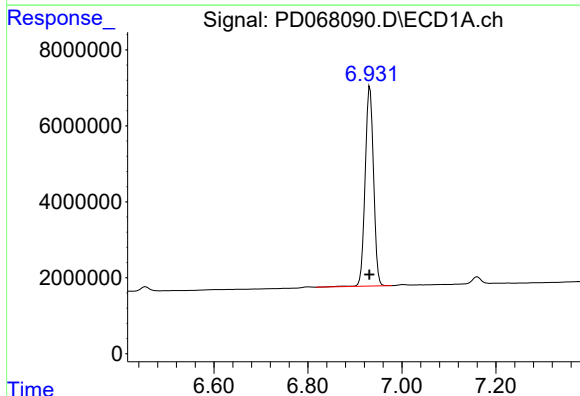


#20 Methoxychlor

R.T.: 6.932 min
Delta R.T.: 0.000 min
Response: 65276524
Conc: 103.23 ng/ml

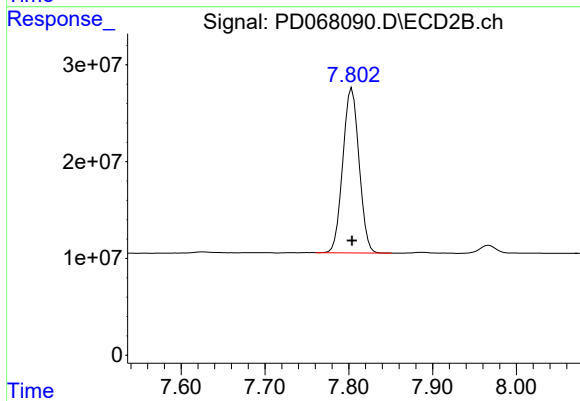

#20 Methoxychlor


R.T.: 7.804 min
Delta R.T.: 0.000 min
Response: 229403326
Conc: 102.87 ng/ml

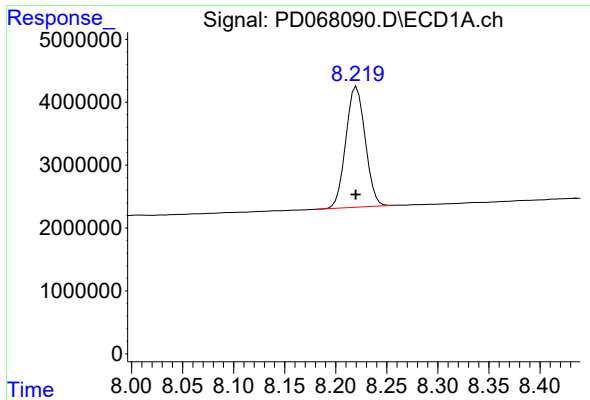

#27 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: 0.000 min
Response: 25328703
Conc: 21.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

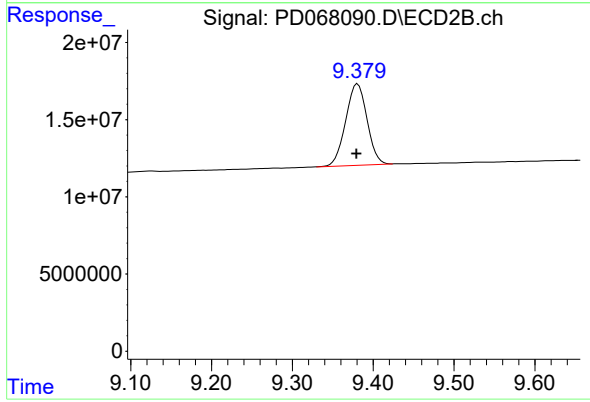

#27 Decachlorobiphenyl

R.T.: 9.381 min
Delta R.T.: 0.001 min
Response: 96750327
Conc: 21.06 ng/ml