

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021822\
 Data File : PD068092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2022 14:29
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 14:59:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 18 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	4.179	27441262	191.4E6	20.000	20.000
27)	SA Decachlor...	8.219	9.379	48178899	183.8E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.892	4.575	37965132	264.0E6	20.000	20.000
3)	MA gamma-BHC...	4.175	4.867	36114955	243.2E6	20.000	20.000
4)	MA Heptachlor	4.475	5.394	33148211	204.8E6	20.000	20.000
9)	A Endosulfan I	5.507	6.458	31412461	181.5E6	20.000	20.000
13)	MA Dieldrin	5.752	6.717	68332212	368.1E6	40.000	40.000
14)	MA Endrin	6.009	6.938	53642146	262.6E6	40.000	40.000
16)	A 4,4'-DDD	6.138	7.048	53952383	271.9E6	40.000	40.000
17)	MA 4,4'-DDT	6.379	7.351	45365450	199.8E6	40.000	40.000
20)	A Methoxychlor	6.931	7.804	126.5E6	446.0E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021822\
Data File : PD068092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2022 14:29
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 14:59:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 18 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

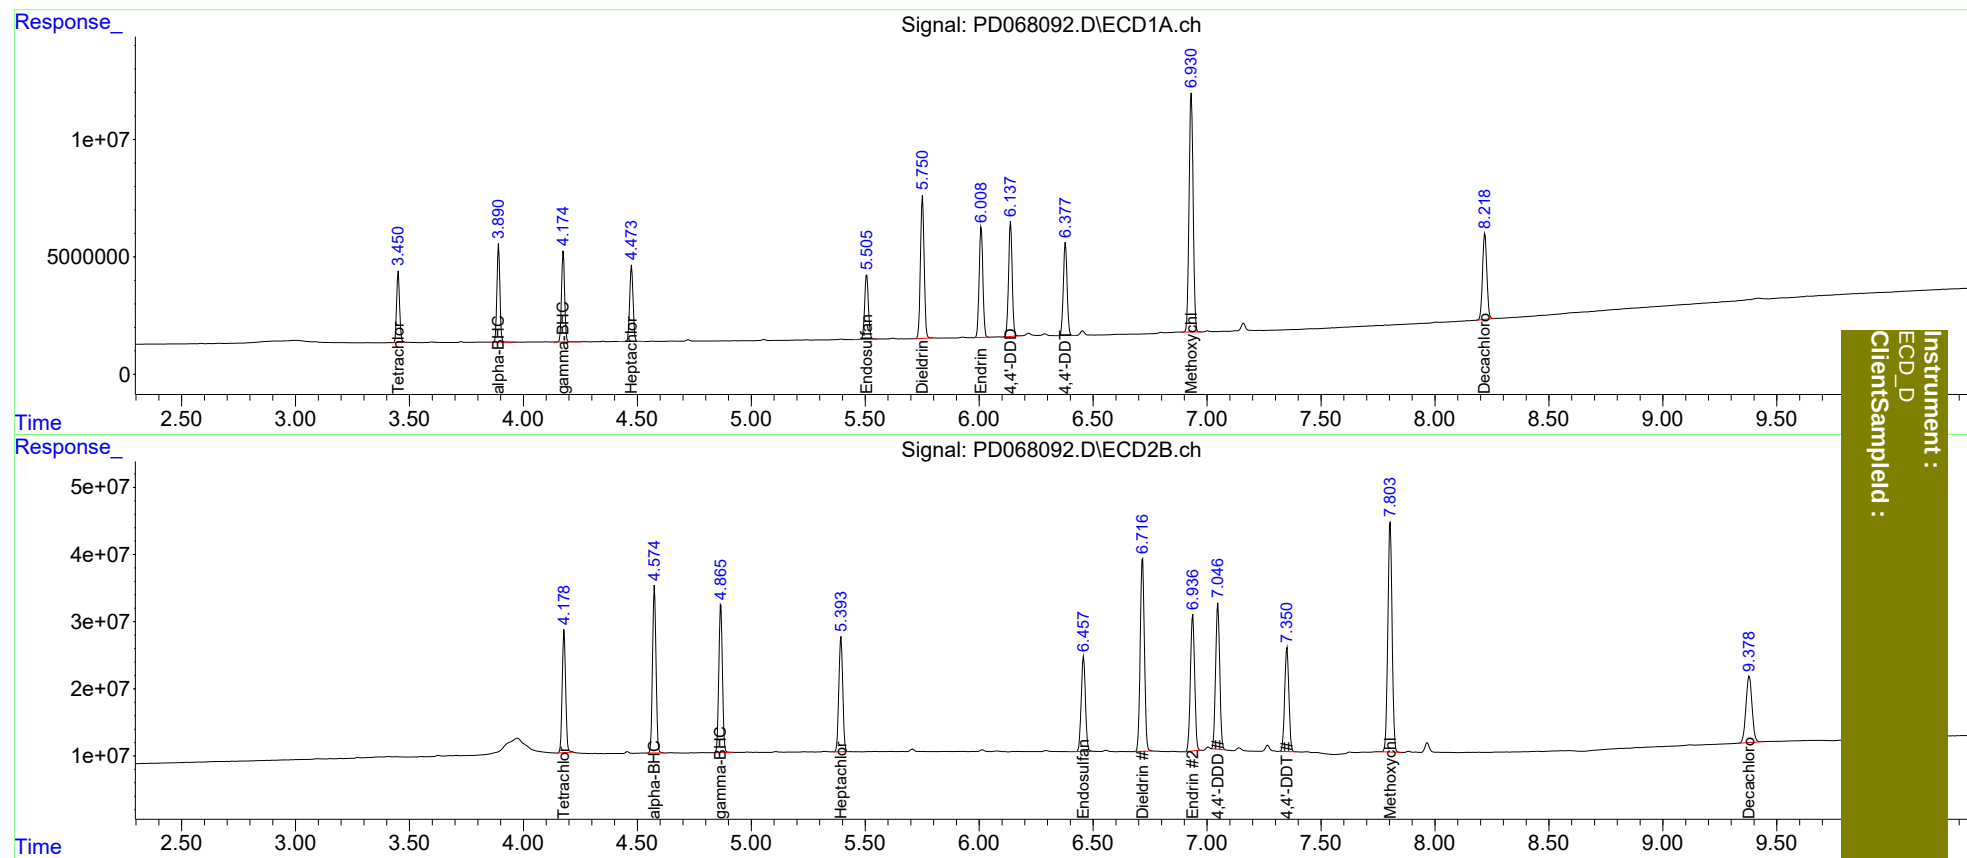


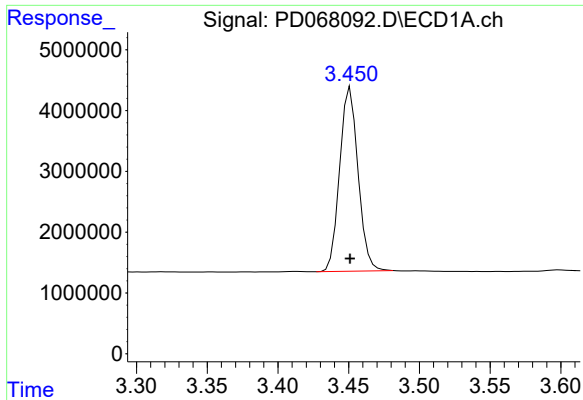

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 27441262
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

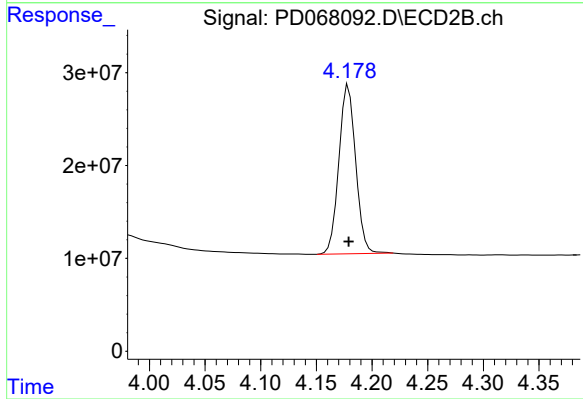


#1 Tetrachloro-m-xylene

R.T.: 4.179 min
Delta R.T.: 0.000 min
Response: 191382593
Conc: 20.00 ng/ml

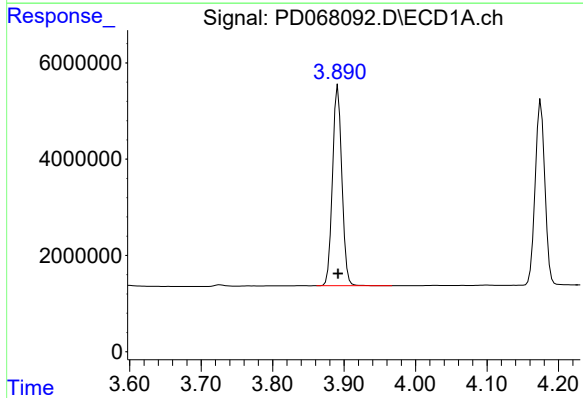


#2 alpha-BHC

R.T.: 3.892 min
Delta R.T.: 0.000 min
Response: 37965132
Conc: 20.00 ng/ml

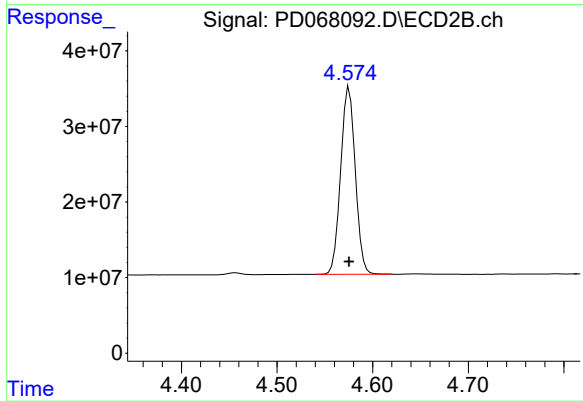

#2 alpha-BHC


R.T.: 4.575 min
Delta R.T.: 0.000 min
Response: 264040214
Conc: 20.00 ng/ml

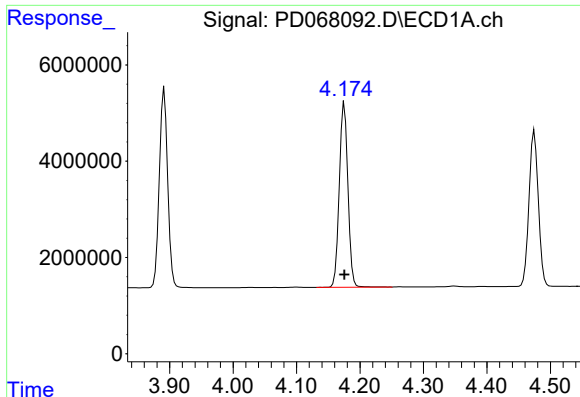

#3 gamma-BHC (Lindane)


R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 36114955
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

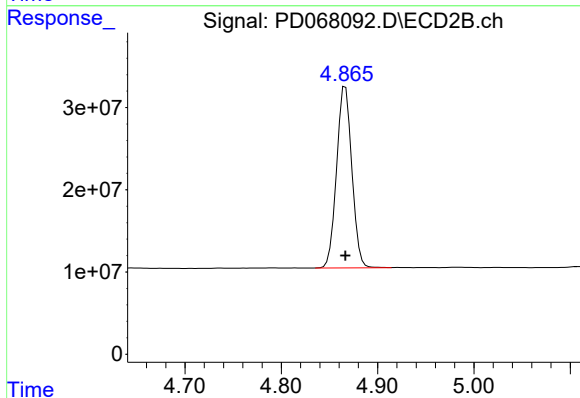


#3 gamma-BHC (Lindane)

R.T.: 4.867 min
Delta R.T.: 0.000 min
Response: 243213208
Conc: 20.00 ng/ml

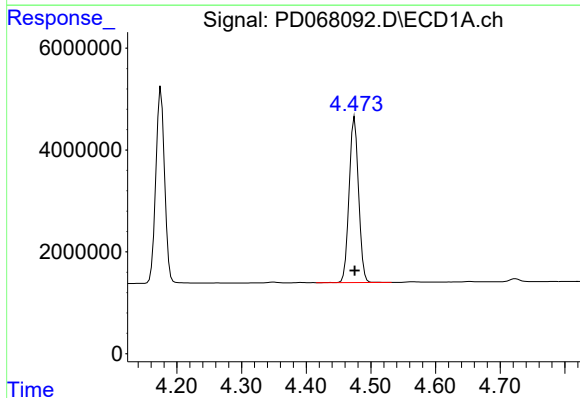


#4 Heptachlor

R.T.: 4.475 min
Delta R.T.: 0.000 min
Response: 33148211
Conc: 20.00 ng/ml

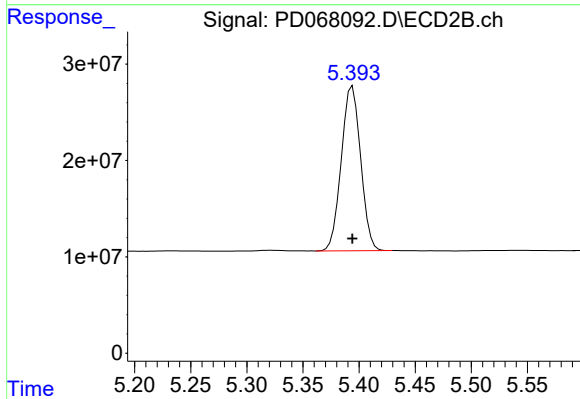

#4 Heptachlor


R.T.: 5.394 min
Delta R.T.: 0.000 min
Response: 204781017
Conc: 20.00 ng/ml

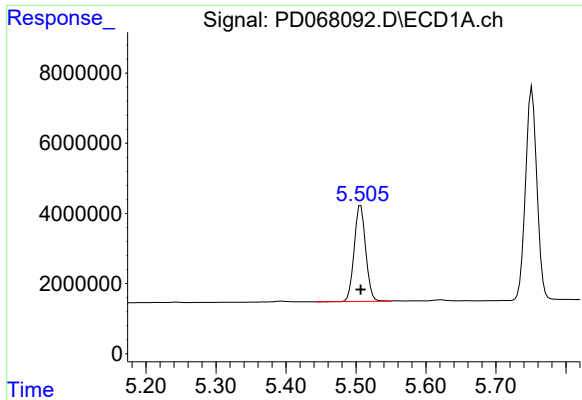

#9 Endosulfan I


R.T.: 5.507 min
Delta R.T.: 0.000 min
Response: 31412461
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

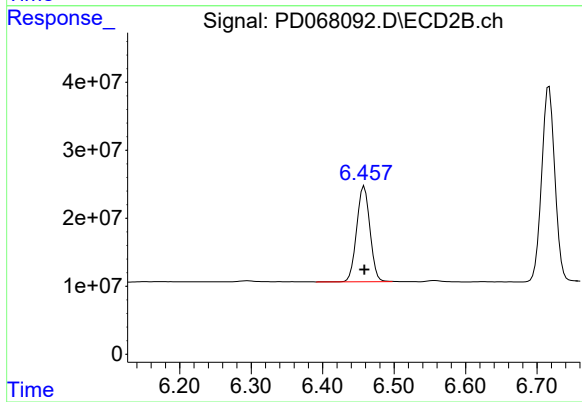


#9 Endosulfan I

R.T.: 6.458 min
Delta R.T.: 0.000 min
Response: 181461924
Conc: 20.00 ng/ml

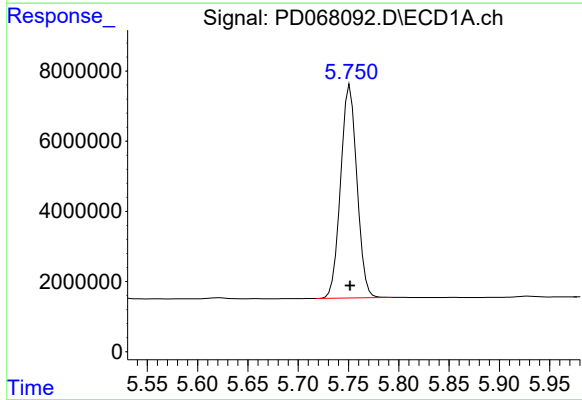


#13 Dieldrin

R.T.: 5.752 min
Delta R.T.: 0.000 min
Response: 68332212
Conc: 40.00 ng/ml

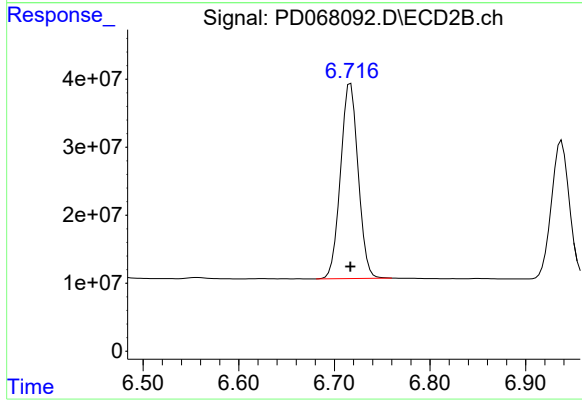

#13 Dieldrin


R.T.: 6.717 min
Delta R.T.: 0.000 min
Response: 368070268
Conc: 40.00 ng/ml

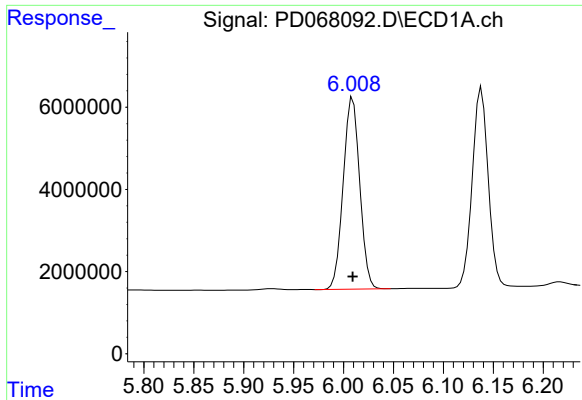

#14 Endrin


R.T.: 6.009 min
Delta R.T.: 0.000 min
Response: 53642146
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

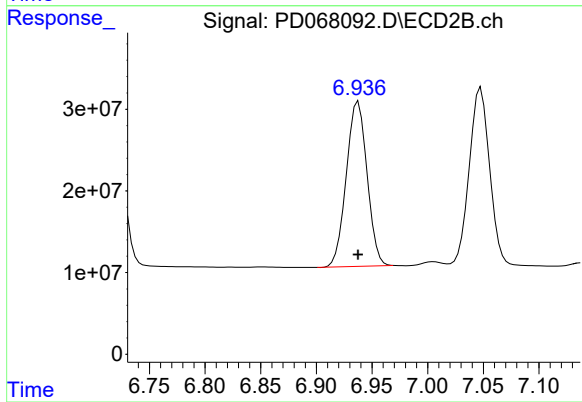


#14 Endrin

R.T.: 6.938 min
Delta R.T.: 0.000 min
Response: 262604806
Conc: 40.00 ng/ml

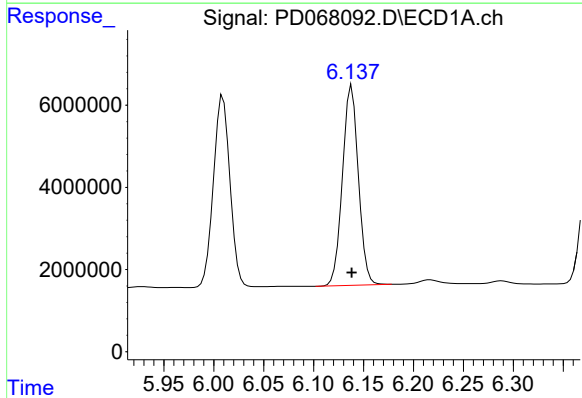


#16 4,4'-DDD

R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 53952383
Conc: 40.00 ng/ml

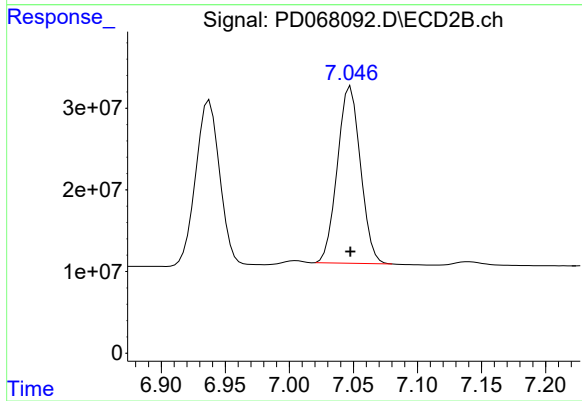

#16 4,4'-DDD


R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 271919890
Conc: 40.00 ng/ml

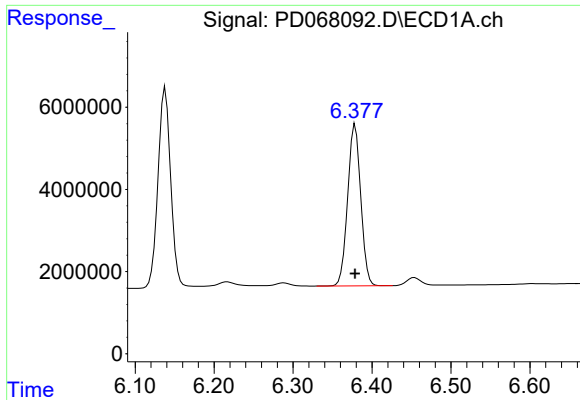

#17 4,4'-DDT


R.T.: 6.379 min
Delta R.T.: 0.000 min
Response: 45365450
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

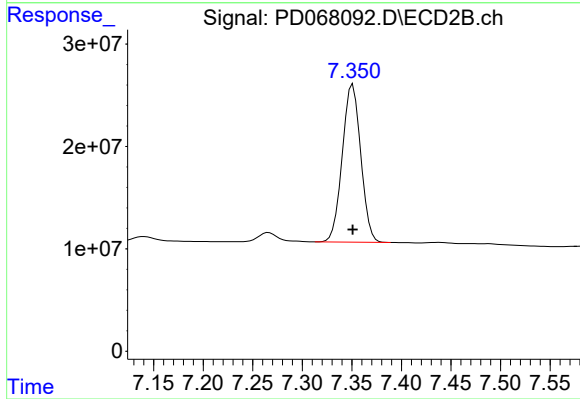


#17 4,4'-DDT

R.T.: 7.351 min
Delta R.T.: 0.000 min
Response: 199797876
Conc: 40.00 ng/ml

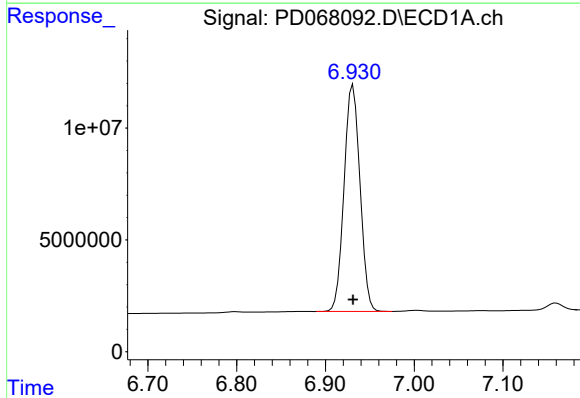


#20 Methoxychlor

R.T.: 6.931 min
Delta R.T.: 0.000 min
Response: 126466246
Conc: 200.00 ng/ml

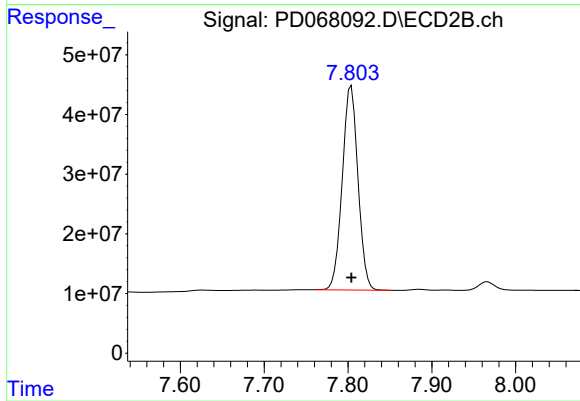

#20 Methoxychlor


R.T.: 7.804 min
Delta R.T.: 0.000 min
Response: 446009484
Conc: 200.00 ng/ml

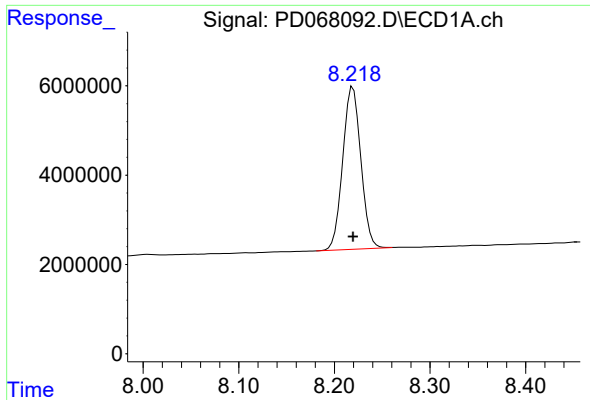

#27 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: 0.000 min
Response: 48178899
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

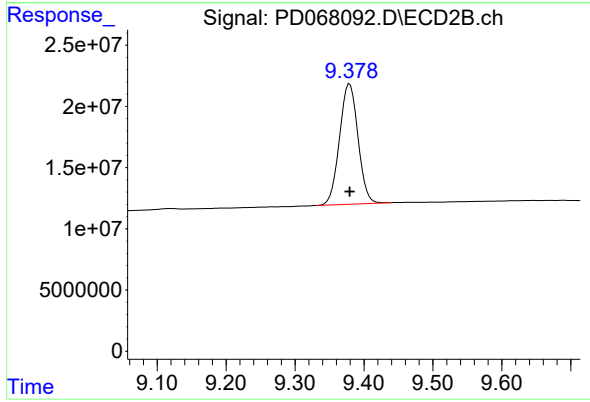

#27 Decachlorobiphenyl

R.T.: 9.379 min
Delta R.T.: 0.000 min
Response: 183767049
Conc: 40.00 ng/ml