

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021822\
 Data File : PD068094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2022 14:57
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 15:14:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 18 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	4.179	54924805	375.0E6	37.810	35.794
27)	SA Decachlor...	8.219	9.378	93863822	348.6E6	74.771	73.415
Target Compounds							
2)	A alpha-BHC	3.891	4.575	80970576	525.2E6	42.099	37.186
3)	MA gamma-BHC...	4.175	4.866	75954050	479.1E6	40.925	36.764
4)	MA Heptachlor	4.475	5.393	68576008	400.0E6	39.763	36.812
9)	A Endosulfan I	5.507	6.458	63026954	345.8E6	38.241	35.946
13)	MA Dieldrin	5.751	6.716	144.0E6	710.2E6	82.777	72.884
14)	MA Endrin	6.010	6.937	110.9E6	503.6E6	81.423	73.327
16)	A 4,4'-DDD	6.138	7.047	111.7E6	527.3E6	81.462	74.591
17)	MA 4,4'-DDT	6.379	7.350	97119639	400.2E6	87.843	79.943
20)	A Methoxychlor	6.931	7.803	255.6E6	876.5E6	400.440	385.119


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021822\
Data File : PD068094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2022 14:57
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 15:14:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 18 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

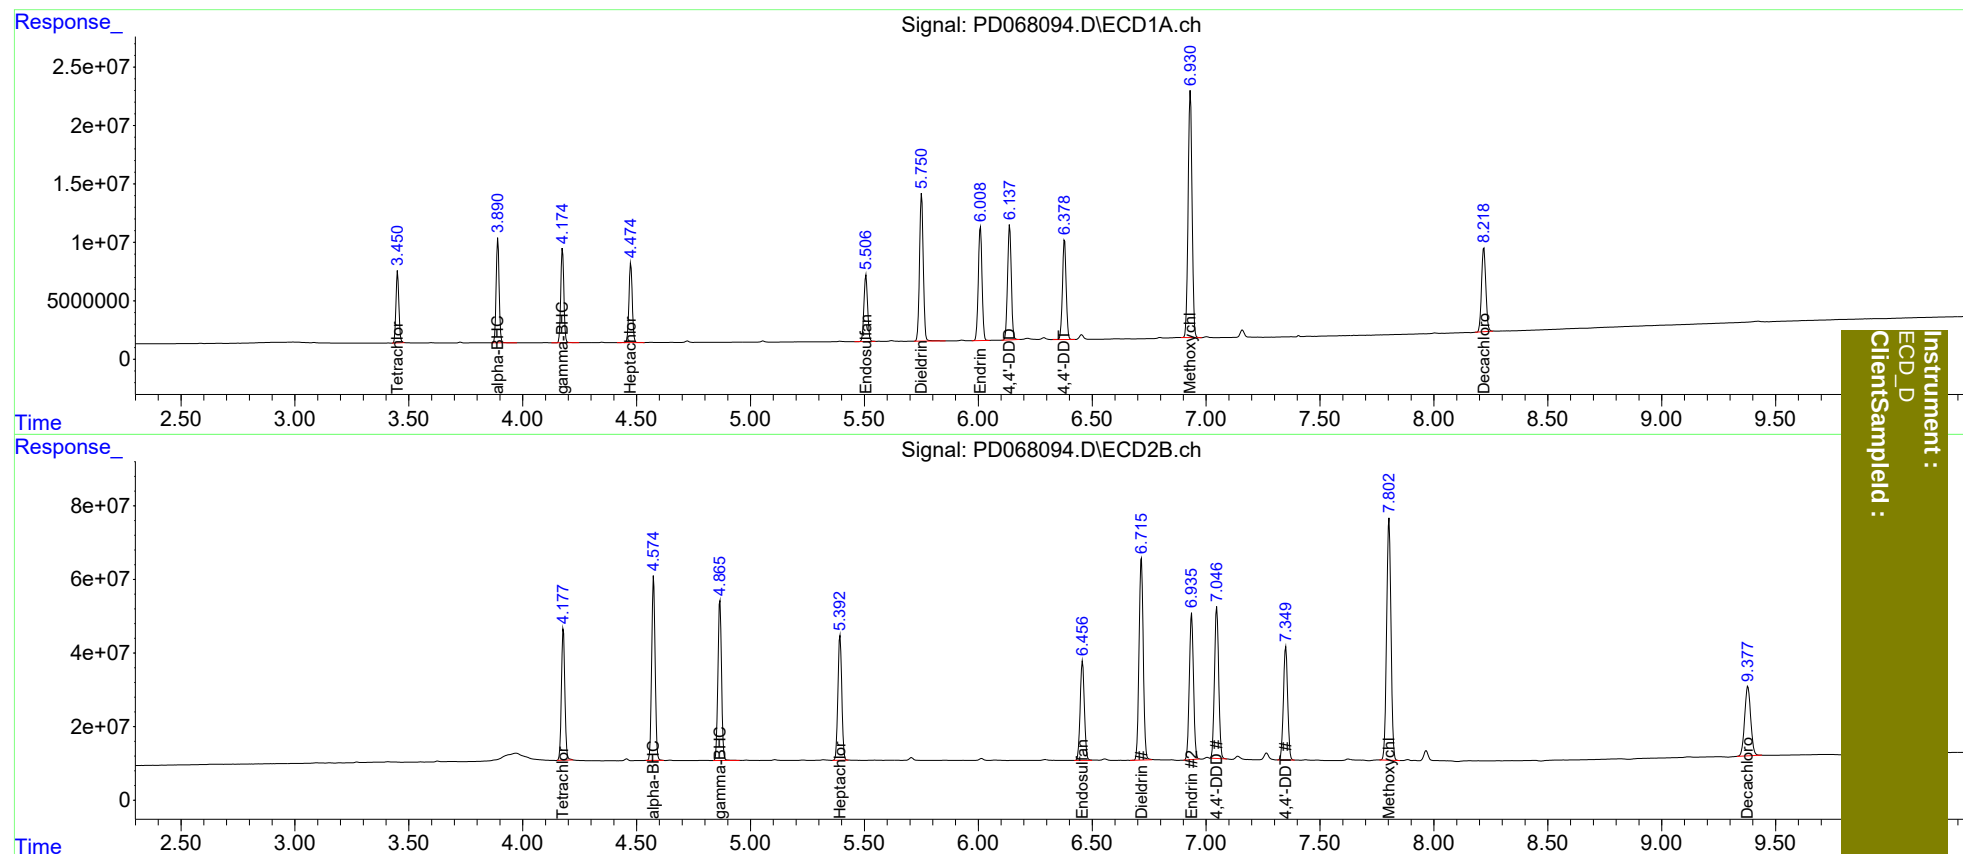


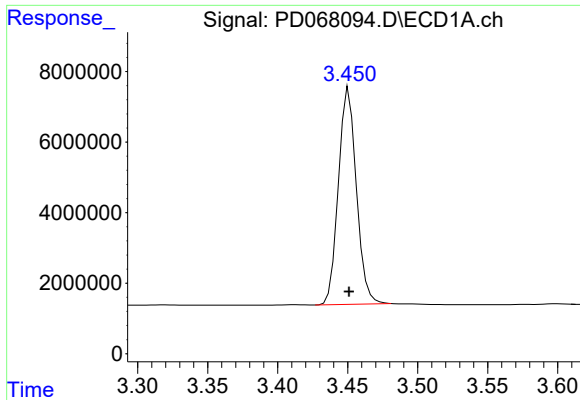

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 54924805
Conc: 37.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

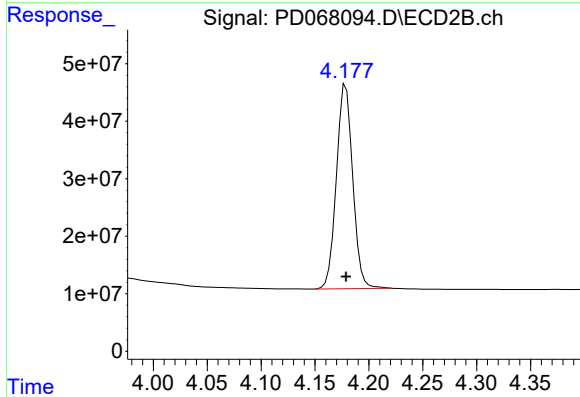


#1 Tetrachloro-m-xylene

R.T.: 4.179 min
Delta R.T.: 0.000 min
Response: 375012109
Conc: 35.79 ng/ml

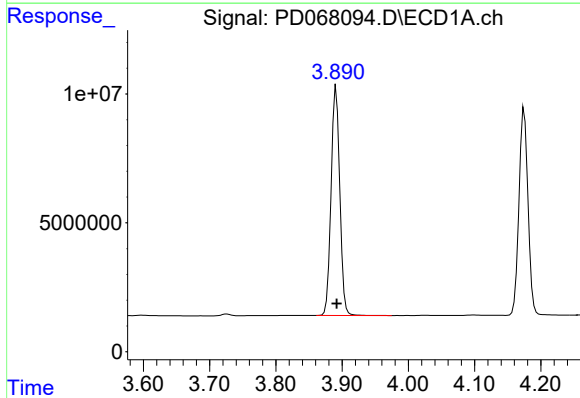


#2 alpha-BHC

R.T.: 3.891 min
Delta R.T.: 0.000 min
Response: 80970576
Conc: 42.10 ng/ml

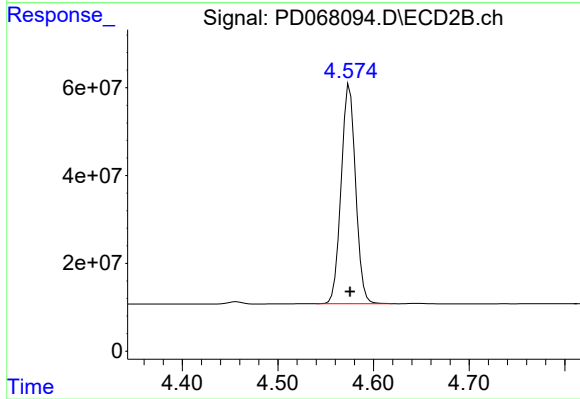

#2 alpha-BHC


R.T.: 4.575 min
Delta R.T.: 0.000 min
Response: 525233688
Conc: 37.19 ng/ml

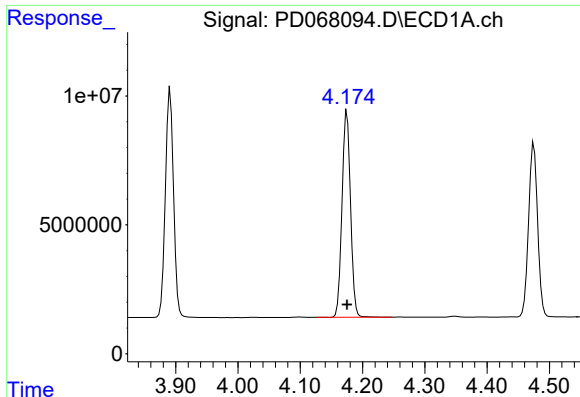

#3 gamma-BHC (Lindane)


R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 75954050
Conc: 40.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

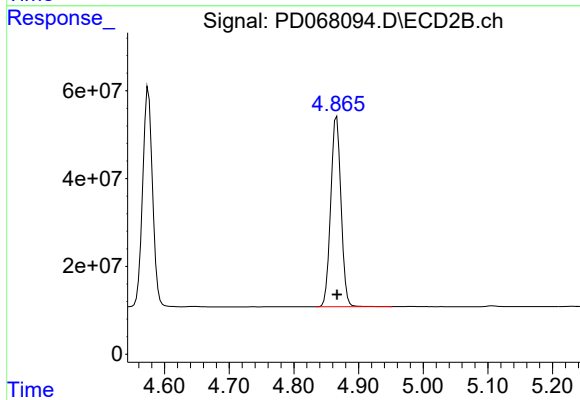


#3 gamma-BHC (Lindane)

R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 479066809
Conc: 36.76 ng/ml

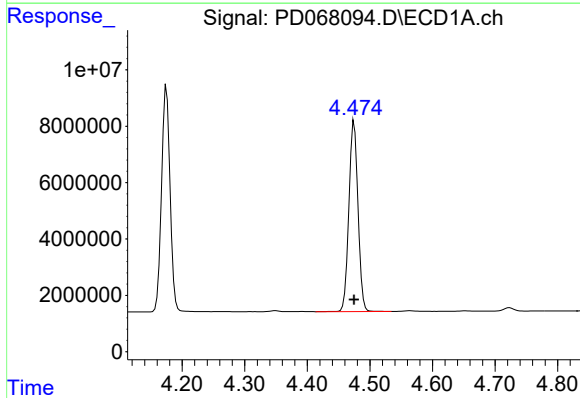


#4 Heptachlor

R.T.: 4.475 min
Delta R.T.: 0.000 min
Response: 68576008
Conc: 39.76 ng/ml

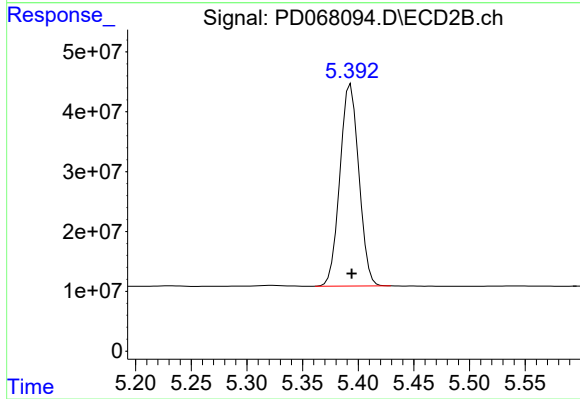

#4 Heptachlor


R.T.: 5.393 min
Delta R.T.: 0.000 min
Response: 400033812
Conc: 36.81 ng/ml

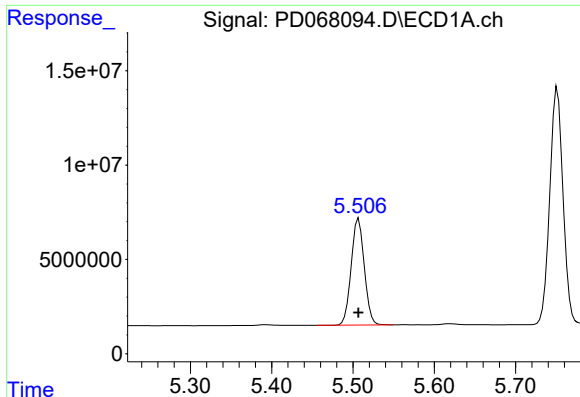

#9 Endosulfan I


R.T.: 5.507 min
Delta R.T.: 0.000 min
Response: 63026954
Conc: 38.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

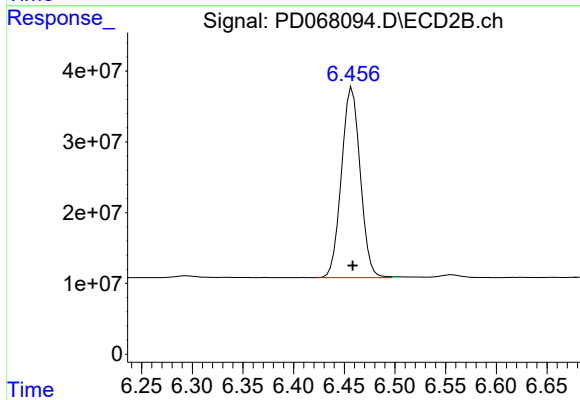


#9 Endosulfan I

R.T.: 6.458 min
Delta R.T.: 0.000 min
Response: 345847792
Conc: 35.95 ng/ml

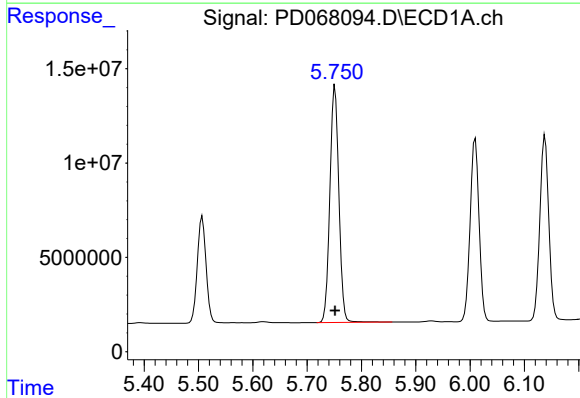


#13 Dieldrin

R.T.: 5.751 min
Delta R.T.: 0.000 min
Response: 143982218
Conc: 82.78 ng/ml

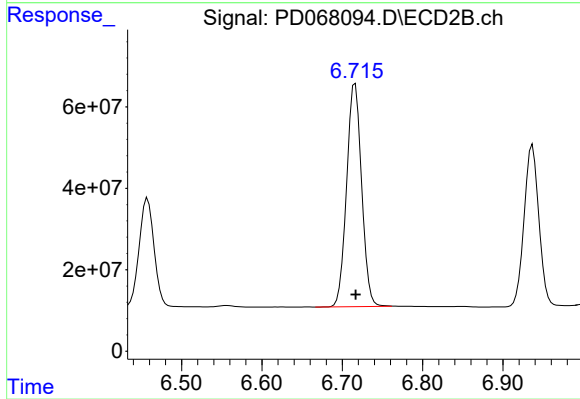

#13 Dieldrin


R.T.: 6.716 min
Delta R.T.: 0.000 min
Response: 710168924
Conc: 72.88 ng/ml

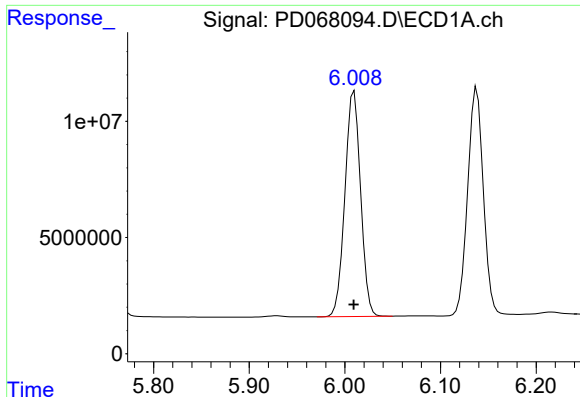

#14 Endrin


R.T.: 6.010 min
Delta R.T.: 0.000 min
Response: 110863828
Conc: 81.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

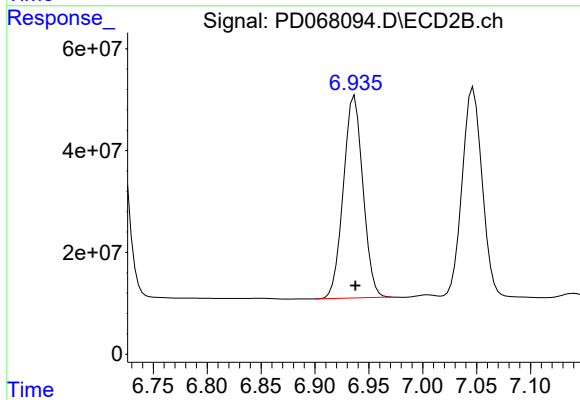


#14 Endrin

R.T.: 6.937 min
Delta R.T.: 0.000 min
Response: 503551175
Conc: 73.33 ng/ml

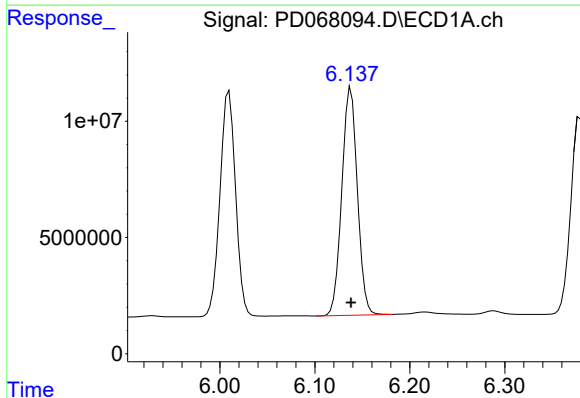


#16 4,4'-DDD

R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 111720470
Conc: 81.46 ng/ml

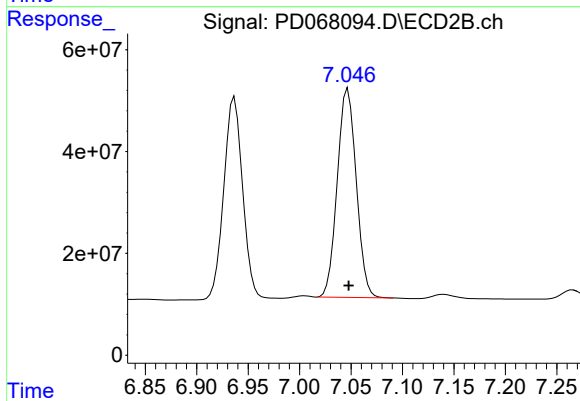

#16 4,4'-DDD


R.T.: 7.047 min
Delta R.T.: 0.000 min
Response: 527263599
Conc: 74.59 ng/ml

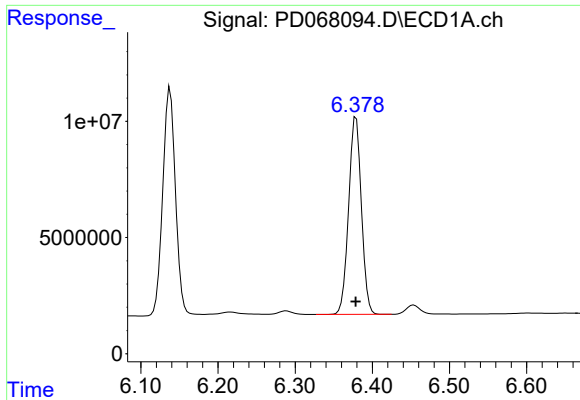

#17 4,4'-DDT


R.T.: 6.379 min
Delta R.T.: 0.000 min
Response: 97119639
Conc: 87.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

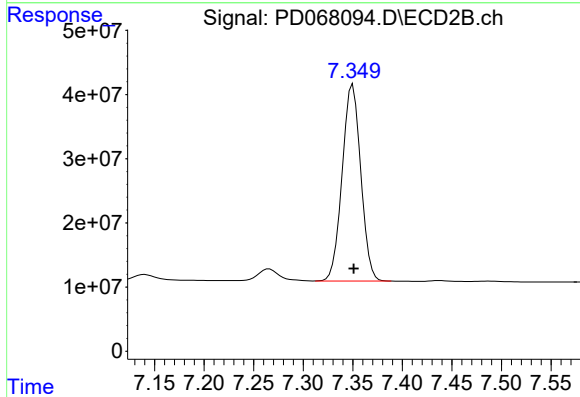


#17 4,4'-DDT

R.T.: 7.350 min
Delta R.T.: 0.000 min
Response: 400163494
Conc: 79.94 ng/ml

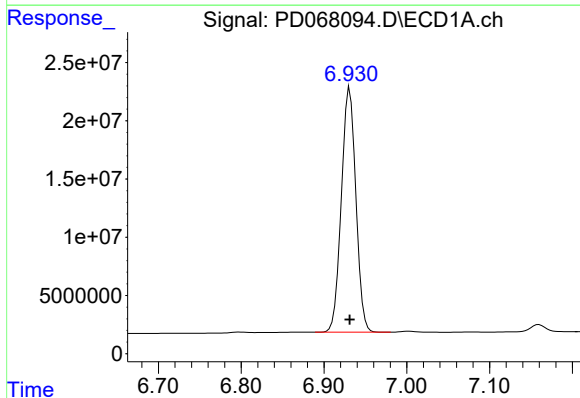


#20 Methoxychlor

R.T.: 6.931 min
Delta R.T.: 0.000 min
Response: 255572486
Conc: 400.44 ng/ml

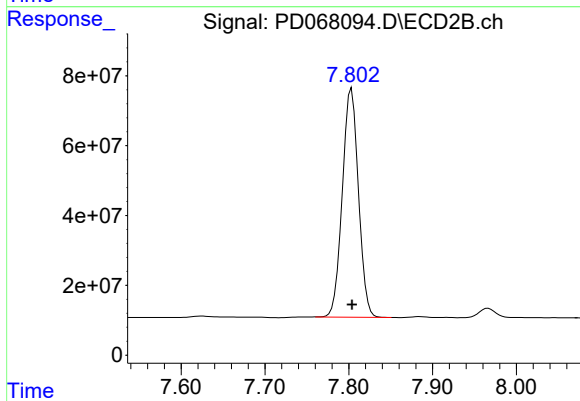

#20 Methoxychlor


R.T.: 7.803 min
Delta R.T.: 0.000 min
Response: 876455544
Conc: 385.12 ng/ml

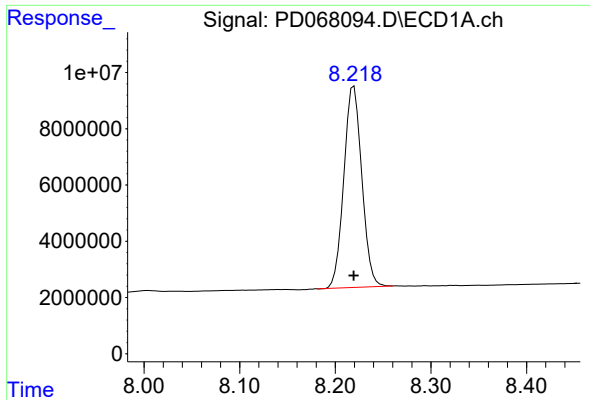

#27 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: 0.000 min
Response: 93863822
Conc: 74.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

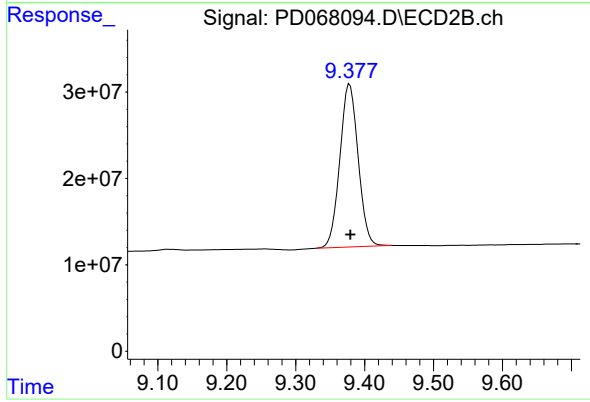

#27 Decachlorobiphenyl

R.T.: 9.378 min
Delta R.T.: 0.000 min
Response: 348561773
Conc: 73.42 ng/ml