

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021822\
 Data File : PD068096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2022 15:25
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 15:44:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 18 15:15:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	4.178	109.9E6	697.2E6	76.728	68.340
27)	SA Decachlor...	8.219	9.379	187.4E6	650.4E6	151.735	139.869
Target Compounds							
2)	A alpha-BHC	3.891	4.574	169.0E6	1006.3E6	86.748	72.520
3)	MA gamma-BHC...	4.175	4.866	157.4E6	915.0E6	84.314	71.669
4)	MA Heptachlor	4.475	5.393	142.1E6	766.9E6	82.494	72.010
9)	A Endosulfan I	5.507	6.457	129.1E6	647.0E6	79.207	68.991
13)	MA Dieldrin	5.752	6.716	300.3E6	1362.2E6	171.183	142.978
14)	MA Endrin	6.009	6.937	230.6E6	964.7E6	168.602	143.475
16)	A 4,4'-DDD	6.138	7.047	231.5E6	1003.7E6	168.016	144.435
17)	MA 4,4'-DDT	6.378	7.350	208.8E6	789.0E6	184.340	157.655
20)	A Methoxychlor	6.931	7.803	516.4E6	1705.0E6	808.832	756.219


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021822\
Data File : PD068096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2022 15:25
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 15:44:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 18 15:15:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

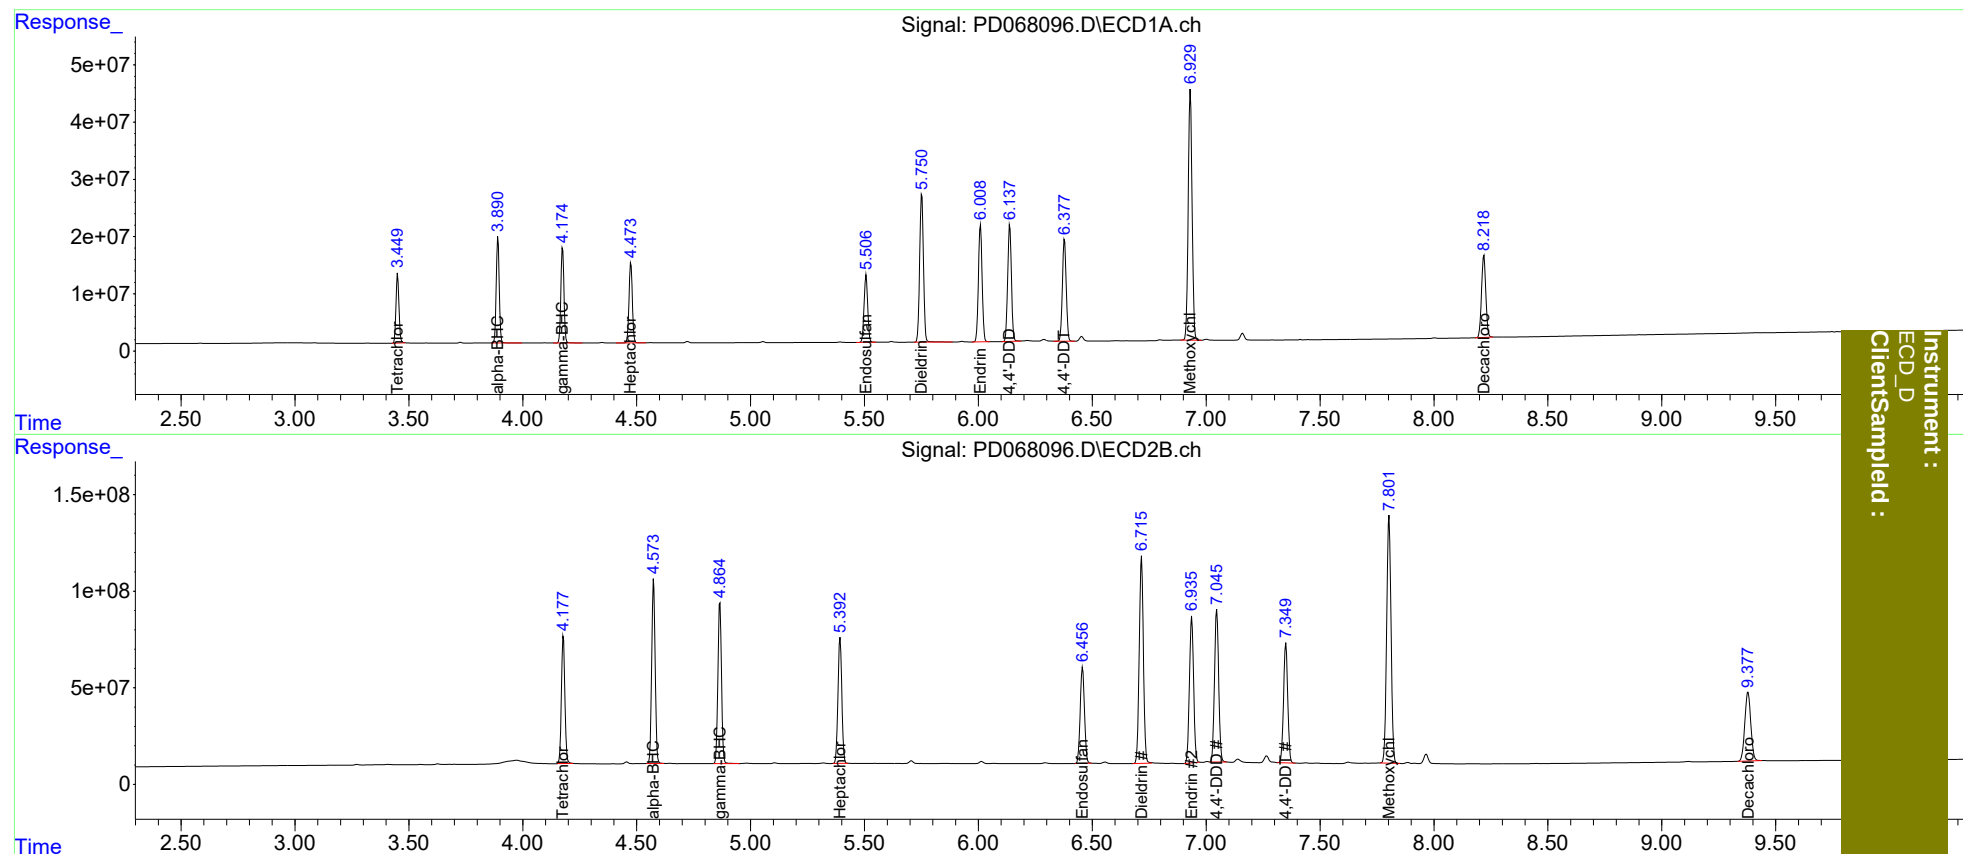


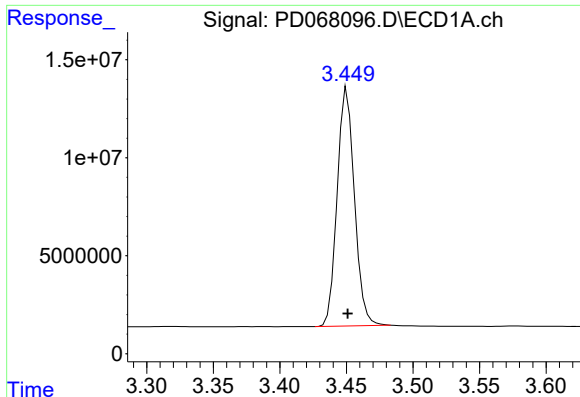

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 109933229
Conc: 76.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

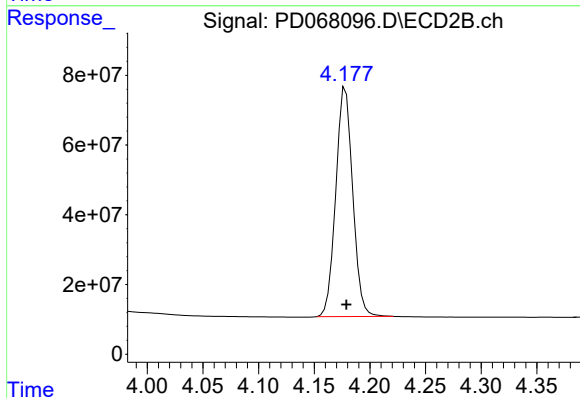


#1 Tetrachloro-m-xylene

R.T.: 4.178 min
Delta R.T.: 0.000 min
Response: 697177215
Conc: 68.34 ng/ml

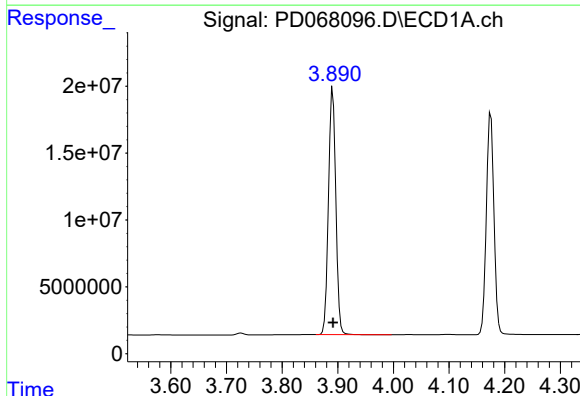


#2 alpha-BHC

R.T.: 3.891 min
Delta R.T.: 0.000 min
Response: 169036117
Conc: 86.75 ng/ml

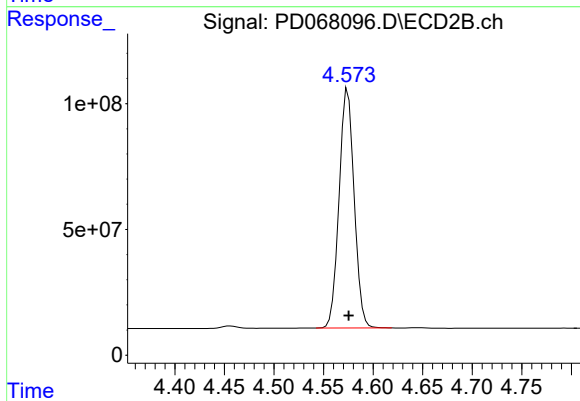

#2 alpha-BHC


R.T.: 4.574 min
Delta R.T.: 0.000 min
Response: 1006298366
Conc: 72.52 ng/ml

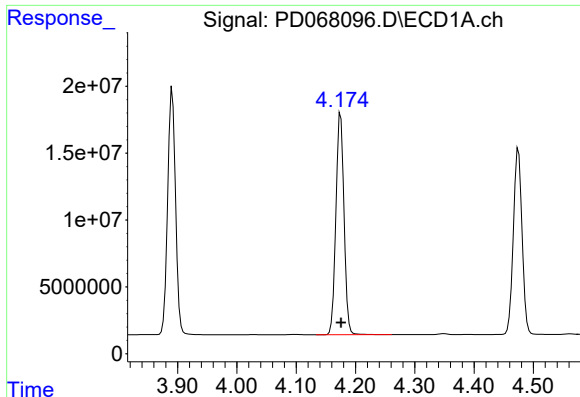

#3 gamma-BHC (Lindane)


R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 157385791
Conc: 84.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

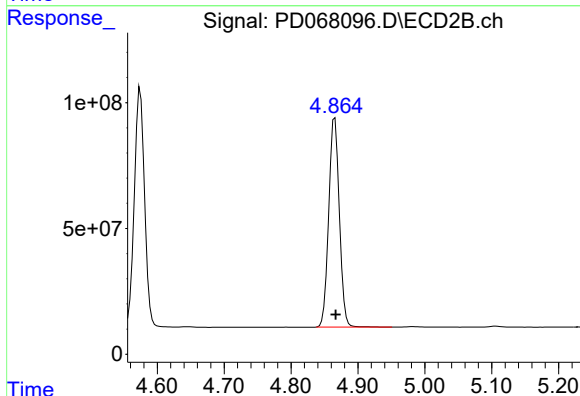


#3 gamma-BHC (Lindane)

R.T.: 4.866 min
Delta R.T.: -0.001 min
Response: 915029476
Conc: 71.67 ng/ml

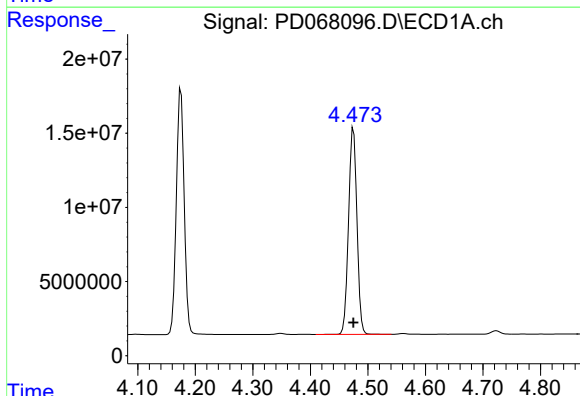


#4 Heptachlor

R.T.: 4.475 min
Delta R.T.: 0.000 min
Response: 142060055
Conc: 82.49 ng/ml

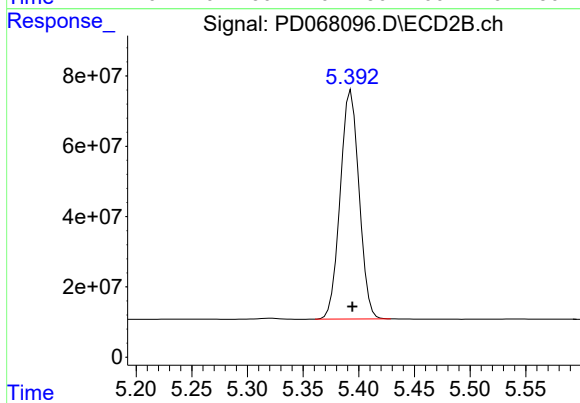

#4 Heptachlor


R.T.: 5.393 min
Delta R.T.: 0.000 min
Response: 766938557
Conc: 72.01 ng/ml

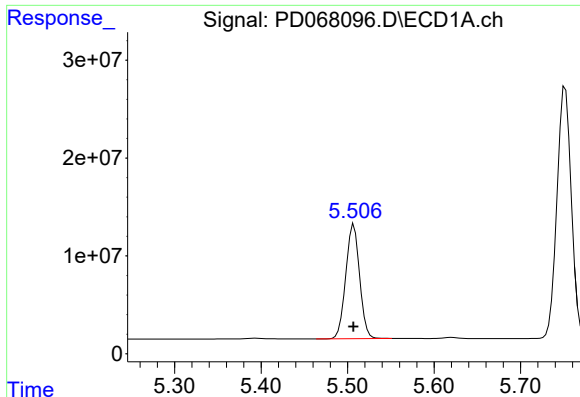

#9 Endosulfan I


R.T.: 5.507 min
Delta R.T.: 0.000 min
Response: 129109977
Conc: 79.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

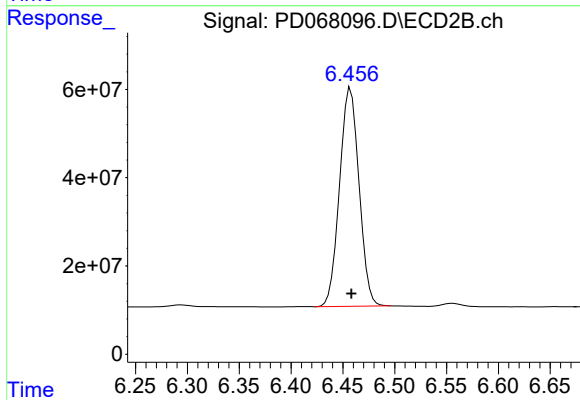


#9 Endosulfan I

R.T.: 6.457 min
Delta R.T.: 0.000 min
Response: 646961107
Conc: 68.99 ng/ml

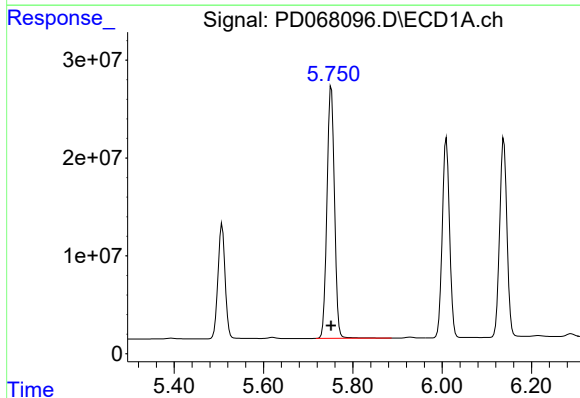


#13 Dieldrin

R.T.: 5.752 min
Delta R.T.: 0.000 min
Response: 300339901
Conc: 171.18 ng/ml

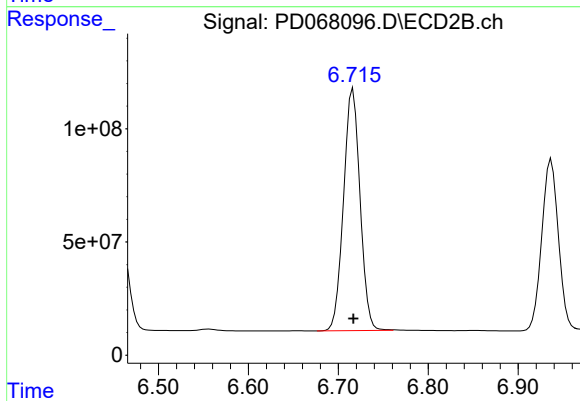

#13 Dieldrin


R.T.: 6.716 min
Delta R.T.: 0.000 min
Response: 1362172124
Conc: 142.98 ng/ml

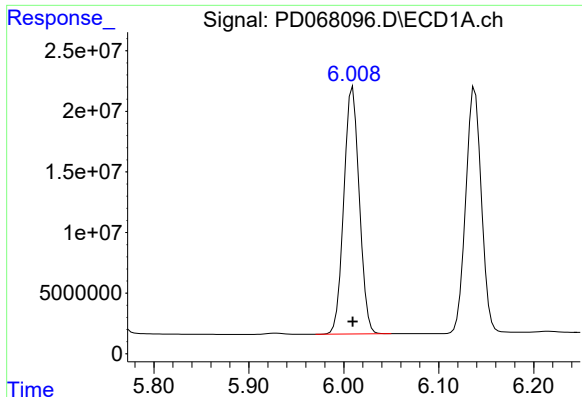

#14 Endrin


R.T.: 6.009 min
Delta R.T.: 0.000 min
Response: 230586442
Conc: 168.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

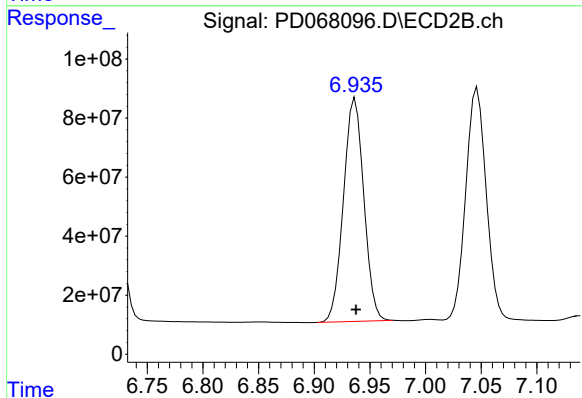


#14 Endrin

R.T.: 6.937 min
Delta R.T.: 0.000 min
Response: 964719505
Conc: 143.47 ng/ml

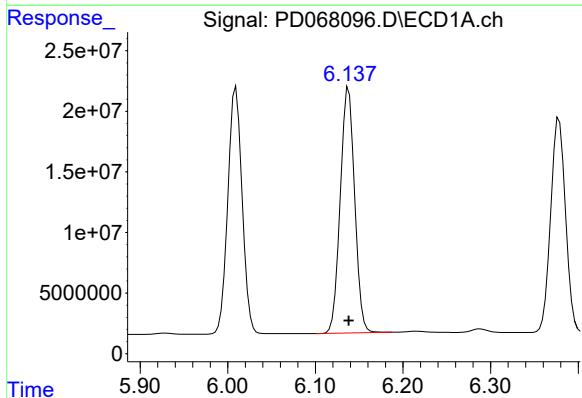


#16 4,4'-DDD

R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 231477995
Conc: 168.02 ng/ml

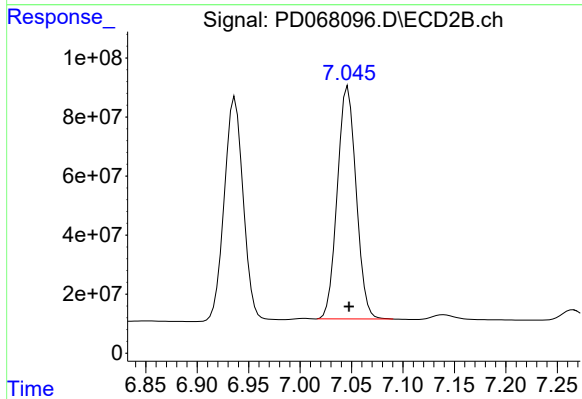

#16 4,4'-DDD


R.T.: 7.047 min
Delta R.T.: -0.001 min
Response: 1003711311
Conc: 144.43 ng/ml

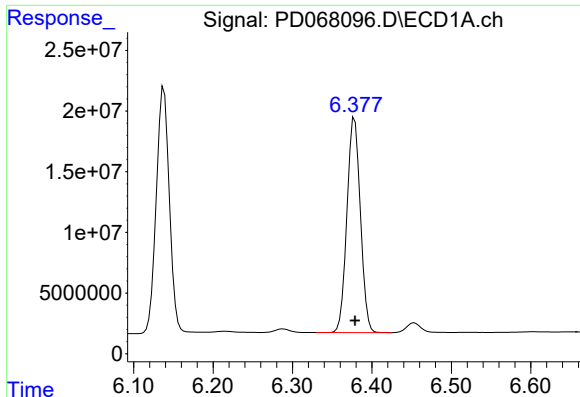

#17 4,4'-DDT


R.T.: 6.378 min
Delta R.T.: 0.000 min
Response: 208802855
Conc: 184.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

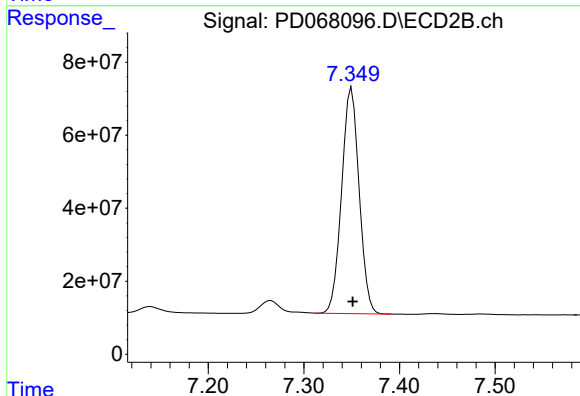


#17 4,4'-DDT

R.T.: 7.350 min
Delta R.T.: 0.000 min
Response: 789021017
Conc: 157.66 ng/ml

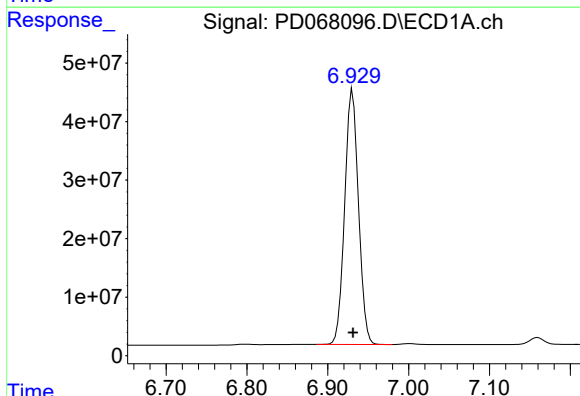


#20 Methoxychlor

R.T.: 6.931 min
Delta R.T.: 0.000 min
Response: 516362307
Conc: 808.83 ng/ml

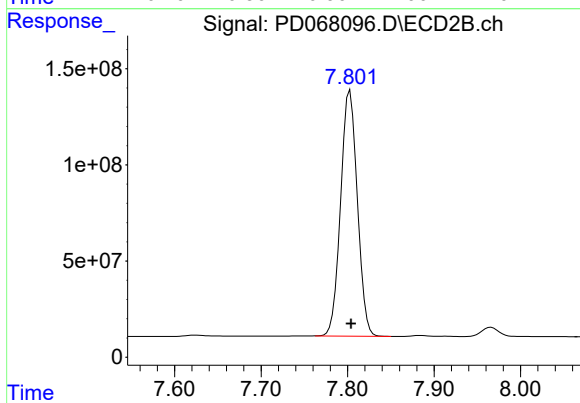

#20 Methoxychlor


R.T.: 7.803 min
Delta R.T.: -0.001 min
Response: 1704999067
Conc: 756.22 ng/ml

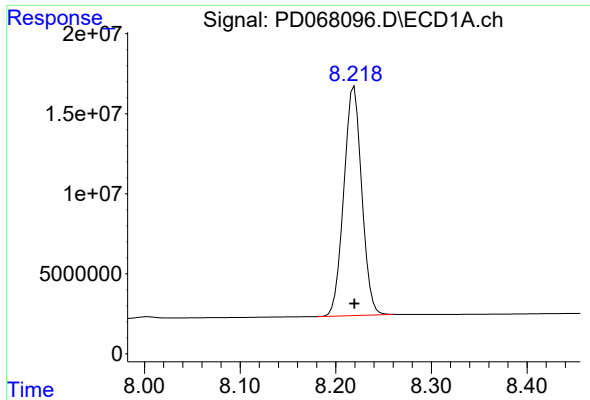

#27 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: 0.000 min
Response: 187368736
Conc: 151.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

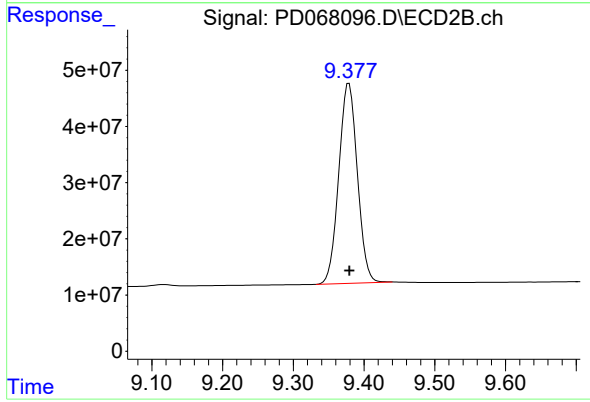

#27 Decachlorobiphenyl

R.T.: 9.379 min
Delta R.T.: 0.000 min
Response: 650410190
Conc: 139.87 ng/ml