

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021822\
 Data File : PD068097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2022 15:39
 Operator : AR\AJ
 Sample : INDB501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 15:53:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 18 15:51:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	4.178	106.9E6	669.7E6	77.675	68.753
27)	SA Decachlor...	8.219	9.379	185.9E6	641.6E6	153.265	140.524
Target Compounds							
5)	MB Aldrin	4.723	5.706	156.7E6	834.5E6	84.318	70.931
6)	B beta-BHC	4.425	5.028	64225159	380.9E6	74.541	67.659
7)	B delta-BHC	4.630	5.254	155.5E6	889.9E6	86.173	72.030
8)	B Heptachlo...	5.168	6.095	138.2E6	716.2E6	81.229	70.002
10)	B trans-Chl...	5.395	6.331	141.9E6	708.9E6	81.890	70.949
11)	B cis-Chlor...	5.454	6.406	137.7E6	675.1E6	80.699	70.098
12)	B 4,4'-DDE	5.621	6.556	271.9E6	1255.0E6	172.140	145.030
15)	B Endosulfa...	6.284	7.141	246.4E6	1038.5E6	165.143	142.492
18)	B Endrin al...	6.454	7.265	173.2E6	737.4E6	161.016	140.341
19)	B Endosulfa...	6.667	7.490	224.1E6	907.7E6	165.392	142.791
21)	B Endrin ke...	7.160	7.966	242.8E6	893.2E6	166.560	144.855


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021822\
Data File : PD068097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2022 15:39
Operator : AR\AJ
Sample : INDB501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 15:53:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 18 15:51:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

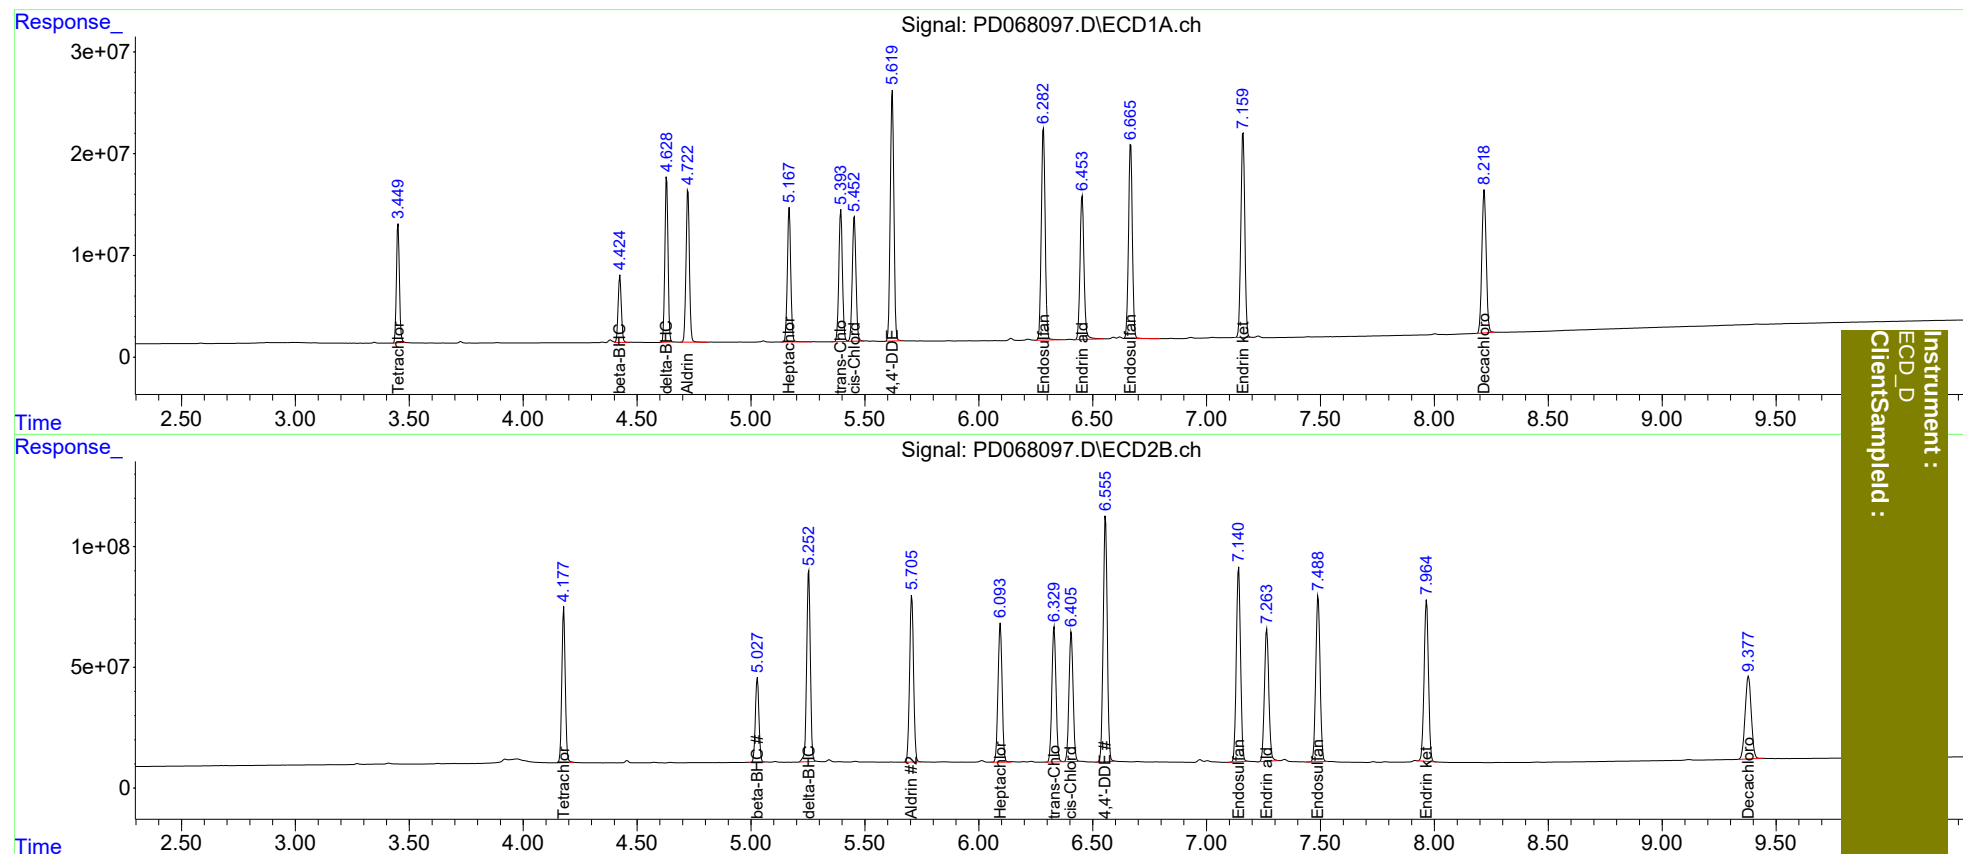


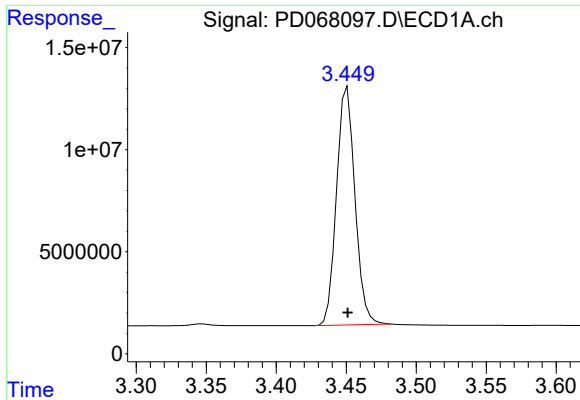

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 106905041
Conc: 77.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

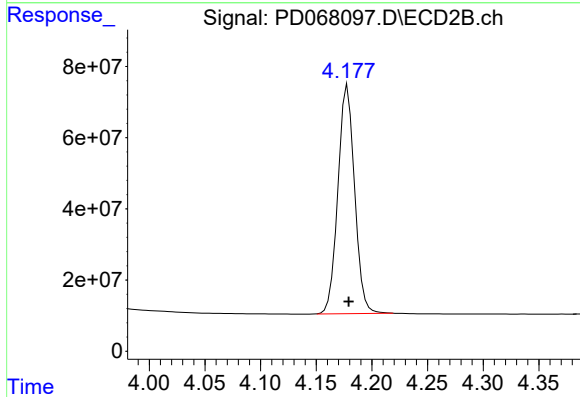


#1 Tetrachloro-m-xylene

R.T.: 4.178 min
Delta R.T.: 0.000 min
Response: 669699642
Conc: 68.75 ng/ml

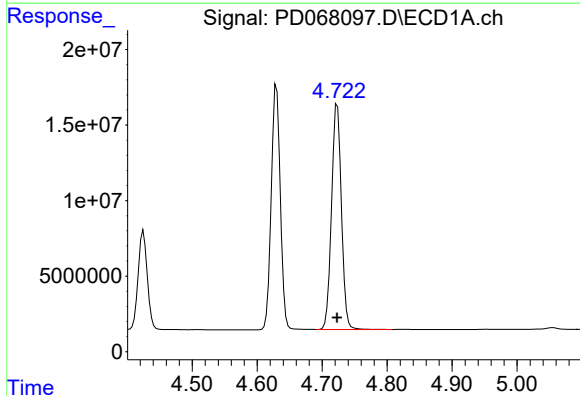


#5 Aldrin

R.T.: 4.723 min
Delta R.T.: 0.000 min
Response: 156676372
Conc: 84.32 ng/ml

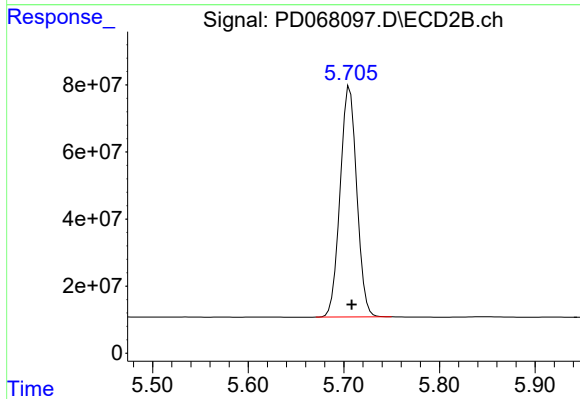

#5 Aldrin


R.T.: 5.706 min
Delta R.T.: -0.002 min
Response: 834481665
Conc: 70.93 ng/ml

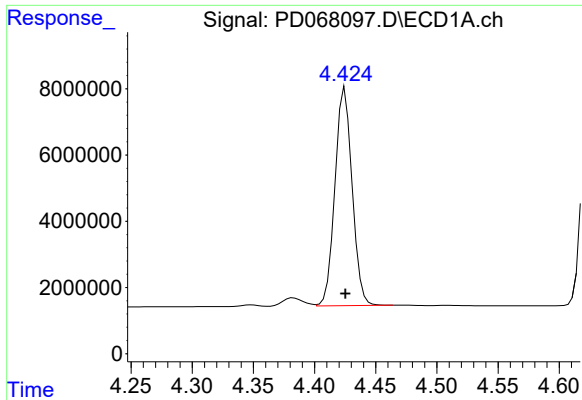

#6 beta-BHC


R.T.: 4.425 min
Delta R.T.: 0.000 min
Response: 64225159
Conc: 74.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

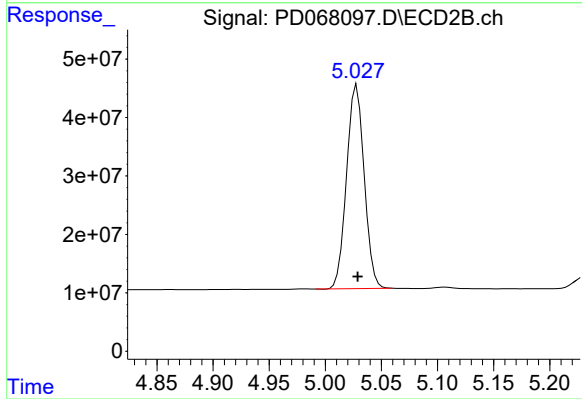


#6 beta-BHC

R.T.: 5.028 min
Delta R.T.: 0.000 min
Response: 380904654
Conc: 67.66 ng/ml

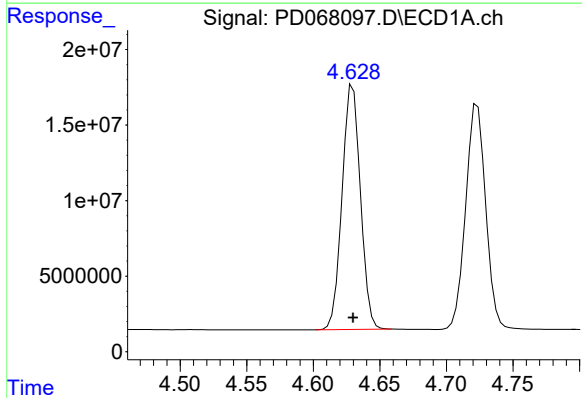


#7 delta-BHC

R.T.: 4.630 min
Delta R.T.: 0.000 min
Response: 155522668
Conc: 86.17 ng/ml

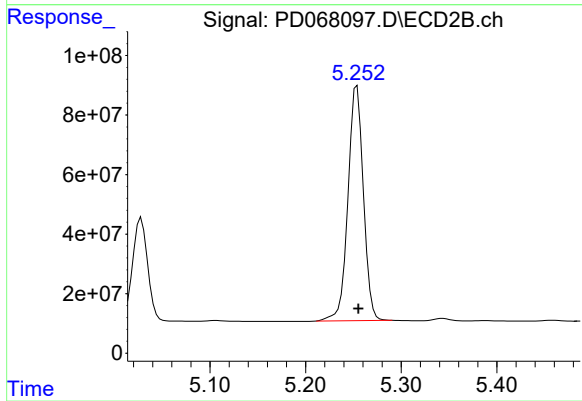

#7 delta-BHC


R.T.: 5.254 min
Delta R.T.: -0.001 min
Response: 889866927
Conc: 72.03 ng/ml

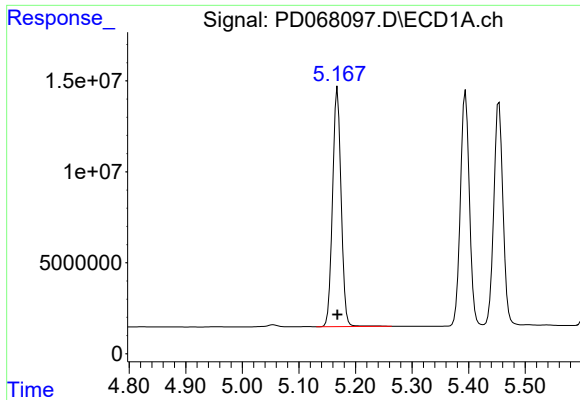

#8 Heptachlor epoxide


R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 138219332
Conc: 81.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

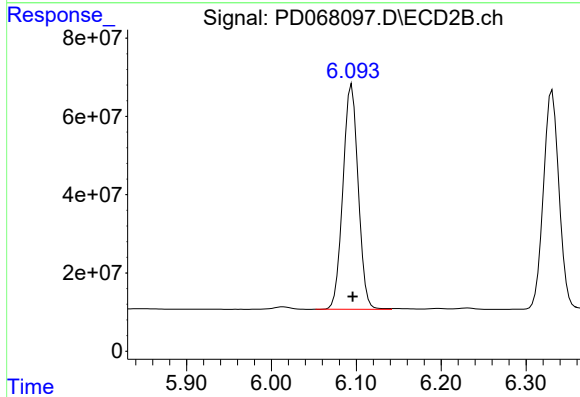


#8 Heptachlor epoxide

R.T.: 6.095 min
Delta R.T.: -0.001 min
Response: 716194266
Conc: 70.00 ng/ml

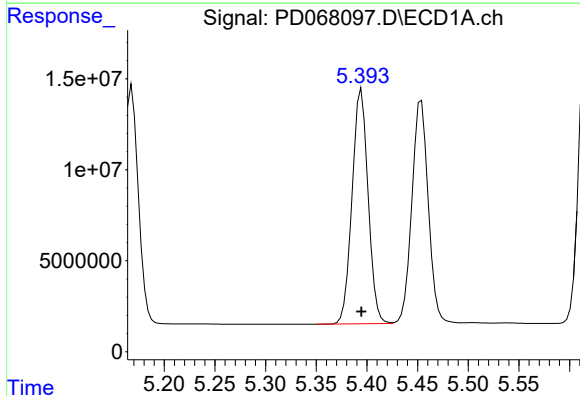


#10 trans-Chlordane

R.T.: 5.395 min
Delta R.T.: 0.000 min
Response: 141912556
Conc: 81.89 ng/ml

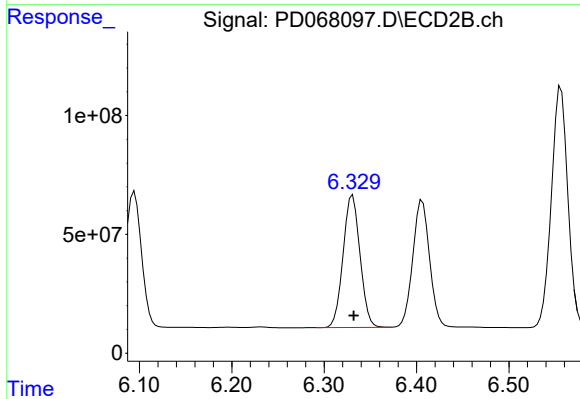

#10 trans-Chlordane


R.T.: 6.331 min
Delta R.T.: -0.001 min
Response: 708903269
Conc: 70.95 ng/ml

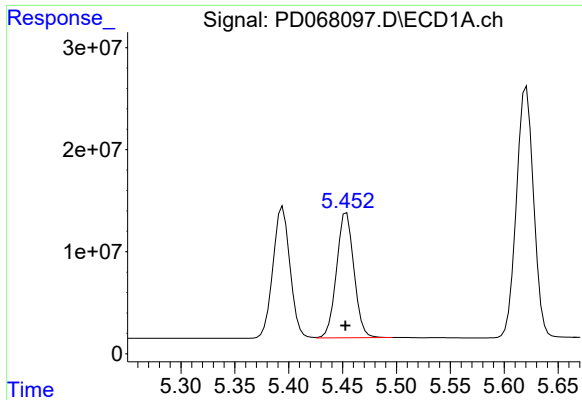

#11 cis-Chlordane


R.T.: 5.454 min
Delta R.T.: 0.001 min
Response: 137684643
Conc: 80.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

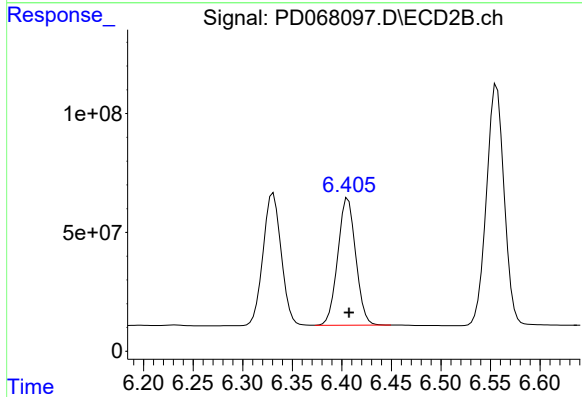


#11 cis-Chlordane

R.T.: 6.406 min
Delta R.T.: -0.001 min
Response: 675074458
Conc: 70.10 ng/ml

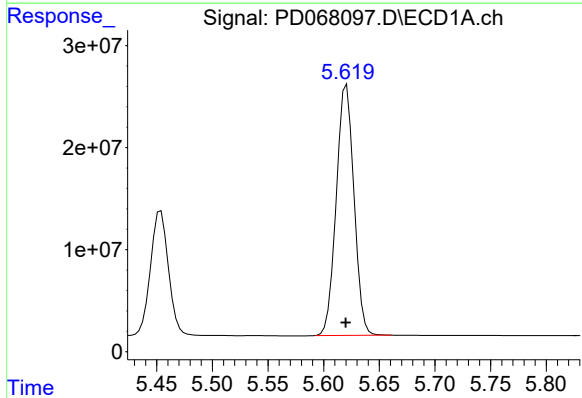


#12 4,4'-DDE

R.T.: 5.621 min
Delta R.T.: 0.000 min
Response: 271949858
Conc: 172.14 ng/ml

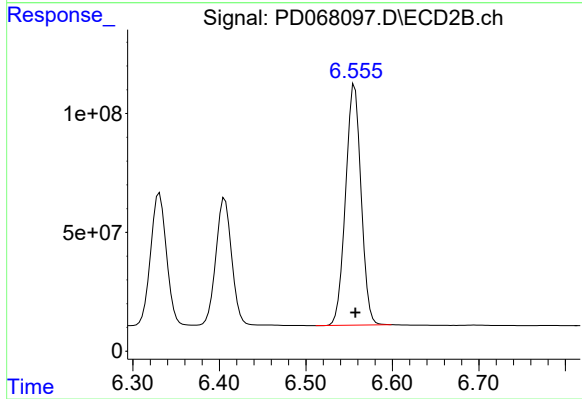

#12 4,4'-DDE


R.T.: 6.556 min
Delta R.T.: 0.000 min
Response: 1255027892
Conc: 145.03 ng/ml

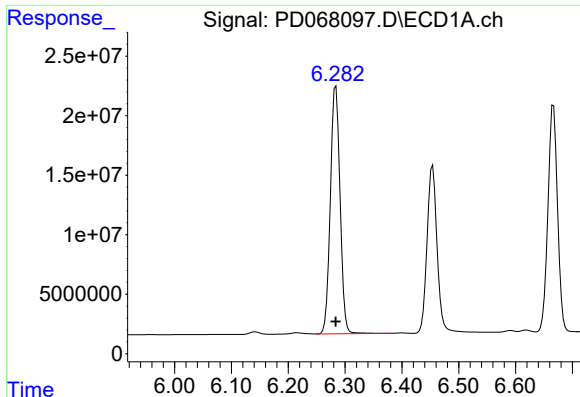

#15 Endosulfan II


R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 246432256
Conc: 165.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

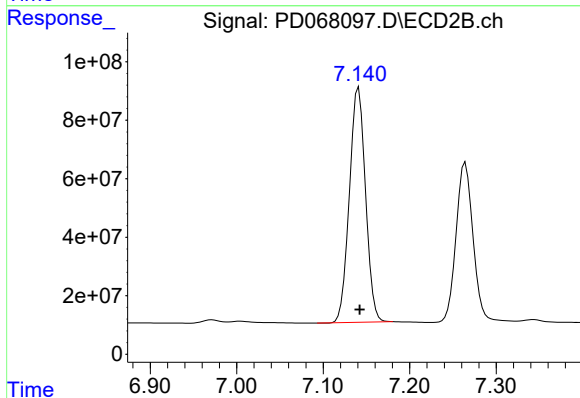


#15 Endosulfan II

R.T.: 7.141 min
Delta R.T.: -0.001 min
Response: 1038501502
Conc: 142.49 ng/ml

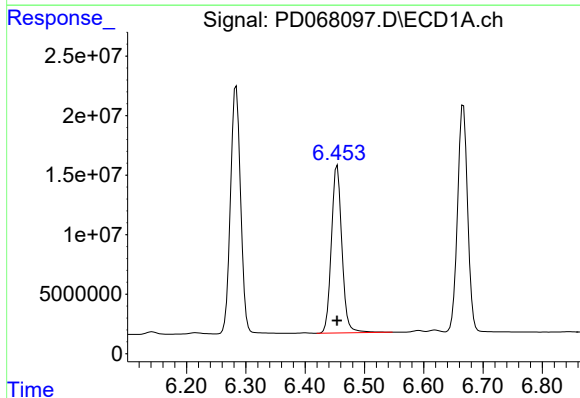


#18 Endrin aldehyde

R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 173195794
Conc: 161.02 ng/ml

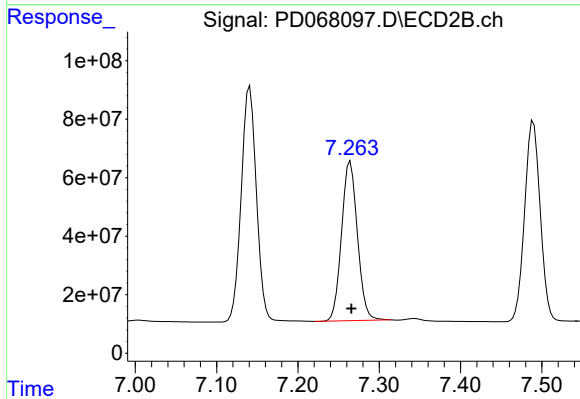

#18 Endrin aldehyde


R.T.: 7.265 min
Delta R.T.: -0.001 min
Response: 737366941
Conc: 140.34 ng/ml

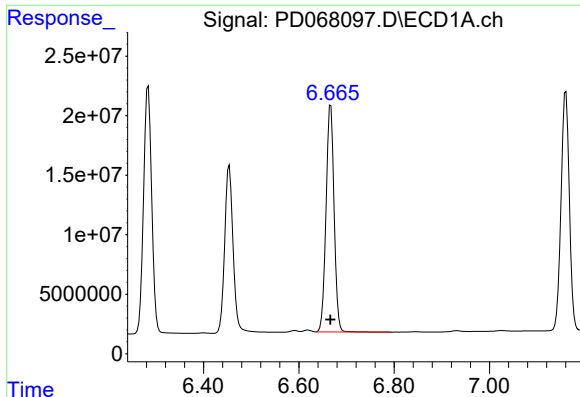

#19 Endosulfan Sulfate


R.T.: 6.667 min
Delta R.T.: 0.000 min
Response: 224142850
Conc: 165.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

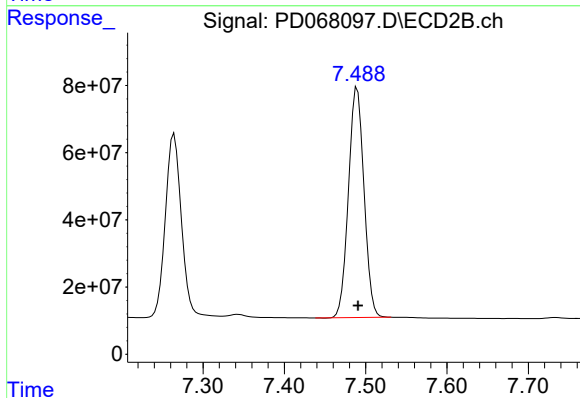


#19 Endosulfan Sulfate

R.T.: 7.490 min
Delta R.T.: 0.000 min
Response: 907679944
Conc: 142.79 ng/ml

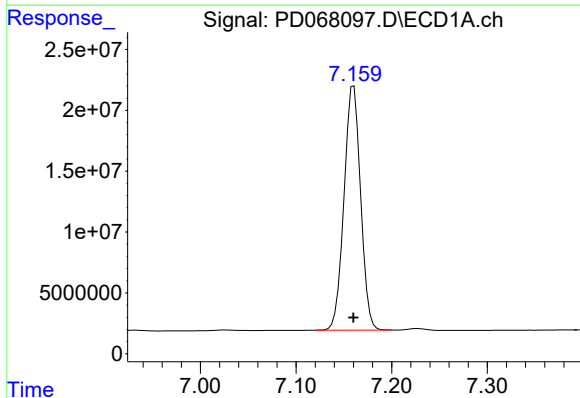


#21 Endrin ketone

R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 242837116
Conc: 166.56 ng/ml

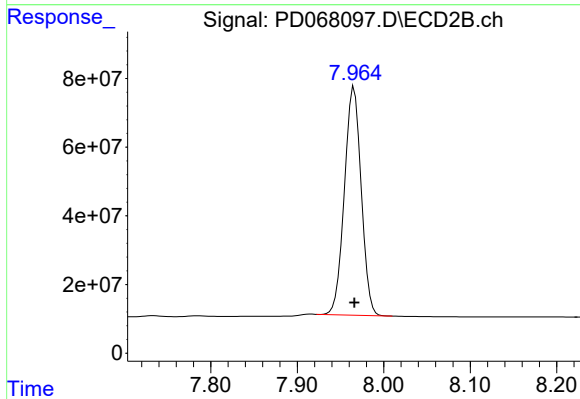

#21 Endrin ketone


R.T.: 7.966 min
Delta R.T.: 0.000 min
Response: 893157379
Conc: 144.85 ng/ml

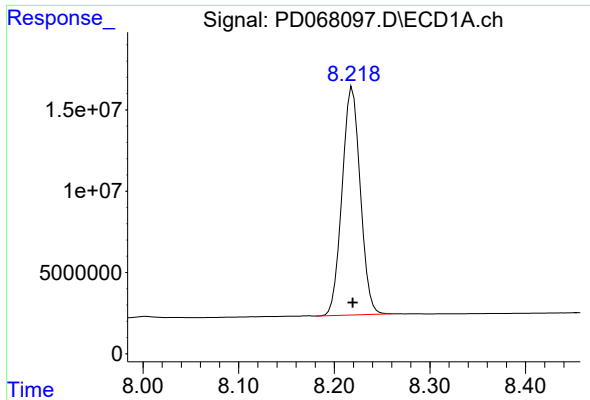

#27 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: 0.000 min
Response: 185902993
Conc: 153.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

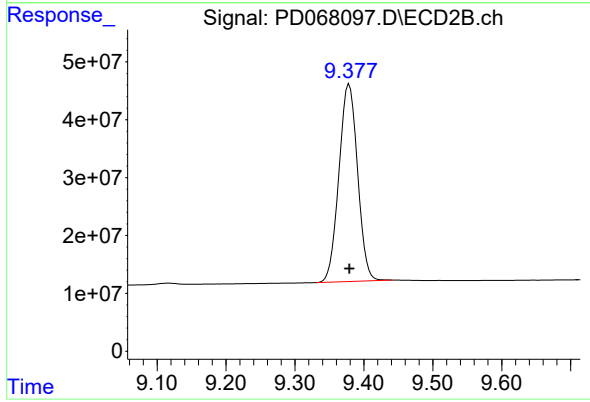

#27 Decachlorobiphenyl

R.T.: 9.379 min
Delta R.T.: 0.000 min
Response: 641581456
Conc: 140.52 ng/ml