

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021920\
 Data File : PD057378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2020 16:55
 Operator : AJ\MA
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 06:26:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021920CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 06:10:15 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.897	4100482	7944764	4.880	4.973
27)	SA Decachlor...	7.866	8.896	10194272	24615266	10.456	10.386
Target Compounds							
2)	A alpha-BHC	3.650	4.280	5314094	11011036	4.556	4.580
3)	MA gamma-BHC...	3.921	4.561	5772954	10856685	5.168	4.578
4)	MA Heptachlor	4.201	5.062	2688270	8894473	4.627	4.606
9)	A Endosulfan I	5.197	6.099	4688657	12195272	4.929	4.925
13)	MA Dieldrin	5.435	6.354	9602375	26629241	9.537	9.530
14)	MA Endrin	5.686	6.570	8136290	22139128	9.783	9.560
16)	A 4,4'-DDD	5.823	6.695	6662515	21517186	9.771	9.427
17)	MA 4,4'-DDT	6.056	6.993	4079794	14367219	8.020	7.929
20)	A Methoxychlor	6.604	7.450	11552404	46419288	45.536	45.741


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021920\
Data File : PD057378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2020 16:55
Operator : AJ\MA
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 06:26:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021920CLP.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 06:10:15 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

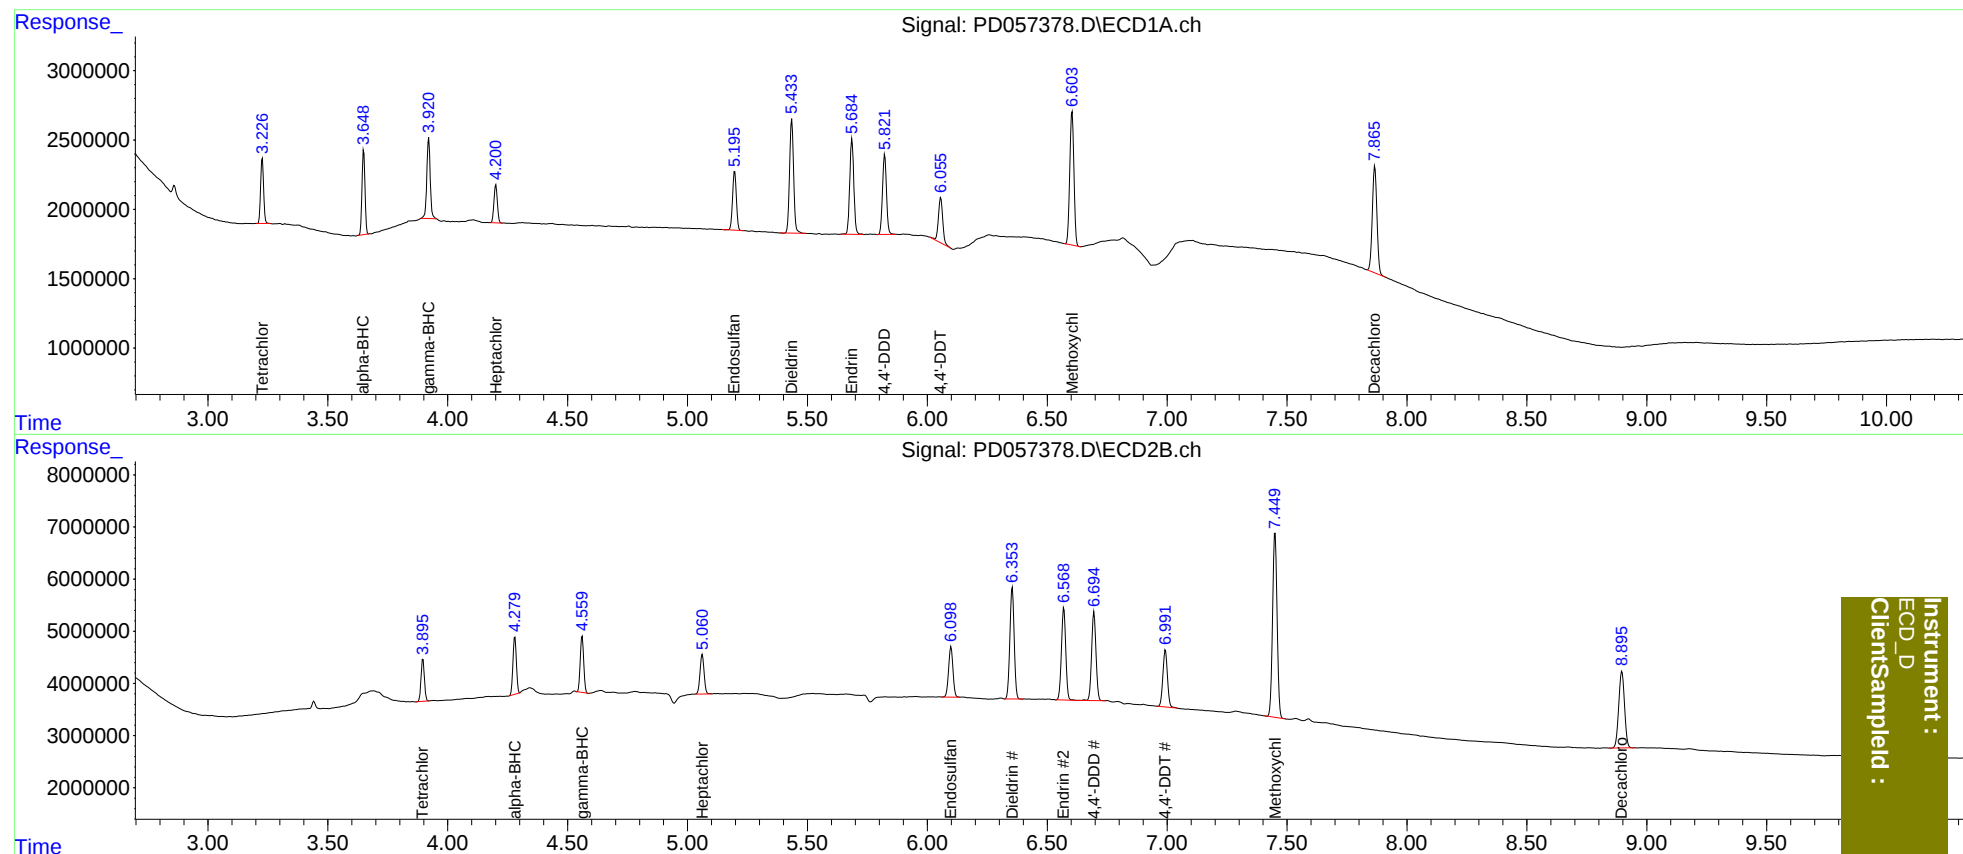


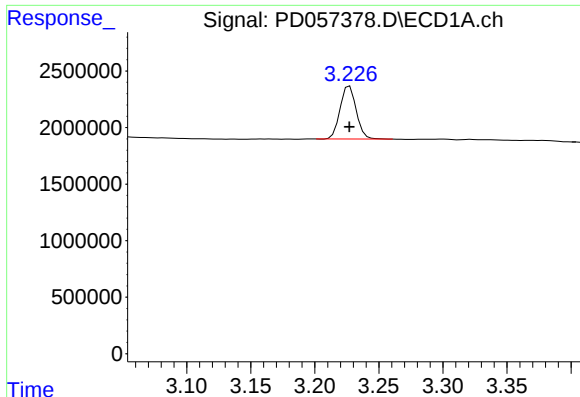

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 4100482
Conc: 4.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

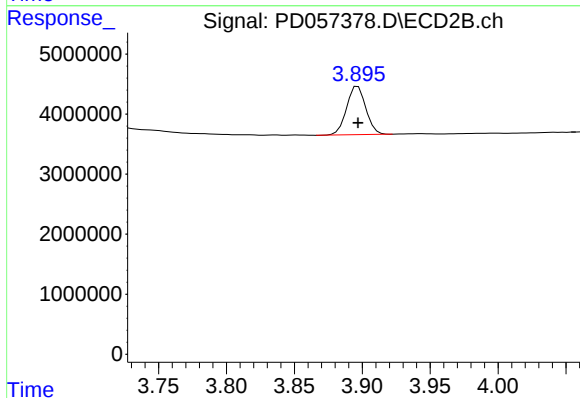


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 7944764
Conc: 4.97 ng/ml

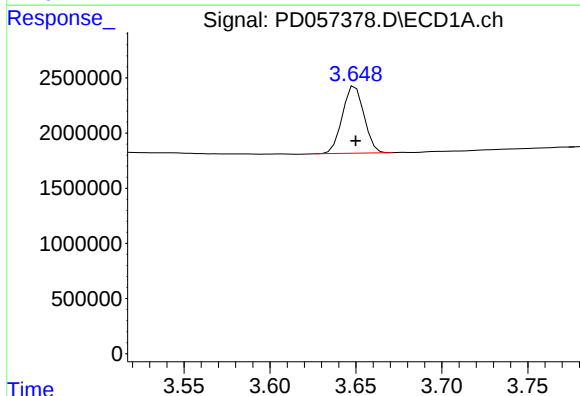


#2 alpha-BHC

R.T.: 3.650 min
Delta R.T.: 0.000 min
Response: 5314094
Conc: 4.56 ng/ml

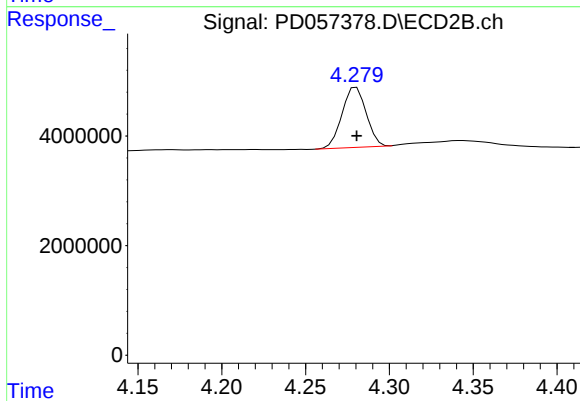

#2 alpha-BHC


R.T.: 4.280 min
Delta R.T.: 0.000 min
Response: 11011036
Conc: 4.58 ng/ml

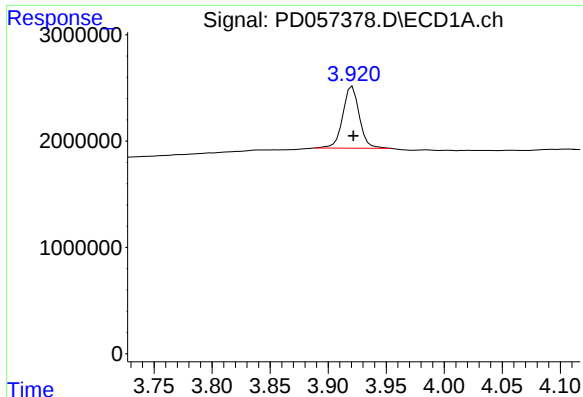

#3 gamma-BHC (Lindane)


R.T.: 3.921 min
Delta R.T.: 0.000 min
Response: 5772954
Conc: 5.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

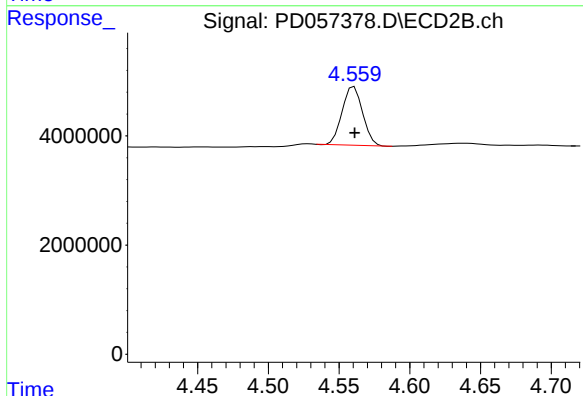


#3 gamma-BHC (Lindane)

R.T.: 4.561 min
Delta R.T.: 0.000 min
Response: 10856685
Conc: 4.58 ng/ml

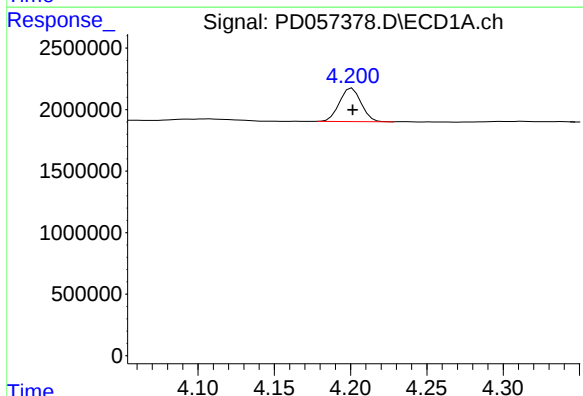


#4 Heptachlor

R.T.: 4.201 min
Delta R.T.: 0.000 min
Response: 2688270
Conc: 4.63 ng/ml

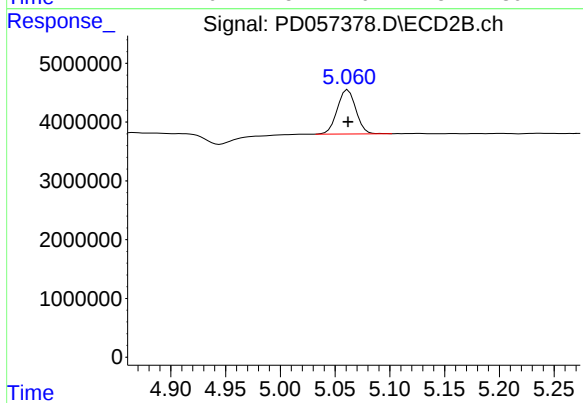

#4 Heptachlor


R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 8894473
Conc: 4.61 ng/ml

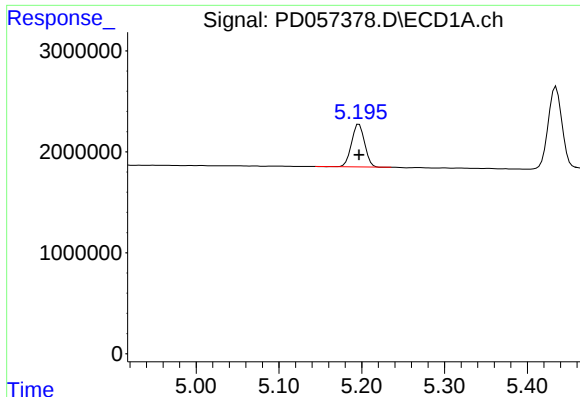

#9 Endosulfan I


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 4688657
Conc: 4.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

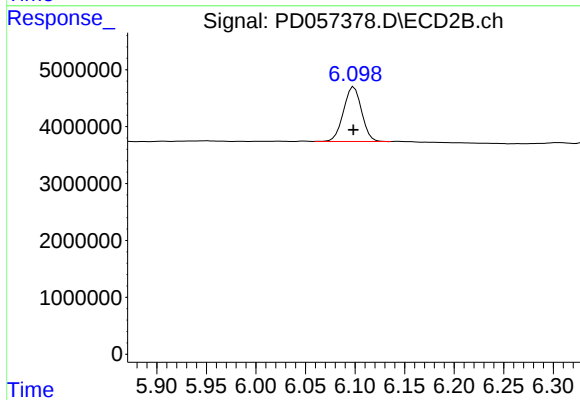


#9 Endosulfan I

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 12195272
Conc: 4.93 ng/ml

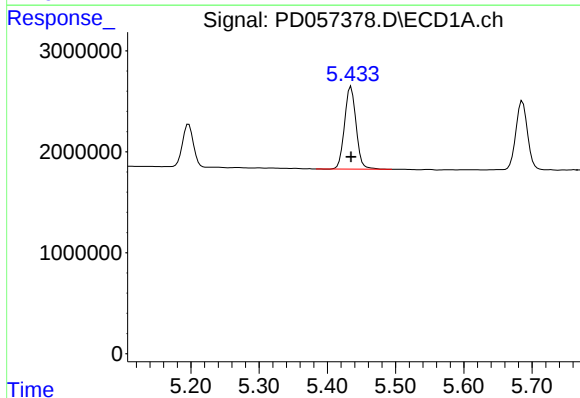


#13 Dieldrin

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 9602375
Conc: 9.54 ng/ml

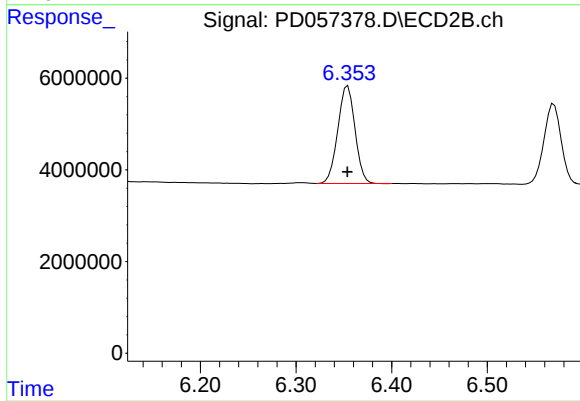

#13 Dieldrin


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 26629241
Conc: 9.53 ng/ml

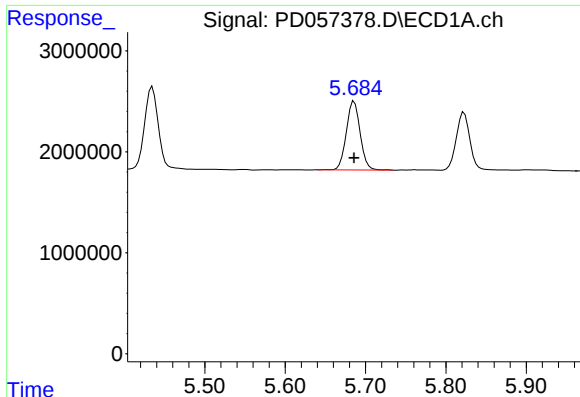

#14 Endrin


R.T.: 5.686 min
Delta R.T.: 0.000 min
Response: 8136290
Conc: 9.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

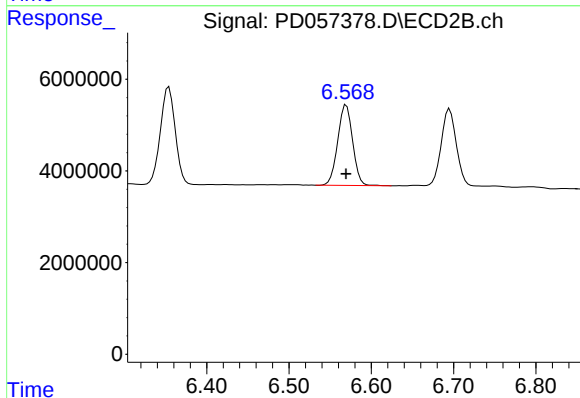


#14 Endrin

R.T.: 6.570 min
Delta R.T.: 0.000 min
Response: 22139128
Conc: 9.56 ng/ml

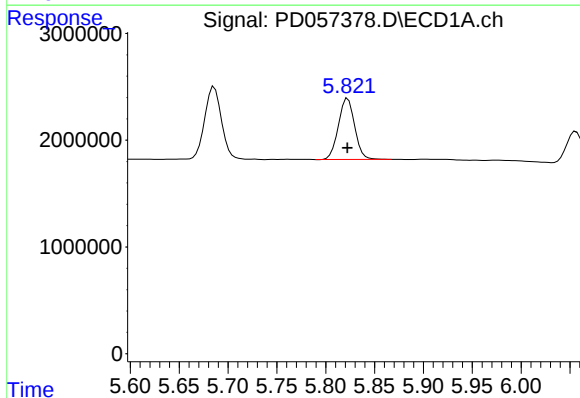


#16 4,4'-DDD

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 6662515
Conc: 9.77 ng/ml

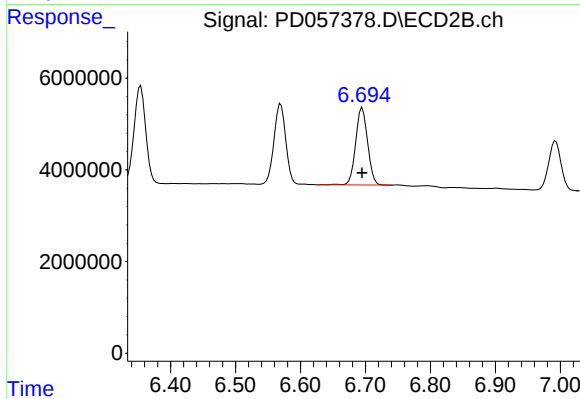

#16 4,4'-DDD


R.T.: 6.695 min
Delta R.T.: 0.000 min
Response: 21517186
Conc: 9.43 ng/ml

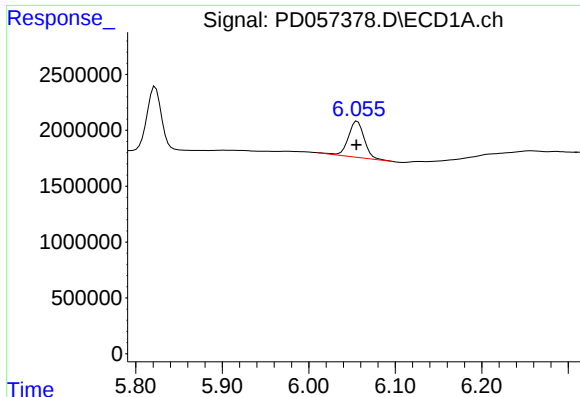

#17 4,4'-DDT


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 4079794
Conc: 8.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

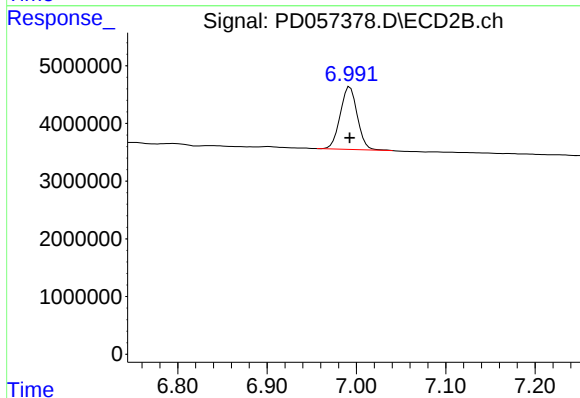


#17 4,4'-DDT

R.T.: 6.993 min
Delta R.T.: 0.000 min
Response: 14367219
Conc: 7.93 ng/ml

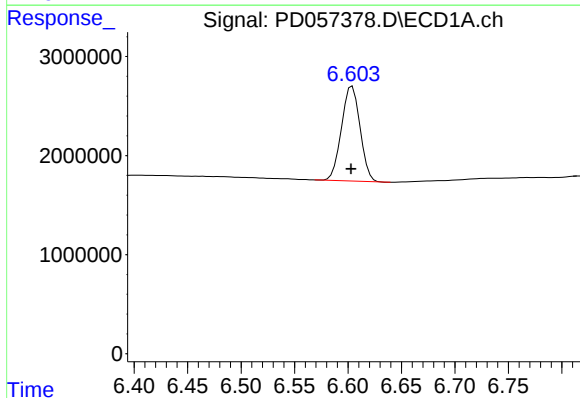


#20 Methoxychlor

R.T.: 6.604 min
Delta R.T.: 0.001 min
Response: 11552404
Conc: 45.54 ng/ml

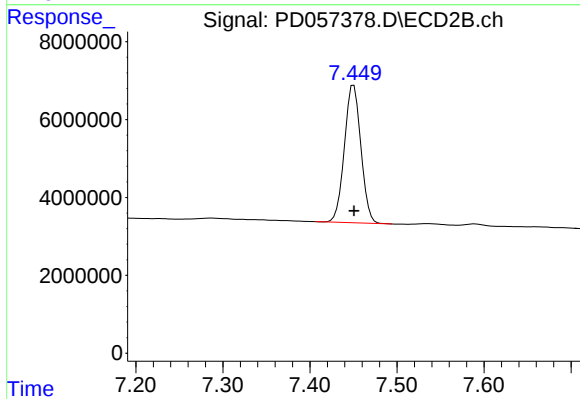

#20 Methoxychlor


R.T.: 7.450 min
Delta R.T.: 0.000 min
Response: 46419288
Conc: 45.74 ng/ml

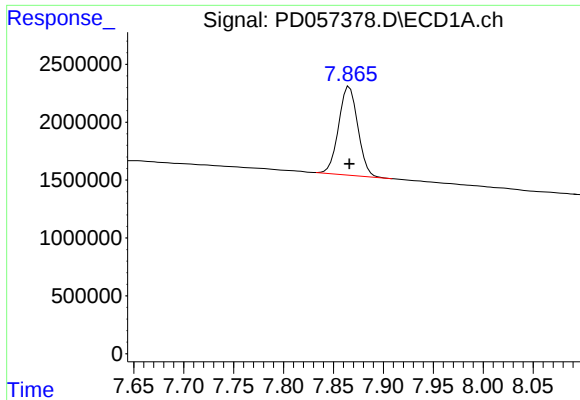

#27 Decachlorobiphenyl

R.T.: 7.866 min
Delta R.T.: 0.000 min
Response: 10194272
Conc: 10.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

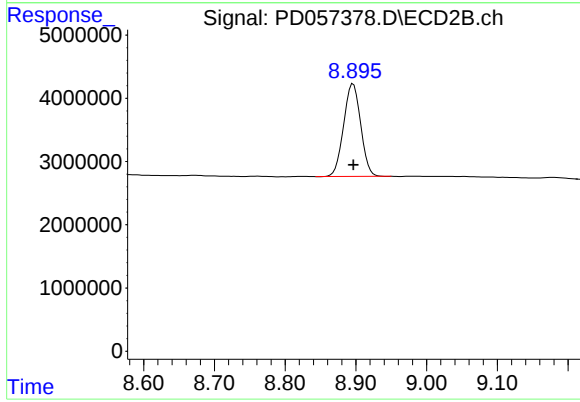

#27 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.000 min
Response: 24615266
Conc: 10.39 ng/ml