

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021920\
 Data File : PD057380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2020 17:24
 Operator : AJ\MA
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 06:14:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021920CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 06:10:15 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.897	8325786	15966048	9.909	9.995
27)	SA Decachlor...	7.866	8.896	20054681	49612447	20.569	20.932
Target Compounds							
2)	A alpha-BHC	3.650	4.280	11063970	22750572	9.485	9.463
3)	MA gamma-BHC...	3.922	4.561	11038410	22866645	9.882	9.642
4)	MA Heptachlor	4.202	5.062	5998306	18640886	10.324	9.654
9)	A Endosulfan I	5.197	6.099	9355379	25049812	9.835	10.117
13)	MA Dieldrin	5.434	6.354	18633306	53237530	18.507	19.052
14)	MA Endrin	5.686	6.570	15464533	44153575	18.595	19.067
16)	A 4,4'-DDD	5.822	6.696	12716395	42710114	18.649	18.712
17)	MA 4,4'-DDT	6.056	6.992	9918725	33321835	19.499	18.390
20)	A Methoxychlor	6.605	7.450	25353529	99417185	99.935	97.964


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021920\
Data File : PD057380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2020 17:24
Operator : AJ\MA
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 06:14:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021920CLP.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 06:10:15 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

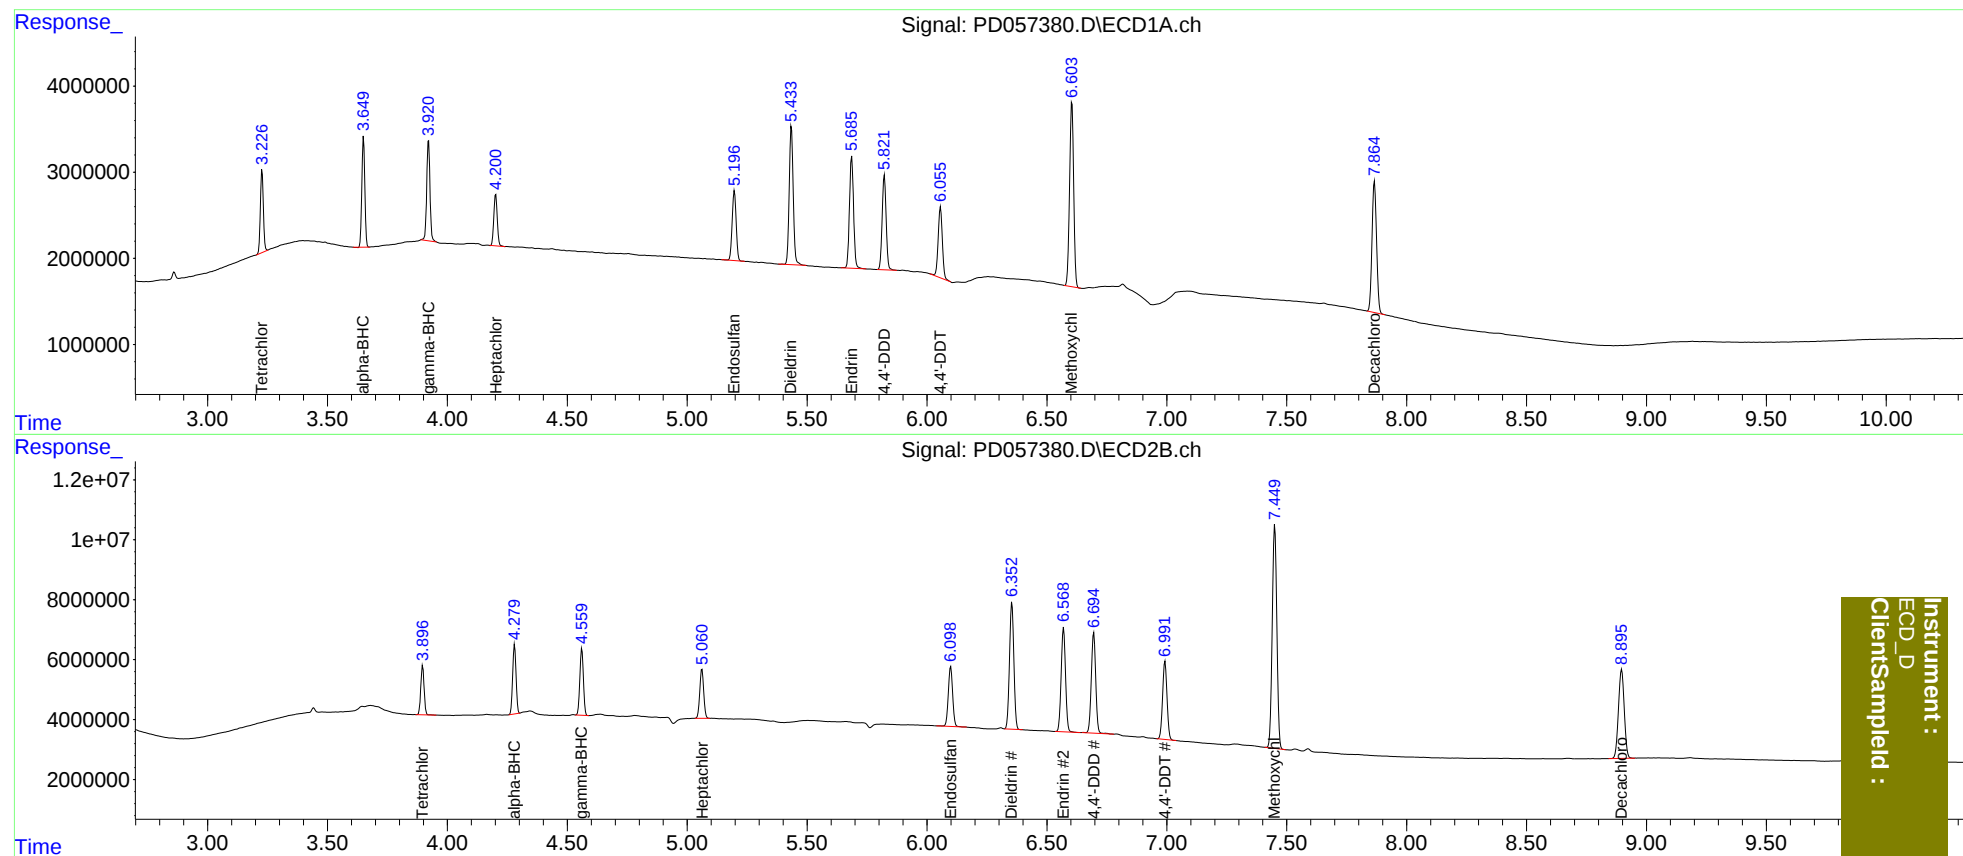


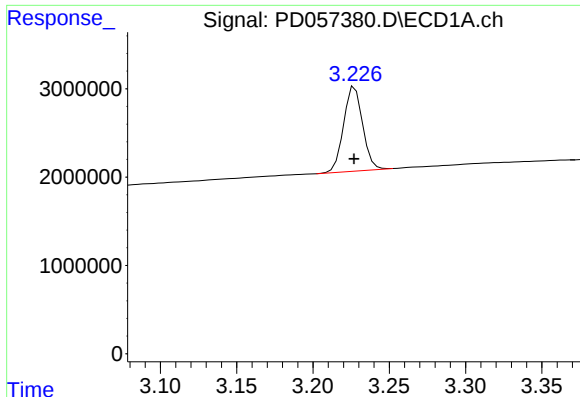

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 8325786
Conc: 9.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

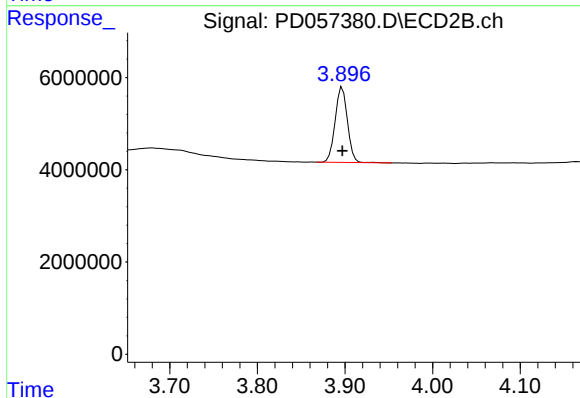


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 15966048
Conc: 9.99 ng/ml

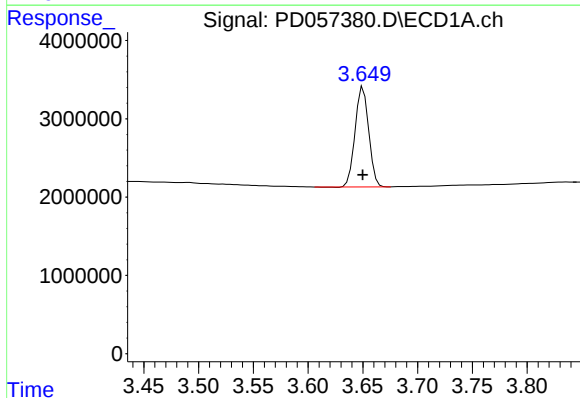


#2 alpha-BHC

R.T.: 3.650 min
Delta R.T.: 0.000 min
Response: 11063970
Conc: 9.48 ng/ml

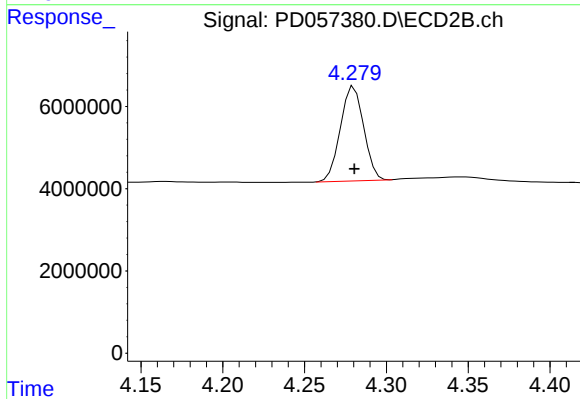

#2 alpha-BHC


R.T.: 4.280 min
Delta R.T.: 0.000 min
Response: 22750572
Conc: 9.46 ng/ml

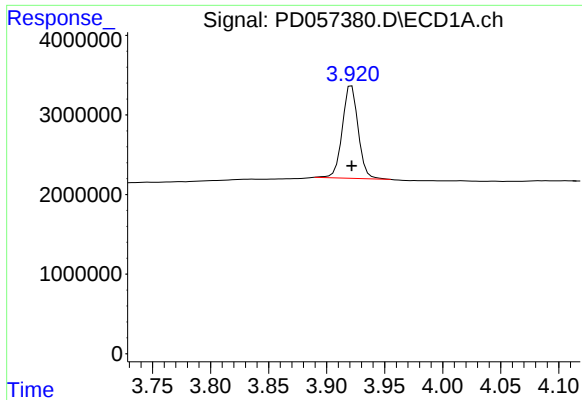

#3 gamma-BHC (Lindane)


R.T.: 3.922 min
Delta R.T.: 0.000 min
Response: 11038410
Conc: 9.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

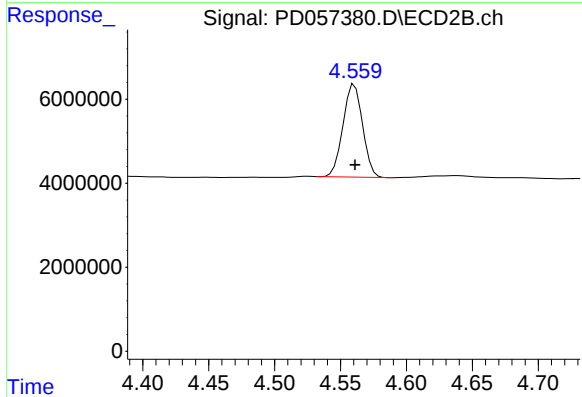


#3 gamma-BHC (Lindane)

R.T.: 4.561 min
Delta R.T.: 0.000 min
Response: 22866645
Conc: 9.64 ng/ml

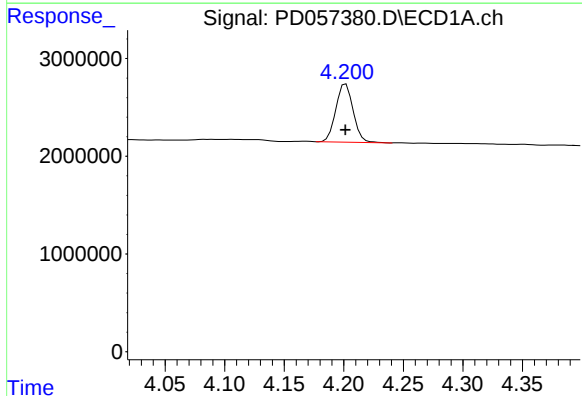


#4 Heptachlor

R.T.: 4.202 min
Delta R.T.: 0.000 min
Response: 5998306
Conc: 10.32 ng/ml

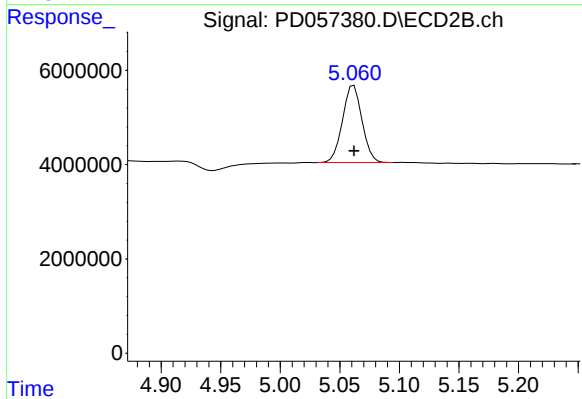

#4 Heptachlor


R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 18640886
Conc: 9.65 ng/ml

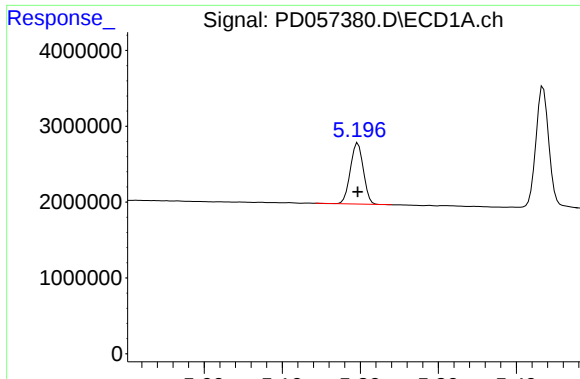

#9 Endosulfan I


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 9355379
Conc: 9.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

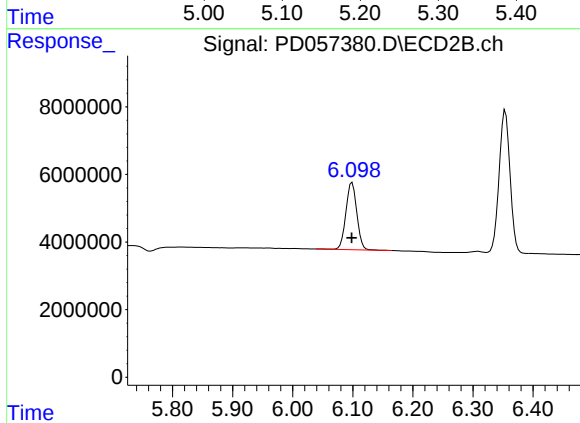


#9 Endosulfan I

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 25049812
Conc: 10.12 ng/ml

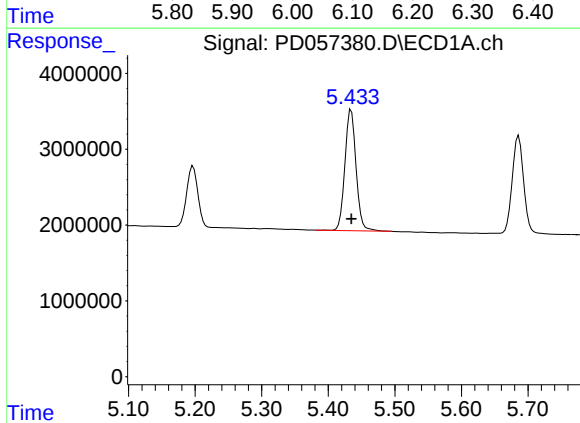


#13 Dieldrin

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 18633306
Conc: 18.51 ng/ml

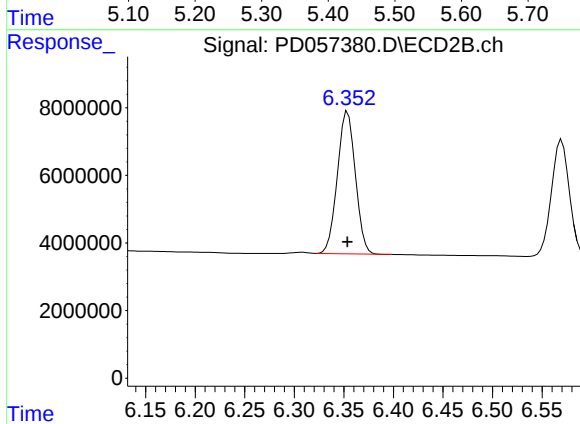

#13 Dieldrin


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 53237530
Conc: 19.05 ng/ml

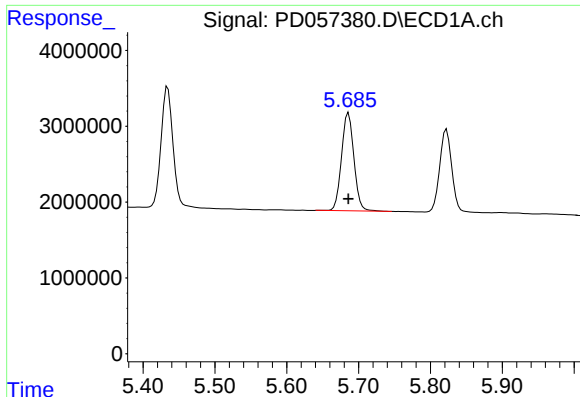

#14 Endrin


R.T.: 5.686 min
Delta R.T.: 0.000 min
Response: 15464533
Conc: 18.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

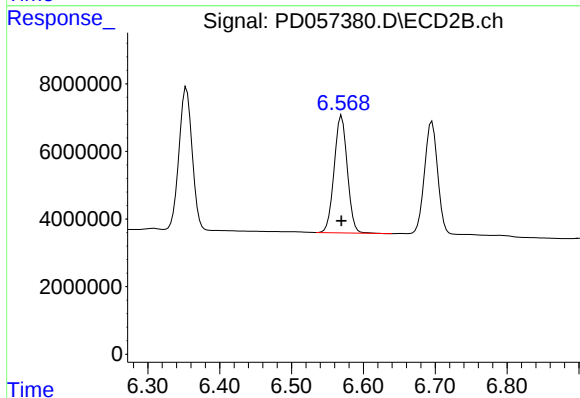


#14 Endrin

R.T.: 6.570 min
Delta R.T.: 0.000 min
Response: 44153575
Conc: 19.07 ng/ml

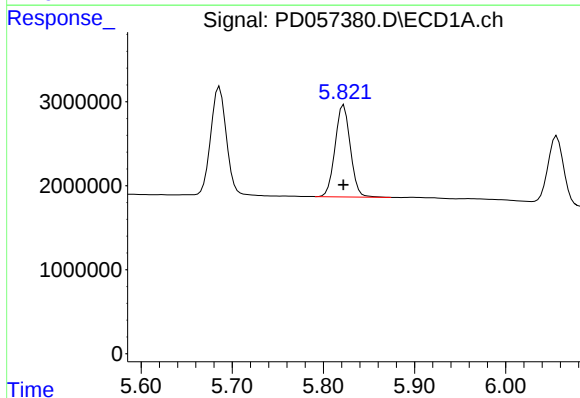


#16 4,4'-DDD

R.T.: 5.822 min
Delta R.T.: 0.000 min
Response: 12716395
Conc: 18.65 ng/ml

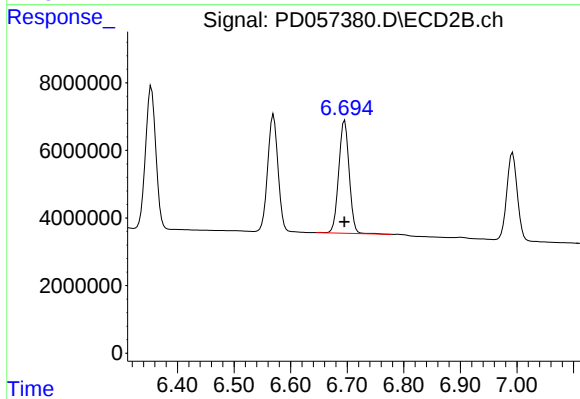

#16 4,4'-DDD


R.T.: 6.696 min
Delta R.T.: 0.000 min
Response: 42710114
Conc: 18.71 ng/ml

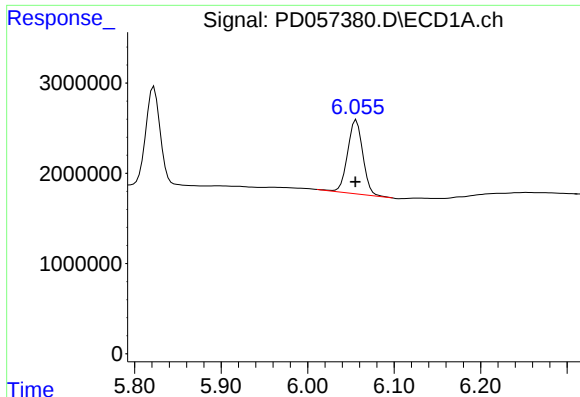

#17 4,4'-DDT


R.T.: 6.056 min
Delta R.T.: 0.001 min
Response: 9918725
Conc: 19.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

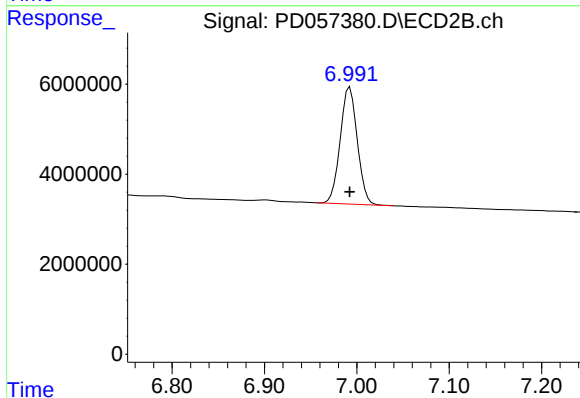


#17 4,4'-DDT

R.T.: 6.992 min
Delta R.T.: 0.000 min
Response: 33321835
Conc: 18.39 ng/ml

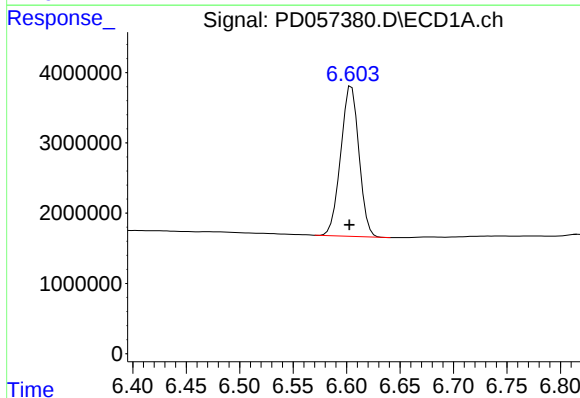


#20 Methoxychlor

R.T.: 6.605 min
Delta R.T.: 0.002 min
Response: 25353529
Conc: 99.94 ng/ml

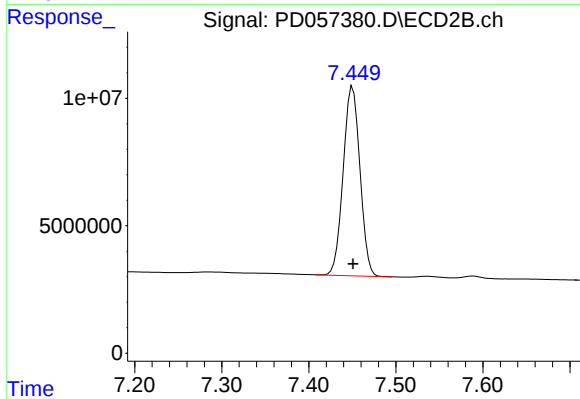

#20 Methoxychlor


R.T.: 7.450 min
Delta R.T.: 0.000 min
Response: 99417185
Conc: 97.96 ng/ml

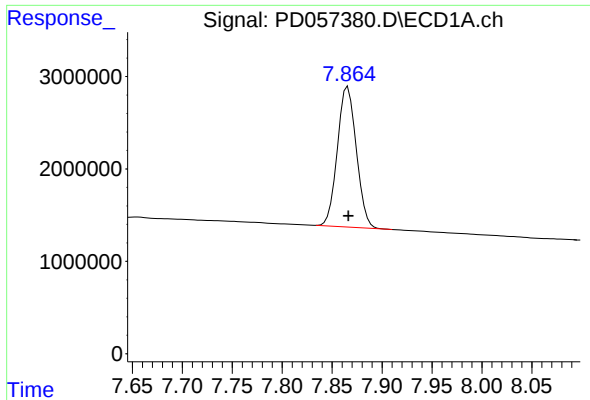

#27 Decachlorobiphenyl

R.T.: 7.866 min
Delta R.T.: 0.000 min
Response: 20054681
Conc: 20.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

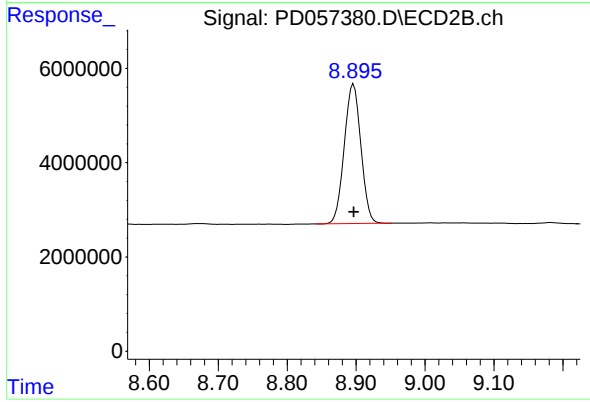

#27 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.000 min
Response: 49612447
Conc: 20.93 ng/ml