

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021920\
 Data File : PD057382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2020 17:52
 Operator : AJ\MA
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 06:14:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021920CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 06:10:15 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.897	16804202	31949496	20.000	20.000
27)	SA Decachlor...	7.866	8.897	38998988	94805628	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.650	4.281	23329626	48083184	20.000	20.000
3)	MA gamma-BHC...	3.922	4.561	22341439	47429355	20.000	20.000
4)	MA Heptachlor	4.201	5.062	11620333	38618047	20.000	20.000
9)	A Endosulfan I	5.197	6.098	19024099	49520139	20.000	20.000
13)	MA Dieldrin	5.435	6.354	40273218	111.8E6	40.000	40.000
14)	MA Endrin	5.686	6.569	33265453	92628669	40.000	40.000
16)	A 4,4'-DDD	5.822	6.695	27274694	91298942	40.000	40.000
17)	MA 4,4'-DDT	6.055	6.992	20346890	72478949	40.000	40.000
20)	A Methoxychlor	6.603	7.451	50739911	203.0E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021920\
Data File : PD057382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2020 17:52
Operator : AJ\MA
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 06:14:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021920CLP.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 06:10:15 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

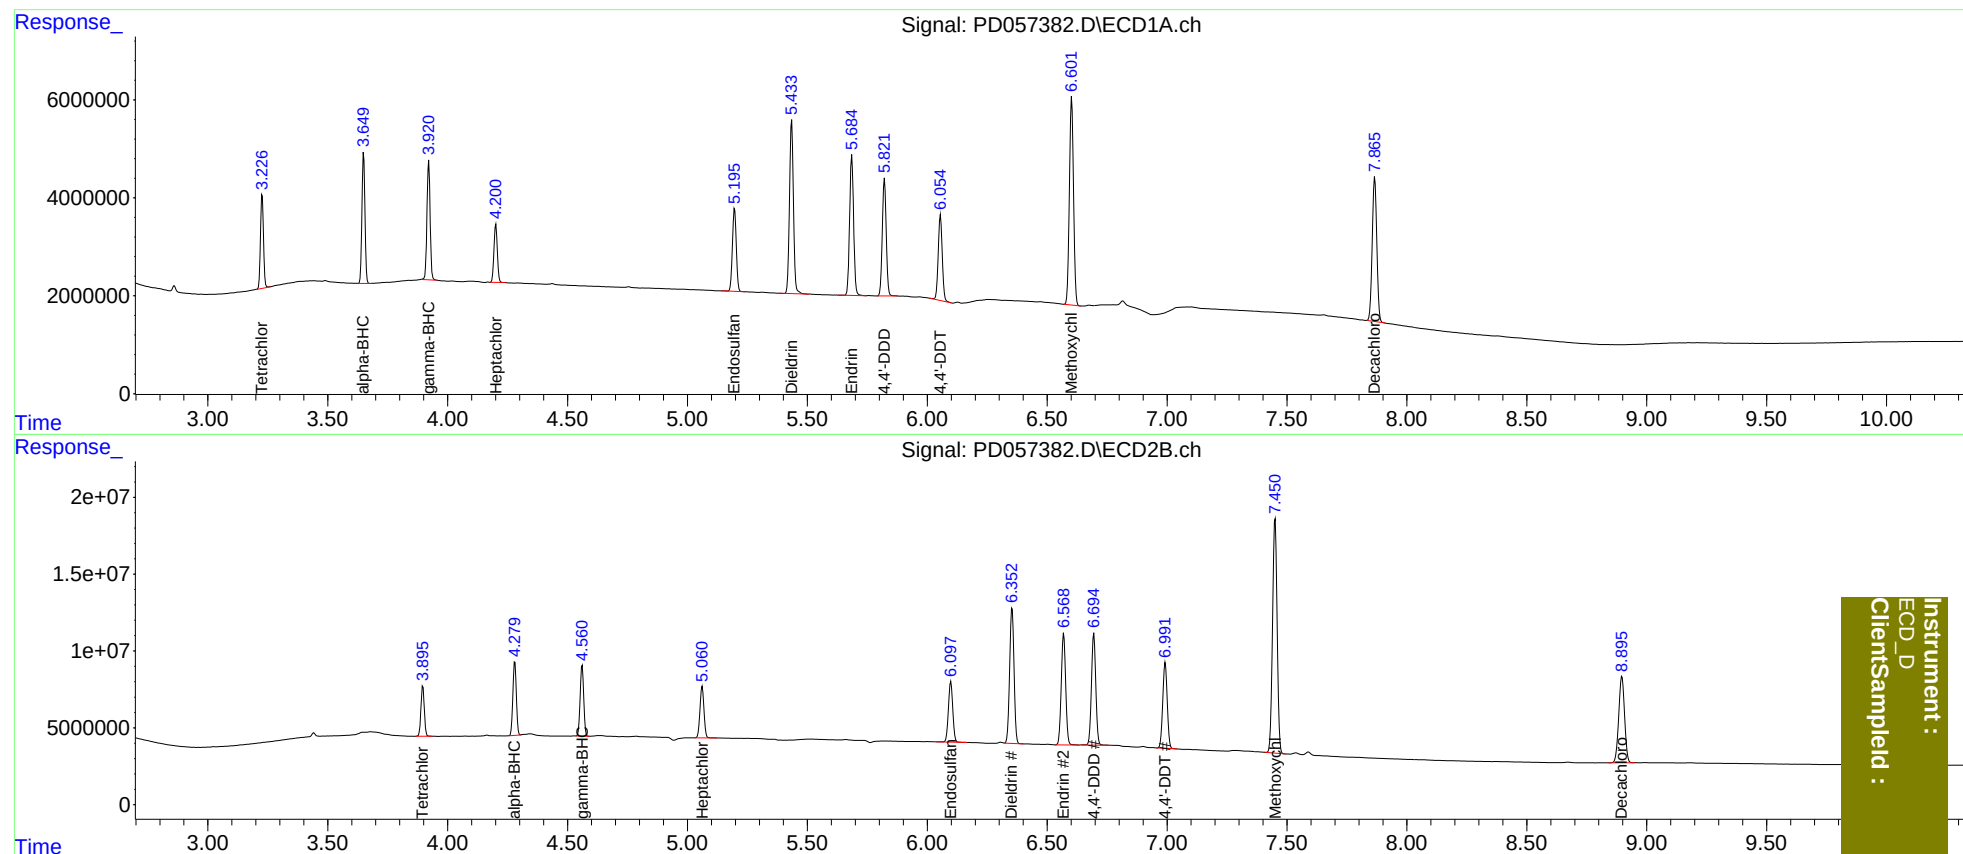


Instrument :
ECD_D
ClientSampled :

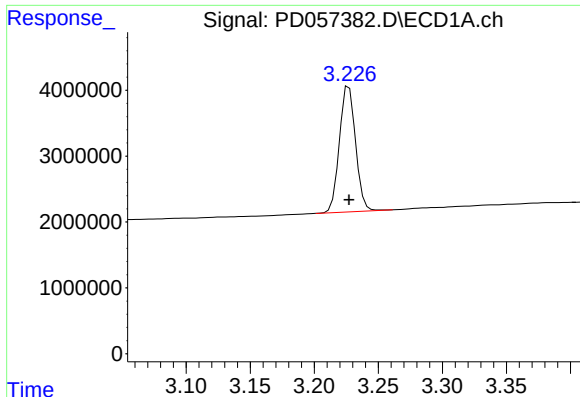

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 16804202
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

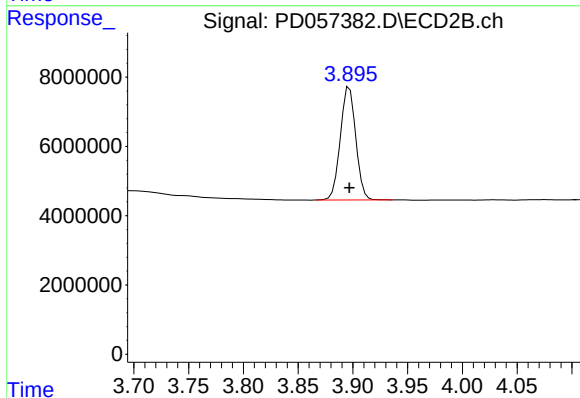


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 31949496
Conc: 20.00 ng/ml

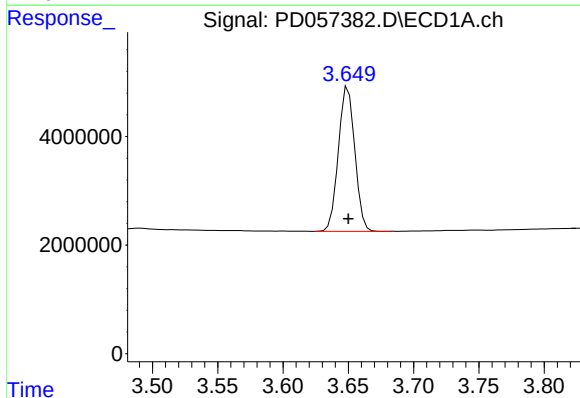


#2 alpha-BHC

R.T.: 3.650 min
Delta R.T.: 0.000 min
Response: 23329626
Conc: 20.00 ng/ml

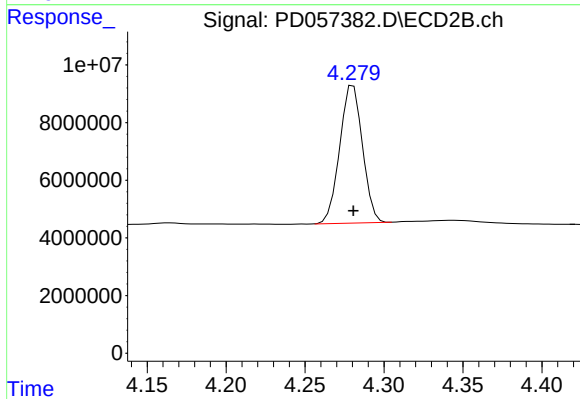

#2 alpha-BHC


R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 48083184
Conc: 20.00 ng/ml

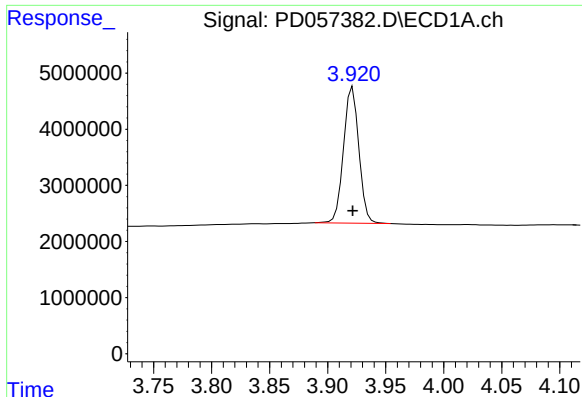

#3 gamma-BHC (Lindane)


R.T.: 3.922 min
Delta R.T.: 0.000 min
Response: 22341439
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

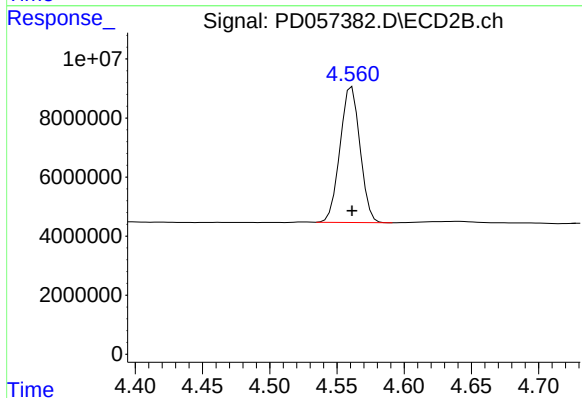


#3 gamma-BHC (Lindane)

R.T.: 4.561 min
Delta R.T.: 0.000 min
Response: 47429355
Conc: 20.00 ng/ml

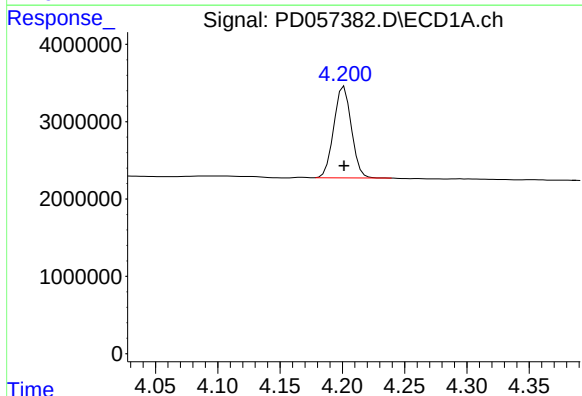


#4 Heptachlor

R.T.: 4.201 min
Delta R.T.: 0.000 min
Response: 11620333
Conc: 20.00 ng/ml

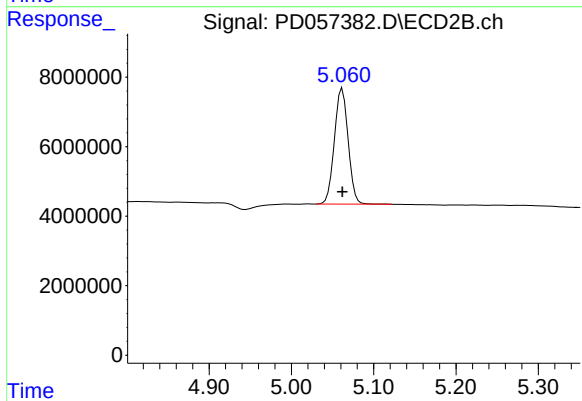

#4 Heptachlor


R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 38618047
Conc: 20.00 ng/ml

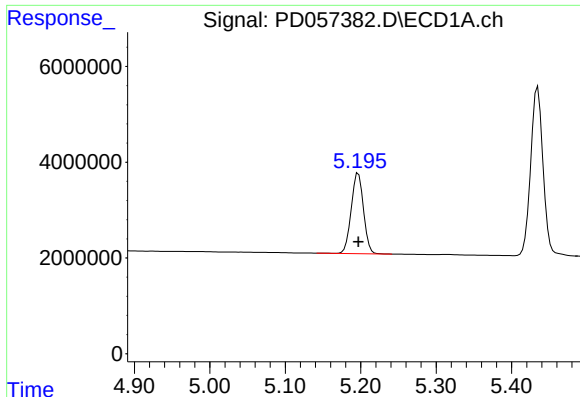

#9 Endosulfan I


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 19024099
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

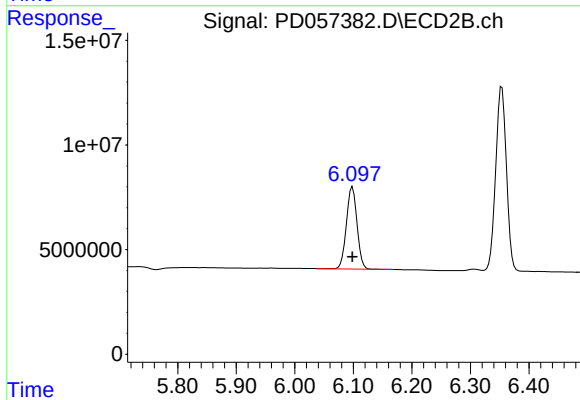


#9 Endosulfan I

R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 49520139
Conc: 20.00 ng/ml

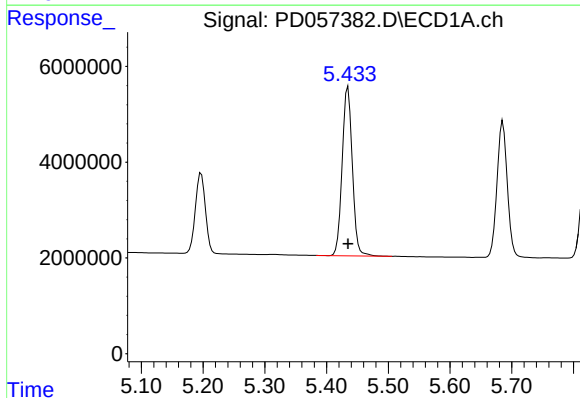


#13 Dieldrin

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 40273218
Conc: 40.00 ng/ml

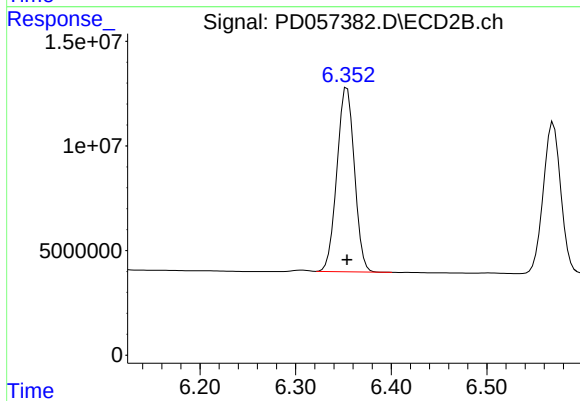

#13 Dieldrin


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 111772985
Conc: 40.00 ng/ml

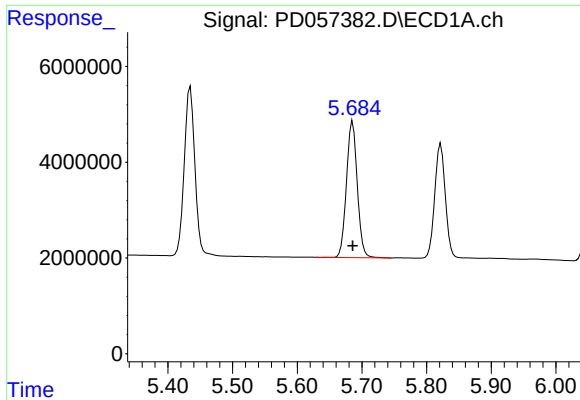

#14 Endrin


R.T.: 5.686 min
Delta R.T.: 0.000 min
Response: 33265453
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

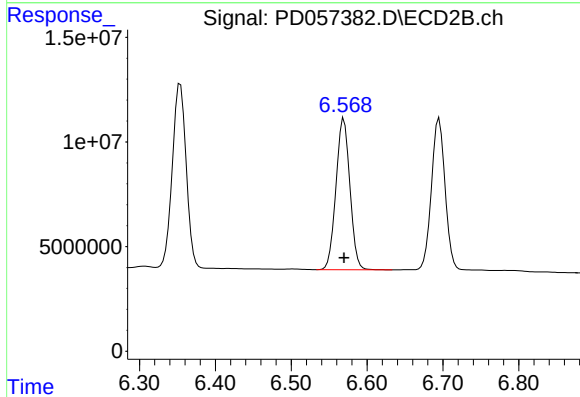


#14 Endrin

R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 92628669
Conc: 40.00 ng/ml

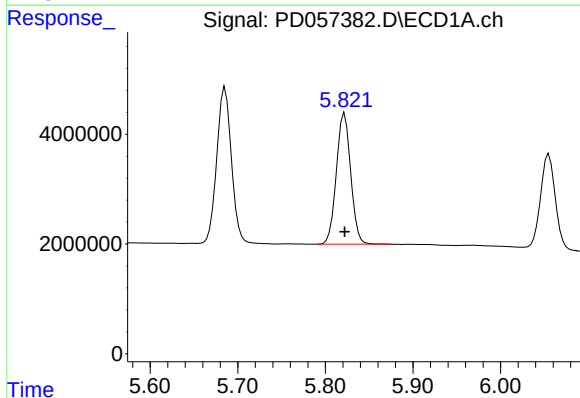


#16 4,4'-DDD

R.T.: 5.822 min
Delta R.T.: 0.000 min
Response: 27274694
Conc: 40.00 ng/ml

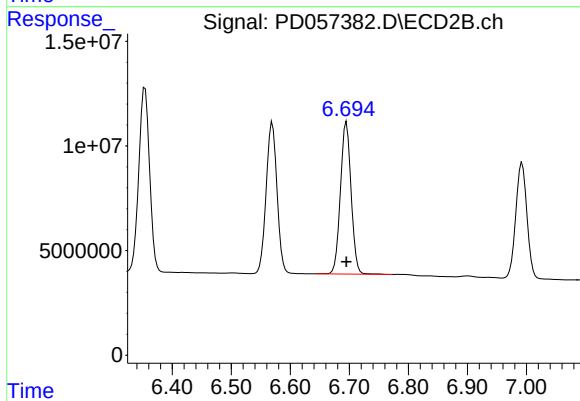

#16 4,4'-DDD


R.T.: 6.695 min
Delta R.T.: 0.000 min
Response: 91298942
Conc: 40.00 ng/ml

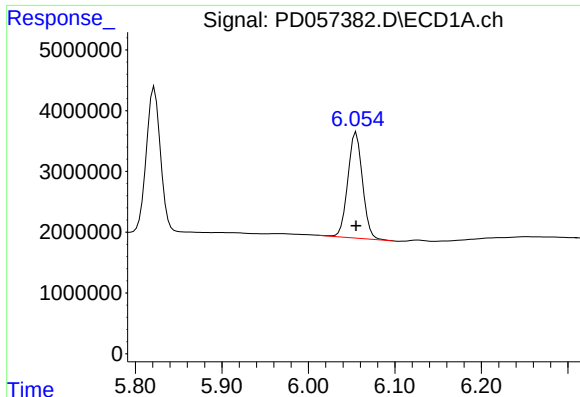

#17 4,4'-DDT


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 20346890
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

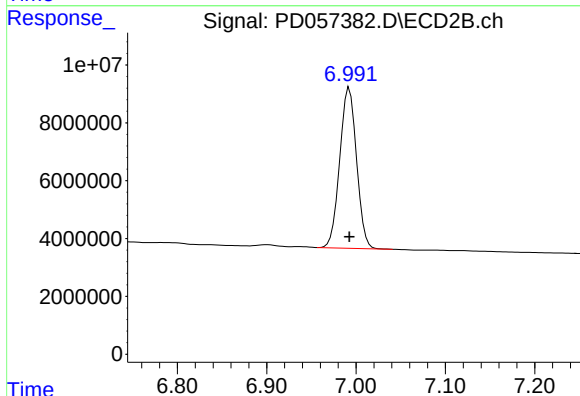


#17 4,4'-DDT

R.T.: 6.992 min
Delta R.T.: 0.000 min
Response: 72478949
Conc: 40.00 ng/ml

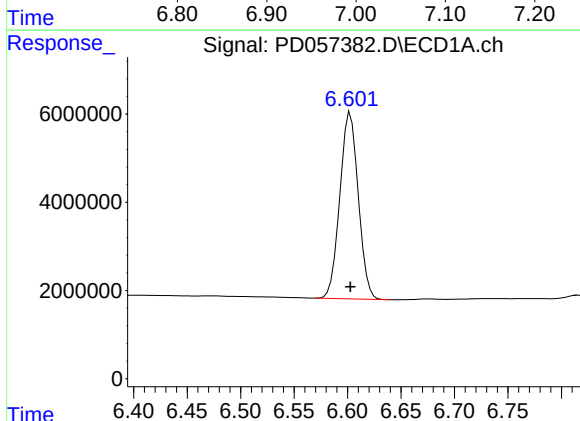


#20 Methoxychlor

R.T.: 6.603 min
Delta R.T.: 0.000 min
Response: 50739911
Conc: 200.00 ng/ml

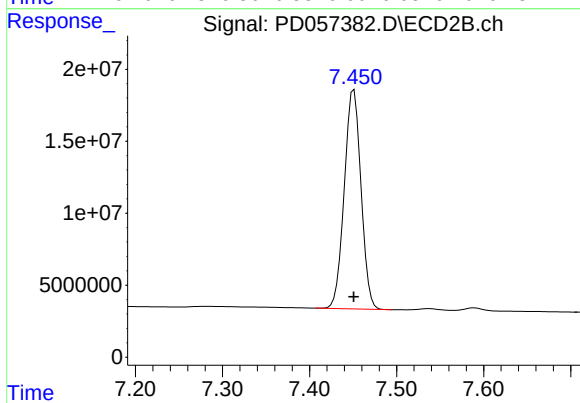

#20 Methoxychlor


R.T.: 7.451 min
Delta R.T.: 0.000 min
Response: 202966568
Conc: 200.00 ng/ml

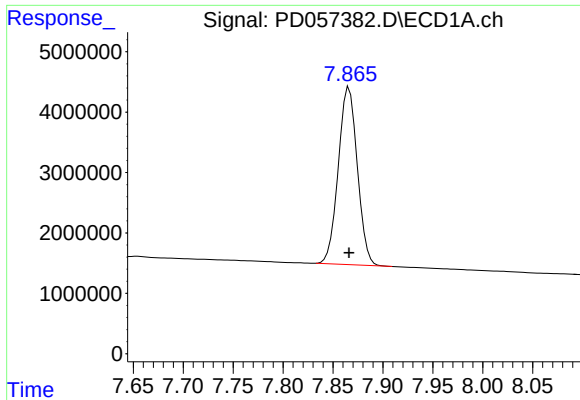

#27 Decachlorobiphenyl

R.T.: 7.866 min
Delta R.T.: 0.000 min
Response: 38998988
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

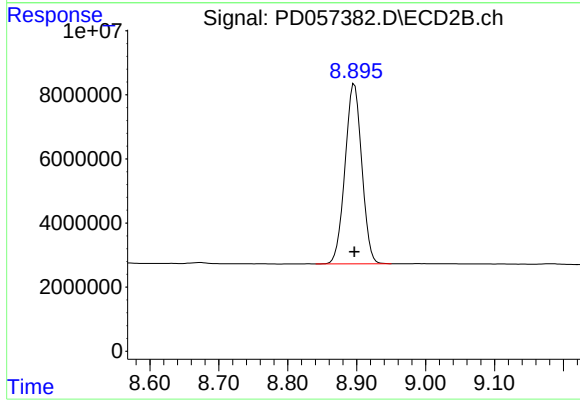

#27 Decachlorobiphenyl

R.T.: 8.897 min
Delta R.T.: 0.000 min
Response: 94805628
Conc: 40.00 ng/ml