

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021920\
 Data File : PD057384.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2020 18:20
 Operator : AJ\MA
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 06:14:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021920CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 06:10:15 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.897	33434337	63043622	39.793	39.465
27)	SA Decachlor...	7.865	8.897	75880475	182.4E6	77.828	76.954
Target Compounds							
2)	A alpha-BHC	3.651	4.281	48641109	98085302	41.699	40.798
3)	MA gamma-BHC...	3.922	4.561	45634937	96212388	40.852	40.571
4)	MA Heptachlor	4.201	5.062	23107145	77617891	39.770	40.198
9)	A Endosulfan I	5.197	6.099	38855951	99285192	40.849	40.099
13)	MA Dieldrin	5.435	6.354	85095943	229.4E6	84.519	82.084
14)	MA Endrin	5.687	6.570	68770762	188.4E6	82.693	81.361
16)	A 4,4'-DDD	5.823	6.696	56764080	185.7E6	83.248	81.359
17)	MA 4,4'-DDT	6.056	6.993	42449299	153.7E6	83.451	84.803
20)	A Methoxychlor	6.603	7.451	99894750	401.8E6	393.752	395.971


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021920\
Data File : PD057384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2020 18:20
Operator : AJ\MA
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 06:14:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021920CLP.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 06:10:15 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

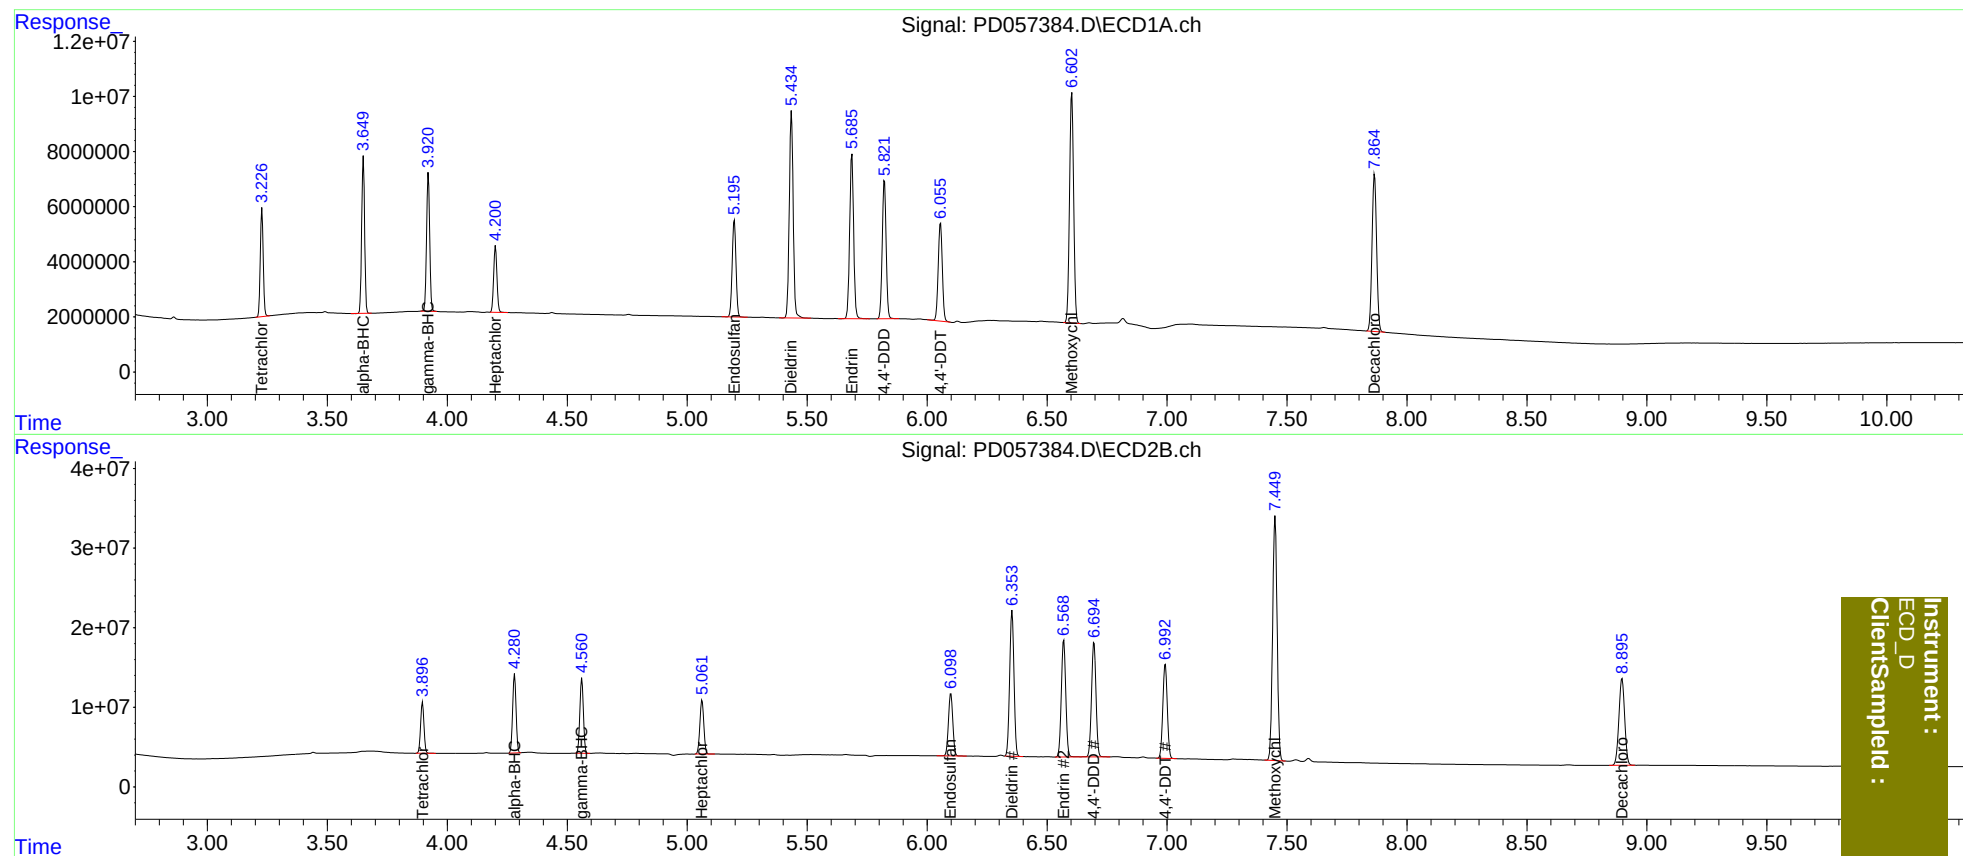


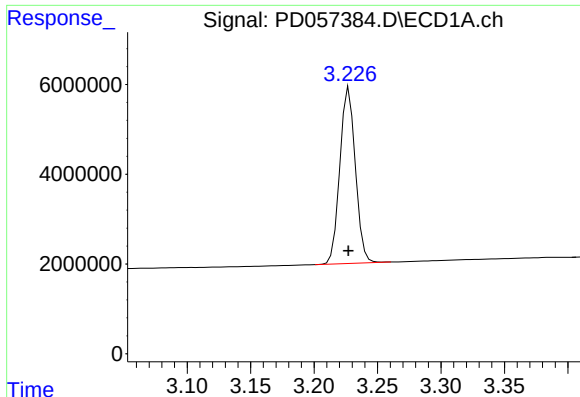

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 33434337
Conc: 39.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

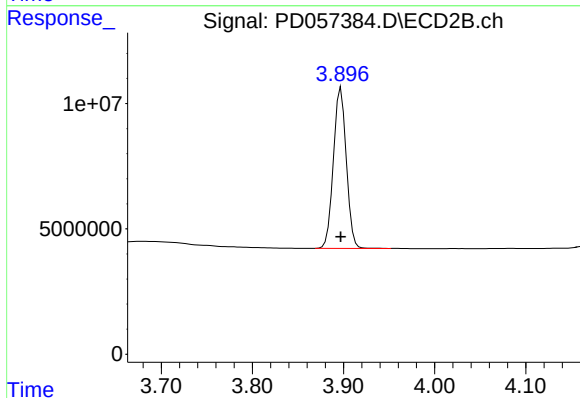


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 63043622
Conc: 39.46 ng/ml

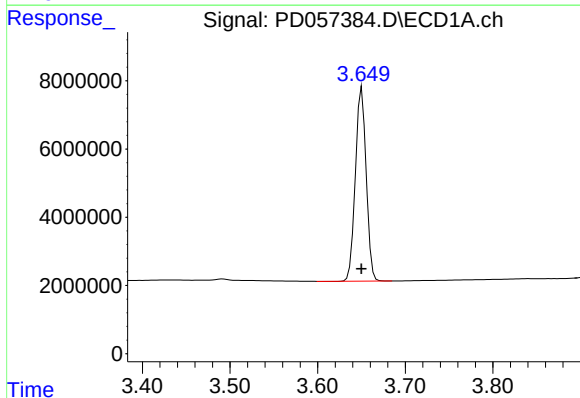


#2 alpha-BHC

R.T.: 3.651 min
Delta R.T.: 0.000 min
Response: 48641109
Conc: 41.70 ng/ml

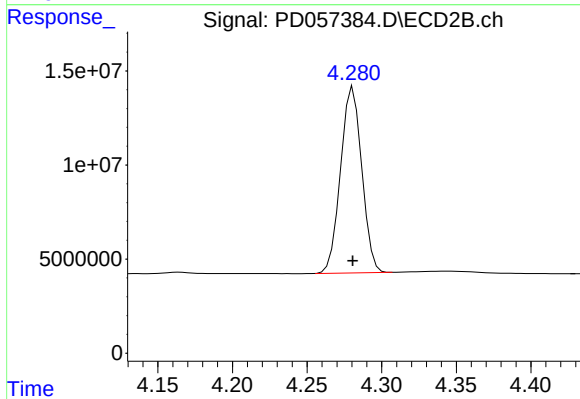

#2 alpha-BHC


R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 98085302
Conc: 40.80 ng/ml

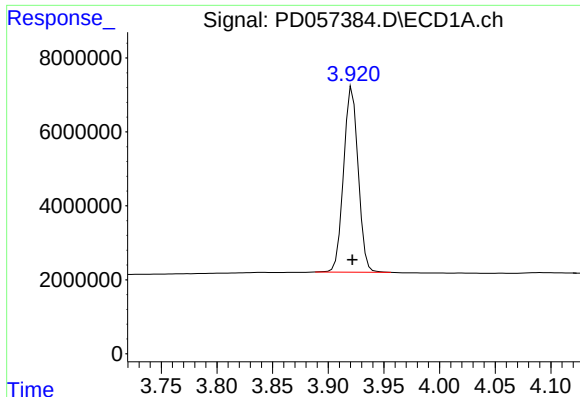

#3 gamma-BHC (Lindane)


R.T.: 3.922 min
Delta R.T.: 0.000 min
Response: 45634937
Conc: 40.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

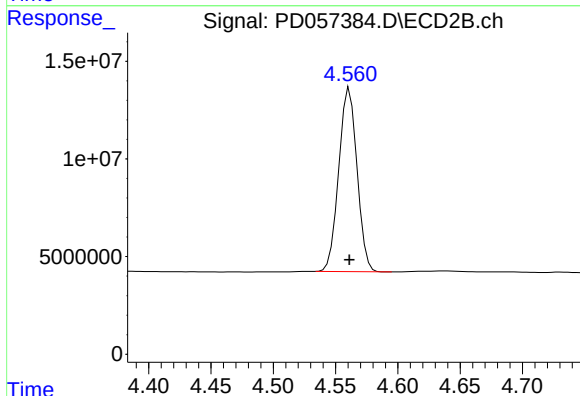


#3 gamma-BHC (Lindane)

R.T.: 4.561 min
Delta R.T.: 0.000 min
Response: 96212388
Conc: 40.57 ng/ml

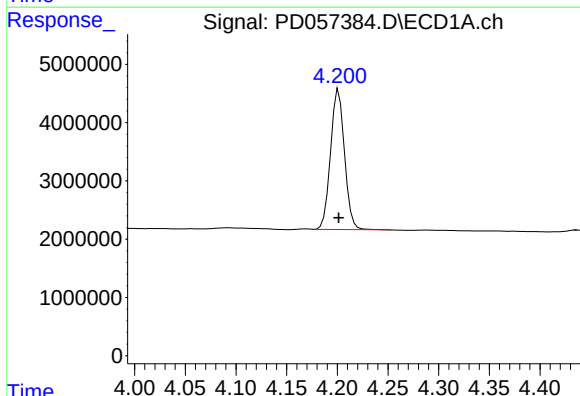


#4 Heptachlor

R.T.: 4.201 min
Delta R.T.: 0.000 min
Response: 23107145
Conc: 39.77 ng/ml

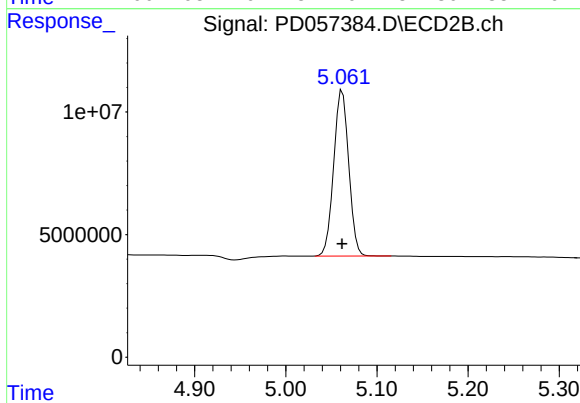

#4 Heptachlor


R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 77617891
Conc: 40.20 ng/ml

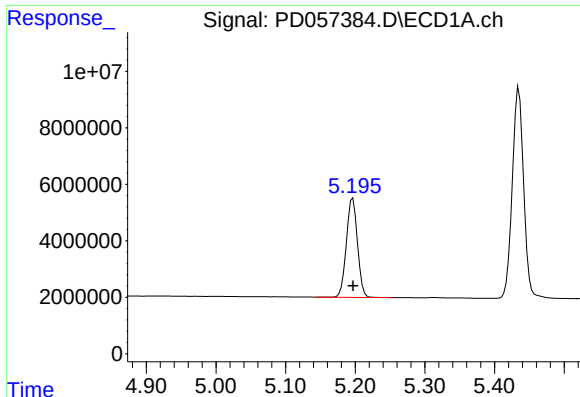

#9 Endosulfan I


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 38855951
Conc: 40.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

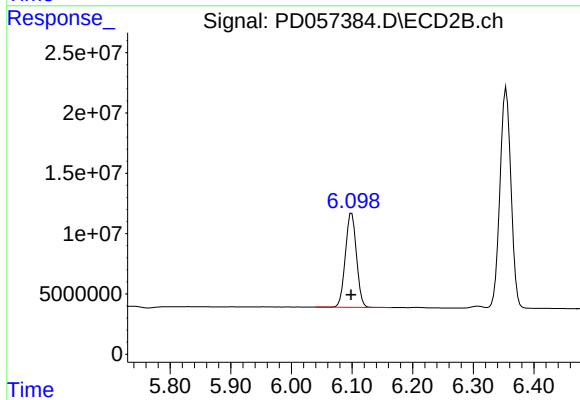


#9 Endosulfan I

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 99285192
Conc: 40.10 ng/ml

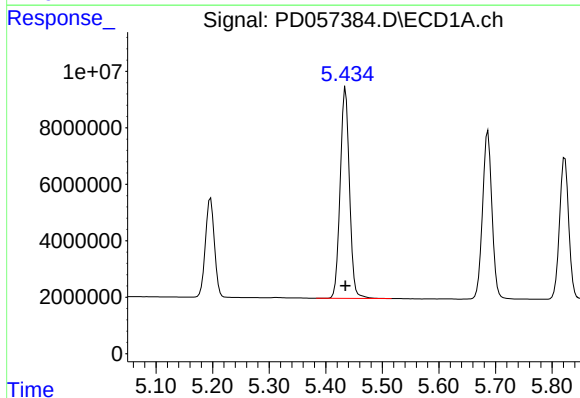


#13 Dieldrin

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 85095943
Conc: 84.52 ng/ml

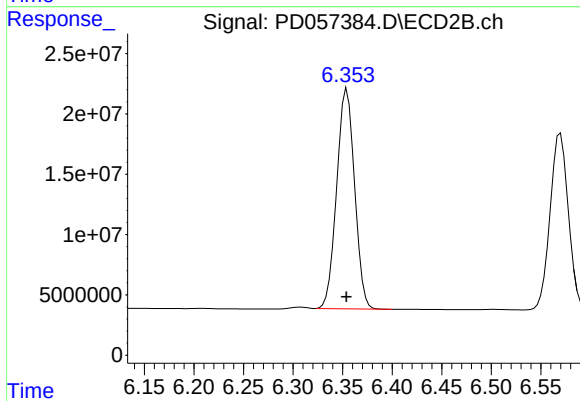

#13 Dieldrin


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 229367969
Conc: 82.08 ng/ml

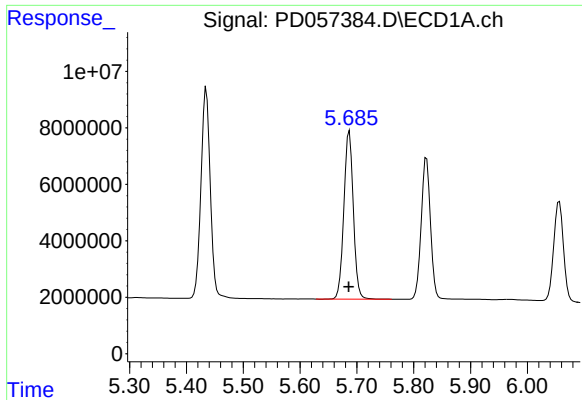

#14 Endrin


R.T.: 5.687 min
Delta R.T.: 0.001 min
Response: 68770762
Conc: 82.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

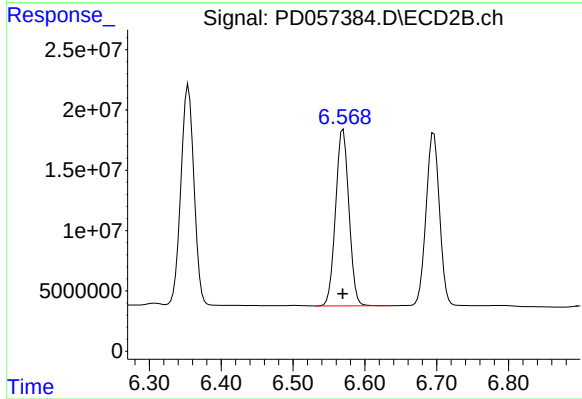


#14 Endrin

R.T.: 6.570 min
Delta R.T.: 0.000 min
Response: 188408340
Conc: 81.36 ng/ml

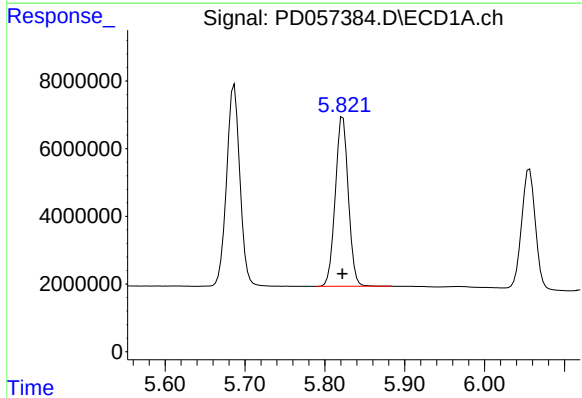


#16 4,4'-DDD

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 56764080
Conc: 83.25 ng/ml

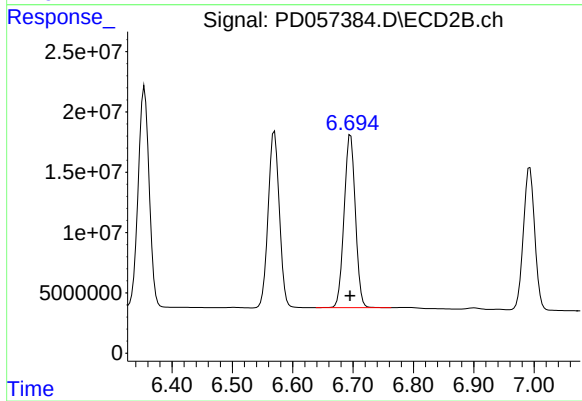

#16 4,4'-DDD


R.T.: 6.696 min
Delta R.T.: 0.000 min
Response: 185699081
Conc: 81.36 ng/ml

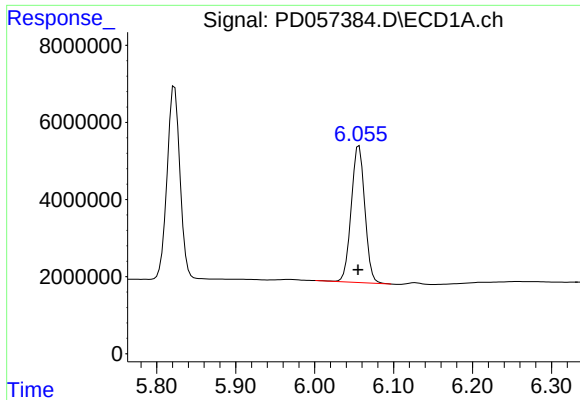

#17 4,4'-DDT


R.T.: 6.056 min
Delta R.T.: 0.001 min
Response: 42449299
Conc: 83.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

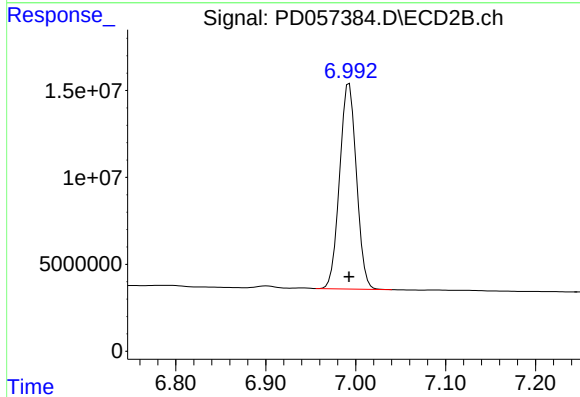


#17 4,4'-DDT

R.T.: 6.993 min
Delta R.T.: 0.000 min
Response: 153660417
Conc: 84.80 ng/ml

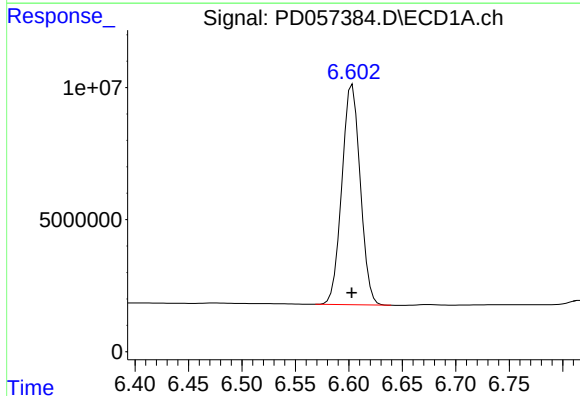


#20 Methoxychlor

R.T.: 6.603 min
Delta R.T.: 0.000 min
Response: 99894750
Conc: 393.75 ng/ml

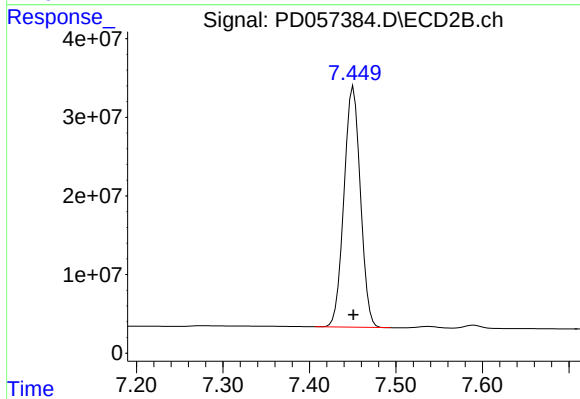

#20 Methoxychlor


R.T.: 7.451 min
Delta R.T.: 0.000 min
Response: 401844505
Conc: 395.97 ng/ml

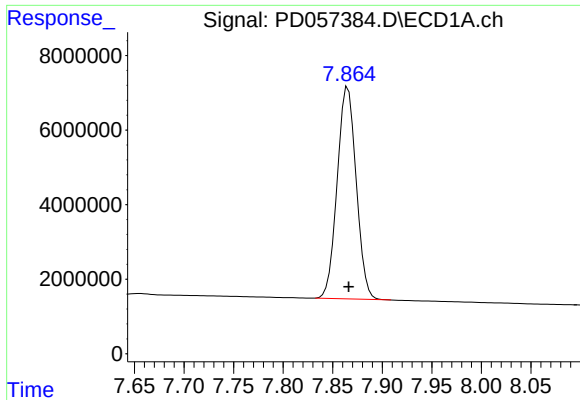

#27 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: 0.000 min
Response: 75880475
Conc: 77.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

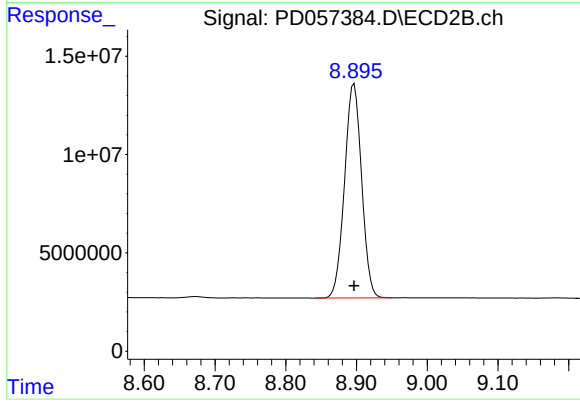

#27 Decachlorobiphenyl

R.T.: 8.897 min
Delta R.T.: 0.000 min
Response: 182390688
Conc: 76.95 ng/ml