

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021920\
 Data File : PD057384.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2020 18:20
 Operator : AJ\MA
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 06:14:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021920CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 06:10:15 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.897	33434337	63043622	39.793	39.465
27)	SA Decachlor...	7.865	8.897	75880475	182.4E6	77.828	76.954
Target Compounds							
2)	A alpha-BHC	3.651	4.281	48641109	98085302	41.699	40.798
3)	MA gamma-BHC...	3.922	4.561	45634937	96212388	40.852	40.571
4)	MA Heptachlor	4.201	5.062	23107145	77617891	39.770	40.198
9)	A Endosulfan I	5.197	6.099	38855951	99285192	40.849	40.099
13)	MA Dieldrin	5.435	6.354	85095943	229.4E6	84.519	82.084
14)	MA Endrin	5.687	6.570	68770762	188.4E6	82.693	81.361
16)	A 4,4'-DDD	5.823	6.696	56764080	185.7E6	83.248	81.359
17)	MA 4,4'-DDT	6.056	6.993	42449299	153.7E6	83.451	84.803
20)	A Methoxychlor	6.603	7.451	99894750	401.8E6	393.752	395.971

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021920\
Data File : PD057384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2020 18:20
Operator : AJ\MA
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 06:14:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021920CLP.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 06:10:15 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

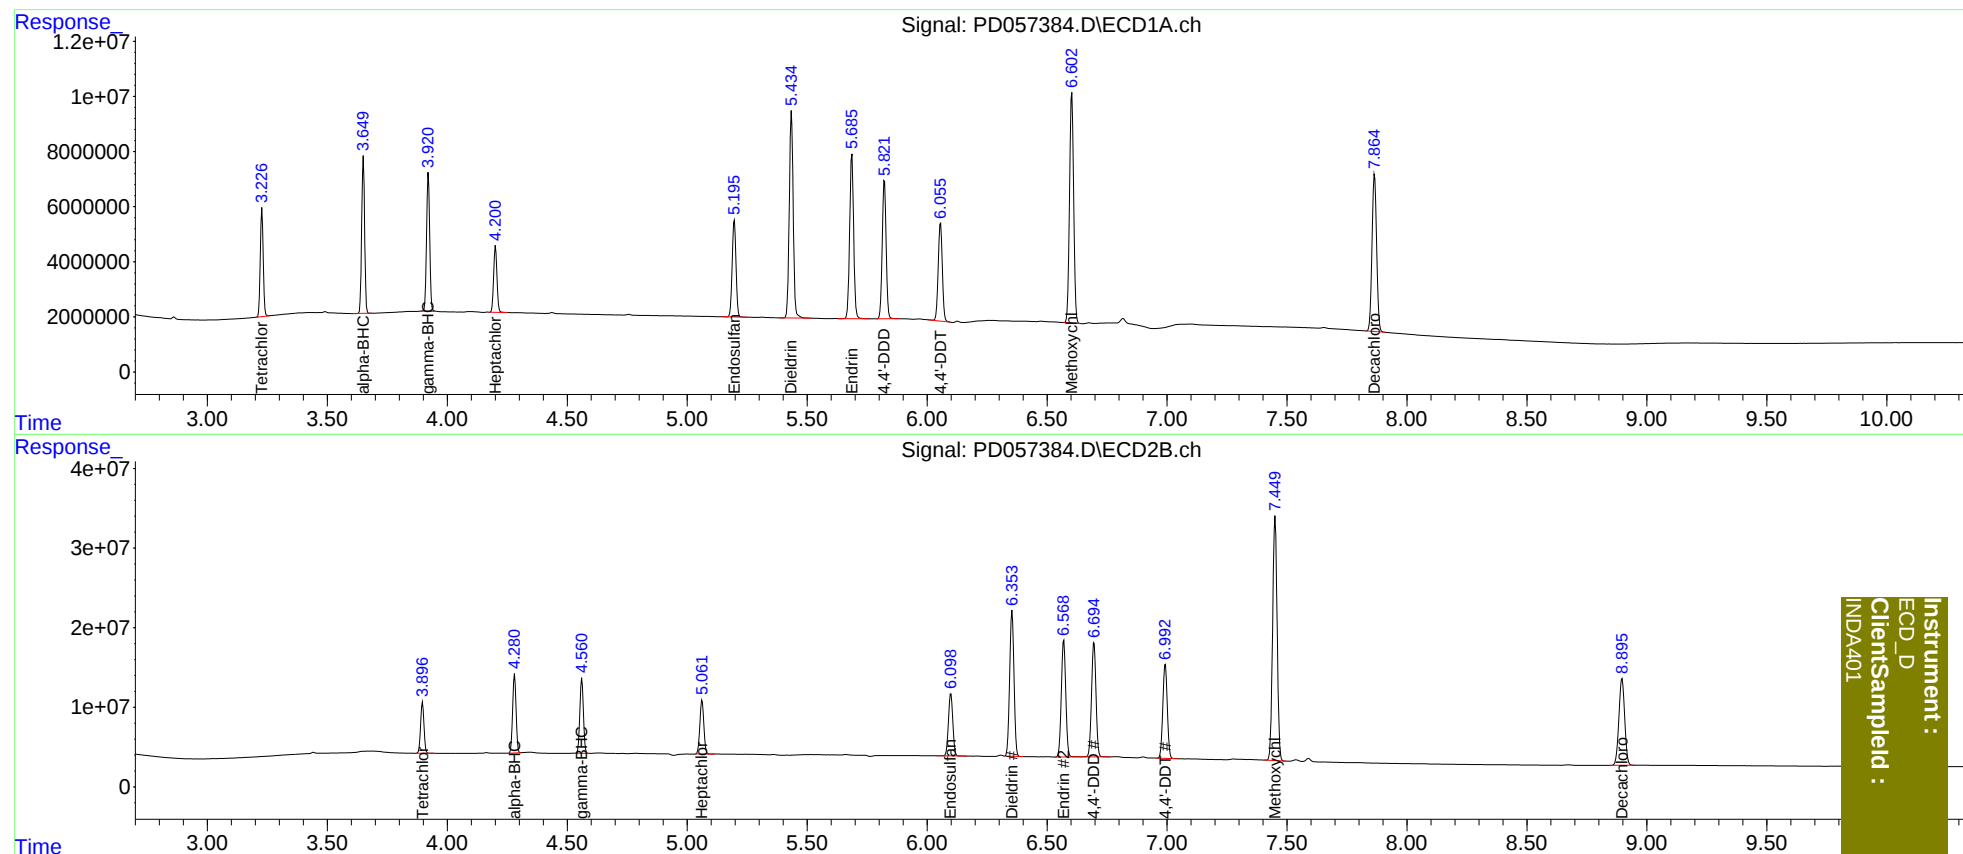

Instrument :
ECD_D
ClientSampled :
INDA401