

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022023\
 Data File : PD074003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 19:58
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:40:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022023.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 21 00:32:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.774	179.4E6	112.4E6	74.568	74.830
28)	SA Decachlor...	9.102	7.931	195.2E6	93593787	73.902	74.391
Target Compounds							
23)	Chlordane-1	4.720	3.777	83679188	35276089	746.267	746.065
24)	Chlordane-2	5.250	4.354	90291362	40621831	742.996	746.502
25)	Chlordane-3	5.964	4.986	372.9E6	120.3E6	743.722	745.691
26)	Chlordane-4	6.046	5.049	448.7E6	114.7E6	743.147	746.978
27)	Chlordane-5	6.898	5.947	77576701	43154532	742.470	744.711



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022023\
Data File : PD074003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 19:58
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:40:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022023.M
Quant Title : GC Extractables
QLast Update : Tue Feb 21 00:32:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

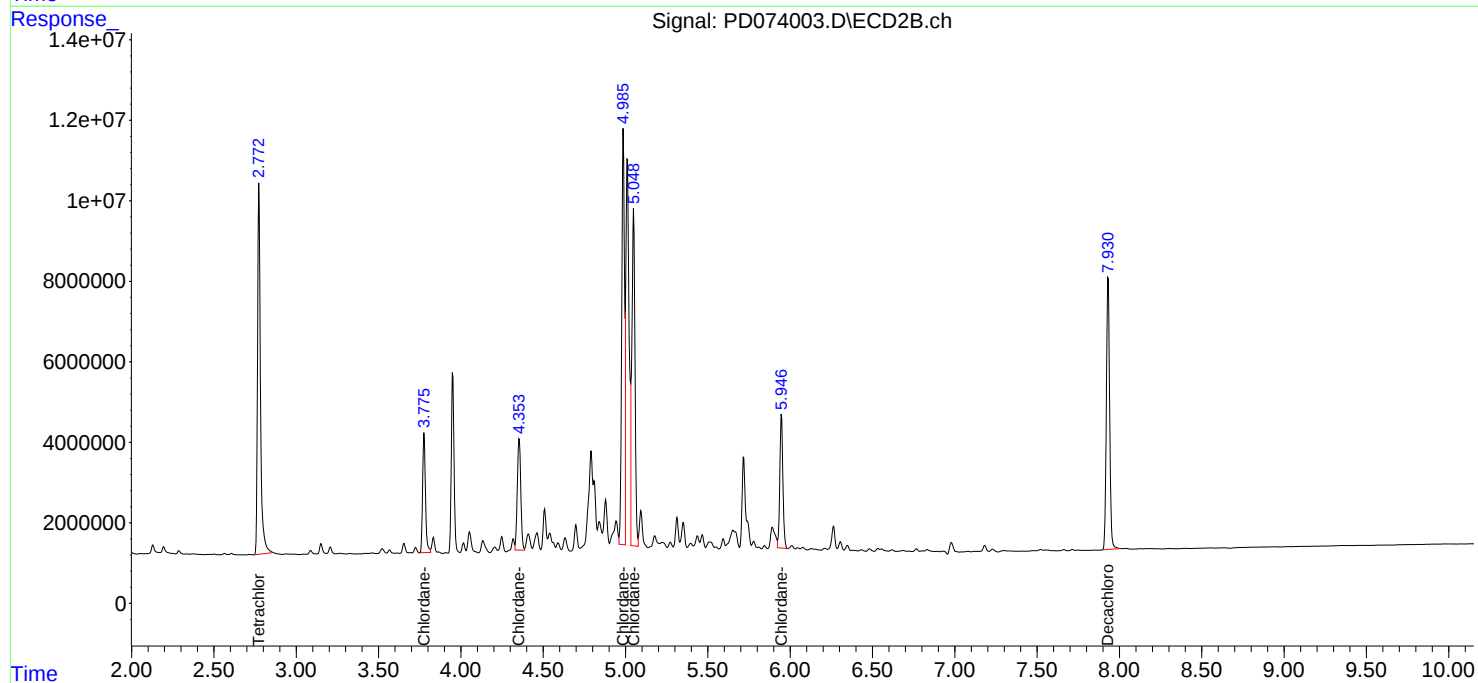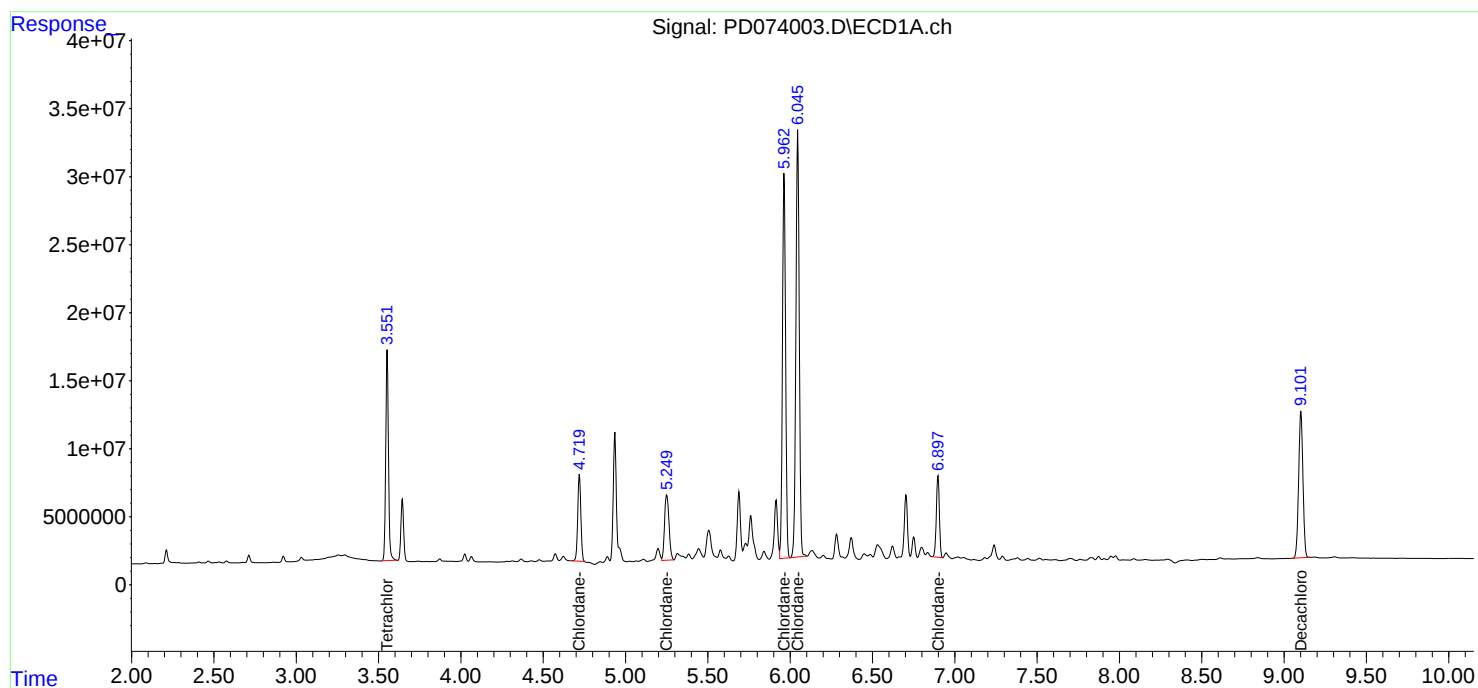


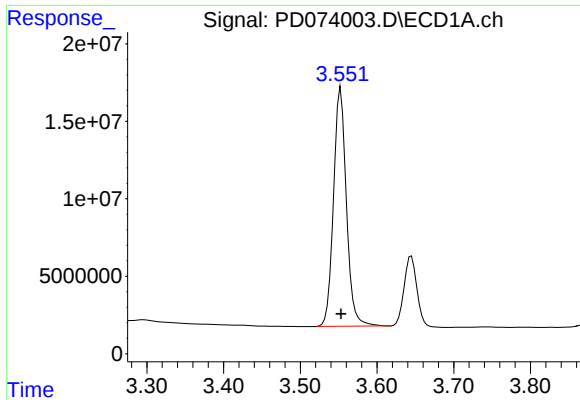

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.000 min
Response: 179423734
Conc: 74.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

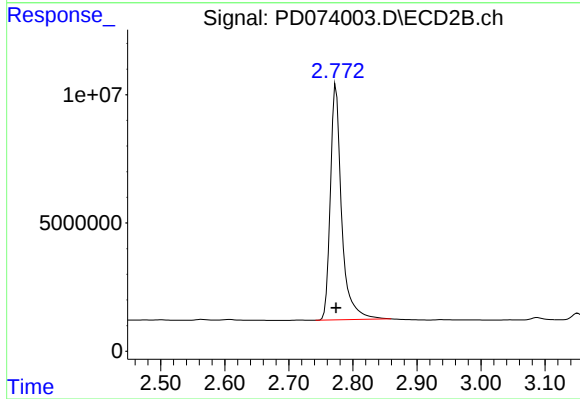


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 112448750
Conc: 74.83 ng/ml

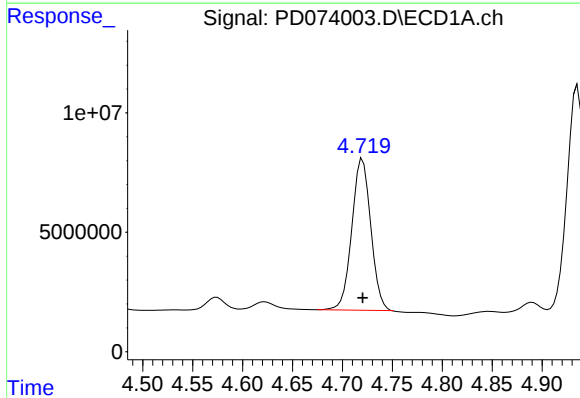


#23 Chlordane-1

R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 83679188
Conc: 746.27 ng/ml

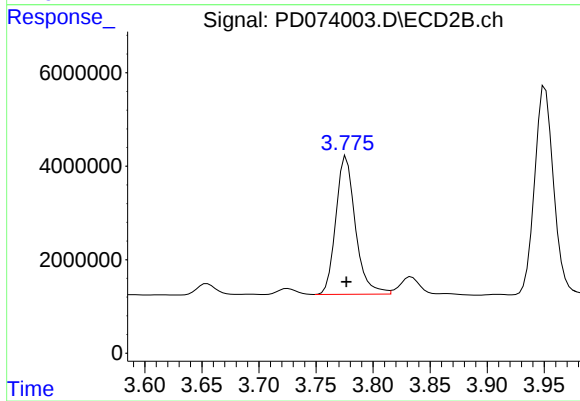

#23 Chlordane-1


R.T.: 3.777 min
Delta R.T.: 0.000 min
Response: 35276089
Conc: 746.07 ng/ml

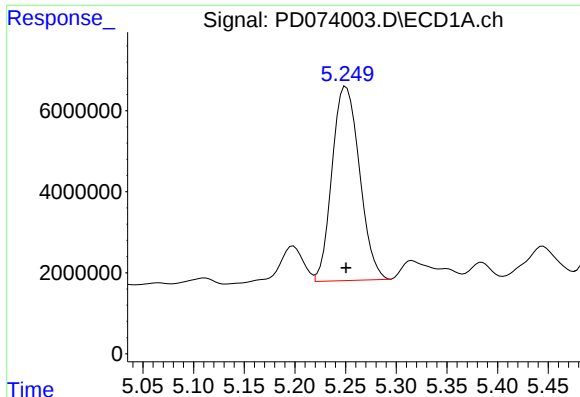

#24 Chlordane-2


R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 90291362
Conc: 743.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

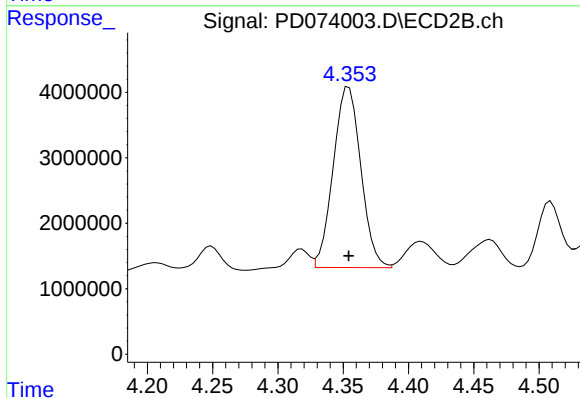


#24 Chlordane-2

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 40621831
Conc: 746.50 ng/ml

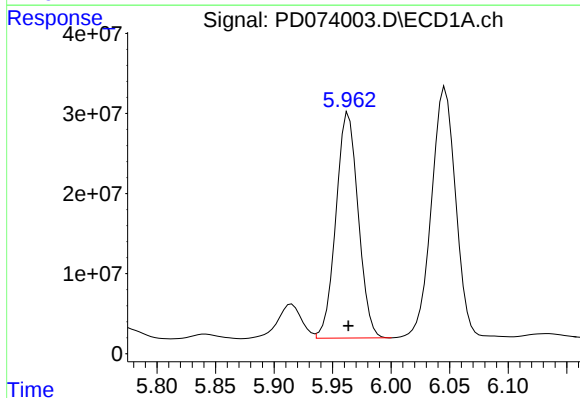


#25 Chlordane-3

R.T.: 5.964 min
Delta R.T.: 0.000 min
Response: 372891390
Conc: 743.72 ng/ml

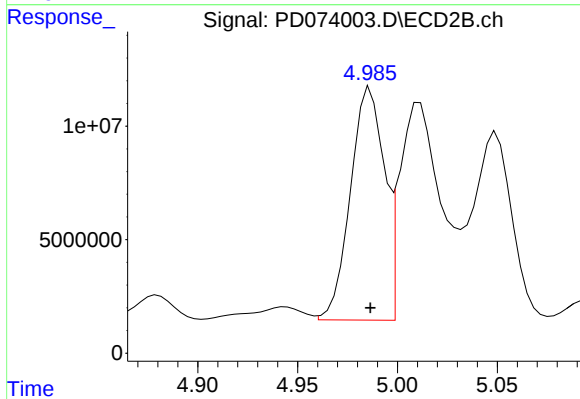

#25 Chlordane-3


R.T.: 4.986 min
Delta R.T.: 0.000 min
Response: 120330963
Conc: 745.69 ng/ml

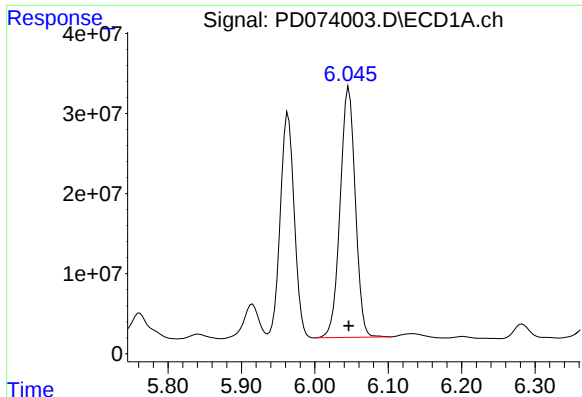

#26 Chlordane-4


R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 448660818
Conc: 743.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

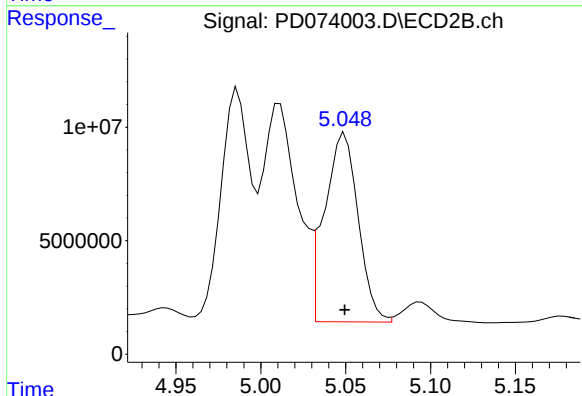


#26 Chlordane-4

R.T.: 5.049 min
Delta R.T.: 0.000 min
Response: 114682534
Conc: 746.98 ng/ml

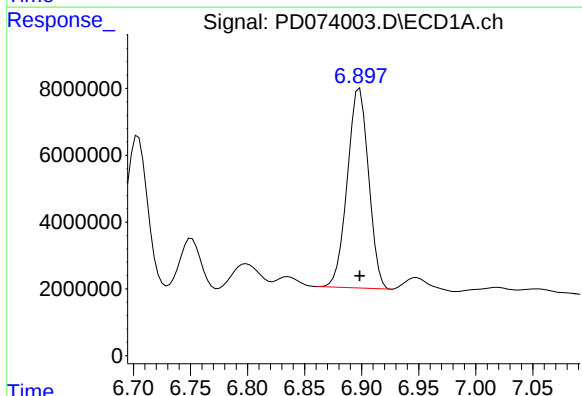


#27 Chlordane-5

R.T.: 6.898 min
Delta R.T.: 0.000 min
Response: 77576701
Conc: 742.47 ng/ml

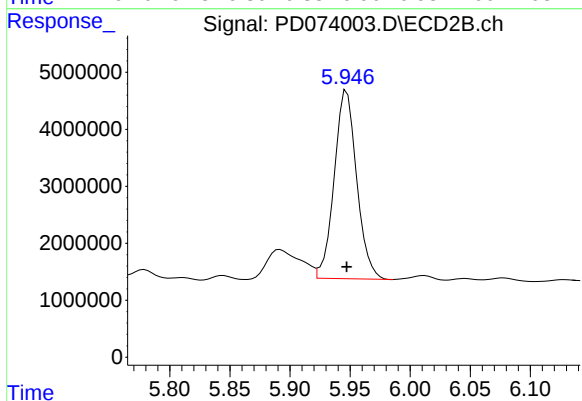

#27 Chlordane-5


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 43154532
Conc: 744.71 ng/ml

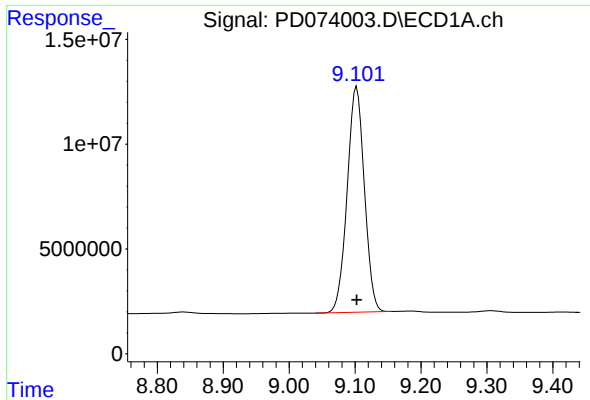

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: 0.000 min
Response: 195220489
Conc: 73.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

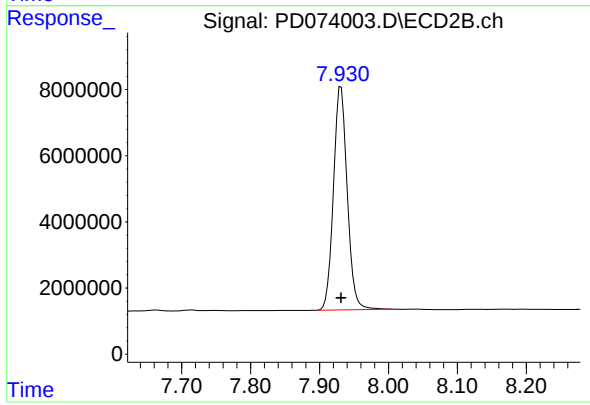

#28 Decachlorobiphenyl

R.T.: 7.931 min
Delta R.T.: 0.000 min
Response: 93593787
Conc: 74.39 ng/ml