

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022023\
 Data File : PD074004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 20:11
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:33:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022023.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 21 00:32:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.774	120.4E6	74818833	50.000	50.000
28)	SA Decachlor...	9.102	7.931	137.0E6	64323286	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.720	3.777	56398758	23601606	500.000	500.000
24)	Chlordane-2	5.251	4.354	62644862	27905722	500.000	500.000
25)	Chlordane-3	5.964	4.987	249.0E6	80253371	500.000	500.000
26)	Chlordane-4	6.047	5.050	302.2E6	75969761	500.000	500.000
27)	Chlordane-5	6.899	5.947	52754161	29084441	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022023\
Data File : PD074004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 20:11
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:33:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022023.M
Quant Title : GC Extractables
QLast Update : Tue Feb 21 00:32:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

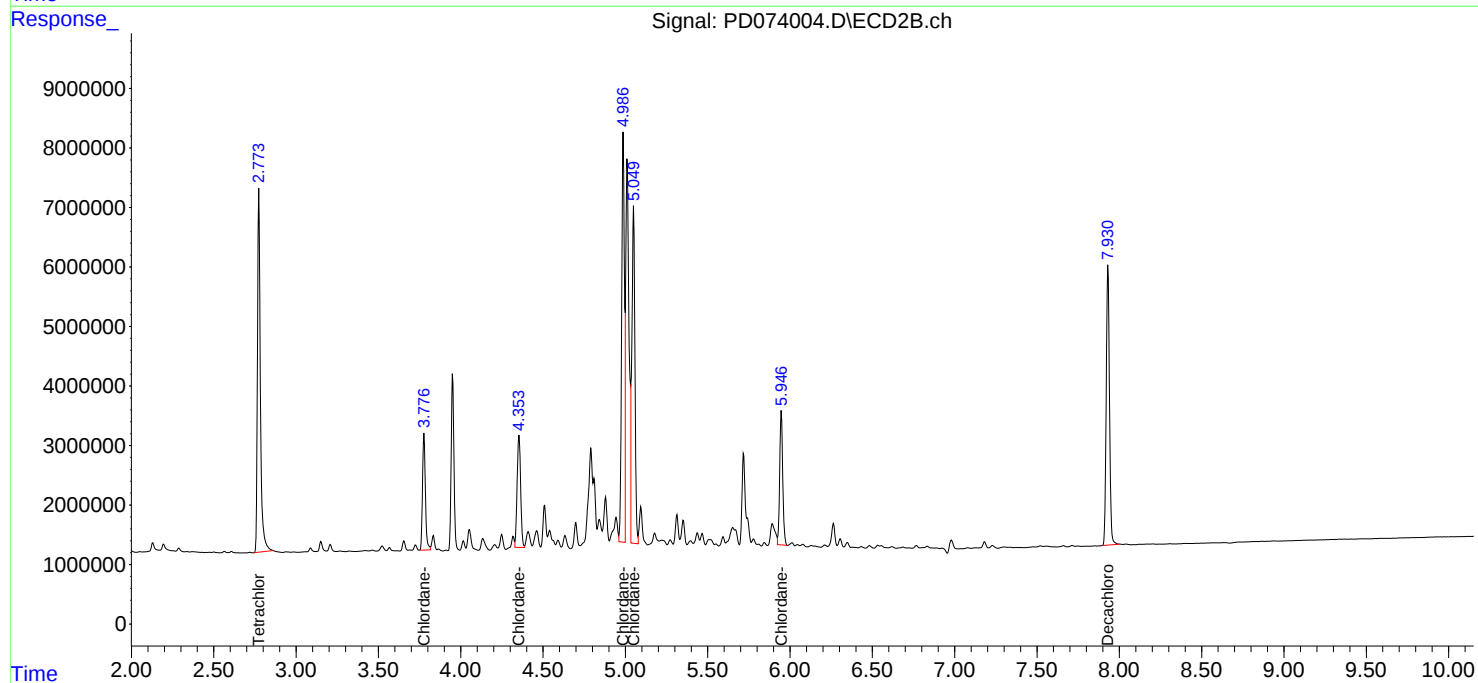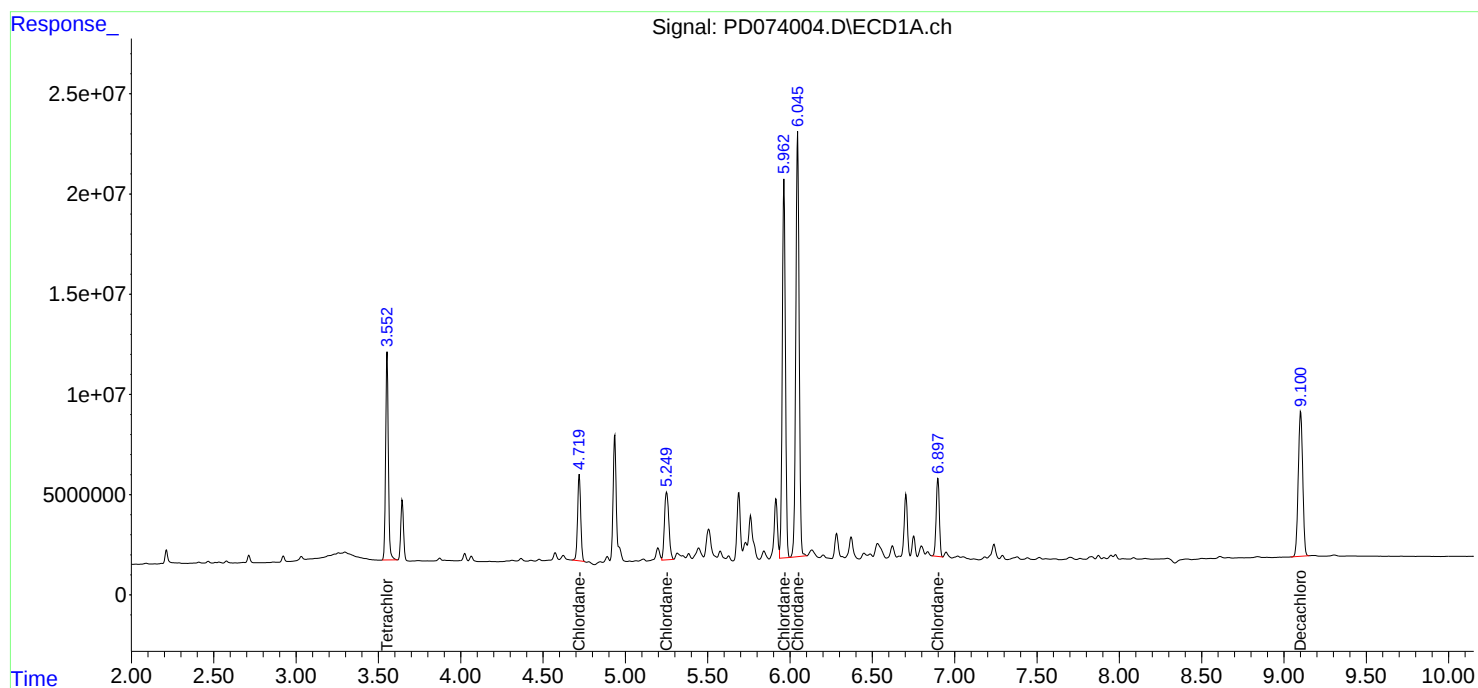


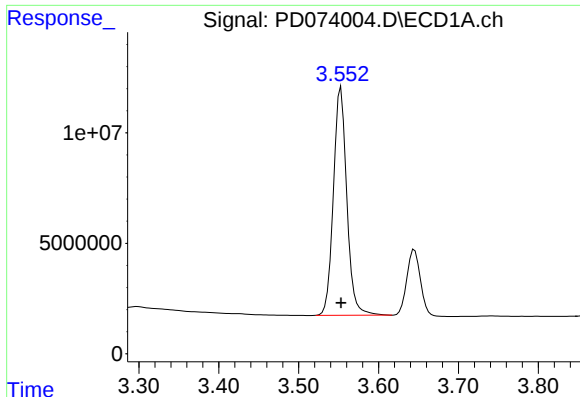

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.000 min
Response: 120382150
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

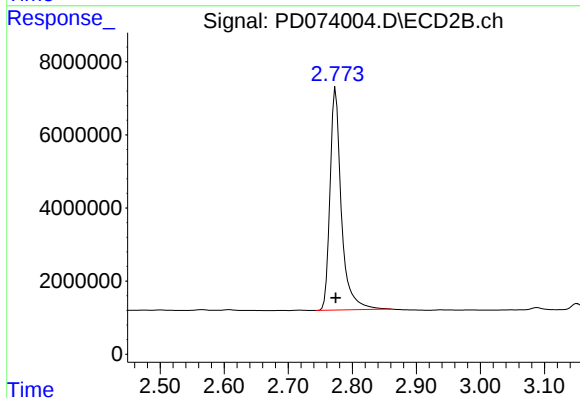


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 74818833
Conc: 50.00 ng/ml

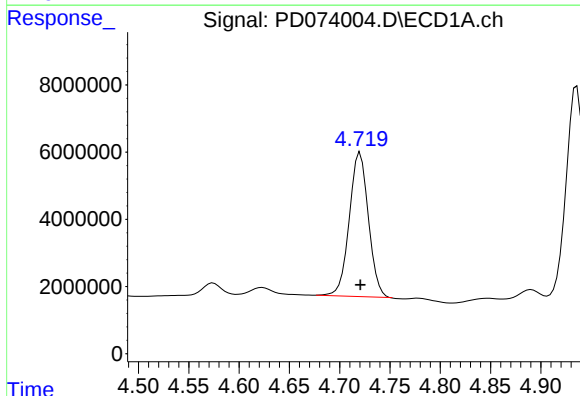


#23 Chlordane-1

R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 56398758
Conc: 500.00 ng/ml

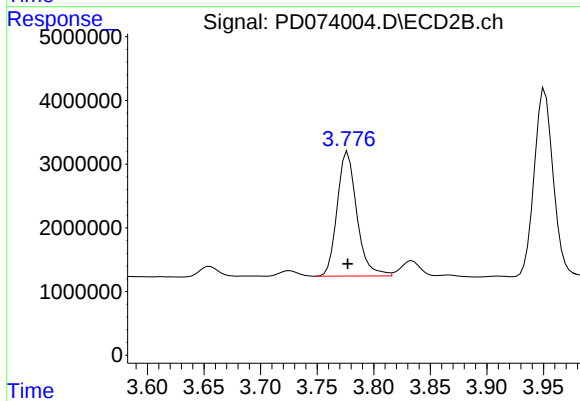

#23 Chlordane-1


R.T.: 3.777 min
Delta R.T.: 0.000 min
Response: 23601606
Conc: 500.00 ng/ml

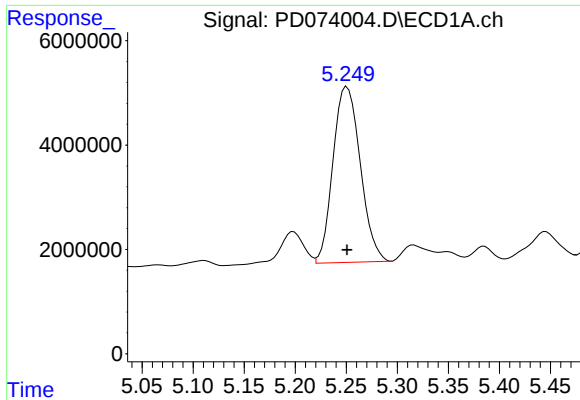

#24 Chlordane-2


R.T.: 5.251 min
Delta R.T.: 0.000 min
Response: 62644862
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

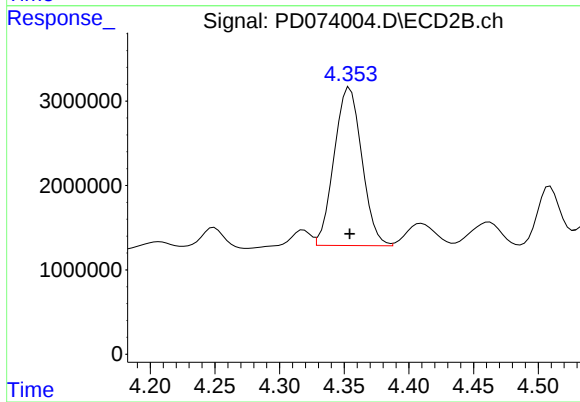


#24 Chlordane-2

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 27905722
Conc: 500.00 ng/ml

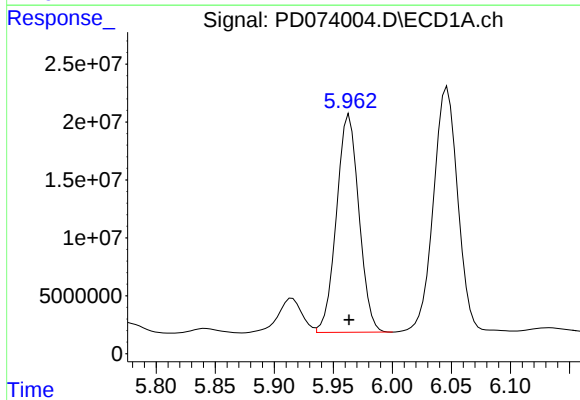


#25 Chlordane-3

R.T.: 5.964 min
Delta R.T.: 0.000 min
Response: 249007083
Conc: 500.00 ng/ml

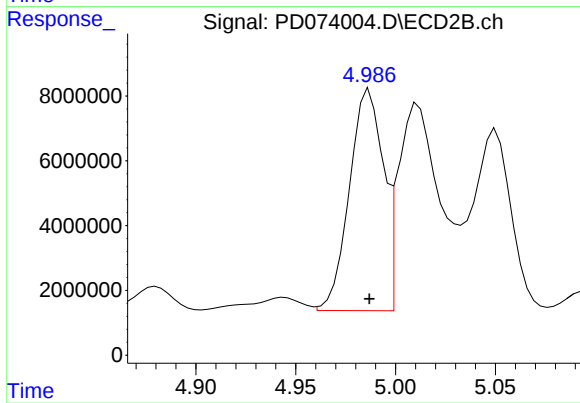

#25 Chlordane-3


R.T.: 4.987 min
Delta R.T.: 0.000 min
Response: 80253371
Conc: 500.00 ng/ml

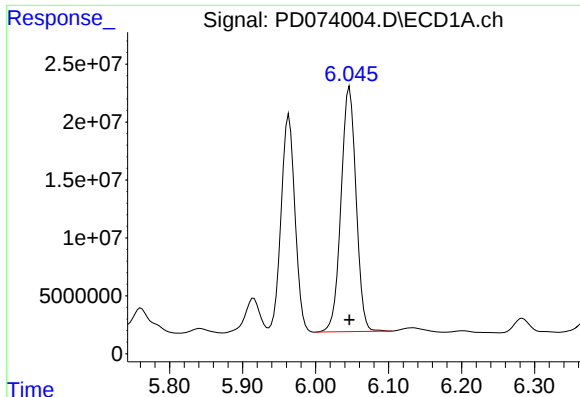

#26 Chlordane-4


R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 302222356
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

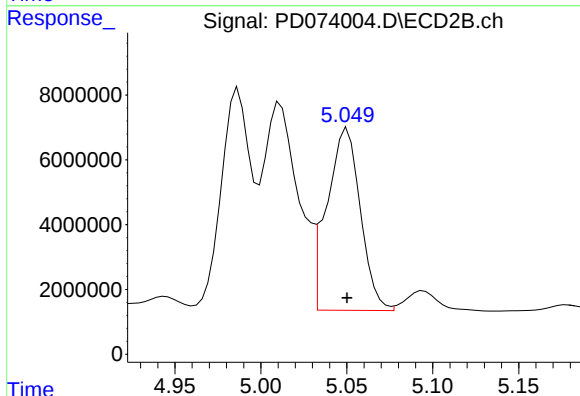


#26 Chlordane-4

R.T.: 5.050 min
Delta R.T.: 0.000 min
Response: 75969761
Conc: 500.00 ng/ml

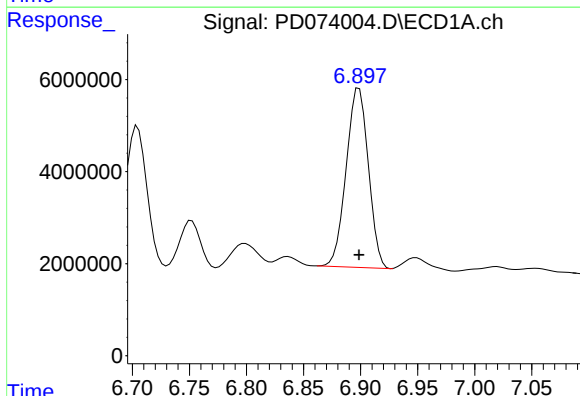


#27 Chlordane-5

R.T.: 6.899 min
Delta R.T.: 0.000 min
Response: 52754161
Conc: 500.00 ng/ml

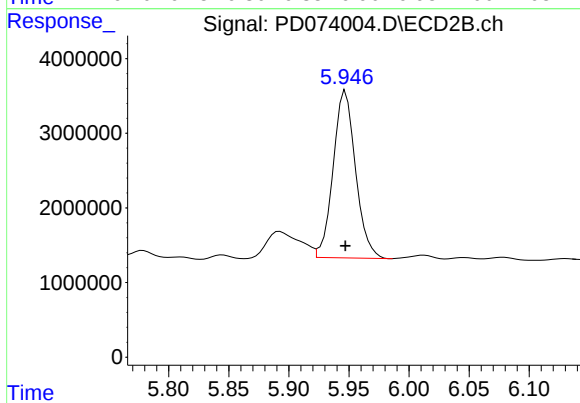

#27 Chlordane-5


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 29084441
Conc: 500.00 ng/ml

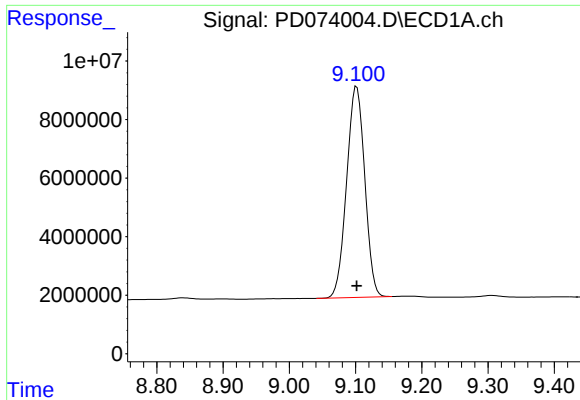

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: 0.000 min
Response: 137033946
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

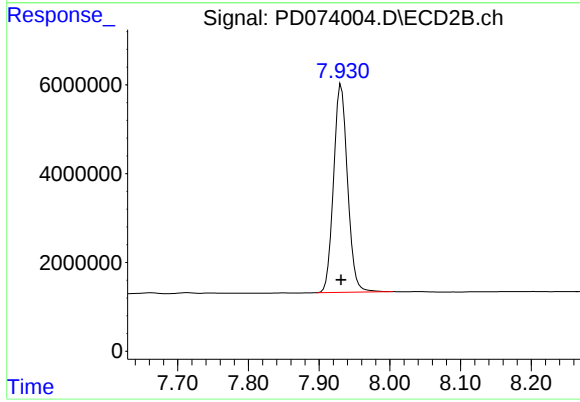

#28 Decachlorobiphenyl

R.T.: 7.931 min
Delta R.T.: 0.000 min
Response: 64323286
Conc: 50.00 ng/ml