

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022023\
 Data File : PD074005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 20:25
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:43:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022023.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 21 00:32:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.774	58241875	36200764	24.399	24.311
28)	SA Decachlor...	9.102	7.931	69719614	33098355	26.030	25.968
Target Compounds							
23)	Chlordane-1	4.720	3.777	27244209	11511346	244.690	245.061
24)	Chlordane-2	5.251	4.355	31641817	14156874	257.702	257.543
25)	Chlordane-3	5.964	4.986	114.4E6	37812708	233.335	238.057
26)	Chlordane-4	6.047	5.050	141.3E6	36818690	237.820	242.284
27)	Chlordane-5	6.899	5.948	25358793	14223070	244.488	246.568



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022023\
Data File : PD074005.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 20:25
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:43:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022023.M
Quant Title : GC Extractables
QLast Update : Tue Feb 21 00:32:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

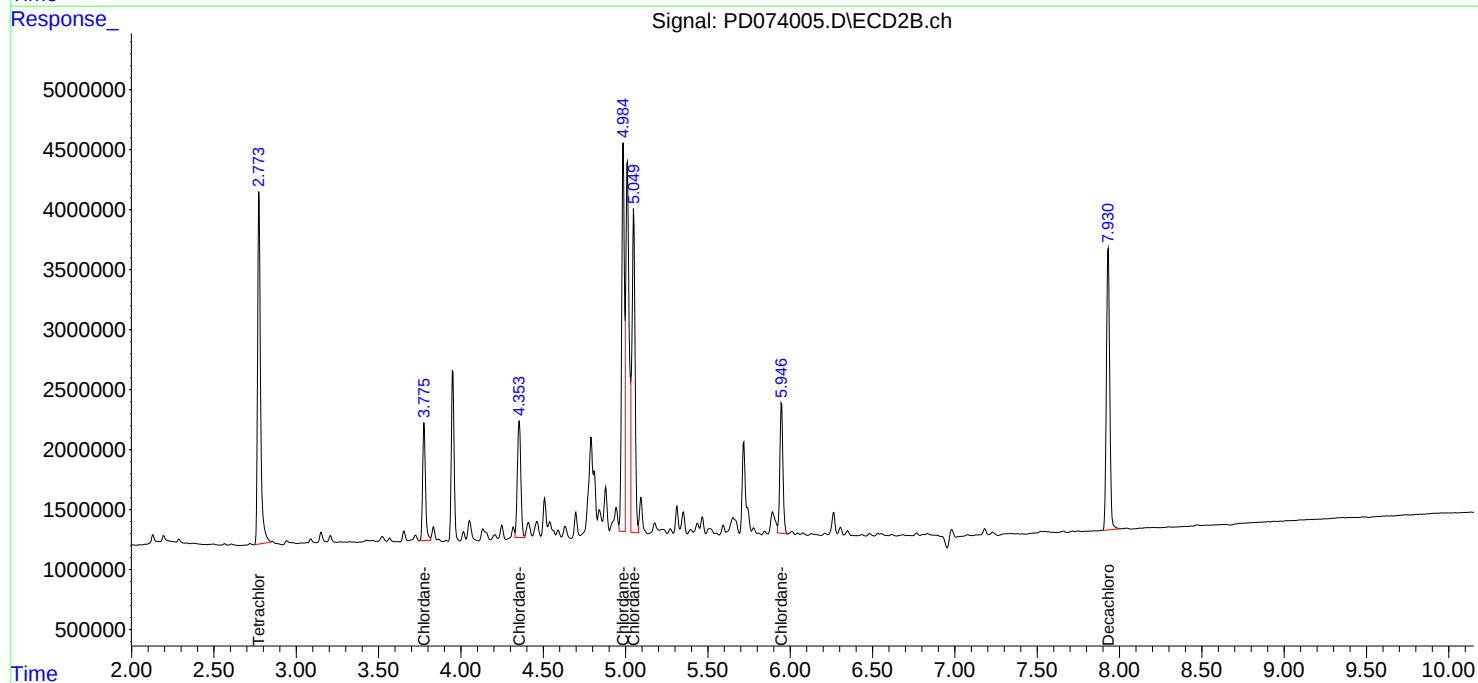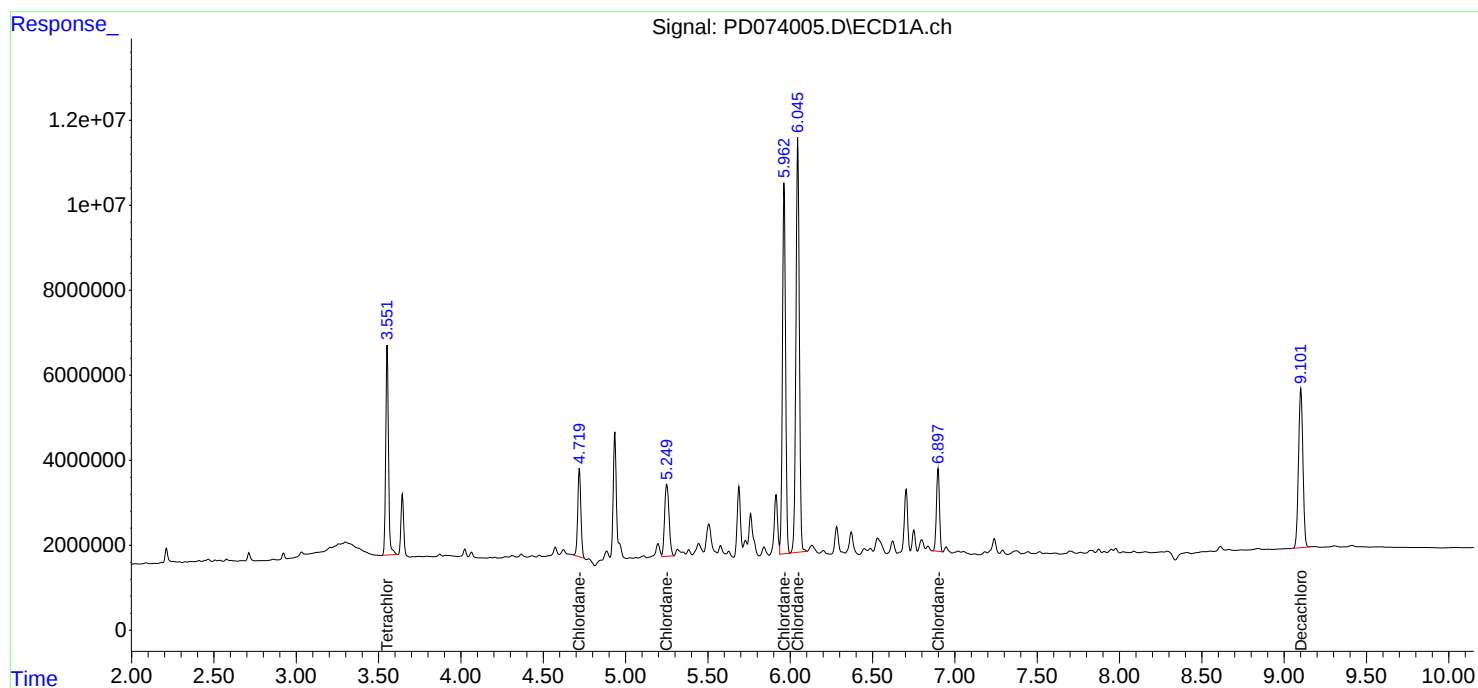


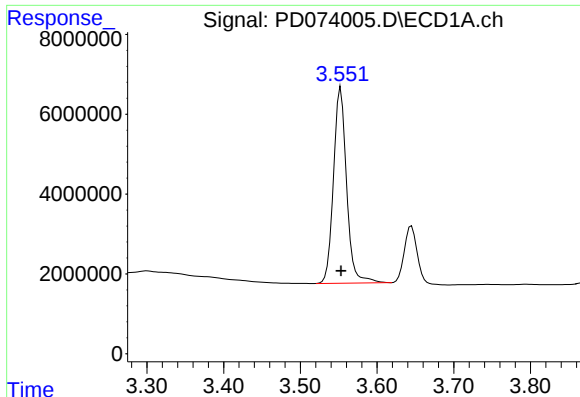

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.000 min
Response: 58241875
Conc: 24.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

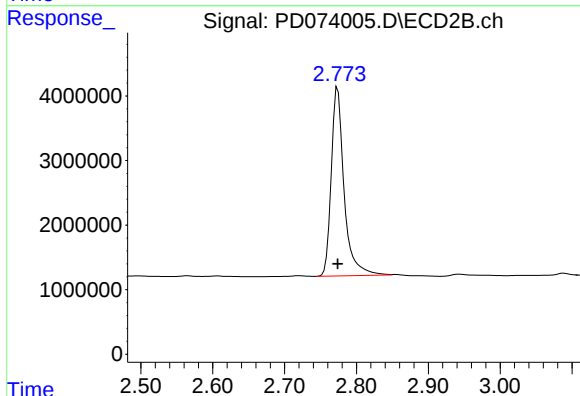


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 36200764
Conc: 24.31 ng/ml

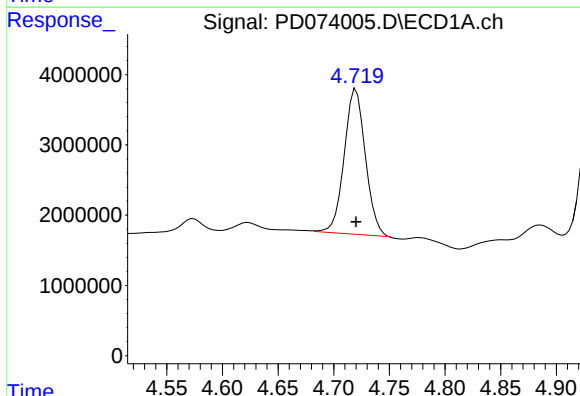


#23 Chlordane-1

R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 27244209
Conc: 244.69 ng/ml

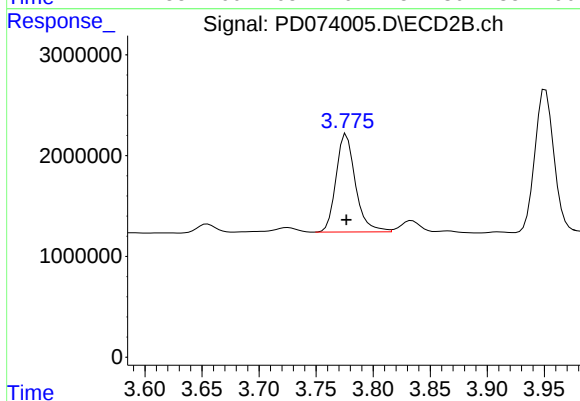

#23 Chlordane-1


R.T.: 3.777 min
Delta R.T.: 0.000 min
Response: 11511346
Conc: 245.06 ng/ml

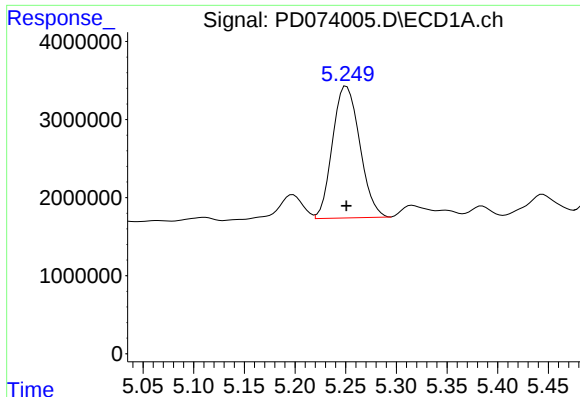

#24 Chlordane-2


R.T.: 5.251 min
Delta R.T.: 0.000 min
Response: 31641817
Conc: 257.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

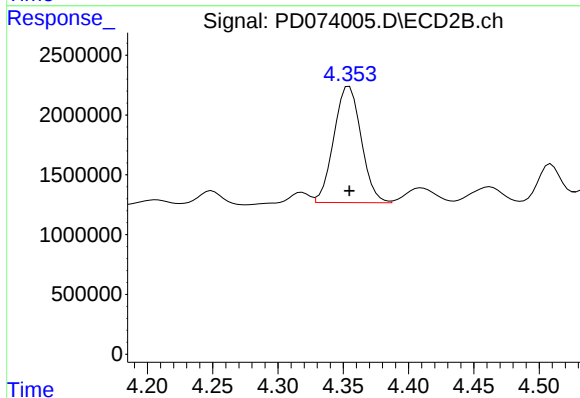


#24 Chlordane-2

R.T.: 4.355 min
Delta R.T.: 0.000 min
Response: 14156874
Conc: 257.54 ng/ml

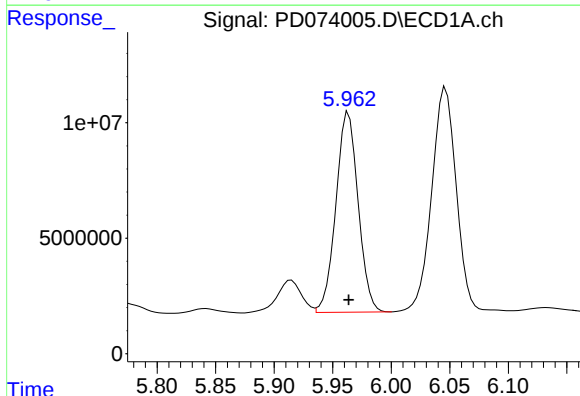


#25 Chlordane-3

R.T.: 5.964 min
Delta R.T.: 0.000 min
Response: 114447950
Conc: 233.34 ng/ml

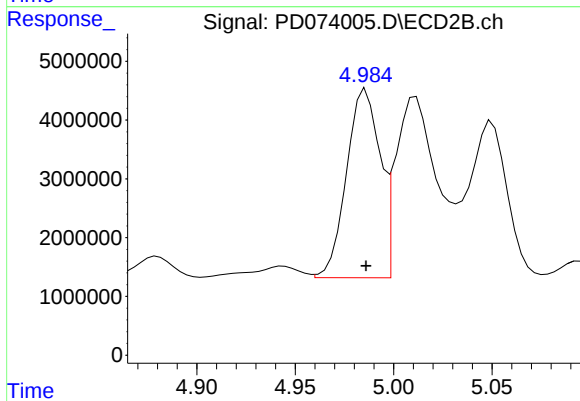

#25 Chlordane-3


R.T.: 4.986 min
Delta R.T.: 0.000 min
Response: 37812708
Conc: 238.06 ng/ml

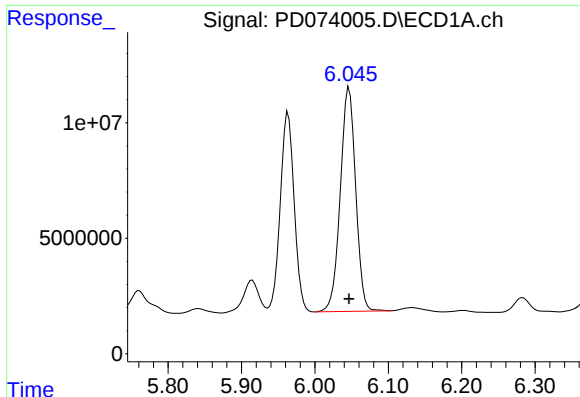

#26 Chlordane-4


R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 141284764
Conc: 237.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

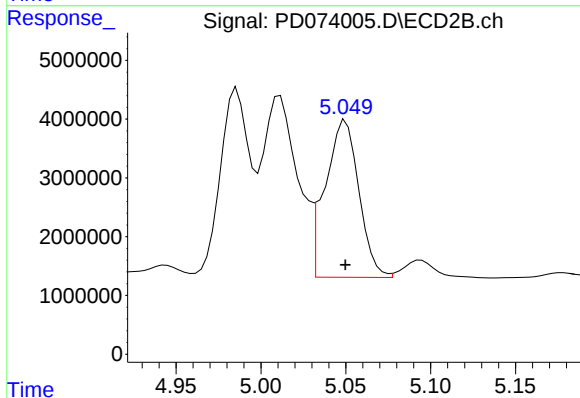


#26 Chlordane-4

R.T.: 5.050 min
Delta R.T.: 0.000 min
Response: 36818690
Conc: 242.28 ng/ml

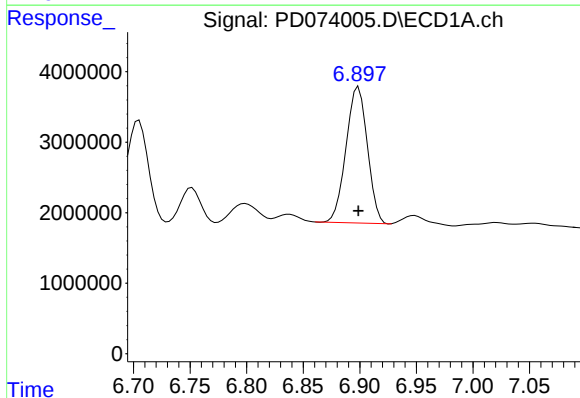


#27 Chlordane-5

R.T.: 6.899 min
Delta R.T.: 0.000 min
Response: 25358793
Conc: 244.49 ng/ml

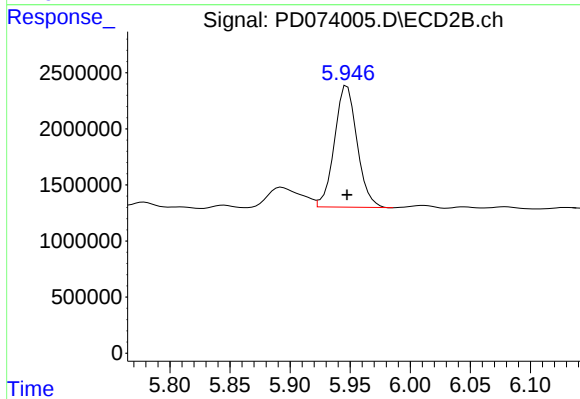

#27 Chlordane-5


R.T.: 5.948 min
Delta R.T.: 0.000 min
Response: 14223070
Conc: 246.57 ng/ml

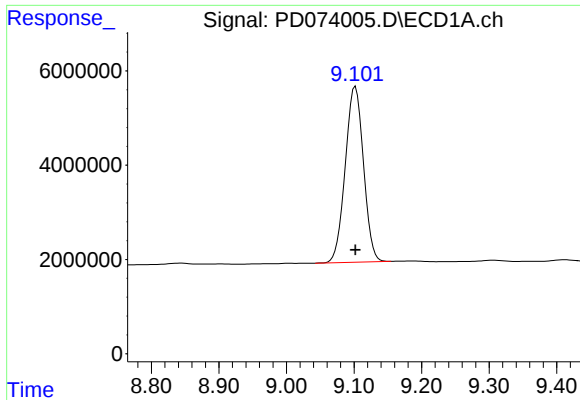

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: 0.000 min
Response: 69719614
Conc: 26.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

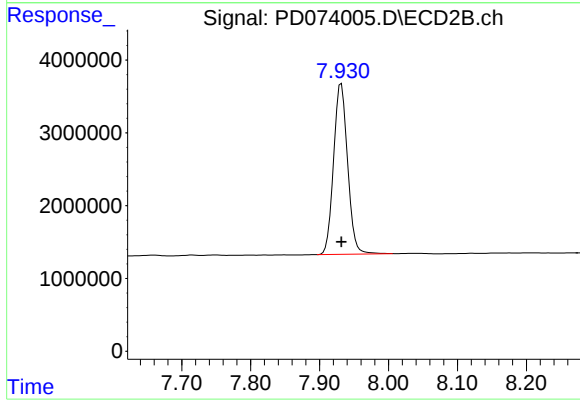

#28 Decachlorobiphenyl

R.T.: 7.931 min
Delta R.T.: 0.000 min
Response: 33098355
Conc: 25.97 ng/ml