

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022023\
 Data File : PD074013.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 22:12
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD022023CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:47:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022023.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 21 00:46:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.774	124.3E6	76410681	52.157	51.738
28)	SA Decachlor...	9.102	7.931	140.4E6	66212846	50.900	50.473
Target Compounds							
23)	Chlordane-1	4.720	3.776	59334882	24294744	529.882	522.926
24)	Chlordane-2	5.251	4.354	65333558	28466558	519.579	509.361
25)	Chlordane-3	5.964	4.986	260.3E6	81819963	540.393	519.263
26)	Chlordane-4	6.045	5.050	314.1E6	79402134	534.122	524.807
27)	Chlordane-5	6.898	5.947	54639392	29747326	527.541	518.132



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022023\
Data File : PD074013.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 22:12
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD022023CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:47:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022023.M
Quant Title : GC Extractables
QLast Update : Tue Feb 21 00:46:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

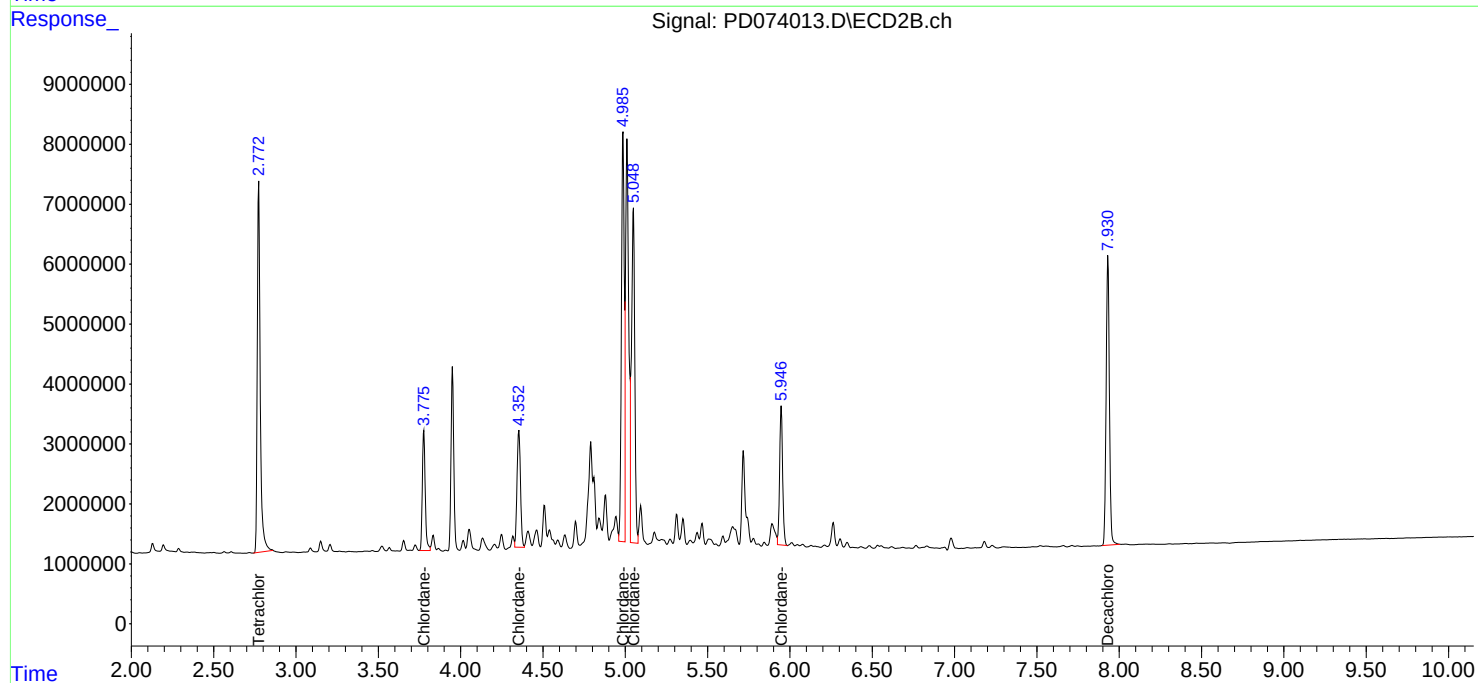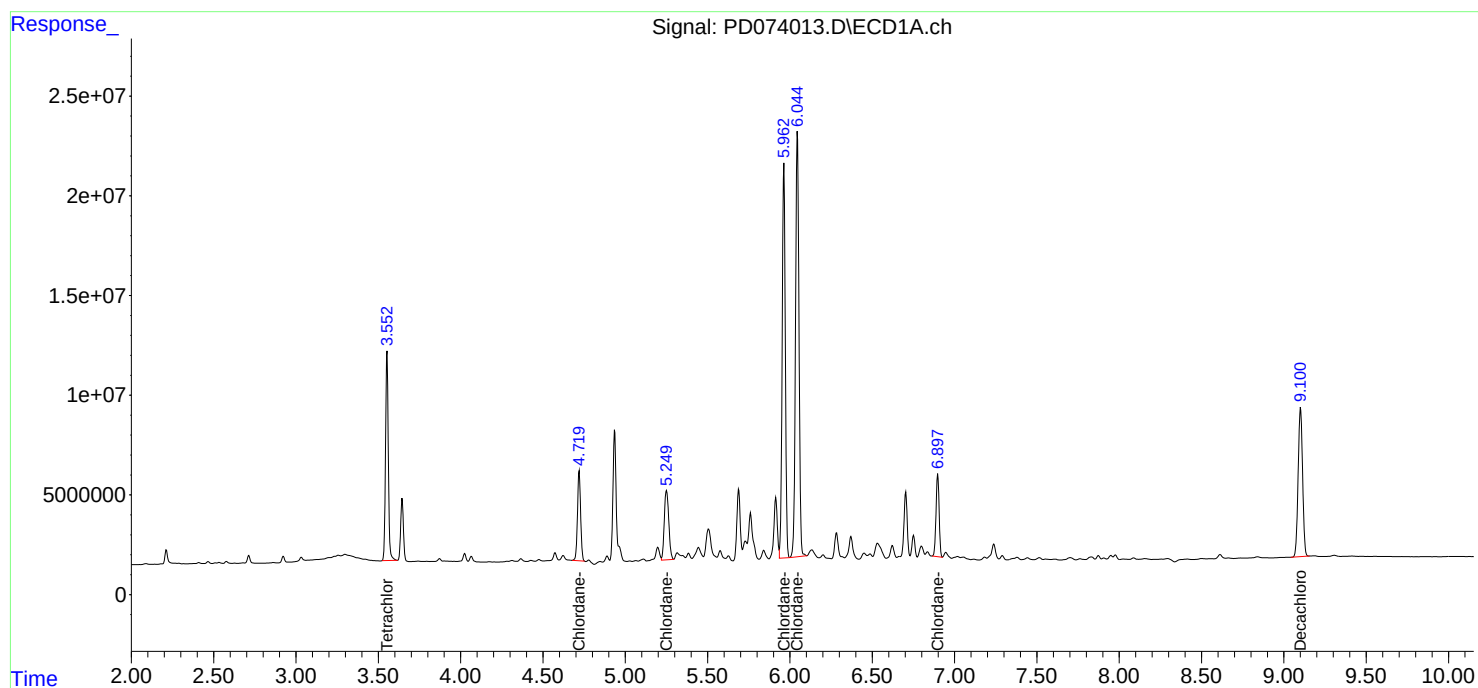


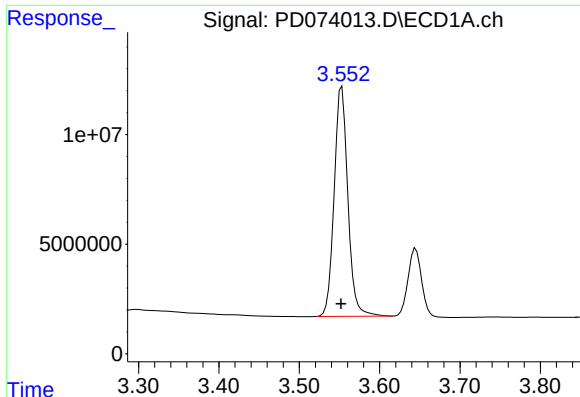

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.001 min
Response: 124251380
Conc: 52.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD022023CHLOR

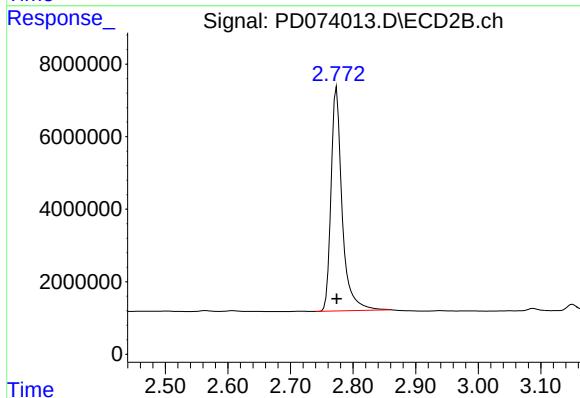


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 76410681
Conc: 51.74 ng/ml

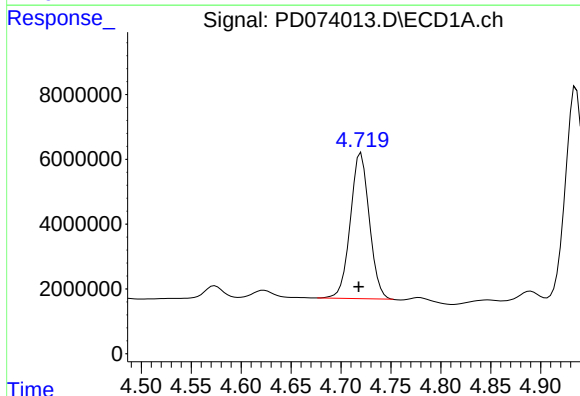


#23 Chlordane-1

R.T.: 4.720 min
Delta R.T.: 0.002 min
Response: 59334882
Conc: 529.88 ng/ml

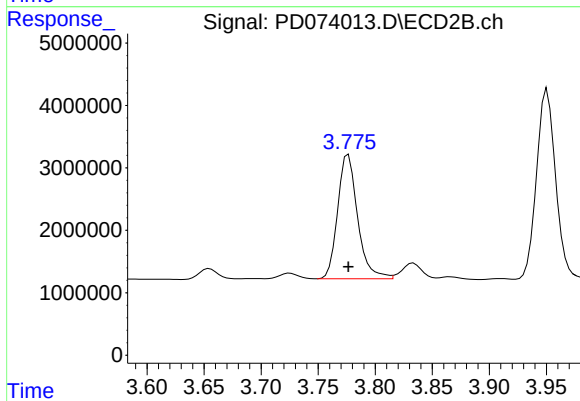

#23 Chlordane-1


R.T.: 3.776 min
Delta R.T.: 0.000 min
Response: 24294744
Conc: 522.93 ng/ml

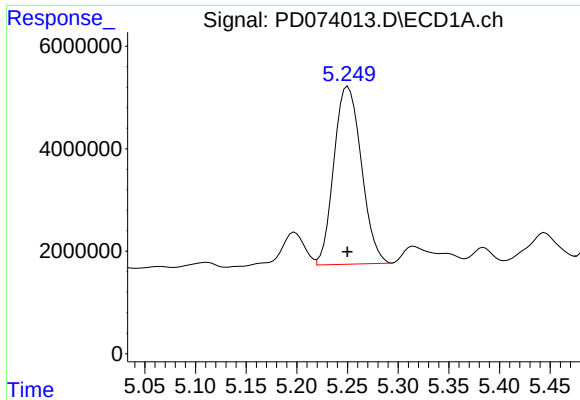

#24 Chlordane-2


R.T.: 5.251 min
Delta R.T.: 0.000 min
Response: 65333558
Conc: 519.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD022023CHLOR

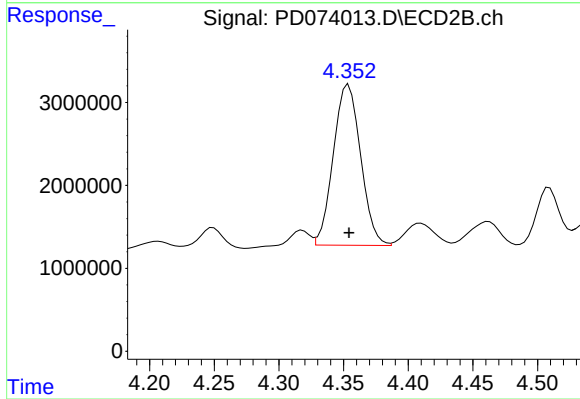


#24 Chlordane-2

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 28466558
Conc: 509.36 ng/ml

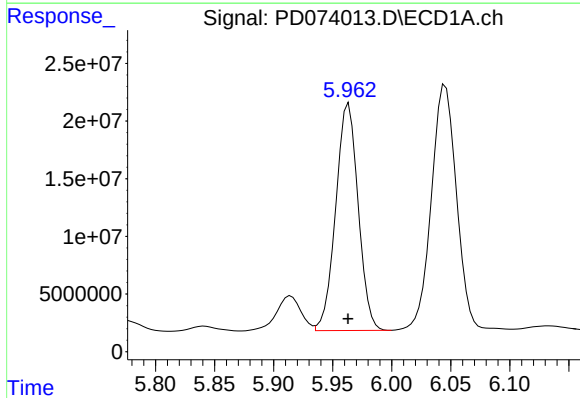


#25 Chlordane-3

R.T.: 5.964 min
Delta R.T.: 0.000 min
Response: 260252730
Conc: 540.39 ng/ml

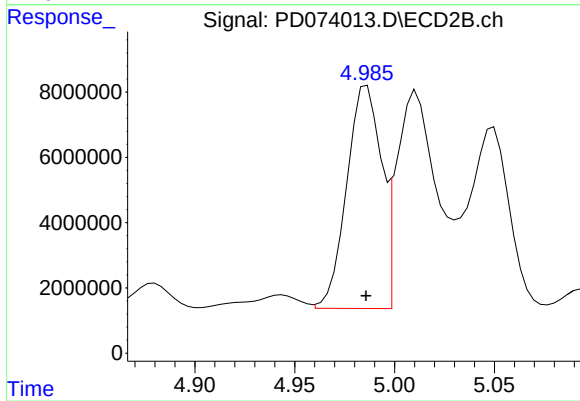

#25 Chlordane-3


R.T.: 4.986 min
Delta R.T.: 0.000 min
Response: 81819963
Conc: 519.26 ng/ml

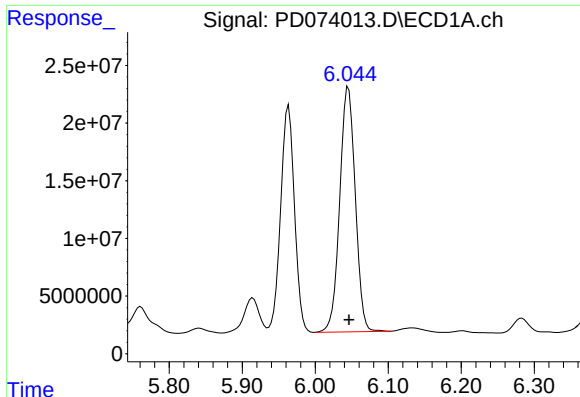

#26 Chlordane-4


R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 314125238
Conc: 534.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD022023CHLOR

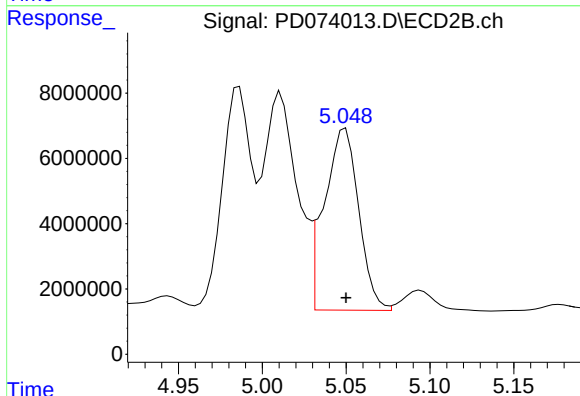


#26 Chlordane-4

R.T.: 5.050 min
Delta R.T.: 0.000 min
Response: 79402134
Conc: 524.81 ng/ml

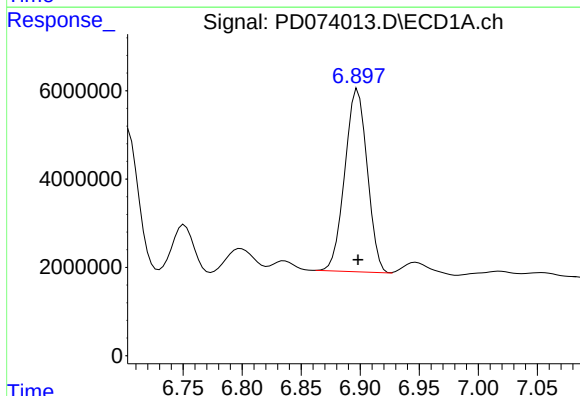


#27 Chlordane-5

R.T.: 6.898 min
Delta R.T.: 0.000 min
Response: 54639392
Conc: 527.54 ng/ml

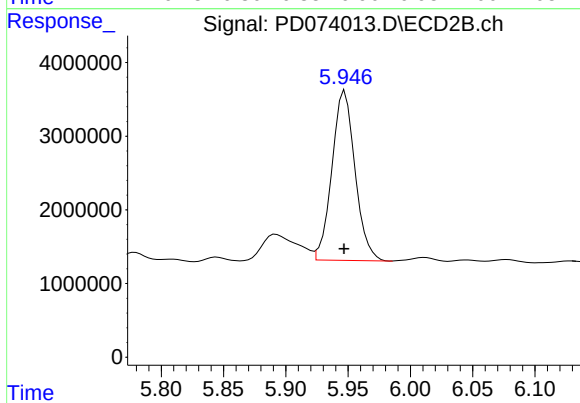

#27 Chlordane-5


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 29747326
Conc: 518.13 ng/ml

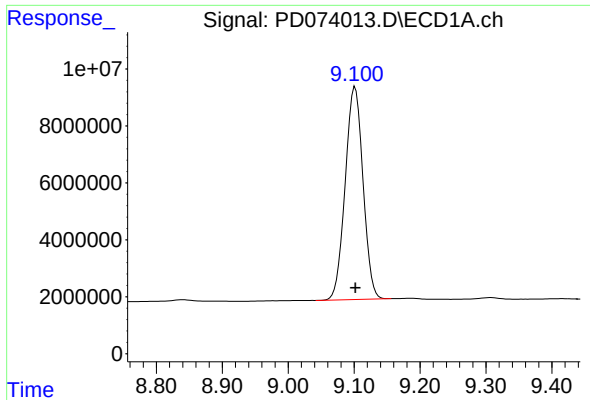

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: 0.000 min
Response: 140376844
Conc: 50.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD022023CHLOR

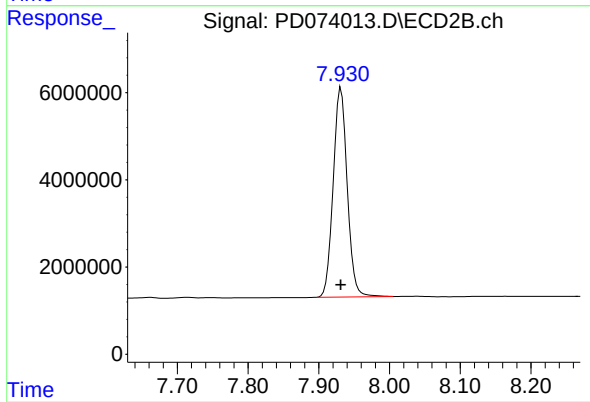

#28 Decachlorobiphenyl

R.T.: 7.931 min
Delta R.T.: 0.000 min
Response: 66212846
Conc: 50.47 ng/ml