

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022024\
 Data File : PD081515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2024 18:14
 Operator : AR\AJ
 Sample : PB158962BS
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS962

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/20/2024
 Supervised By : Ankita Jodhani 02/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 20:36:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021324CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 14 00:57:42 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.793	25856793	44269020	18.852	17.858
27)	SA Decachlor...	9.109	7.929	45592713	60797952	23.692	23.631
Target Compounds							
2)	A alpha-BHC	4.021	3.294	9341290	16557880	3.914	4.102
3)	MA gamma-BHC...	4.355	3.624	9142937	15230090	3.882	4.041
4)	MA Heptachlor	4.947	3.964	11001497	15636543	4.367	4.339
5)	MB Aldrin	5.290	4.245	10406768	15795012	4.413	4.387
6)	B beta-BHC	4.549	3.919	4797610	7146175	4.564	4.153
7)	B delta-BHC	4.797	4.149	11625095	15380817	4.705	3.875
8)	B Heptachlo...	5.717	4.746	10241725	14710286	4.633	4.414
9)	A Endosulfan I	6.104	5.114	9756812	13255439	4.455	4.257m
10)	B trans-Chl...	5.973	4.996	9769118	14285381	4.543	4.405
11)	B cis-Chlor...	6.053	5.059	10046537	14534593	4.569	4.441m
12)	B 4,4'-DDE	6.224	5.248	18088814	25900351	8.511	8.323
13)	MA Dieldrin	6.379	5.380	20326386	28645921	8.833	8.345
14)	MA Endrin	6.610	5.655	17699287	28661236	9.480	9.718
15)	B Endosulfa...	6.827	5.948	19715214	25875394	10.070	9.003
16)	A 4,4'-DDD	6.741	5.801	15495142	22318911	9.152	8.418
17)	MA 4,4'-DDT	7.056	6.053	16387753	21838394	9.098	8.049
18)	B Endrin al...	6.958	6.127	15208371	20969601	10.085	9.353
19)	B Endosulfa...	7.192	6.350	18415300	25777446	9.783	9.308
20)	A Methoxychlor	7.531	6.627	44229229	64269576	46.827	47.889
21)	B Endrin ke...	7.678	6.855	19278767	29291699	9.565	9.364

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022024\
Data File : PD081515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2024 18:14
Operator : AR\AJ
Sample : PB158962BS
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 20:36:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021324CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Feb 14 00:57:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

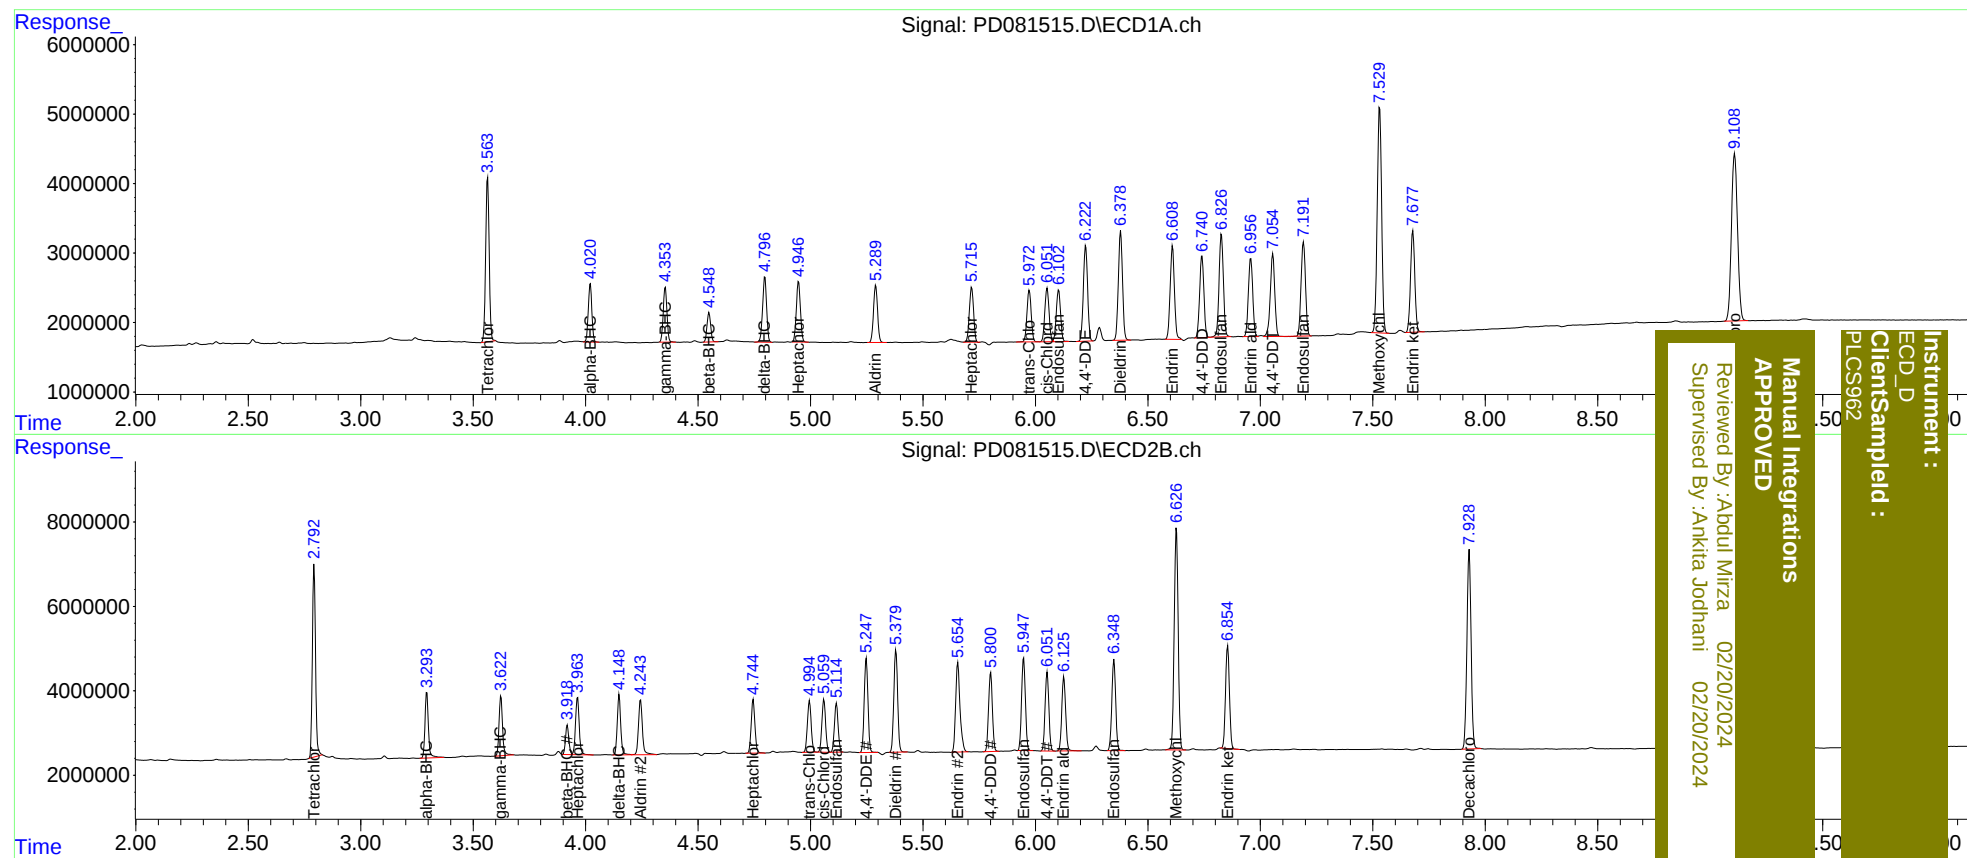

Instrument :
ECD_D
ClientSampled :
PLCS962

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 02/20/2024
Supervised By: Ankita Jodhani 02/20/2024