

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022119\
 Data File : PD051307.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Feb 2019 9:53
 Operator : AJ\SJ
 Sample : PIBLK46
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK46

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 03:53:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012419CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 25 03:30:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.226	4.046	29412340	636.9E6	21.078	22.337
27) SA Decachlor...	7.830	9.161	46569136	730.0E6	38.118	39.249
Target Compounds						
6) B beta-BHC	0.000	4.933f	0 59276229	N.D.	3.211	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022119\
Data File : PD051307.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Feb 2019 9:53
Operator : AJ\SJ
Sample : PIBLK46
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK46

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 03:53:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012419CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 25 03:30:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

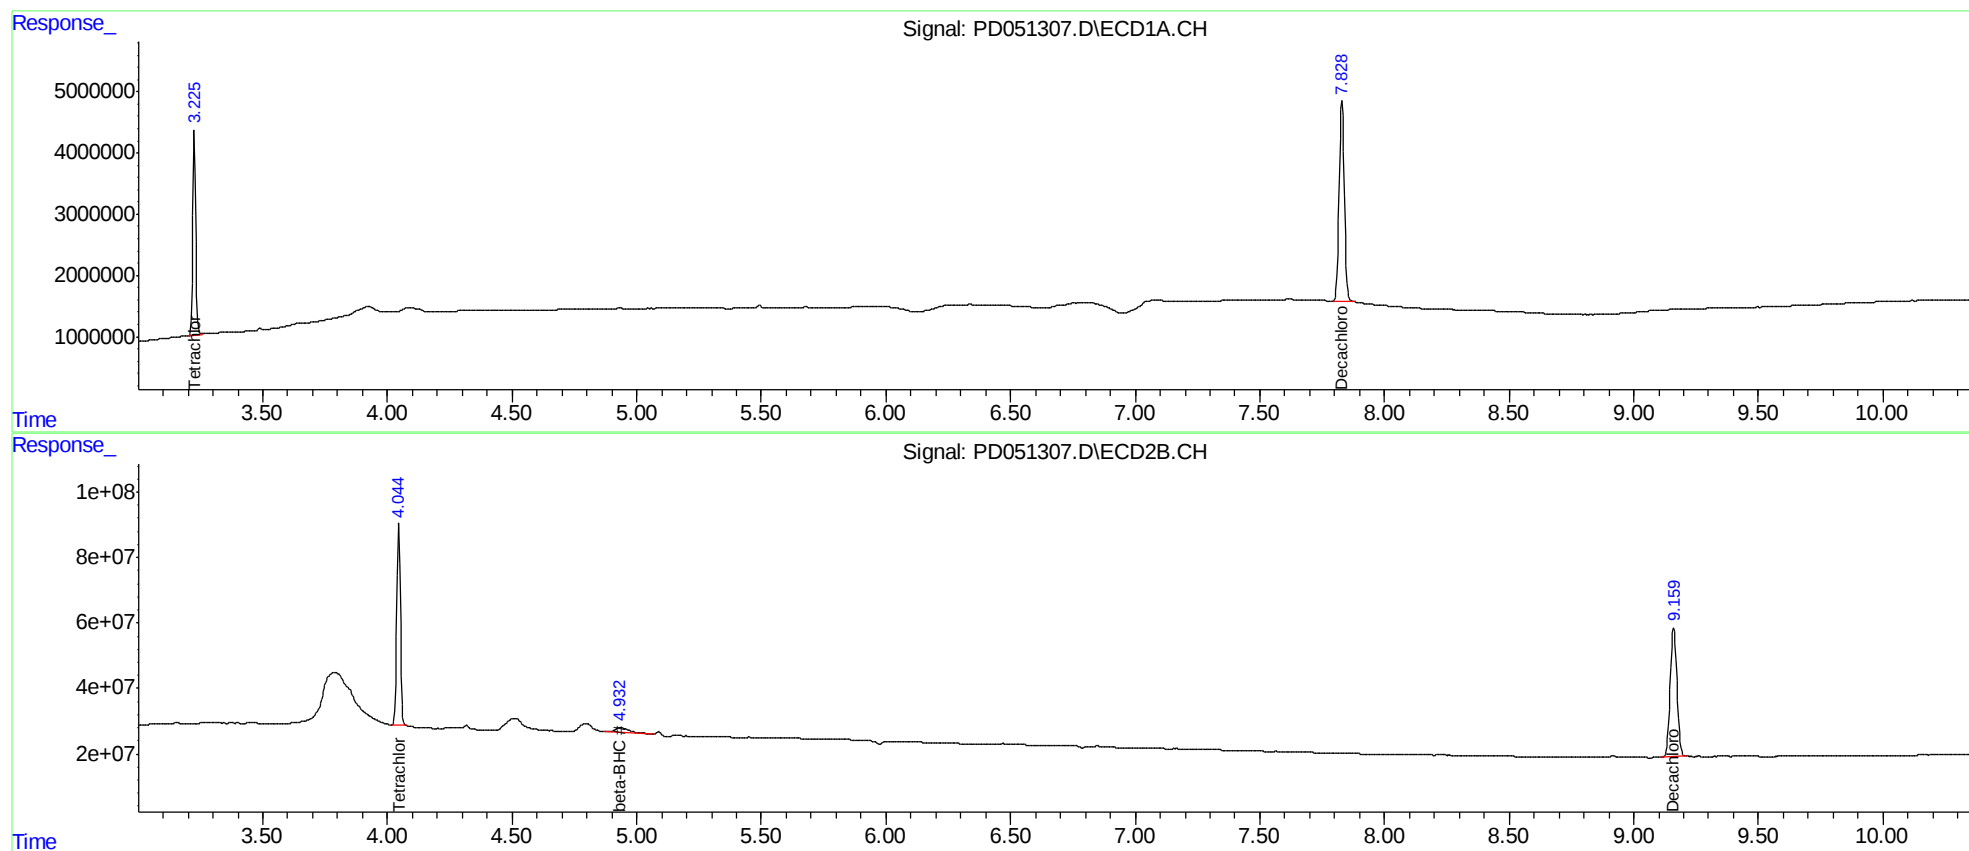


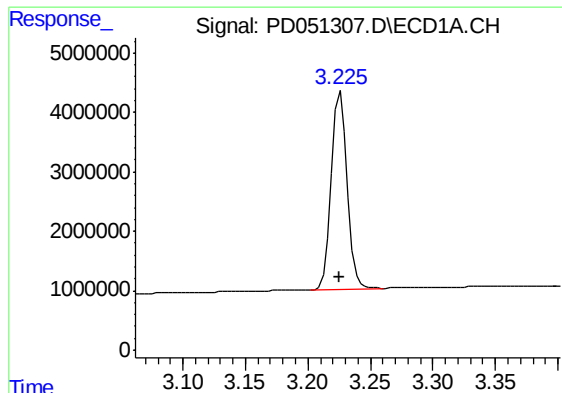

#1 Tetrachloro-m-xylene


R.T.: 3.226 min
Delta R.T.: 0.001 min
Response: 29412340
Conc: 21.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK46

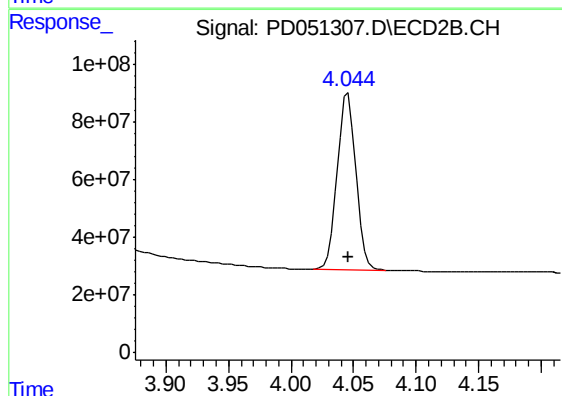


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 636872898
Conc: 22.34 ng/ml

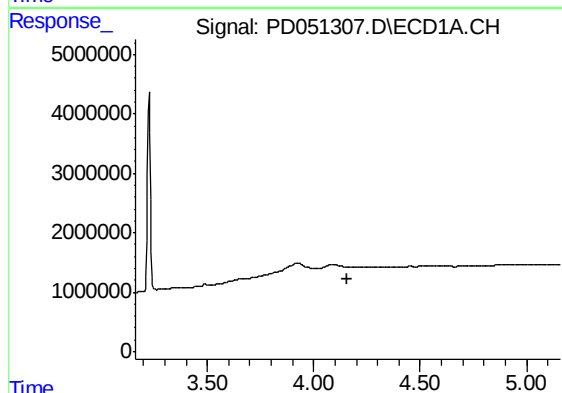


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.160 min
Response: 0
Conc: N.D.

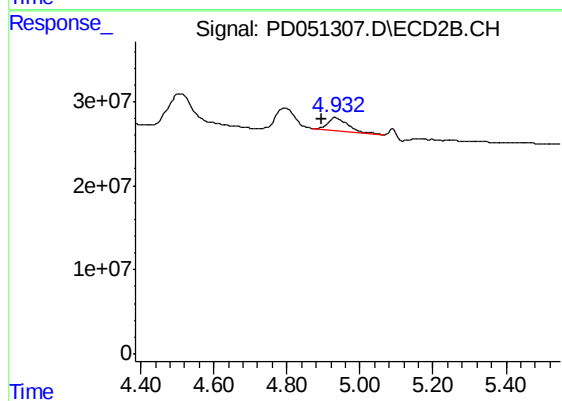

#6 beta-BHC


R.T.: 4.933 min
Delta R.T.: 0.037 min
Response: 59276229
Conc: 3.21 ng/ml

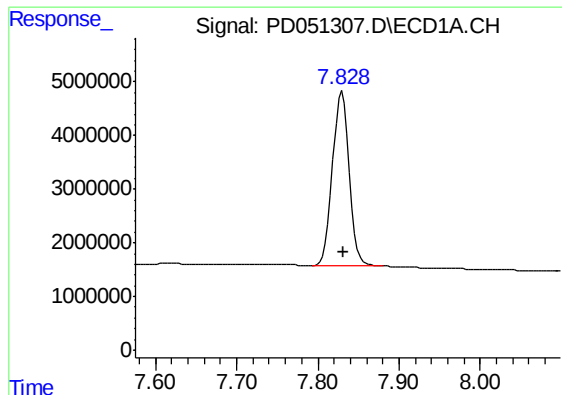

#27 Decachlorobiphenyl

R.T.: 7.830 min
Delta R.T.: -0.002 min
Response: 46569136
Conc: 38.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK46

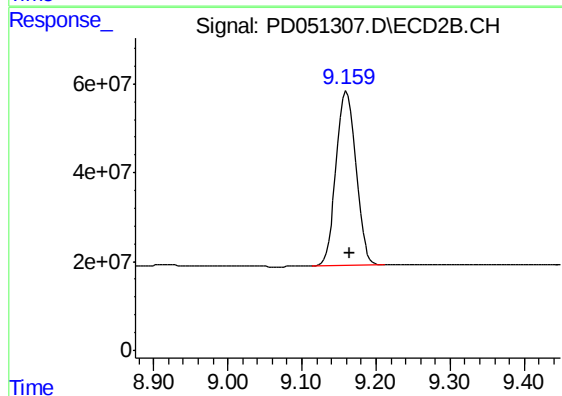

#27 Decachlorobiphenyl

R.T.: 9.161 min
Delta R.T.: -0.003 min
Response: 729980199
Conc: 39.25 ng/ml