

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022120\
 Data File : PD057427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2020 19:08
 Operator : AJ\MA
 Sample : L1418-19
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5B21

Manual Integrations
 APPROVED

mohammad
 2/25/2020 10:38:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 17:23:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022120CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 24 16:58:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.896	7077353	15156093	8.238	7.475
27)	SA Decachlor...	7.863	8.893	13318095	29449631	14.654m	13.439m
Target Compounds							
10)	B trans-Chl...	5.093	5.959	40365974	114.4E6	39.595	36.014
11)	B cis-Chlor...	5.145	6.048	11436487	47242970	11.137	15.038 #
12)	B 4,4'-DDE	5.314	6.207	54720469	123.5E6	53.328	41.408
16)	A 4,4'-DDD	5.822	6.694	275.8E6	811.2E6	360.163	323.080
17)	MA 4,4'-DDT	6.054	6.991	10759879	37599167	15.377	16.539

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022120\
Data File : PD057427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2020 19:08
Operator : AJ\MA
Sample : L1418-19
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 17:23:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022120CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 24 16:58:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

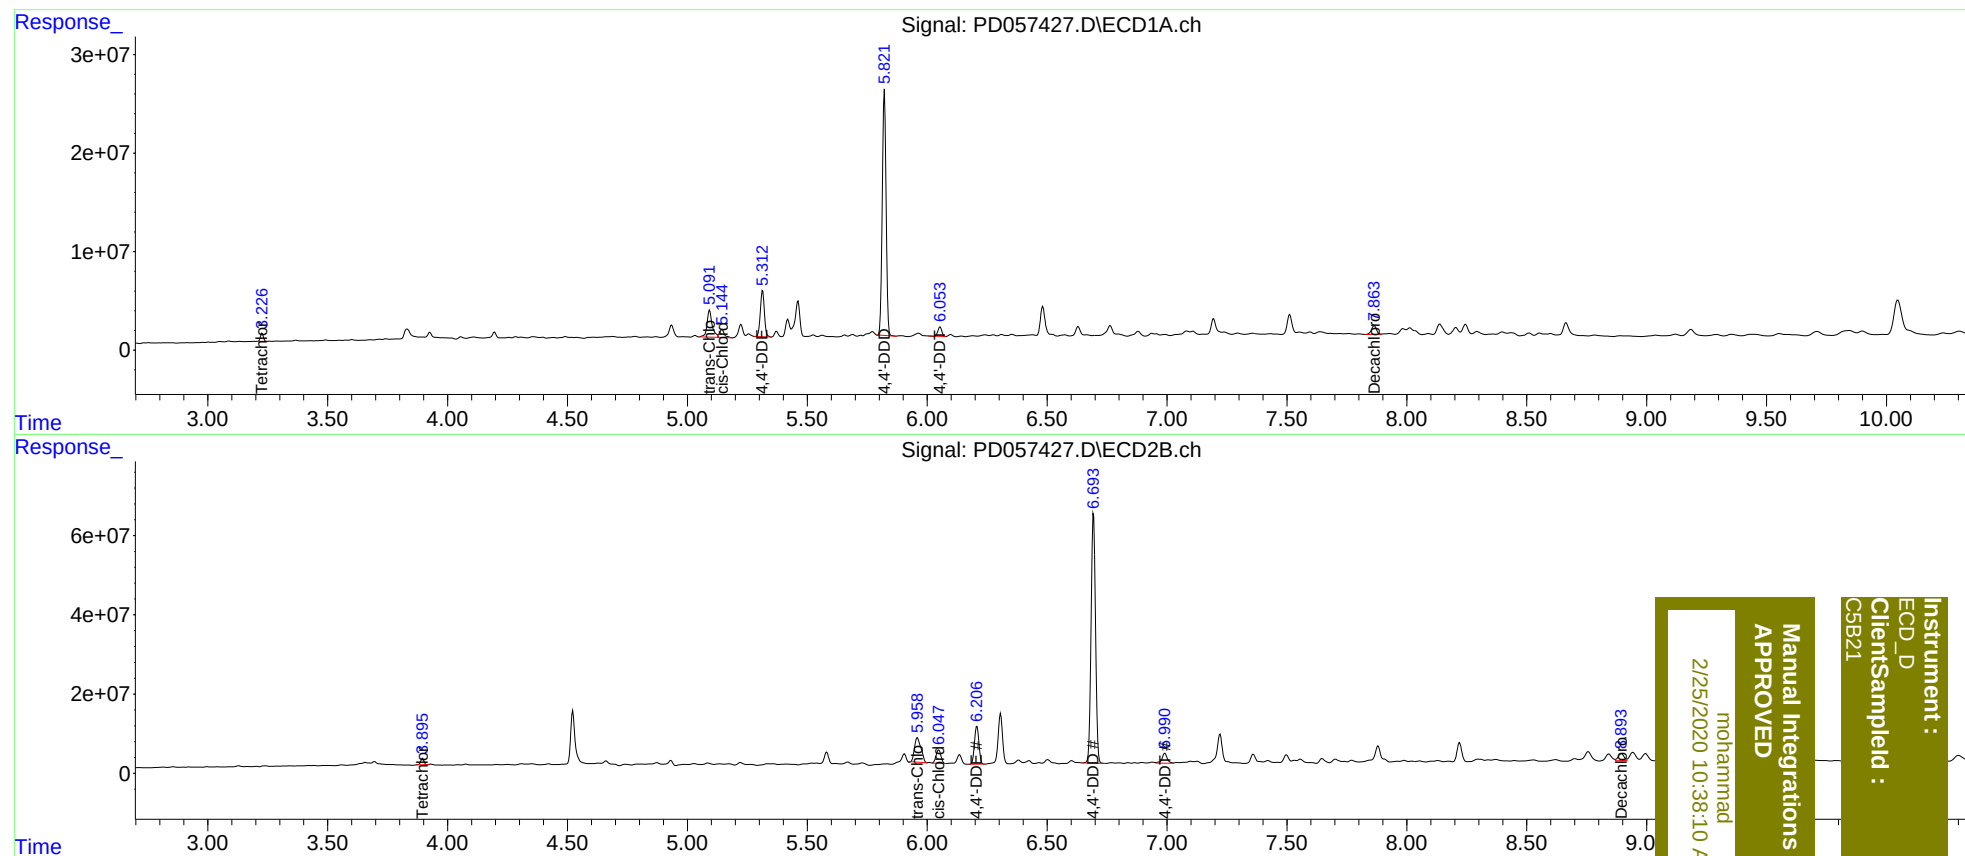

Manual Integrations
APPROVED

mohammad
2/25/2020 10:38:10 AM

Instrument :
ECD_D
ClientSample :
C5B21