

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022120\
 Data File : PD057428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2020 19:50
 Operator : AJ\MA
 Sample : L1418-19DL 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 C5B21DL

Manual Integrations
 APPROVED

mohammad
 2/26/2020 11:01:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 17:23:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022120CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 24 16:58:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.896	1412609	3217100	1.644	1.587
27)	SA Decachlor...	7.862	8.892	3012632	8667116	3.315m	3.955m
Target Compounds							
10)	B trans-Chl...	5.091	5.961	8156413	24853662	8.001m	7.824
11)	B cis-Chlor...	5.143	6.048	1583128	10135513	1.542m	3.226 #
12)	B 4,4'-DDE	5.313	6.206	11021986	25219858	10.742	8.459
16)	A 4,4'-DDD	5.822	6.693	54803949	168.3E6	71.574	67.026
17)	MA 4,4'-DDT	6.054	6.991	1935177	6116539	2.766	2.691

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022120\
Data File : PD057428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2020 19:50
Operator : AJ\MA
Sample : L1418-19DL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 17:23:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022120CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 24 16:58:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

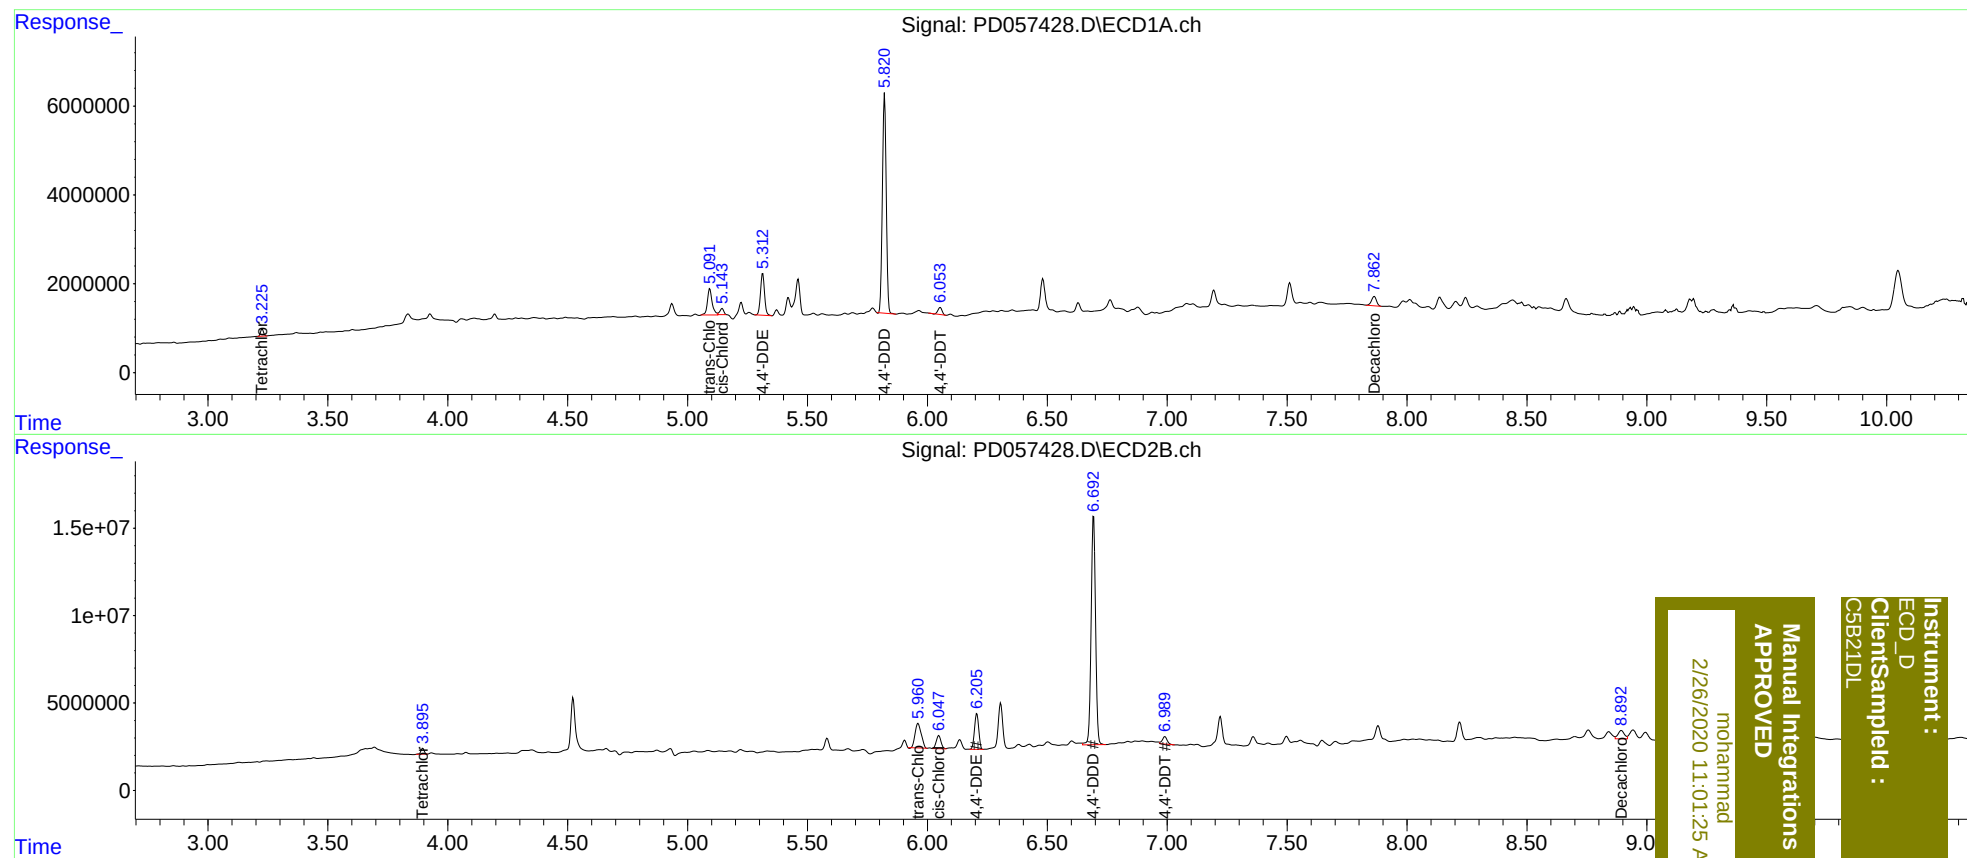

Manual Integrations
APPROVED

mohammad
2/26/2020 11:01:25 AM

Instrument :
ECD_D
ClientSample :
C5B21DL