

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022121\
 Data File : PD061328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2021 13:36
 Operator : DD\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 04:22:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022121CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 22 04:21:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	3.982	4881126	43706184	5.299	5.113
27)	SA Decachlor...	8.260	9.036	13913214	79175457	11.362	10.910
Target Compounds							
2)	A alpha-BHC	3.926	4.370	6419757	66526521	4.879	5.100
3)	MA gamma-BHC...	4.211	4.655	6488886	60355829	5.053	5.101
4)	MA Heptachlor	4.515	5.163	6757692	62972941	5.129	5.292
9)	A Endosulfan I	5.550	6.209	6283924	48640067	5.378	5.230
13)	MA Dieldrin	5.794	6.466	12726524	102.2E6	9.954	10.308
14)	MA Endrin	6.053	6.684	11116510	80198147	10.575	10.259
16)	A 4,4'-DDD	6.176	6.805	10032966	79935662	9.842	10.314
17)	MA 4,4'-DDT	6.419	7.103	9502350	78461712	9.433	10.532
20)	A Methoxychlor	6.965	7.561	29617002	190.0E6	52.872	54.032


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022121\
Data File : PD061328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2021 13:36
Operator : DD\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 04:22:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022121CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 22 04:21:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

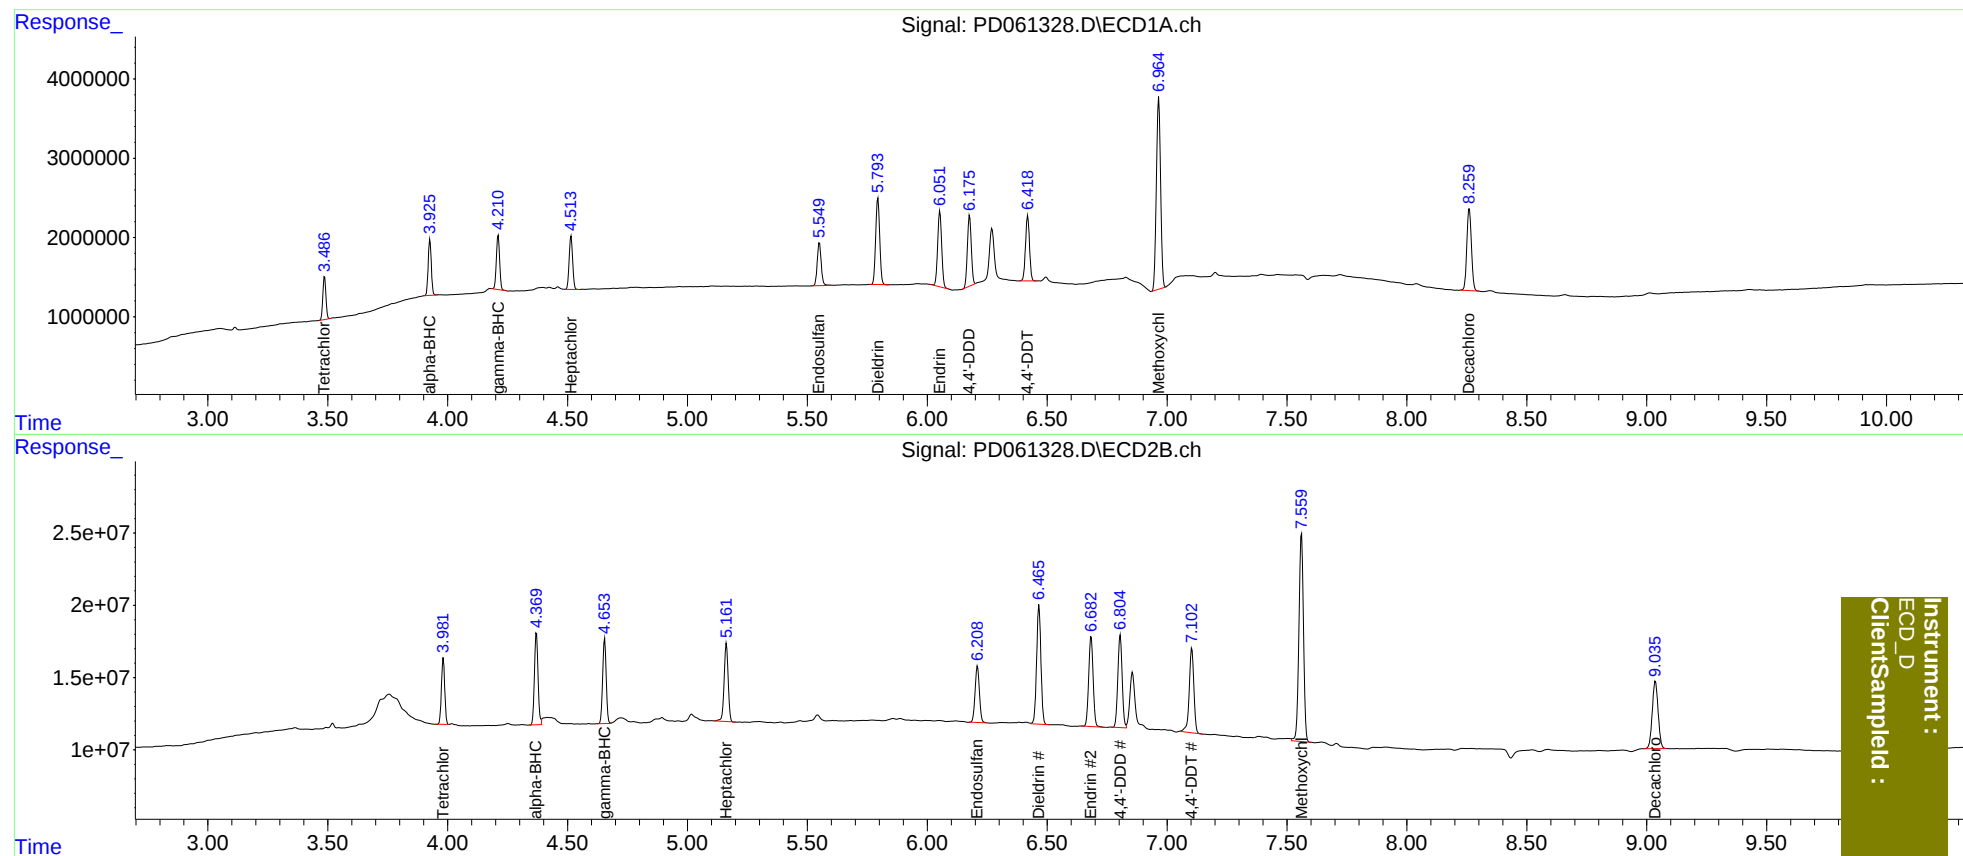


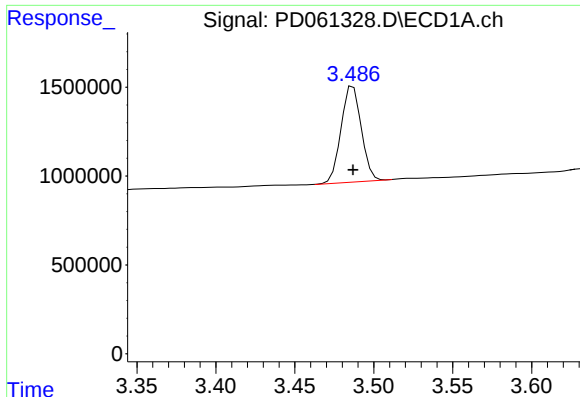

#1 Tetrachloro-m-xylene


R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 4881126
Conc: 5.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

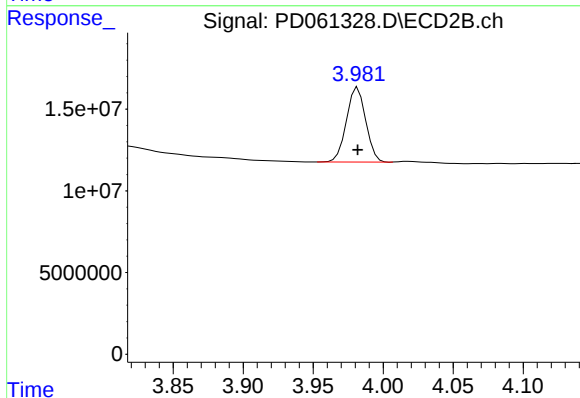


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 43706184
Conc: 5.11 ng/ml

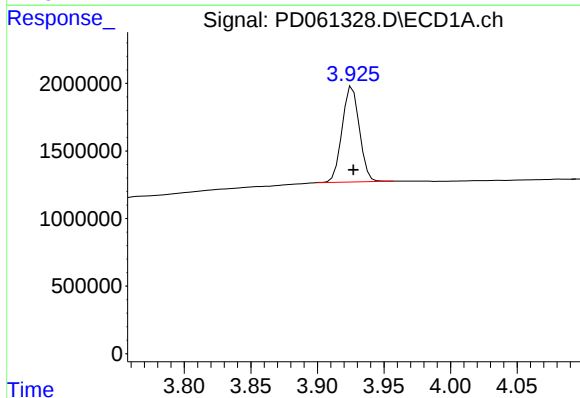


#2 alpha-BHC

R.T.: 3.926 min
Delta R.T.: 0.000 min
Response: 6419757
Conc: 4.88 ng/ml

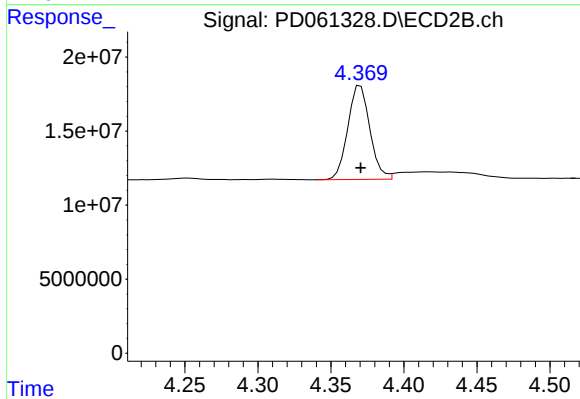

#2 alpha-BHC


R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 66526521
Conc: 5.10 ng/ml

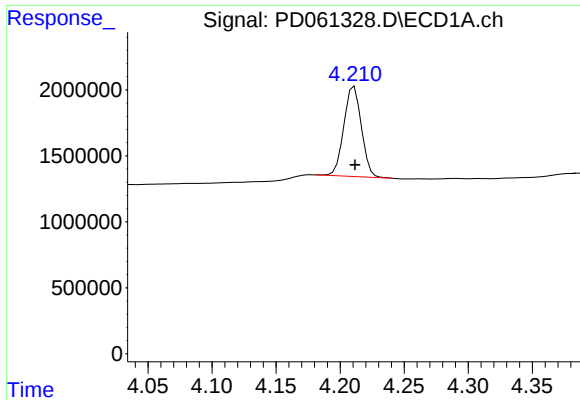

#3 gamma-BHC (Lindane)


R.T.: 4.211 min
Delta R.T.: 0.000 min
Response: 6488886
Conc: 5.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

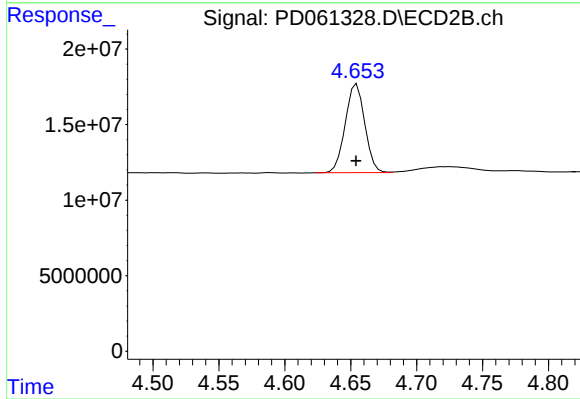


#3 gamma-BHC (Lindane)

R.T.: 4.655 min
Delta R.T.: 0.000 min
Response: 60355829
Conc: 5.10 ng/ml

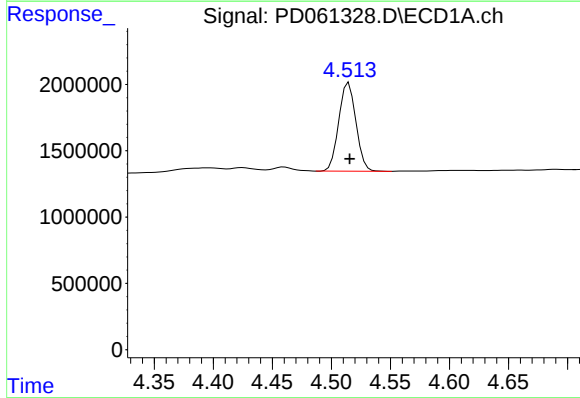


#4 Heptachlor

R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 6757692
Conc: 5.13 ng/ml

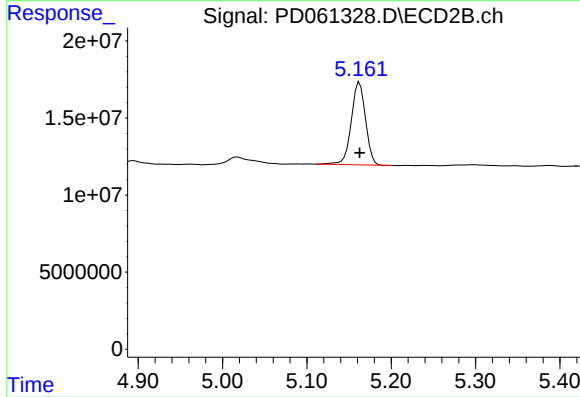

#4 Heptachlor


R.T.: 5.163 min
Delta R.T.: 0.000 min
Response: 62972941
Conc: 5.29 ng/ml

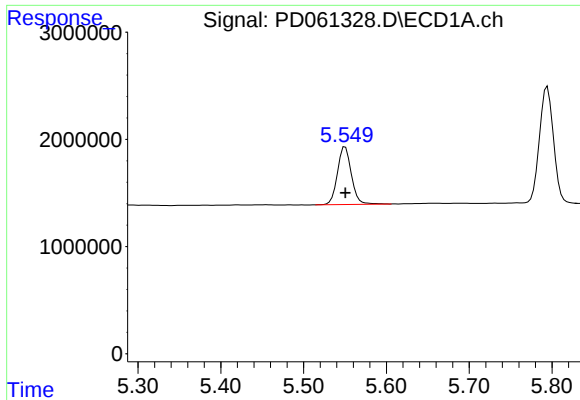

#9 Endosulfan I


R.T.: 5.550 min
Delta R.T.: 0.000 min
Response: 6283924
Conc: 5.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

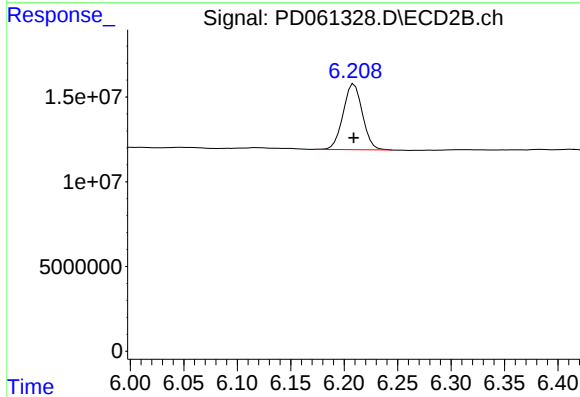


#9 Endosulfan I

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 48640067
Conc: 5.23 ng/ml

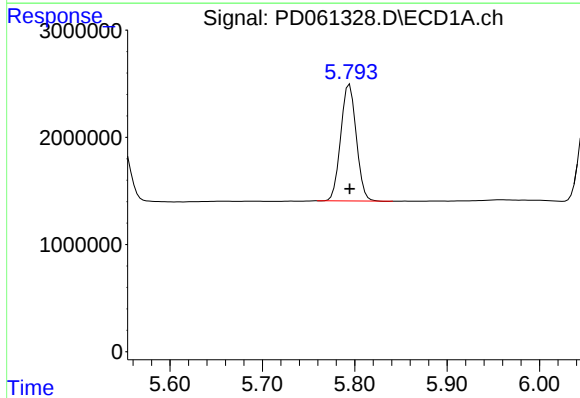


#13 Dieldrin

R.T.: 5.794 min
Delta R.T.: 0.000 min
Response: 12726524
Conc: 9.95 ng/ml

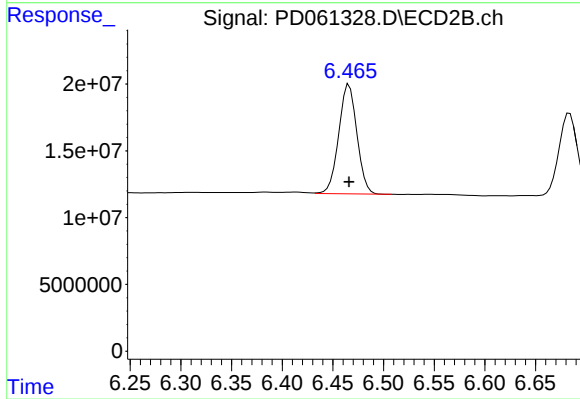

#13 Dieldrin


R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 102229513
Conc: 10.31 ng/ml

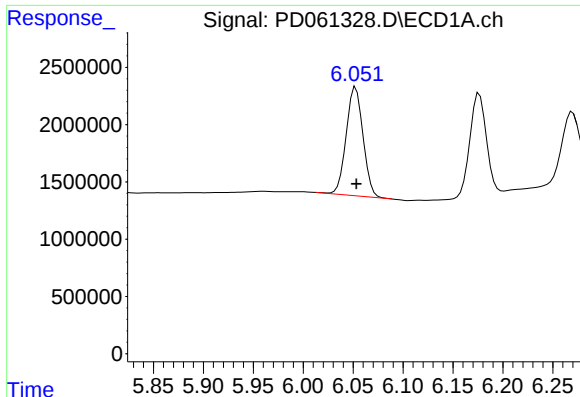

#14 Endrin


R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 11116510
Conc: 10.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

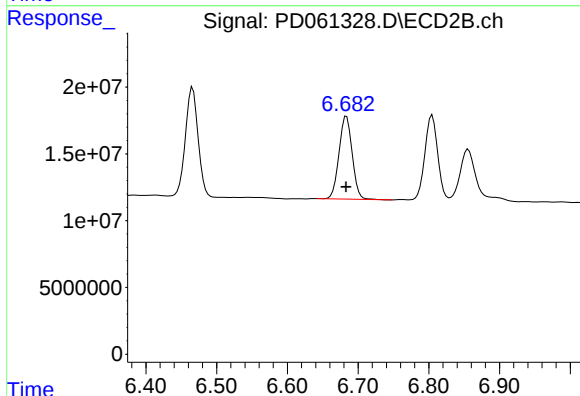


#14 Endrin

R.T.: 6.684 min
Delta R.T.: 0.000 min
Response: 80198147
Conc: 10.26 ng/ml

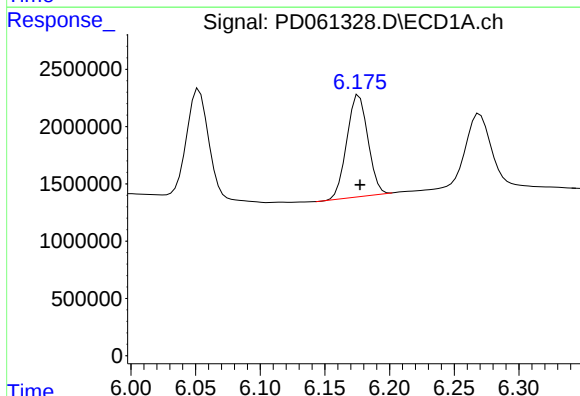


#16 4,4'-DDD

R.T.: 6.176 min
Delta R.T.: 0.000 min
Response: 10032966
Conc: 9.84 ng/ml

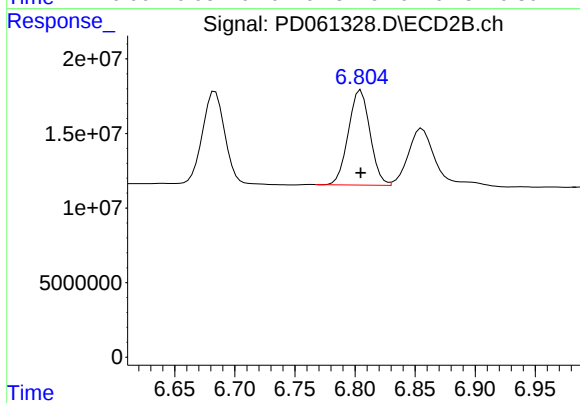

#16 4,4'-DDD


R.T.: 6.805 min
Delta R.T.: 0.000 min
Response: 79935662
Conc: 10.31 ng/ml

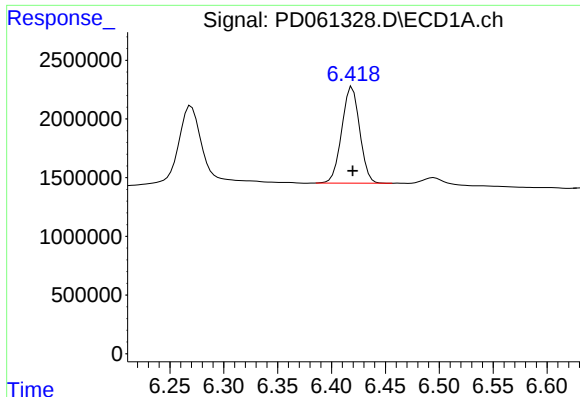

#17 4,4'-DDT


R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 9502350
Conc: 9.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

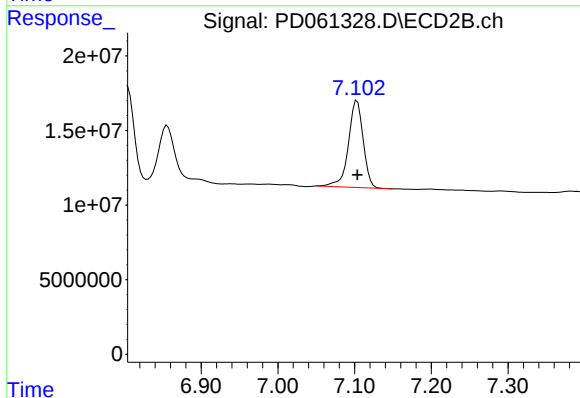


#17 4,4'-DDT

R.T.: 7.103 min
Delta R.T.: 0.000 min
Response: 78461712
Conc: 10.53 ng/ml

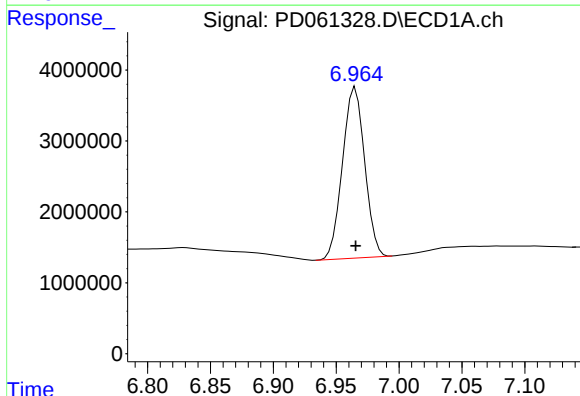


#20 Methoxychlor

R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 29617002
Conc: 52.87 ng/ml

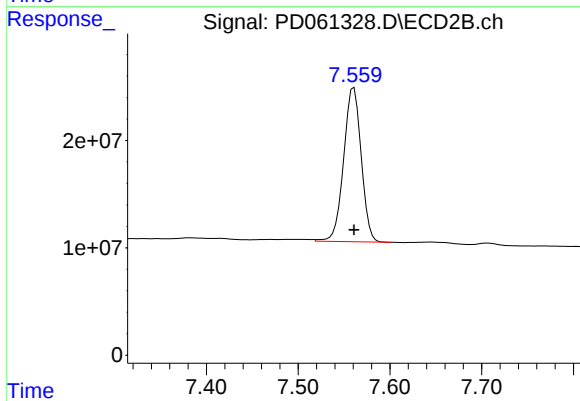

#20 Methoxychlor


R.T.: 7.561 min
Delta R.T.: 0.000 min
Response: 189991581
Conc: 54.03 ng/ml

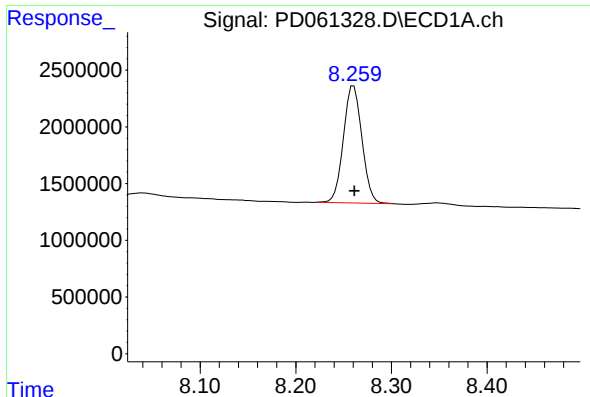

#27 Decachlorobiphenyl

R.T.: 8.260 min
Delta R.T.: 0.000 min
Response: 13913214
Conc: 11.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

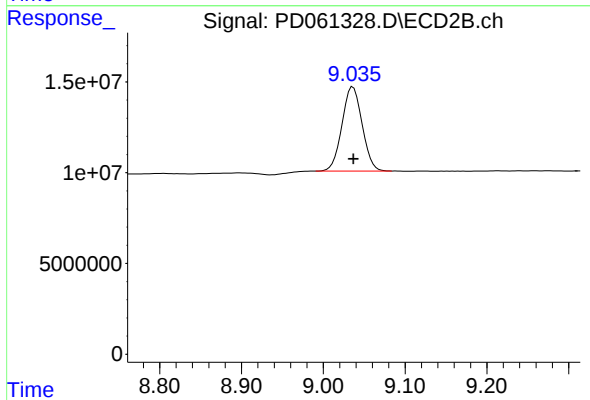

#27 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: 0.000 min
Response: 79175457
Conc: 10.91 ng/ml