

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022121\
 Data File : PD061330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2021 14:04
 Operator : DD\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 04:22:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022121CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 22 04:21:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	3.982	9517047	85117014	10.332	9.957
27)	SA Decachlor...	8.260	9.037	26008542	151.7E6	21.239	20.910
Target Compounds							
2)	A alpha-BHC	3.926	4.370	13039011	130.2E6	9.910	9.984
3)	MA gamma-BHC...	4.211	4.654	12770759	118.8E6	9.945	10.040
4)	MA Heptachlor	4.515	5.163	13391539	122.0E6	10.163	10.249
9)	A Endosulfan I	5.550	6.209	12251758	94973215	10.485	10.212
13)	MA Dieldrin	5.794	6.466	25445471	202.0E6	19.903	20.365
14)	MA Endrin	6.052	6.684	21734278	161.8E6	20.676	20.695
16)	A 4,4'-DDD	6.176	6.805	20249389	156.5E6	19.864	20.199
17)	MA 4,4'-DDT	6.419	7.104	19774215	153.9E6	19.631	20.651
20)	A Methoxychlor	6.964	7.561	57871260	373.0E6	103.312	106.065

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022121\
Data File : PD061330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2021 14:04
Operator : DD\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 04:22:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022121CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 22 04:21:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

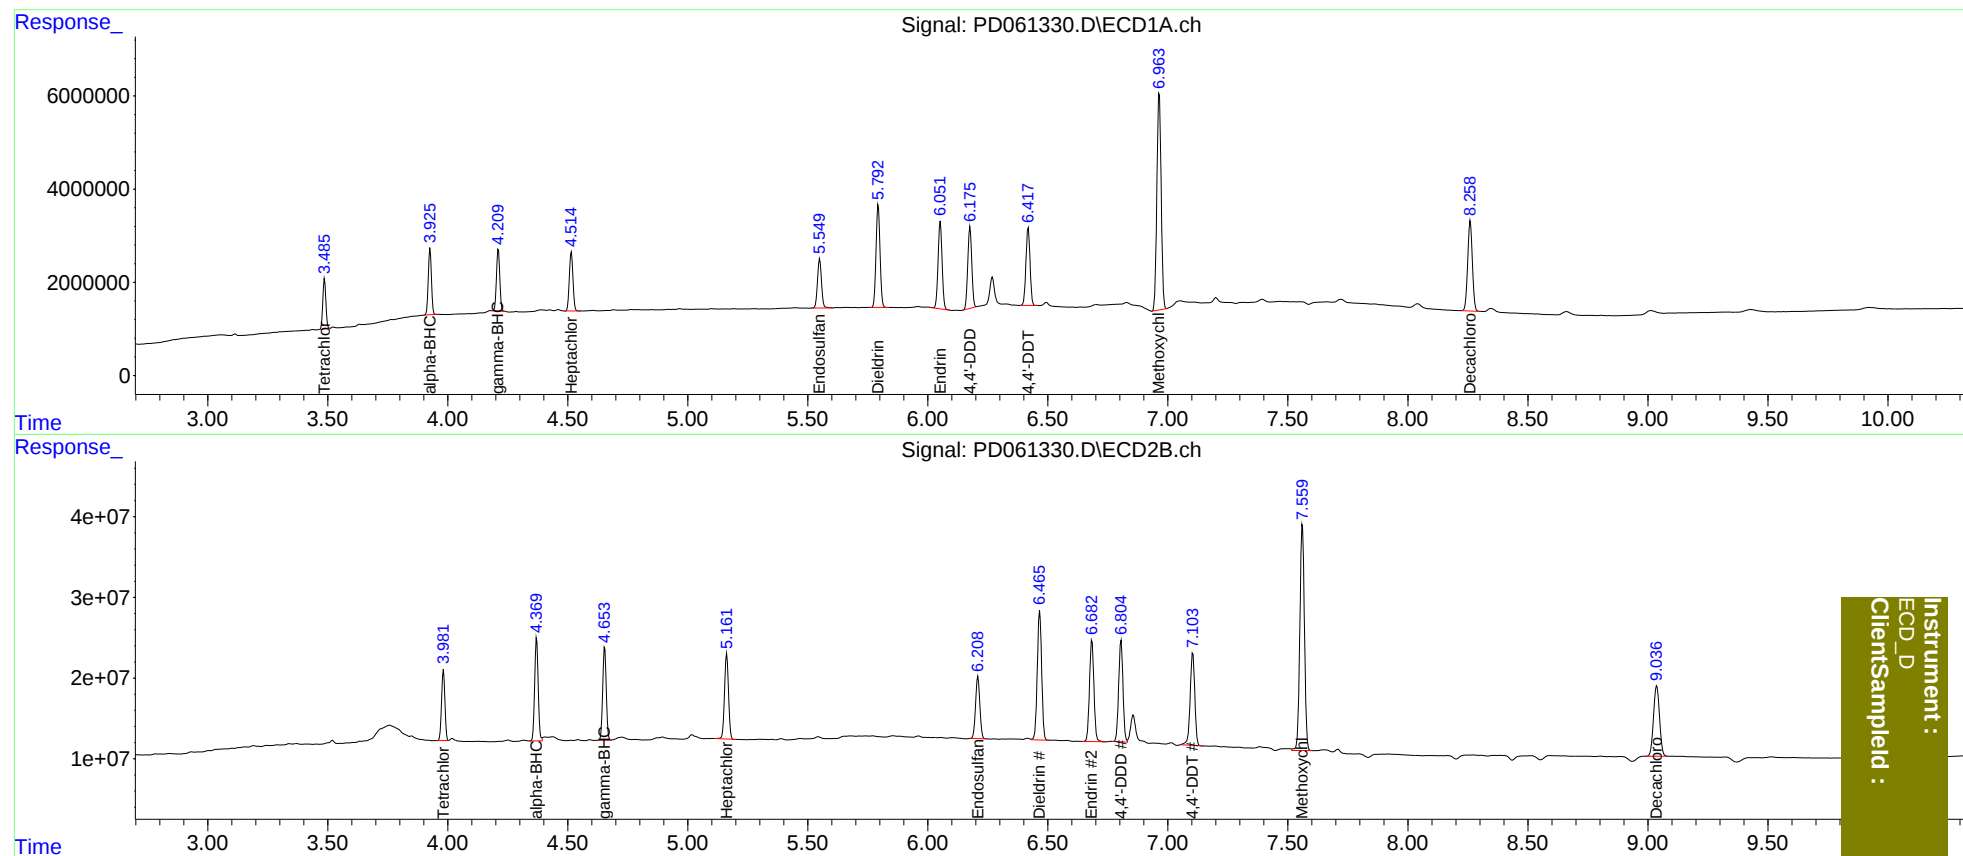


Instrument :
ECD_D
ClientSampled :

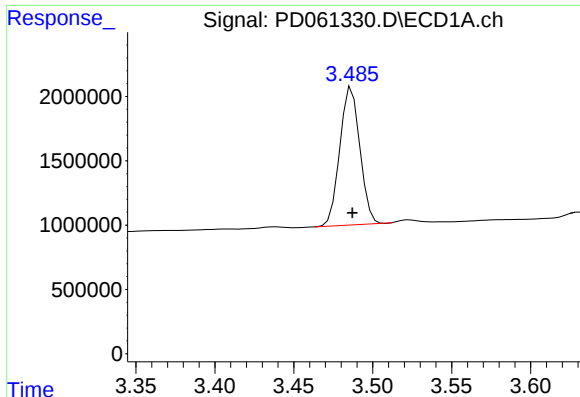

#1 Tetrachloro-m-xylene


R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 9517047
Conc: 10.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

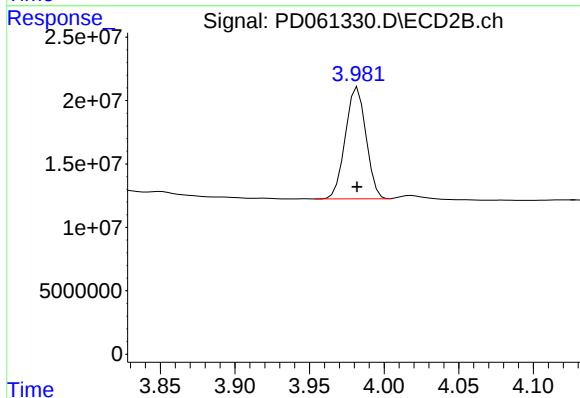


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 85117014
Conc: 9.96 ng/ml

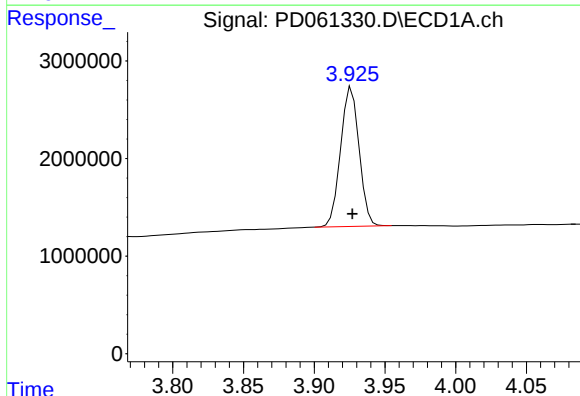


#2 alpha-BHC

R.T.: 3.926 min
Delta R.T.: 0.000 min
Response: 13039011
Conc: 9.91 ng/ml

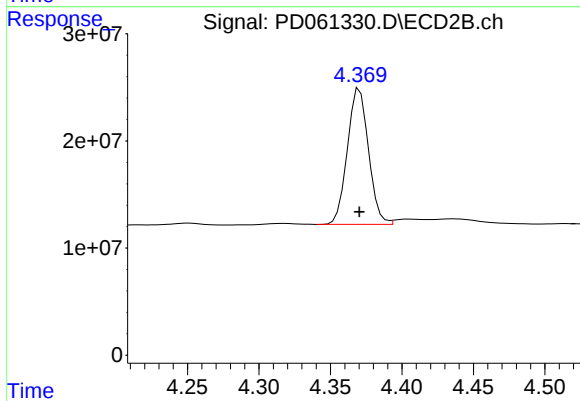

#2 alpha-BHC


R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 130225015
Conc: 9.98 ng/ml

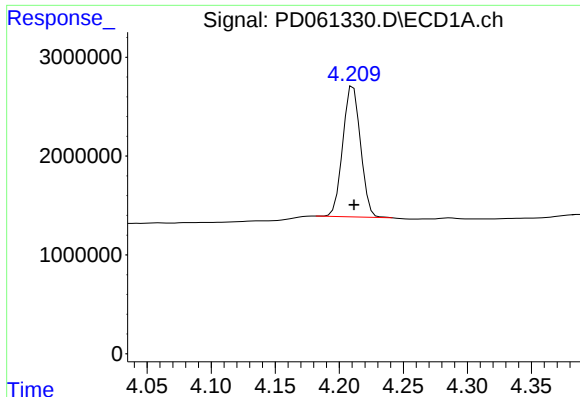

#3 gamma-BHC (Lindane)


R.T.: 4.211 min
Delta R.T.: 0.000 min
Response: 12770759
Conc: 9.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

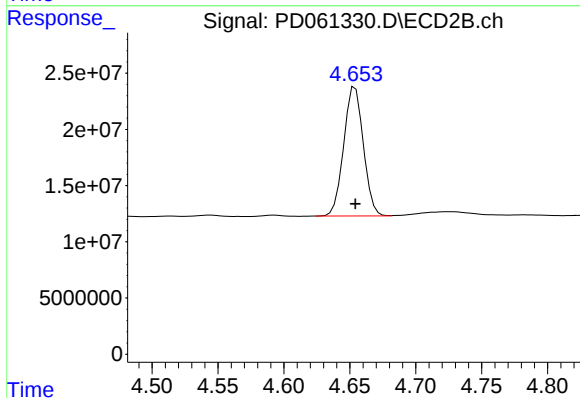


#3 gamma-BHC (Lindane)

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 118803218
Conc: 10.04 ng/ml

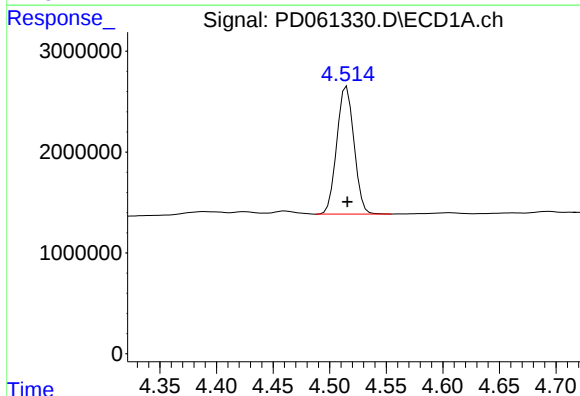


#4 Heptachlor

R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 13391539
Conc: 10.16 ng/ml

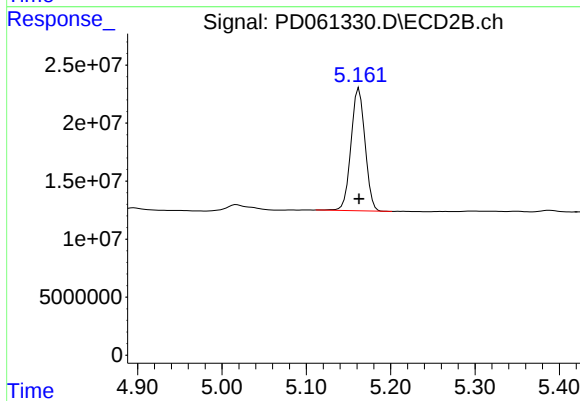

#4 Heptachlor


R.T.: 5.163 min
Delta R.T.: 0.000 min
Response: 121952819
Conc: 10.25 ng/ml

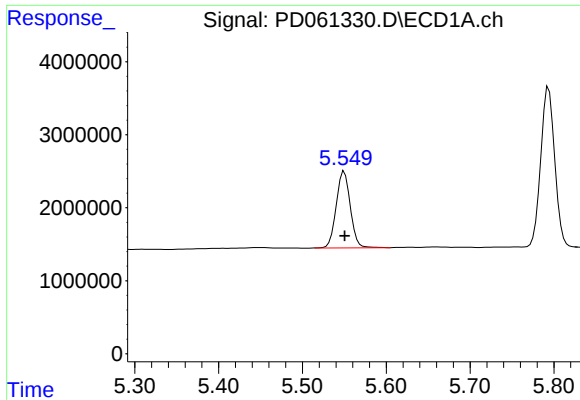

#9 Endosulfan I


R.T.: 5.550 min
Delta R.T.: 0.000 min
Response: 12251758
Conc: 10.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

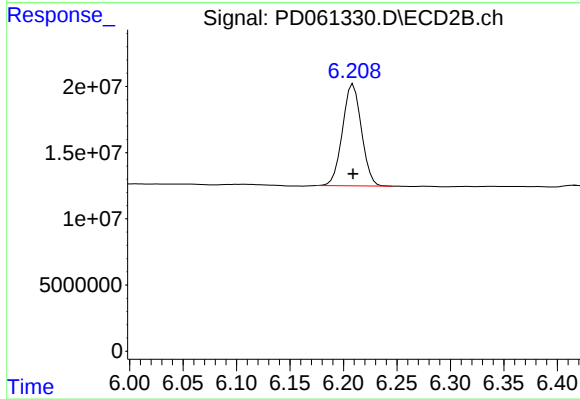


#9 Endosulfan I

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 94973215
Conc: 10.21 ng/ml

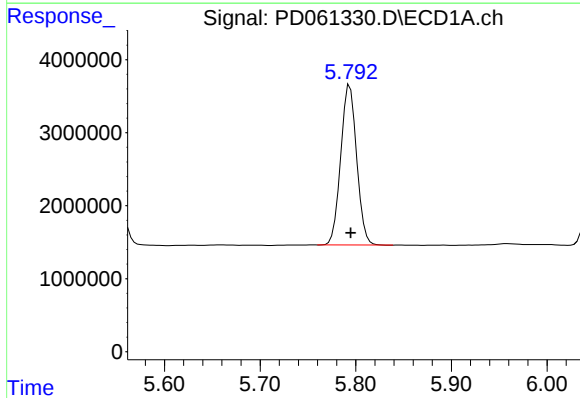


#13 Dieldrin

R.T.: 5.794 min
Delta R.T.: 0.000 min
Response: 25445471
Conc: 19.90 ng/ml

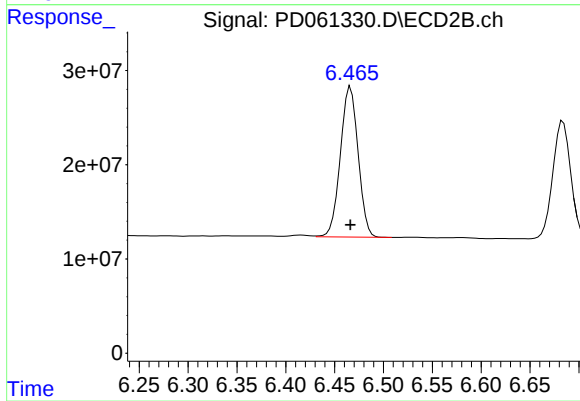

#13 Dieldrin


R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 201976703
Conc: 20.36 ng/ml

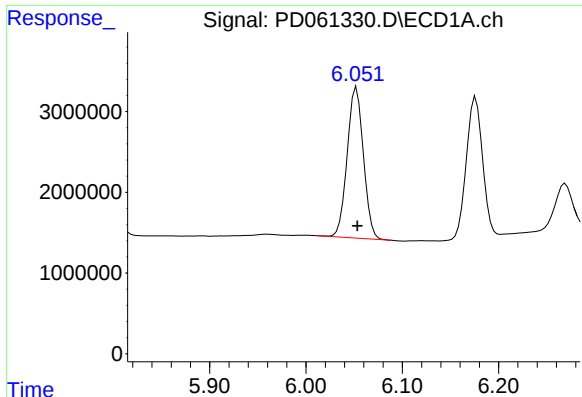

#14 Endrin


R.T.: 6.052 min
Delta R.T.: 0.000 min
Response: 21734278
Conc: 20.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

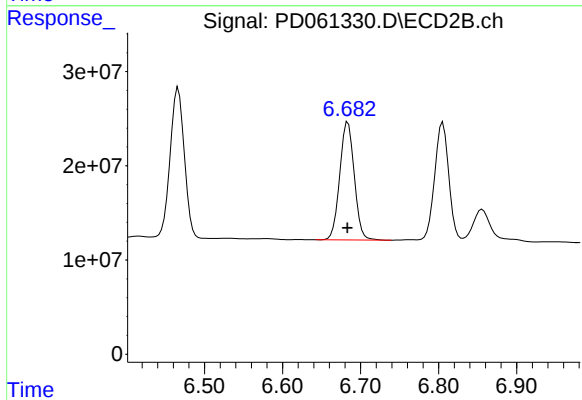


#14 Endrin

R.T.: 6.684 min
Delta R.T.: 0.000 min
Response: 161781064
Conc: 20.70 ng/ml

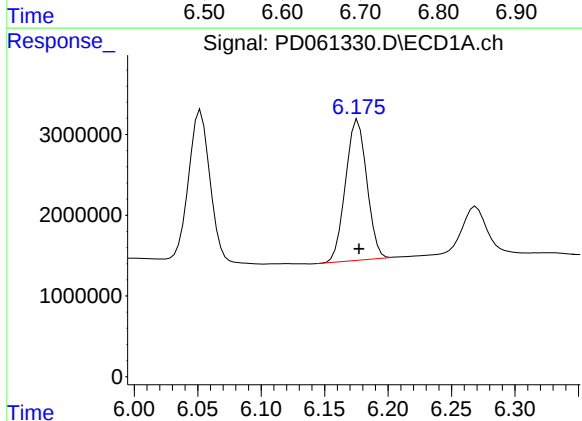


#16 4,4'-DDD

R.T.: 6.176 min
Delta R.T.: 0.000 min
Response: 20249389
Conc: 19.86 ng/ml

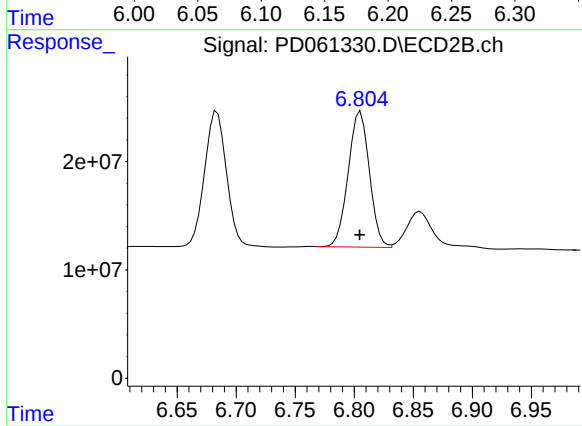

#16 4,4'-DDD


R.T.: 6.805 min
Delta R.T.: 0.000 min
Response: 156543419
Conc: 20.20 ng/ml

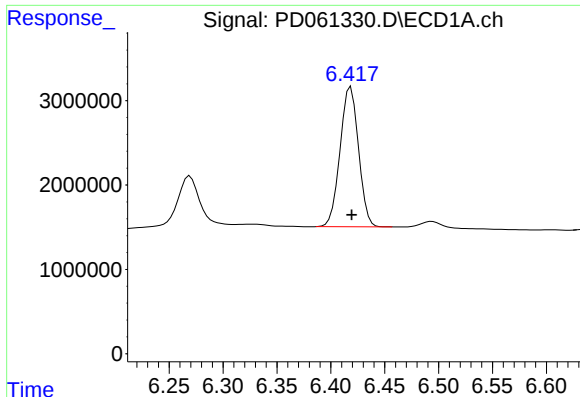

#17 4,4'-DDT


R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 19774215
Conc: 19.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

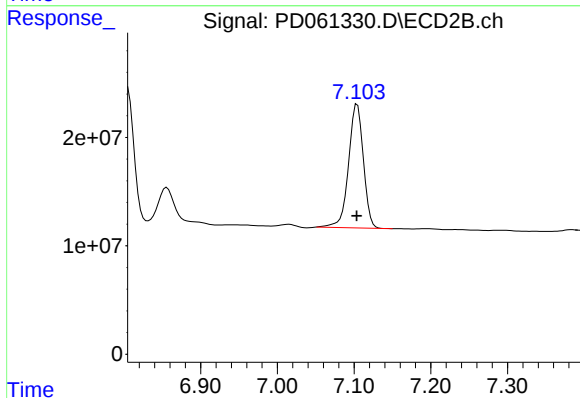


#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 153853619
Conc: 20.65 ng/ml

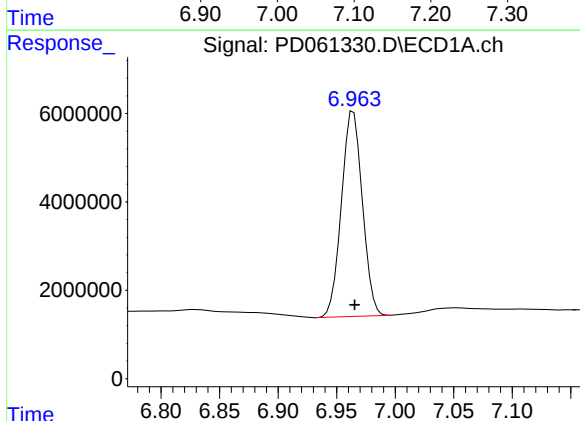


#20 Methoxychlor

R.T.: 6.964 min
Delta R.T.: -0.001 min
Response: 57871260
Conc: 103.31 ng/ml

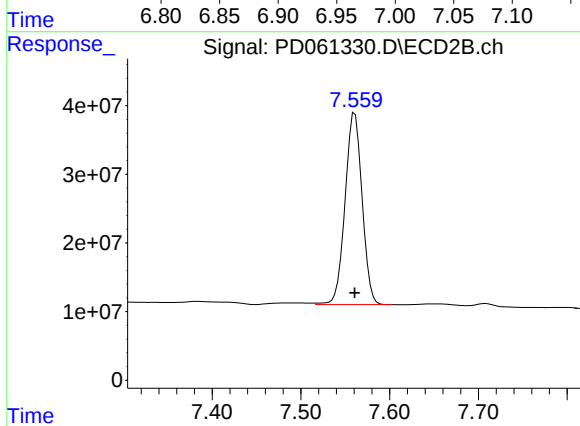

#20 Methoxychlor


R.T.: 7.561 min
Delta R.T.: 0.000 min
Response: 372951775
Conc: 106.06 ng/ml

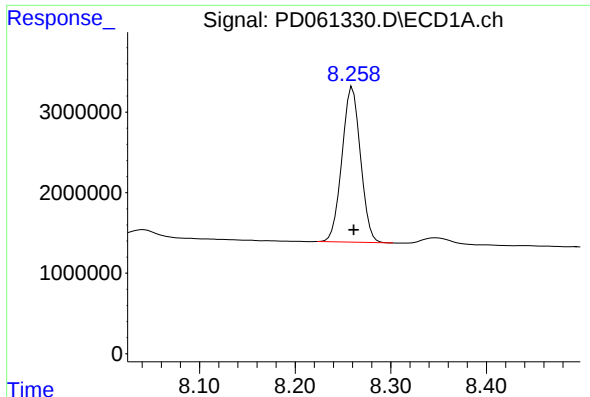

#27 Decachlorobiphenyl

R.T.: 8.260 min
Delta R.T.: -0.001 min
Response: 26008542
Conc: 21.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

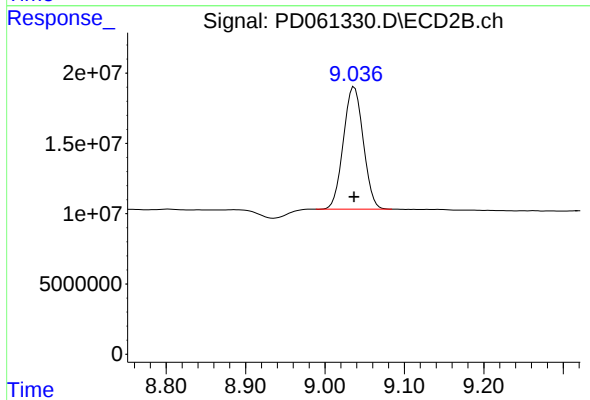

#27 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: 0.000 min
Response: 151748788
Conc: 20.91 ng/ml