

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022121\
 Data File : PD061332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2021 14:33
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 04:23:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022121CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 22 04:21:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	3.982	18422817	171.0E6	20.000	20.000
27)	SA Decachlor...	8.261	9.037	48982292	290.3E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.927	4.370	26314403	260.9E6	20.000	20.000
3)	MA gamma-BHC...	4.212	4.654	25682363	236.7E6	20.000	20.000
4)	MA Heptachlor	4.516	5.163	26353016	238.0E6	20.000	20.000
9)	A Endosulfan I	5.550	6.209	23369786	186.0E6	20.000	20.000
13)	MA Dieldrin	5.795	6.466	51139665	396.7E6	40.000	40.000
14)	MA Endrin	6.053	6.683	42046791	312.7E6	40.000	40.000
16)	A 4,4'-DDD	6.177	6.805	40776337	310.0E6	40.000	40.000
17)	MA 4,4'-DDT	6.419	7.103	40292806	298.0E6	40.000	40.000
20)	A Methoxychlor	6.966	7.561	112.0E6	703.3E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022121\
Data File : PD061332.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2021 14:33
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 04:23:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022121CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 22 04:21:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

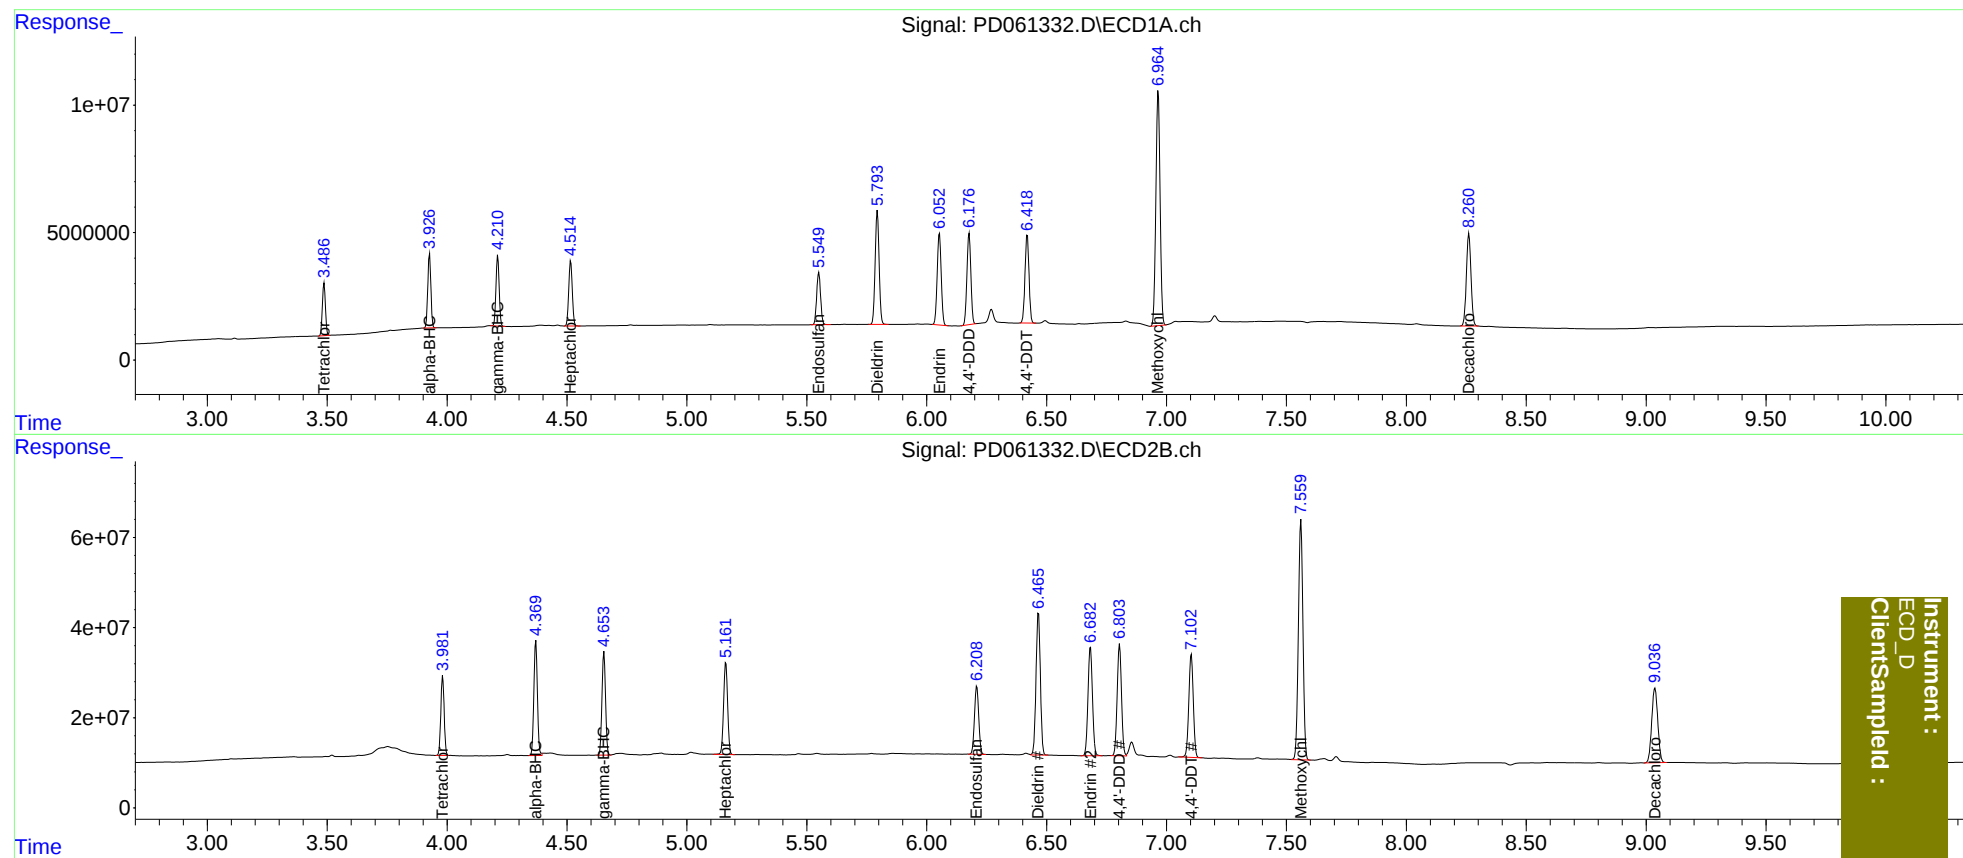


Instrument :
ECD_D
ClientSample :
Sample

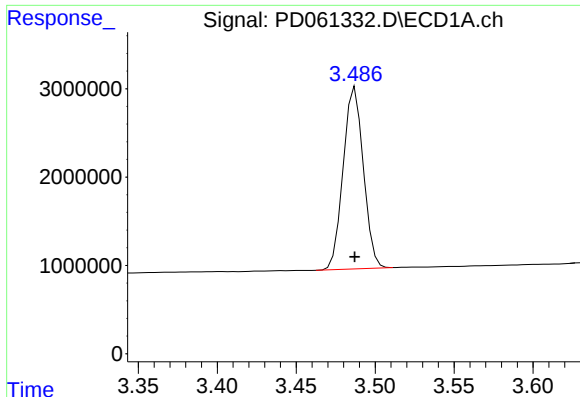

#1 Tetrachloro-m-xylene


R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 18422817
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

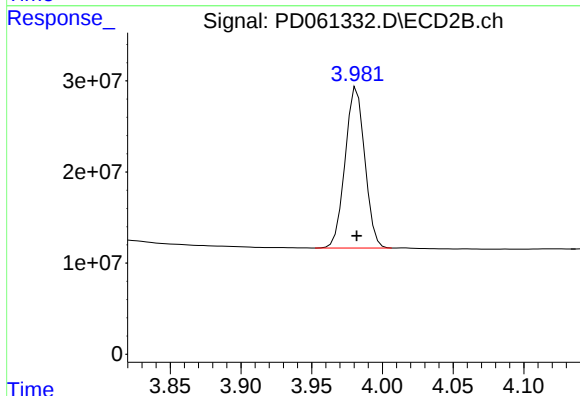


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 170972505
Conc: 20.00 ng/ml

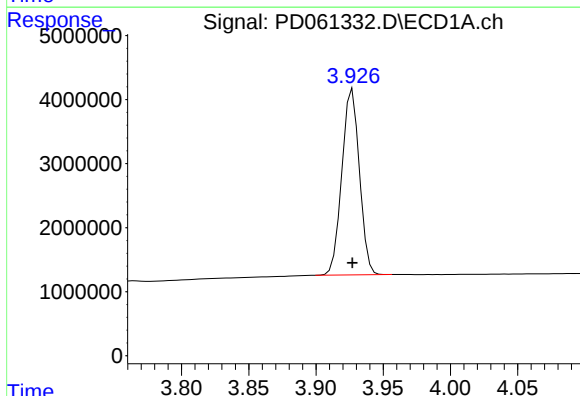


#2 alpha-BHC

R.T.: 3.927 min
Delta R.T.: 0.000 min
Response: 26314403
Conc: 20.00 ng/ml

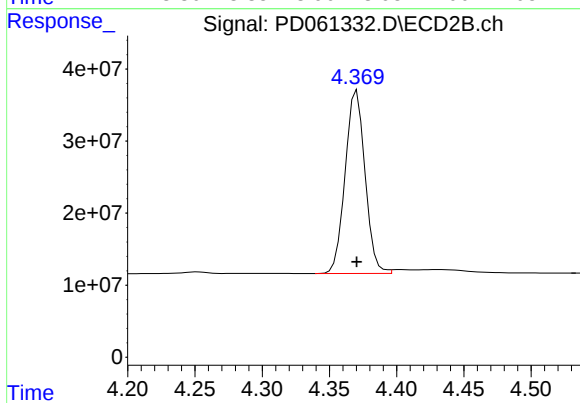

#2 alpha-BHC


R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 260865556
Conc: 20.00 ng/ml

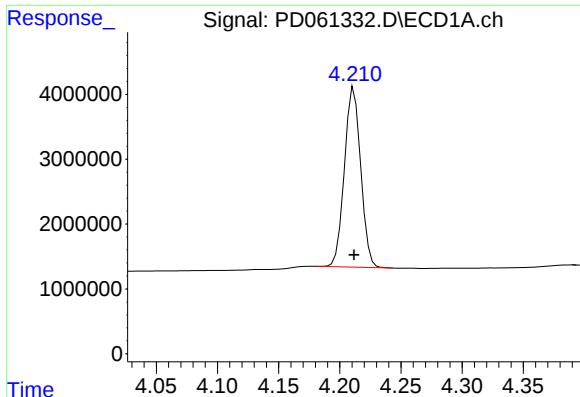

#3 gamma-BHC (Lindane)


R.T.: 4.212 min
Delta R.T.: 0.000 min
Response: 25682363
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

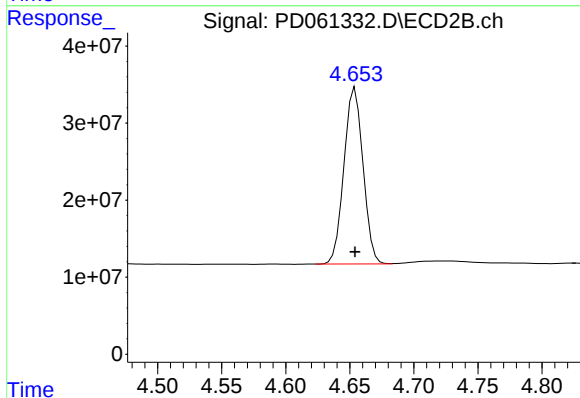


#3 gamma-BHC (Lindane)

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 236657701
Conc: 20.00 ng/ml

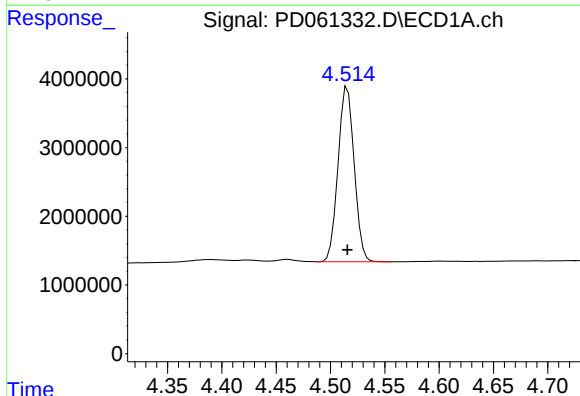


#4 Heptachlor

R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 26353016
Conc: 20.00 ng/ml

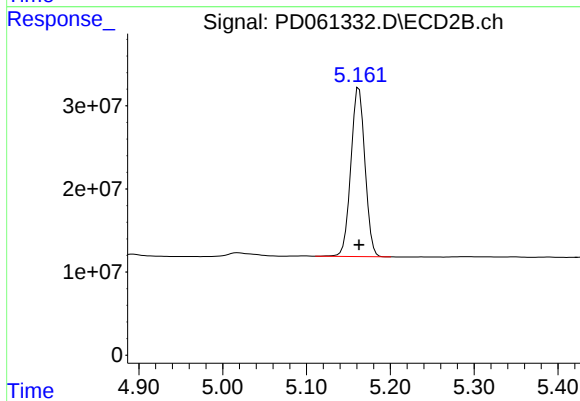

#4 Heptachlor


R.T.: 5.163 min
Delta R.T.: 0.000 min
Response: 237979236
Conc: 20.00 ng/ml

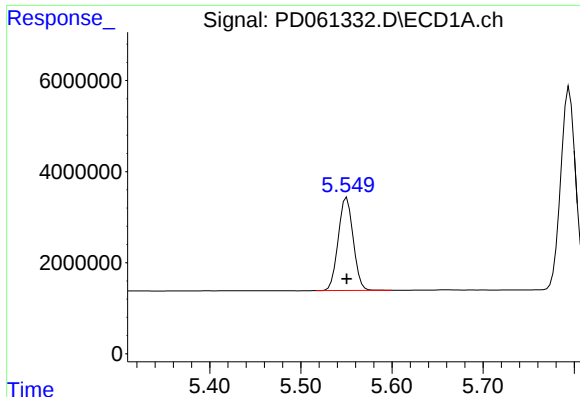

#9 Endosulfan I


R.T.: 5.550 min
Delta R.T.: 0.000 min
Response: 23369786
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

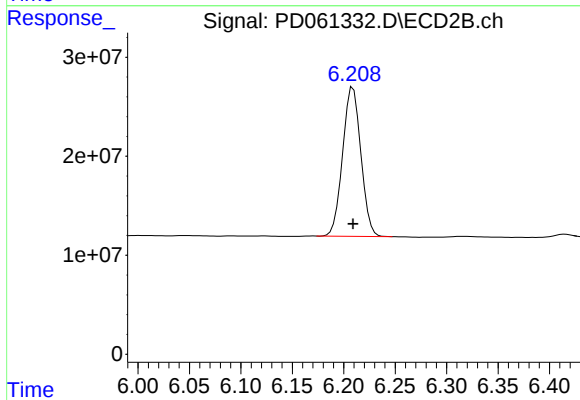


#9 Endosulfan I

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 185995101
Conc: 20.00 ng/ml

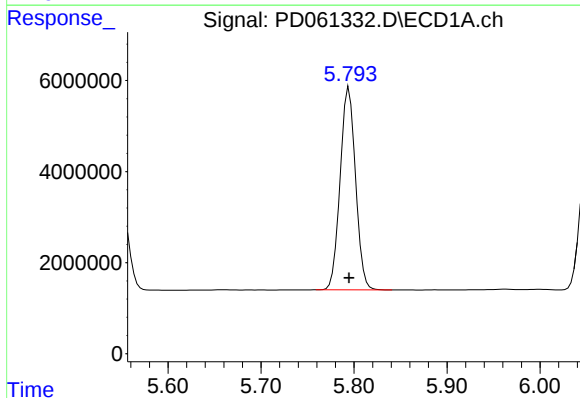


#13 Dieldrin

R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 51139665
Conc: 40.00 ng/ml

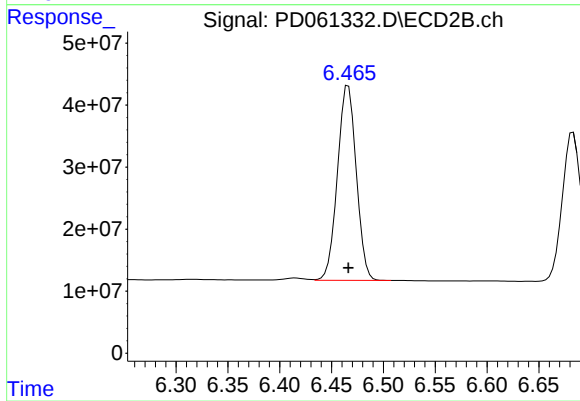

#13 Dieldrin


R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 396714145
Conc: 40.00 ng/ml

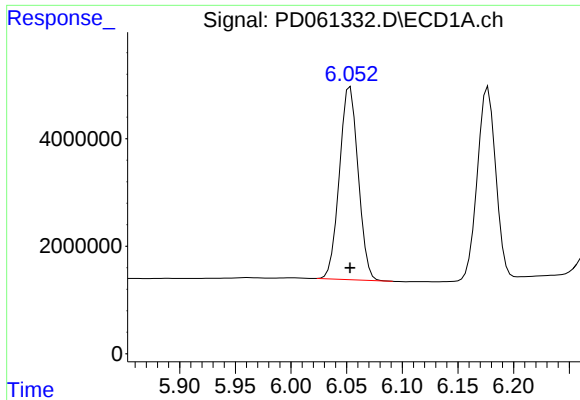

#14 Endrin


R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 42046791
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

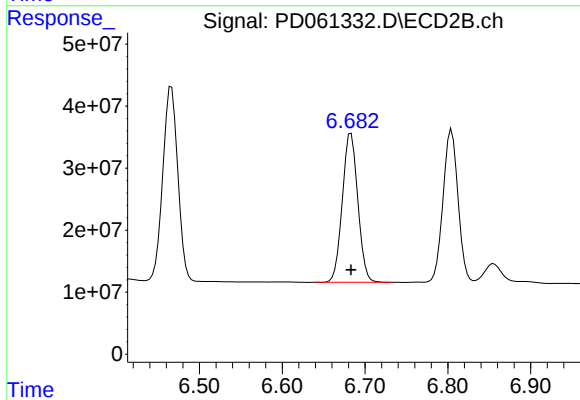


#14 Endrin

R.T.: 6.683 min
Delta R.T.: 0.000 min
Response: 312689896
Conc: 40.00 ng/ml

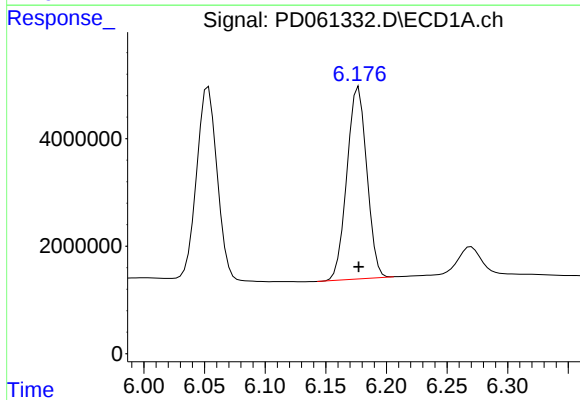


#16 4,4'-DDD

R.T.: 6.177 min
Delta R.T.: 0.000 min
Response: 40776337
Conc: 40.00 ng/ml

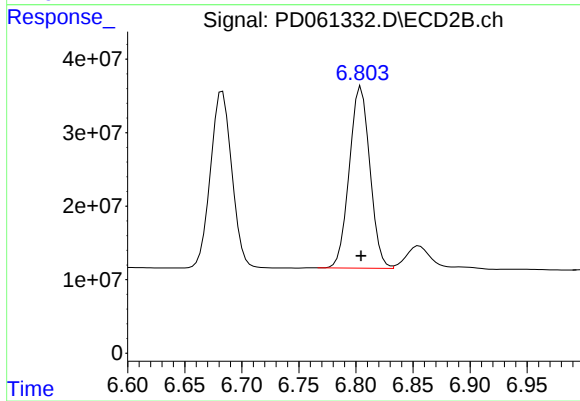

#16 4,4'-DDD


R.T.: 6.805 min
Delta R.T.: 0.000 min
Response: 310009144
Conc: 40.00 ng/ml

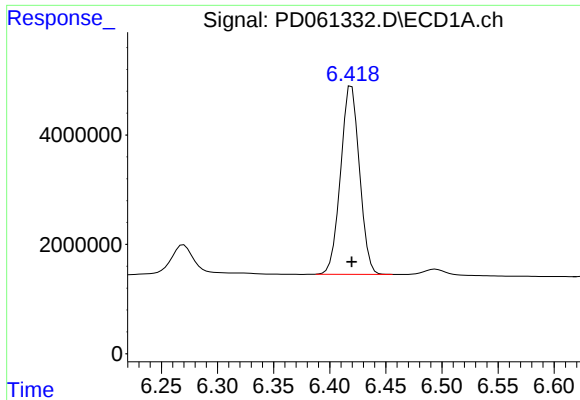

#17 4,4'-DDT


R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 40292806
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

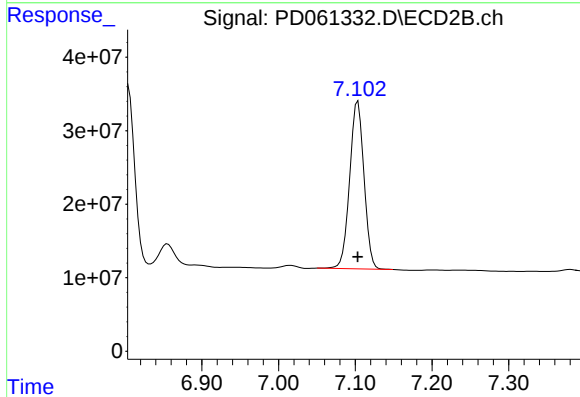


#17 4,4'-DDT

R.T.: 7.103 min
Delta R.T.: 0.000 min
Response: 298007466
Conc: 40.00 ng/ml

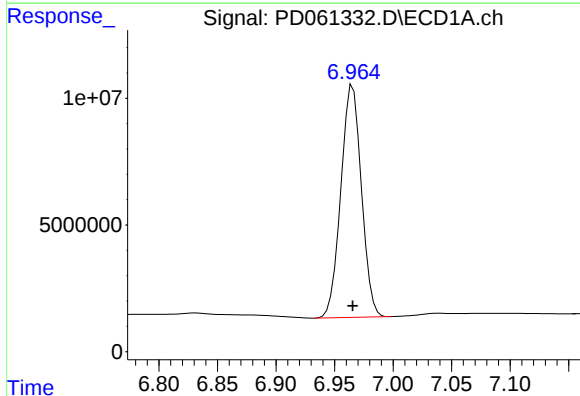


#20 Methoxychlor

R.T.: 6.966 min
Delta R.T.: 0.000 min
Response: 112032436
Conc: 200.00 ng/ml

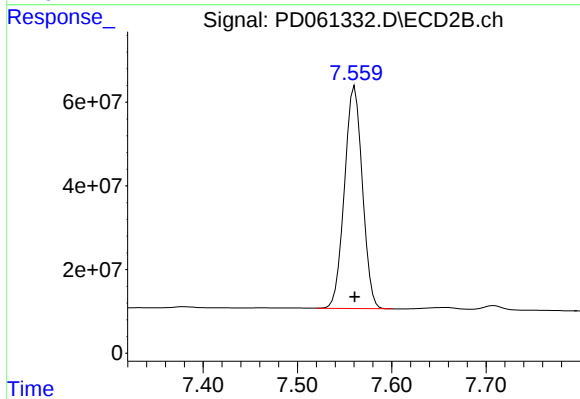

#20 Methoxychlor

R.T.: 7.561 min
Delta R.T.: 0.000 min
Response: 703253008
Conc: 200.00 ng/ml

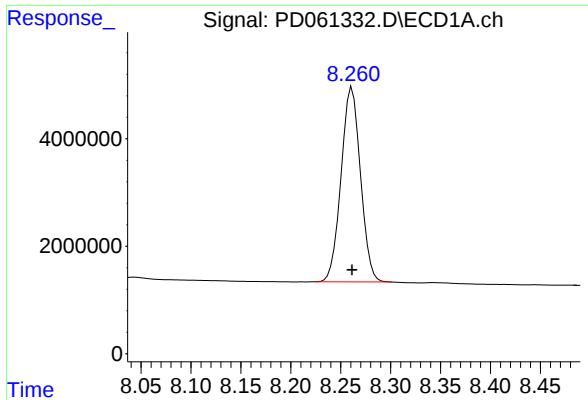

#27 Decachlorobiphenyl


R.T.: 8.261 min

Delta R.T.: 0.000 min

Response: 48982292

Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

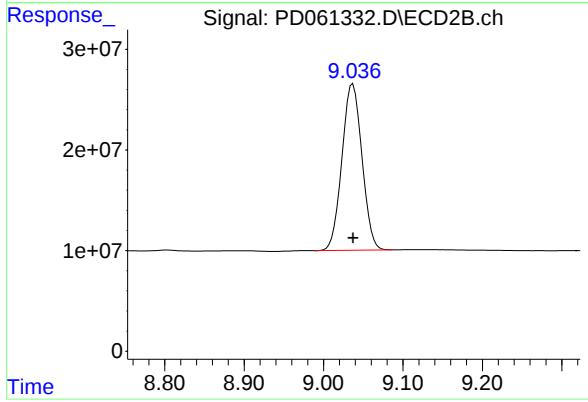

#27 Decachlorobiphenyl

R.T.: 9.037 min

Delta R.T.: 0.000 min

Response: 290286272

Conc: 40.00 ng/ml