

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022121\
 Data File : PD061336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2021 15:29
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 04:23:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022121CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 22 04:21:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	3.982	68723598	619.9E6	74.607	72.511
27)	SA Decachlor...	8.260	9.037	172.7E6	1015.3E6	141.026	139.898
Target Compounds							
2)	A alpha-BHC	3.927	4.370	108.5E6	968.2E6	82.483	74.229
3)	MA gamma-BHC...	4.212	4.654	102.6E6	882.1E6	79.869	74.545
4)	MA Heptachlor	4.515	5.162	102.5E6	867.5E6	77.821	72.908
9)	A Endosulfan I	5.550	6.209	88406659	686.5E6	75.659	73.816
13)	MA Dieldrin	5.795	6.466	203.7E6	1475.7E6	159.296	148.789
14)	MA Endrin	6.053	6.684	162.6E6	1144.3E6	154.664	146.385
16)	A 4,4'-DDD	6.177	6.804	161.9E6	1150.5E6	158.809	148.451
17)	MA 4,4'-DDT	6.419	7.103	167.0E6	1126.3E6	165.753	151.180
20)	A Methoxychlor	6.965	7.561	411.0E6	2473.5E6	733.746	703.456

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022121\
Data File : PD061336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2021 15:29
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 04:23:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022121CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 22 04:21:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

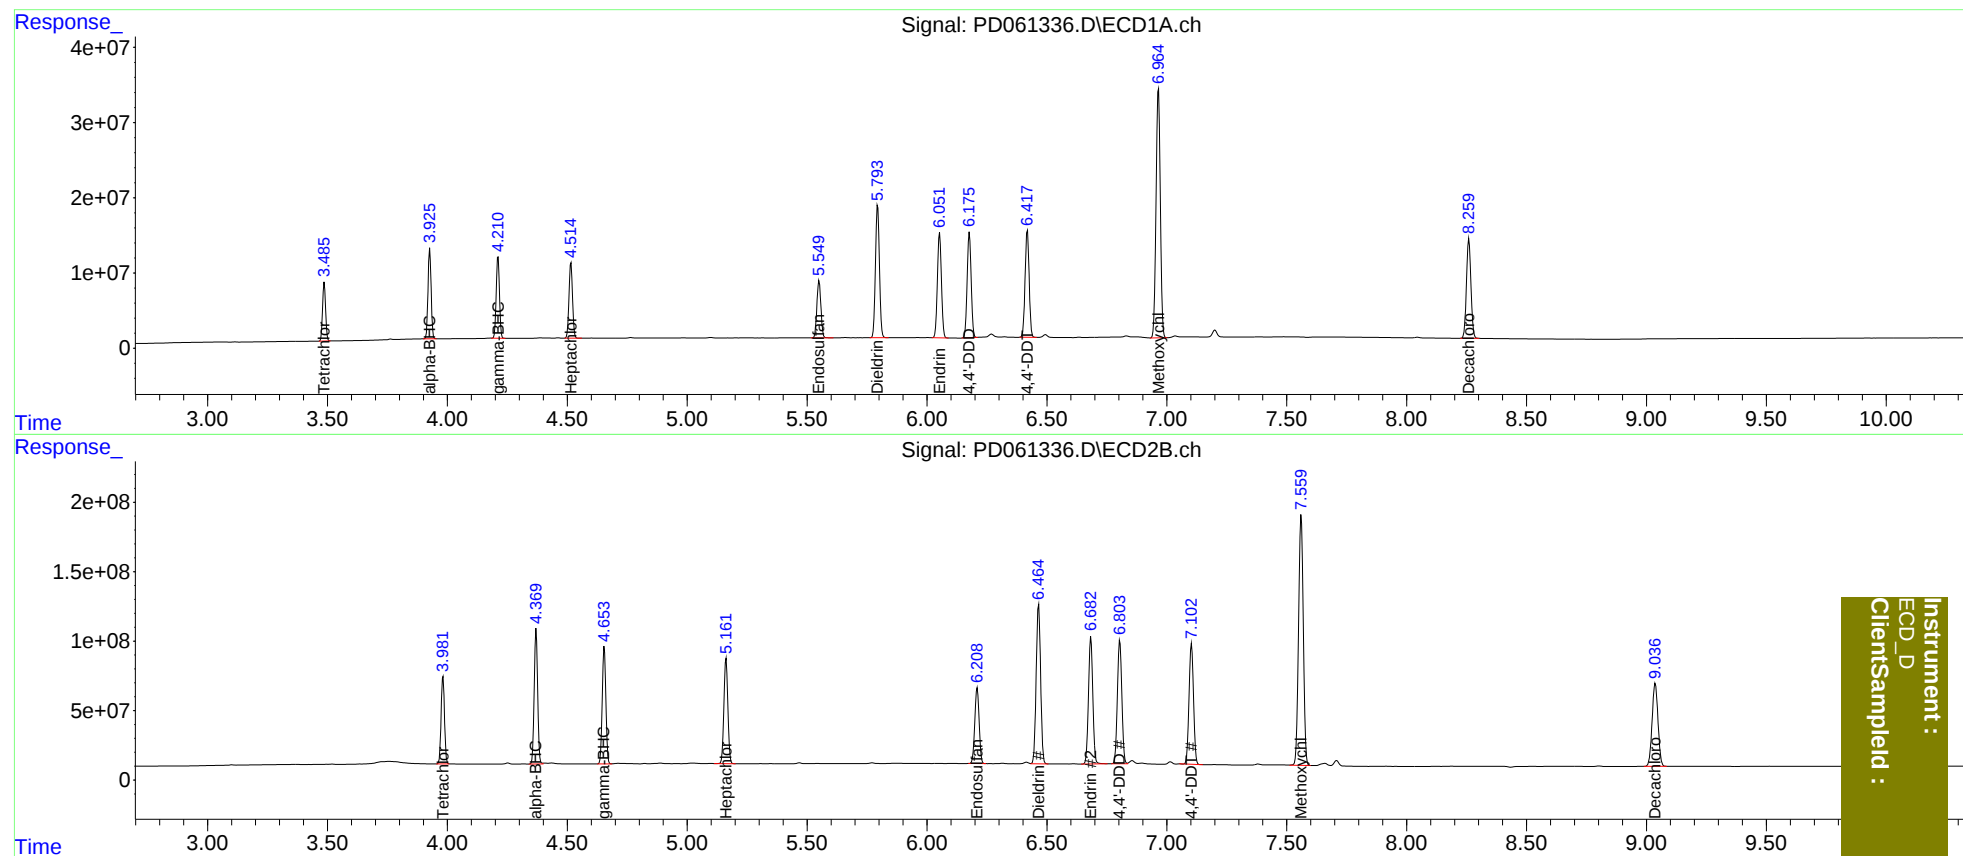


Instrument :
ECD_D
ClientSample :
Sample

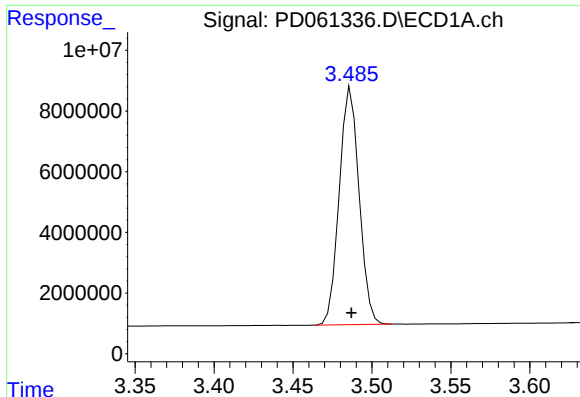

#1 Tetrachloro-m-xylene


R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 68723598
Conc: 74.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

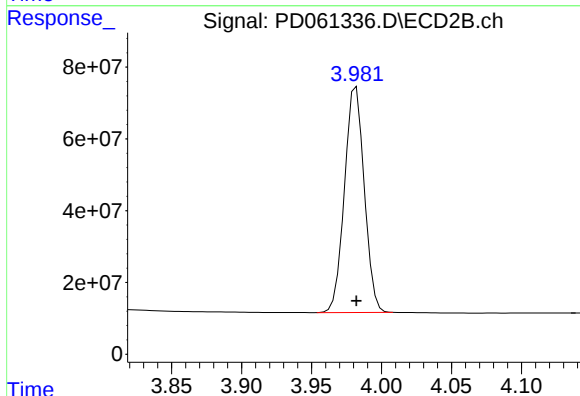


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 619871082
Conc: 72.51 ng/ml

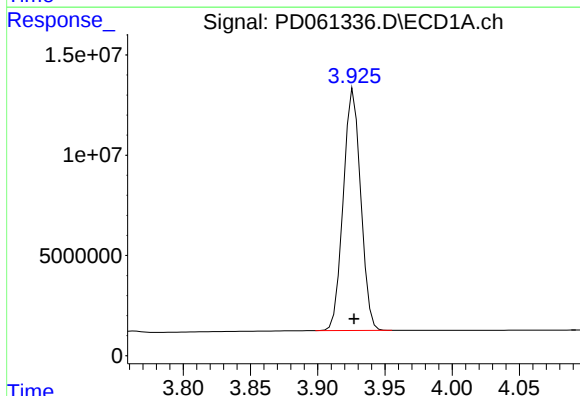


#2 alpha-BHC

R.T.: 3.927 min
Delta R.T.: 0.000 min
Response: 108525175
Conc: 82.48 ng/ml

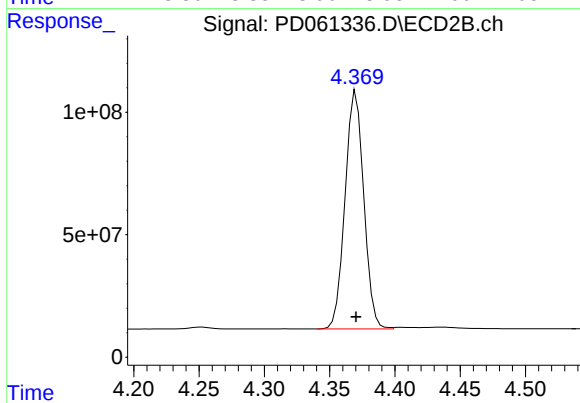

#2 alpha-BHC


R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 968193117
Conc: 74.23 ng/ml

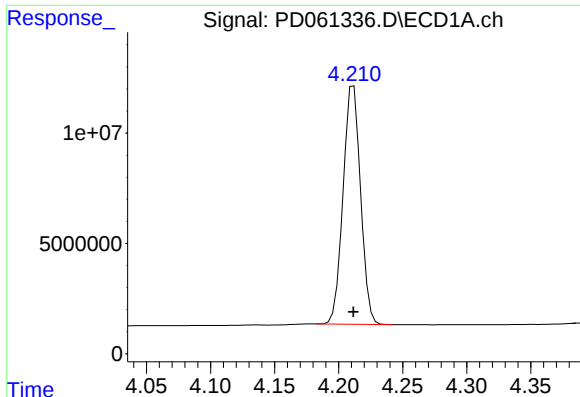

#3 gamma-BHC (Lindane)


R.T.: 4.212 min
Delta R.T.: 0.000 min
Response: 102561768
Conc: 79.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

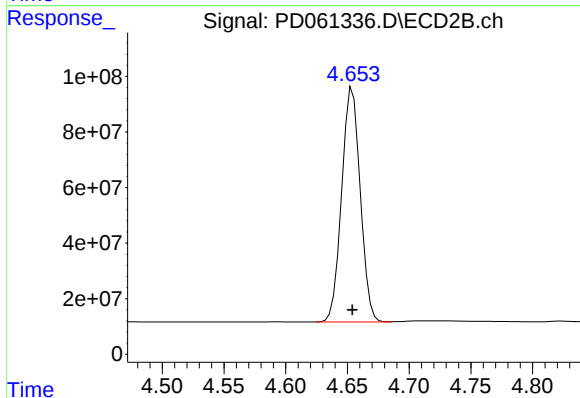


#3 gamma-BHC (Lindane)

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 882085546
Conc: 74.55 ng/ml

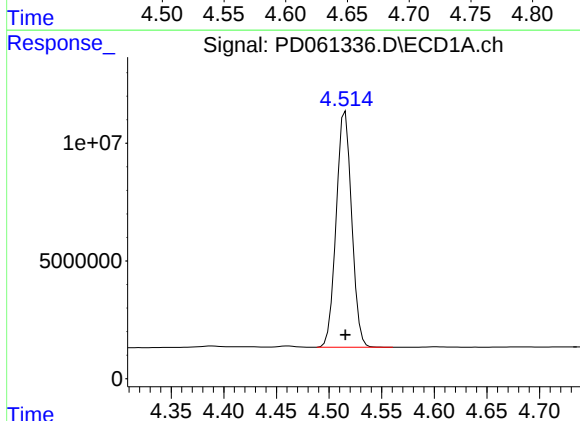


#4 Heptachlor

R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 102540698
Conc: 77.82 ng/ml

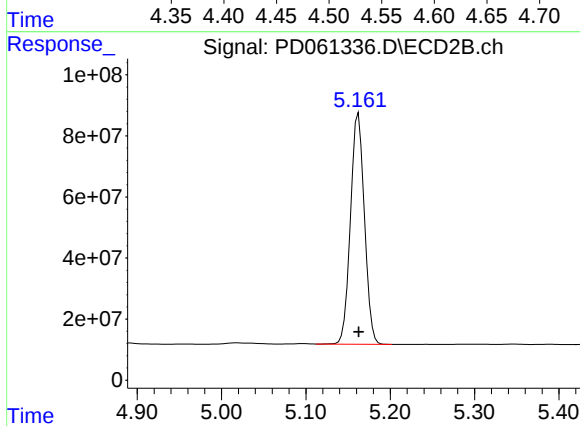

#4 Heptachlor


R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 867533835
Conc: 72.91 ng/ml

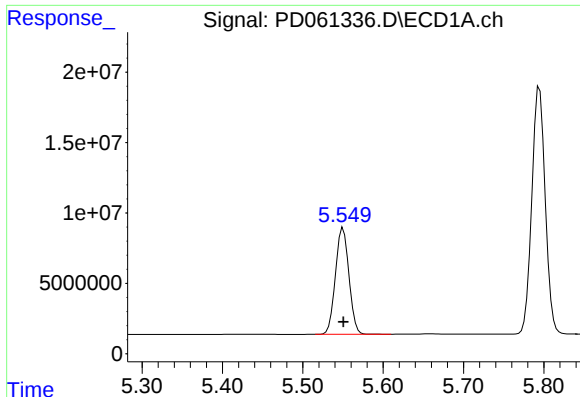

#9 Endosulfan I


R.T.: 5.550 min
Delta R.T.: 0.000 min
Response: 88406659
Conc: 75.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

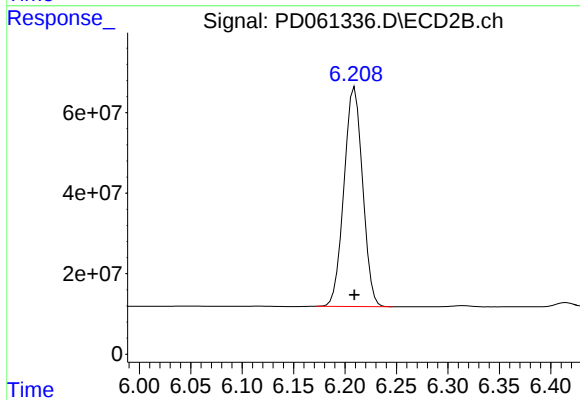


#9 Endosulfan I

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 686472507
Conc: 73.82 ng/ml

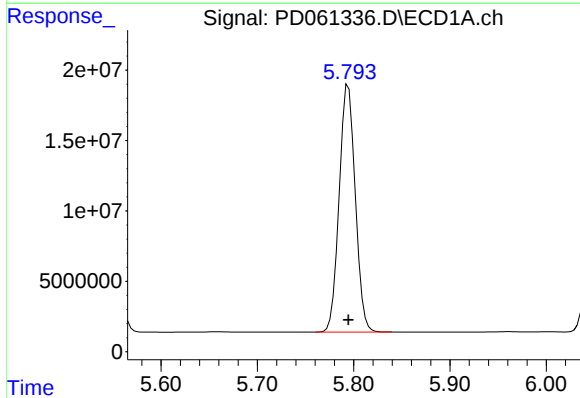


#13 Dieldrin

R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 203658660
Conc: 159.30 ng/ml

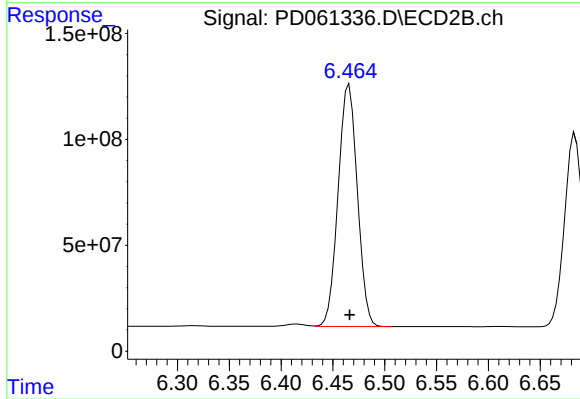

#13 Dieldrin


R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 1475665456
Conc: 148.79 ng/ml

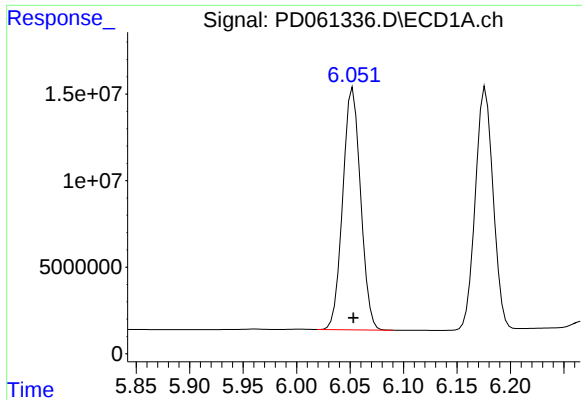

#14 Endrin


R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 162578018
Conc: 154.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

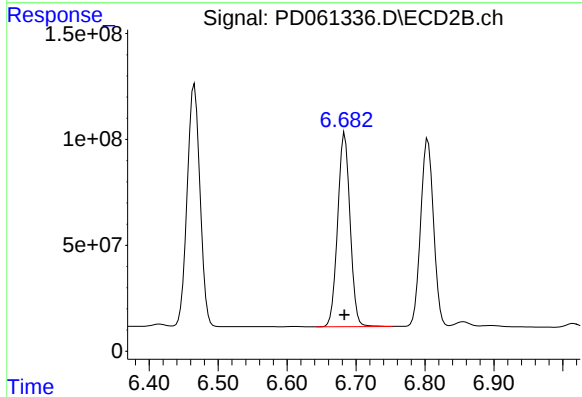


#14 Endrin

R.T.: 6.684 min
Delta R.T.: 0.000 min
Response: 1144330179
Conc: 146.39 ng/ml

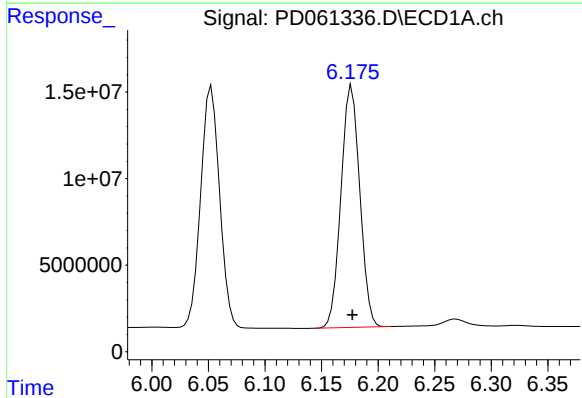


#16 4,4'-DDD

R.T.: 6.177 min
Delta R.T.: 0.000 min
Response: 161891347
Conc: 158.81 ng/ml

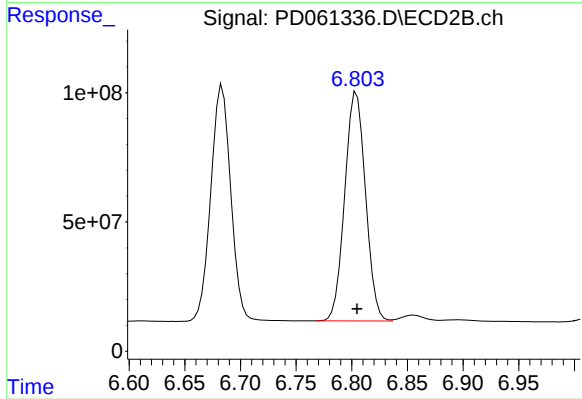

#16 4,4'-DDD


R.T.: 6.804 min
Delta R.T.: 0.000 min
Response: 1150532512
Conc: 148.45 ng/ml

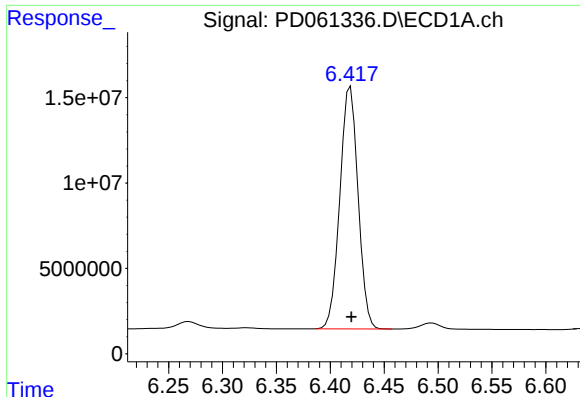

#17 4,4'-DDT


R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 166965891
Conc: 165.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

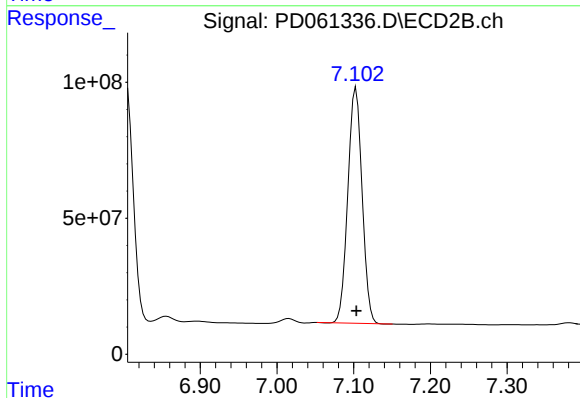


#17 4,4'-DDT

R.T.: 7.103 min
Delta R.T.: 0.000 min
Response: 1126321615
Conc: 151.18 ng/ml

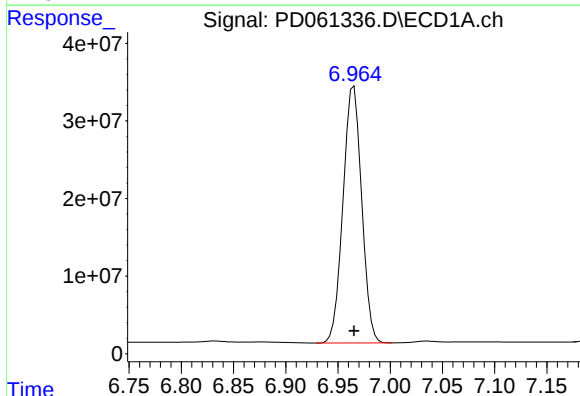


#20 Methoxychlor

R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 411016737
Conc: 733.75 ng/ml

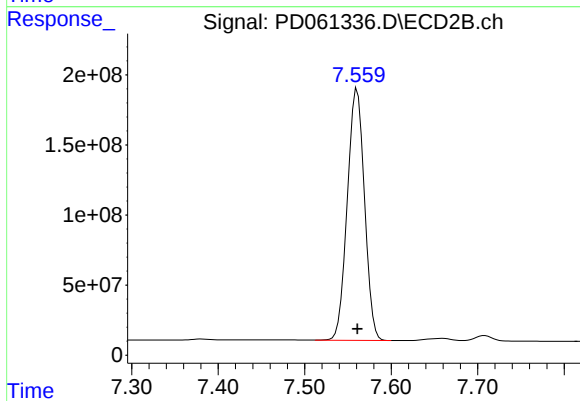

#20 Methoxychlor


R.T.: 7.561 min
Delta R.T.: 0.000 min
Response: 2473537041
Conc: 703.46 ng/ml

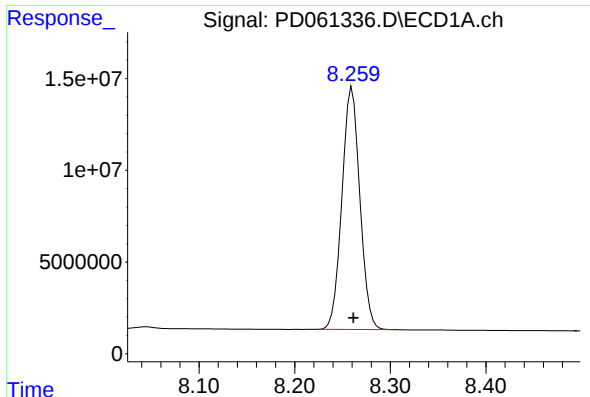

#27 Decachlorobiphenyl

R.T.: 8.260 min
Delta R.T.: -0.001 min
Response: 172694120
Conc: 141.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

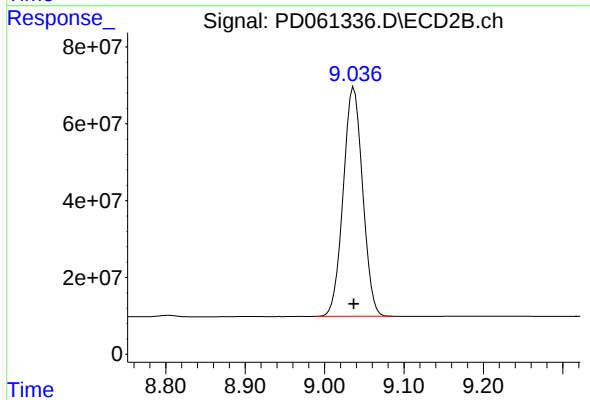

#27 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: 0.000 min
Response: 1015260205
Conc: 139.90 ng/ml