

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022121\
 Data File : PD061321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2021 11:58
 Operator : DD\AJ
 Sample : RESC01
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 04:52:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022121CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 22 04:35:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	3.983	17601449	154.4E6	19.114	18.463
2)	SA Decachlor...	8.260	9.038	45086719	270.8E6	36.646	37.677
Target Compounds							
2)	A alpha-BHC	3.927	4.371	12364571	115.9E6	9.350	9.023
3)	MA gamma-BHC...	4.212	4.655	12175280	106.4E6	9.464	9.109
4)	MA Heptachlor	4.515	5.164	12632330	108.6E6	9.571	9.196
5)	MB Aldrin	4.765	5.468	12020158	101.4E6	9.771	9.301
6)	B beta-BHC	4.461	4.824	6302360	44781281	10.193	9.115
7)	B delta-BHC	4.668	5.041	12265701	110.2E6	9.491	9.448
8)	B Heptachlo...	5.209	5.854	11658090	92865050	9.748	9.356
9)	A Endosulfan I	5.551	6.210	11698026	86605919	9.918	9.376
10)	B trans-Chl...	5.437	6.087	12035023	92776907	9.646	9.292
11)	B cis-Chlor...	5.496	6.160	11848583	89000498	9.756	9.359
12)	B 4,4'-DDE	5.660	6.316	21802230	180.8E6	18.768	18.961
13)	MA Dieldrin	5.795	6.466	23744267	184.7E6	18.590	18.795
14)	MA Endrin	6.053	6.684	20056577	147.7E6	18.896	19.131
15)	B Endosulfa...	6.326	6.892	18811287	150.4E6	18.556	19.582
16)	A 4,4'-DDD	6.177	6.805	18844935	145.4E6	18.562	18.981
17)	MA 4,4'-DDT	6.419	7.103	17738219	142.2E6	17.631	19.076
18)	B Endrin al...	6.495	7.016	18053928	118.1E6	20.102	18.907
19)	B Endosulfa...	6.709	7.239	19978174	138.2E6	19.205	18.915
20)	A Methoxychlor	6.965	7.561	52908925	338.9E6	94.919	96.997
21)	B Endrin ke...	7.202	7.709	23981103	141.9E6	20.065	19.640

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022121\
Data File : PD061321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2021 11:58
Operator : DD\AJ
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 04:52:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022121CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 22 04:35:05 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

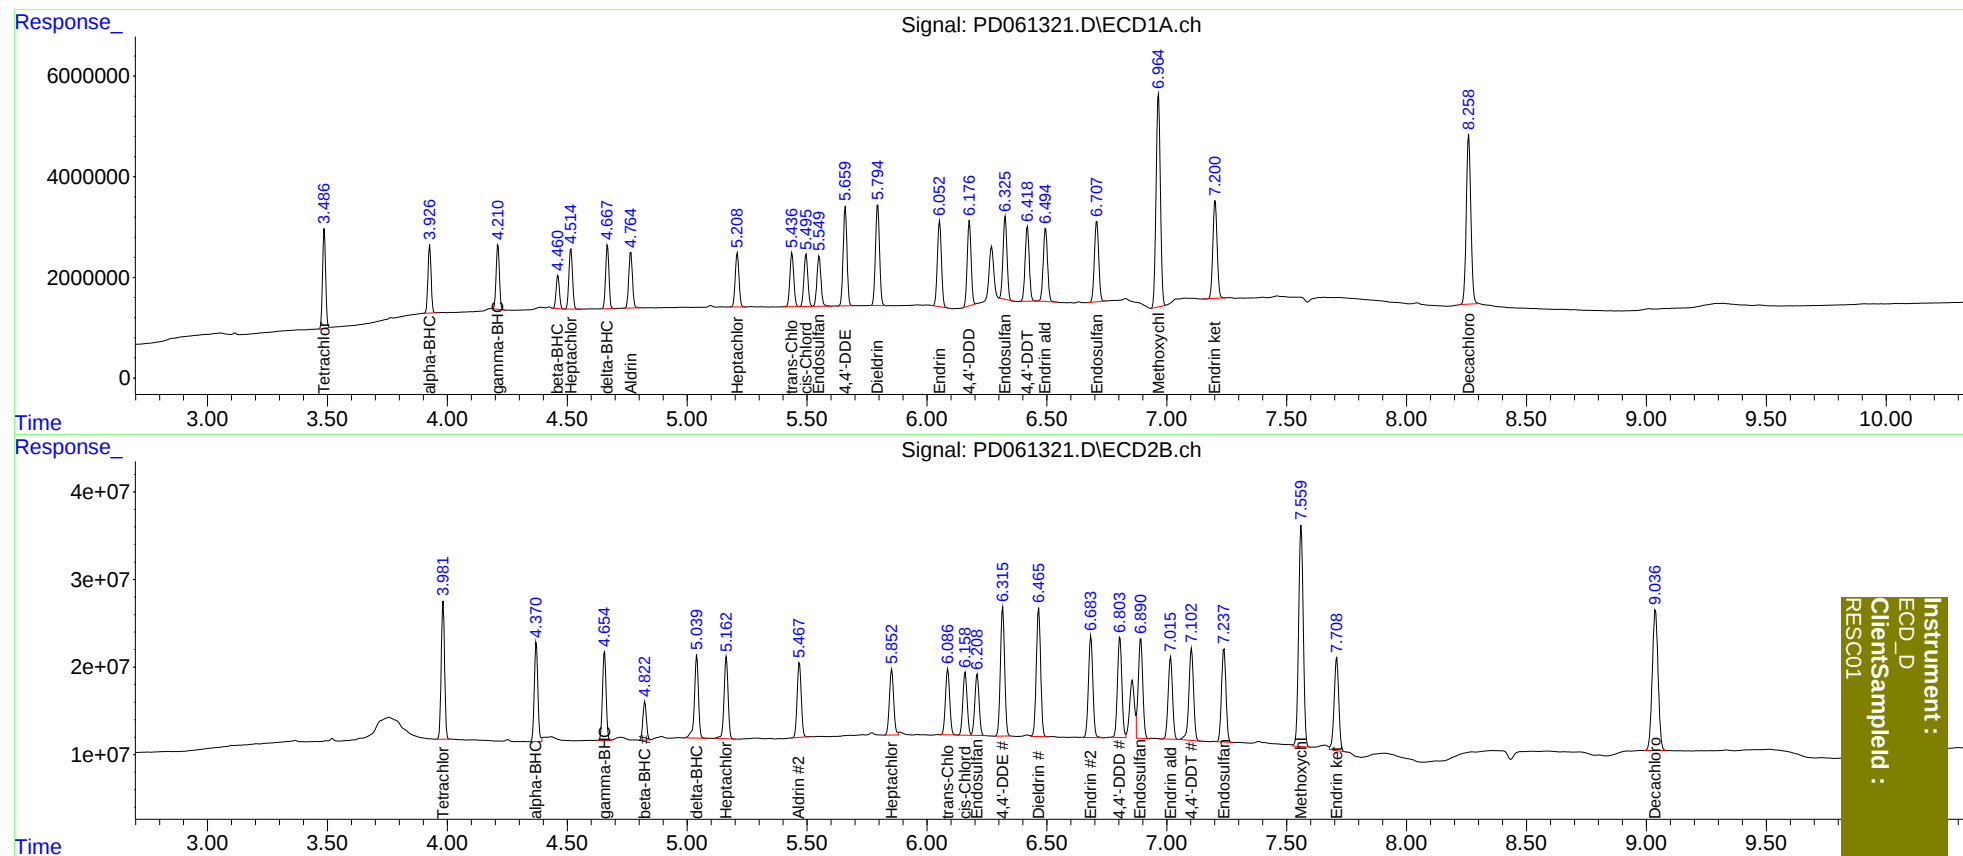

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022121\
Data File : PD061321.D
Acq On : 21 Feb 2021 11:58
Operator : DD\AJ
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022121CLP.M
Title : GC Extractables
Last Update : Mon Feb 22 04:35:05 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
3.487	3.927	100.00%
3.927	4.212	100.00%
4.212	4.461	100.00%
4.461	4.515	100.00%
4.515	4.668	100.00%
4.668	4.765	100.00%
4.765	5.209	100.00%
5.209	5.437	100.00%
5.437	5.496	100.00%
5.496	5.551	100.00%
5.551	5.660	100.00%
5.660	5.795	100.00%
5.795	6.053	100.00%
6.053	6.177	100.00%
6.177	6.326	100.00%
6.326	6.419	100.00%
6.419	6.495	100.00%
6.495	6.709	100.00%
6.709	6.966	100.00%
6.966	7.202	100.00%
7.202	8.260	100.00%

Signal #2


3.983	4.371	100.00%
4.371	4.655	100.00%
4.655	4.824	100.00%
4.824	5.041	100.00%
5.041	5.164	100.00%
5.164	5.468	100.00%
5.468	5.854	100.00%
5.854	6.087	100.00%
6.087	6.160	100.00%
6.160	6.210	99.16%
6.210	6.316	100.00%
6.316	6.466	100.00%
6.466	6.684	100.00%
6.684	6.805	100.00%
6.805	6.892	100.00%
6.892	7.016	100.00%
7.016	7.103	100.00%
7.103	7.239	100.00%
7.239	7.561	100.00%
7.561	7.709	100.00%
7.709	9.038	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022121\
Data File : PD061321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2021 11:58
Operator : DD\AJ
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 04:52:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022121CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 22 04:35:05 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

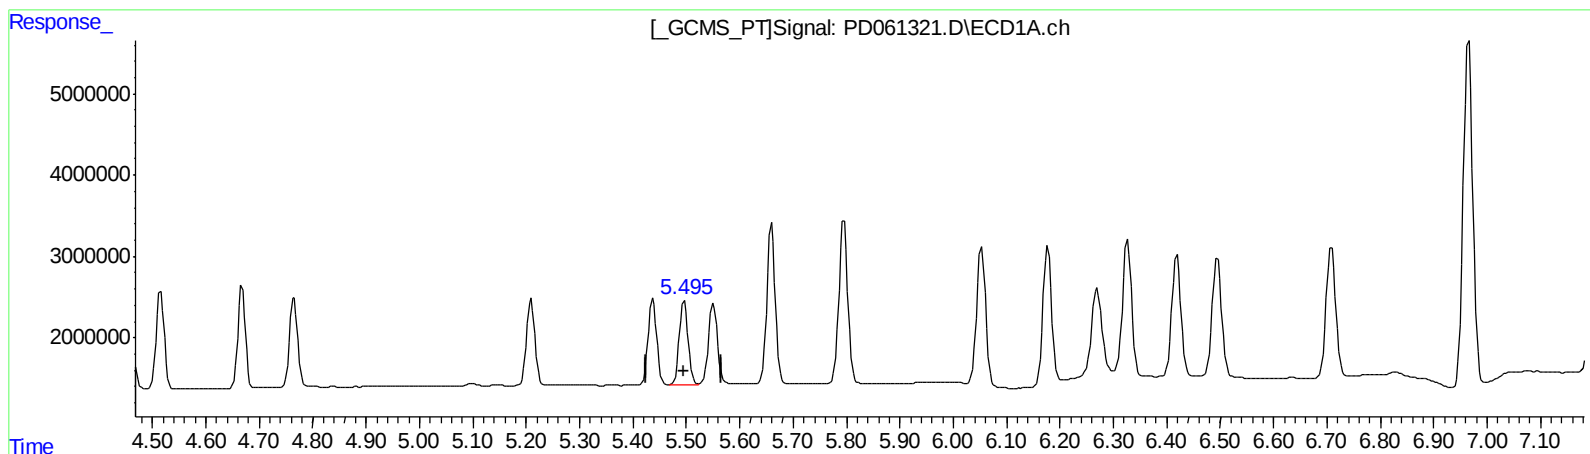

(11) cis-Chlordane (B)

5.496min 9.756 ng/ml

response 11848583

(11) cis-Chlordane #2 (B)

6.160min 9.359 ng/ml

response 89000498