

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022222\
 Data File : PD068136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2022 11:02
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 13:05:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 13:00:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.176	167.0E6	841.1E6	95.298	90.934
28)	SA Decachlor...	8.215	9.369	140.8E6	469.5E6	94.544	92.179
Target Compounds							
23)	Chlordane-1	4.322	5.198	59087947	373.5E6	962.021	912.928
24)	Chlordane-2	4.824	5.671	64508160	356.5E6	912.632	891.582
25)	Chlordane-3	5.393	6.327	212.6E6	1335.5E6	986.233	937.590
26)	Chlordane-4	5.451	6.404	173.6E6	1513.6E6	958.285	932.678
27)	Chlordane-5	6.290	7.215	68042640	252.6E6	976.410	939.235



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022222\
Data File : PD068136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2022 11:02
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 13:05:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 13:00:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

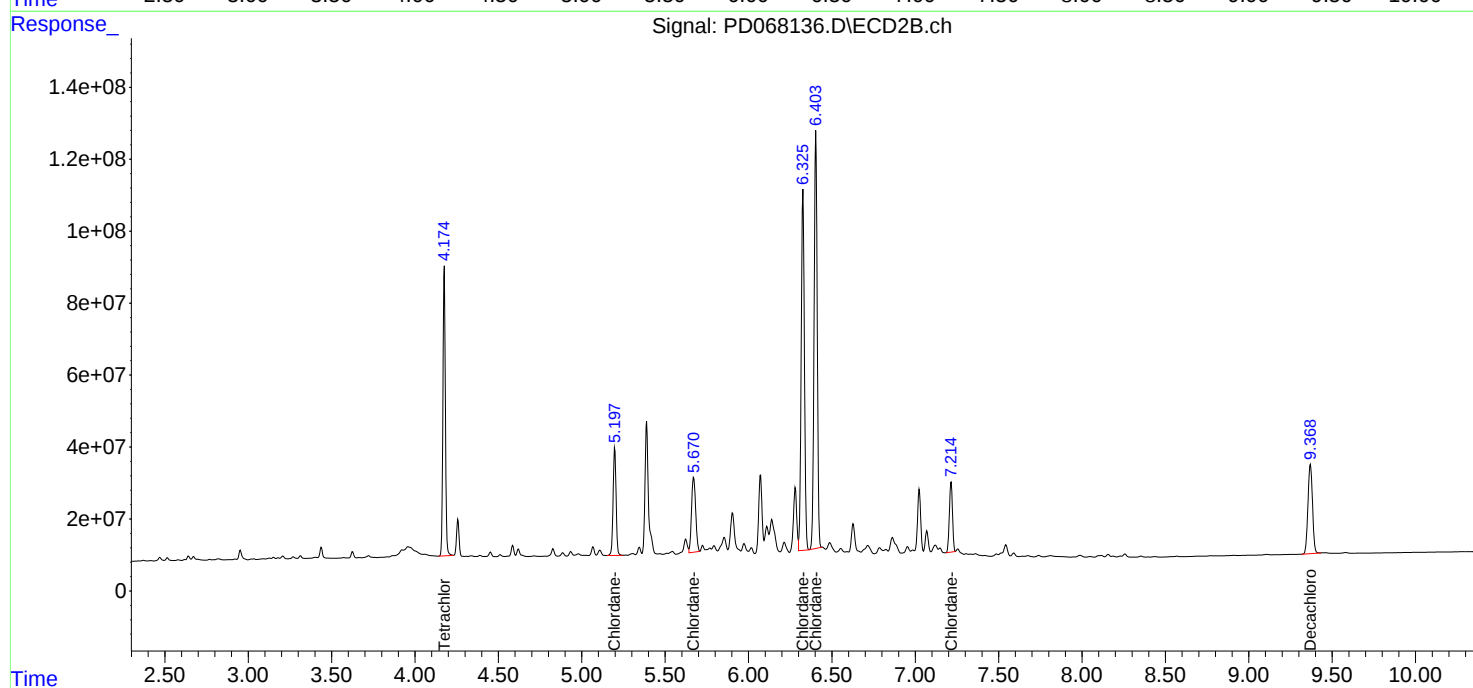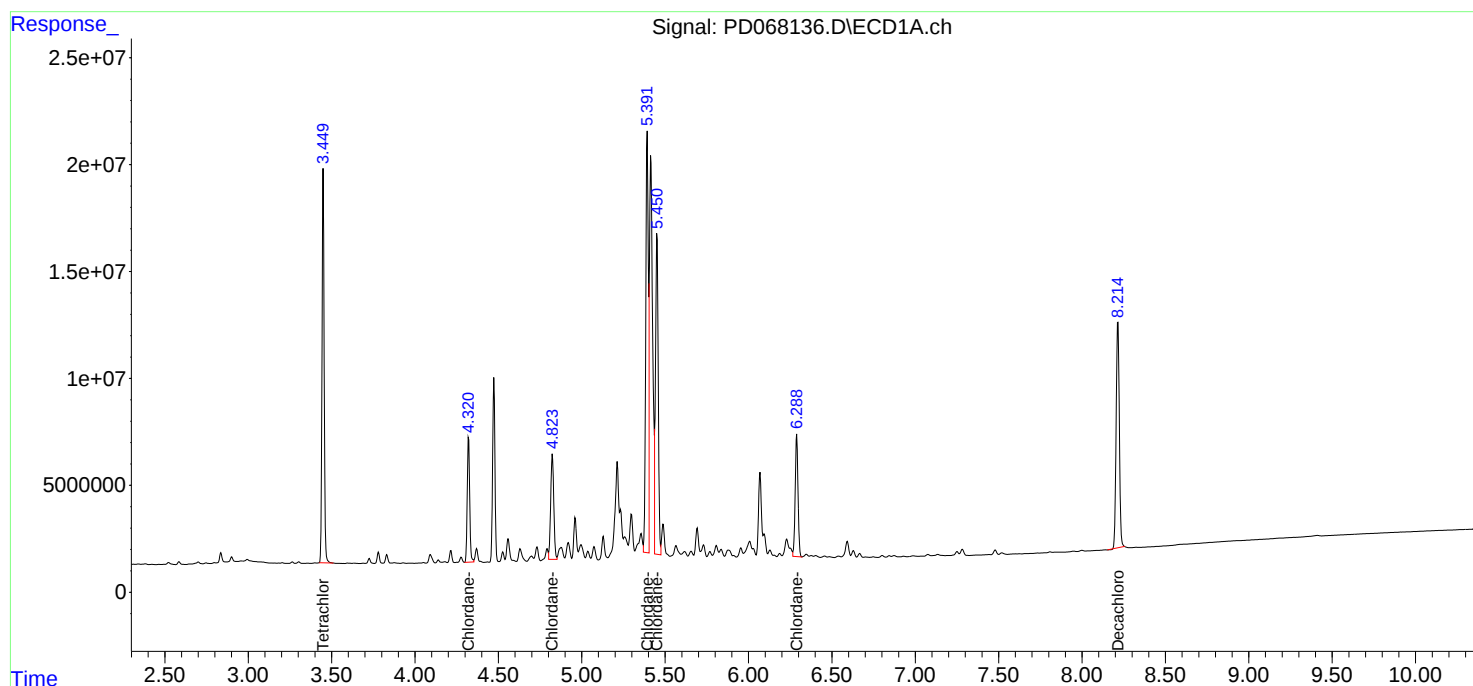


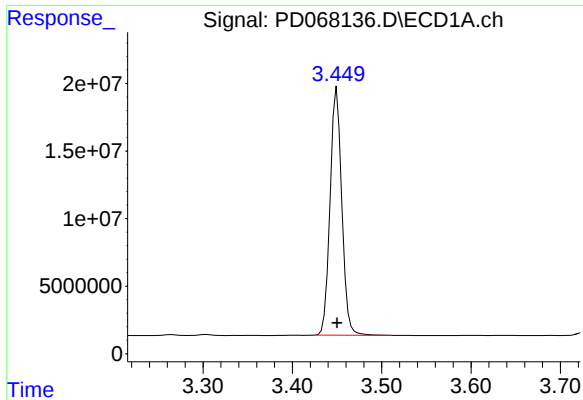

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 167039463
Conc: 95.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

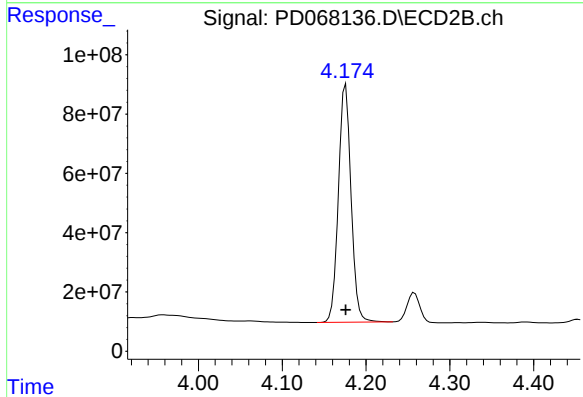


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 841128415
Conc: 90.93 ng/ml

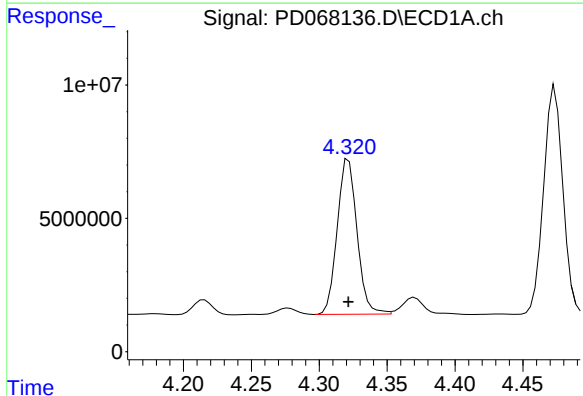


#23 Chlordane-1

R.T.: 4.322 min
Delta R.T.: 0.000 min
Response: 59087947
Conc: 962.02 ng/ml

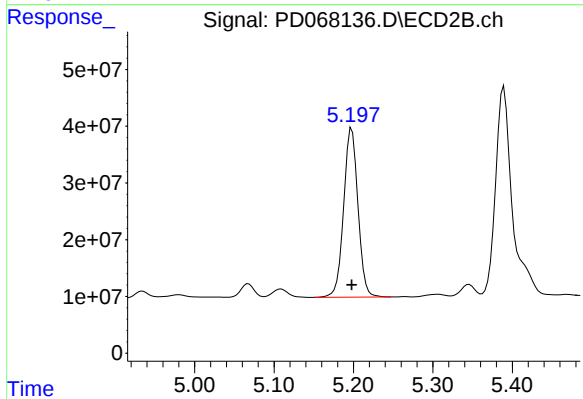

#23 Chlordane-1


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 373524808
Conc: 912.93 ng/ml

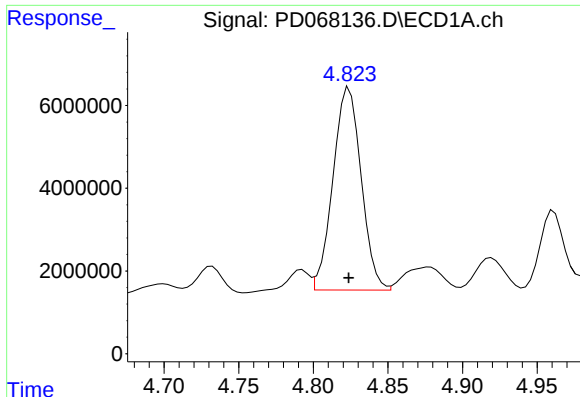

#24 Chlordane-2


R.T.: 4.824 min
Delta R.T.: 0.000 min
Response: 64508160
Conc: 912.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

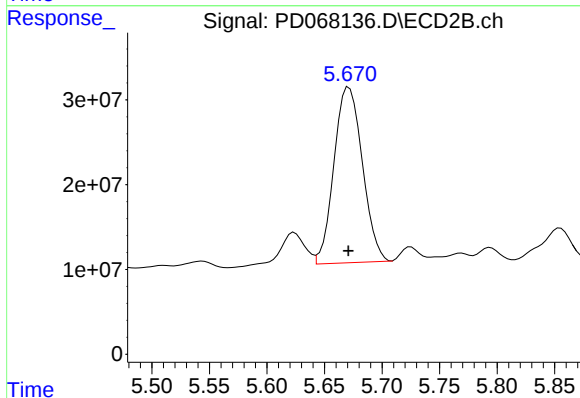


#24 Chlordane-2

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 356516984
Conc: 891.58 ng/ml

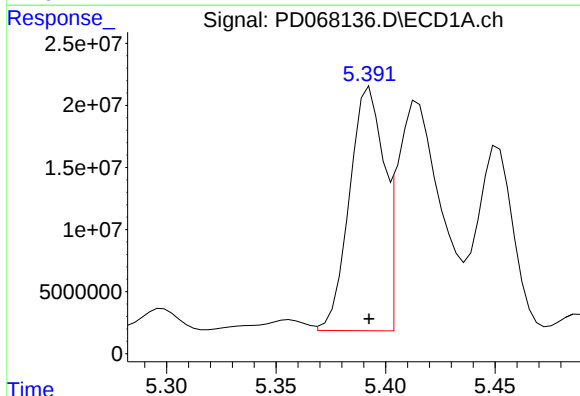


#25 Chlordane-3

R.T.: 5.393 min
Delta R.T.: 0.000 min
Response: 212600176
Conc: 986.23 ng/ml

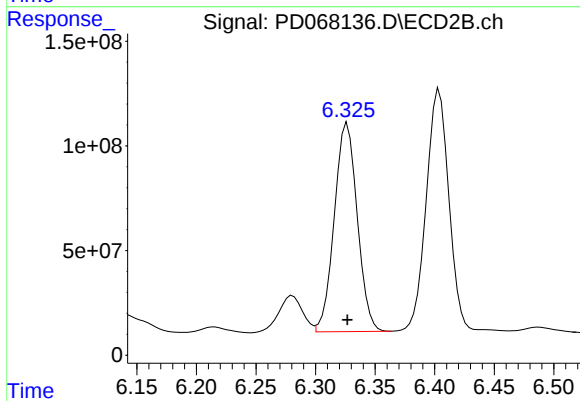

#25 Chlordane-3


R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 1335489744
Conc: 937.59 ng/ml

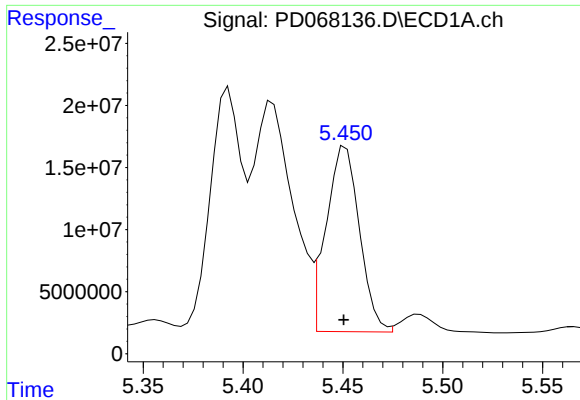

#26 Chlordane-4


R.T.: 5.451 min
Delta R.T.: 0.000 min
Response: 173639894
Conc: 958.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

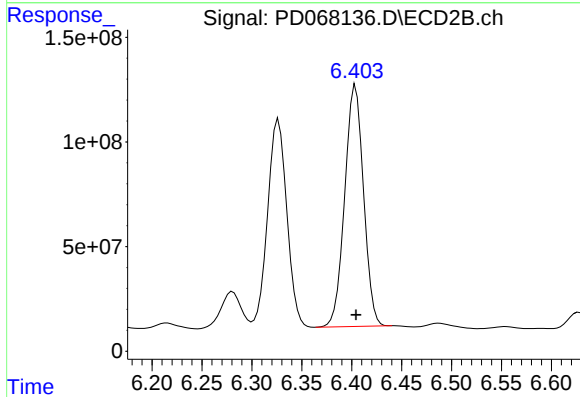


#26 Chlordane-4

R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 1513633365
Conc: 932.68 ng/ml

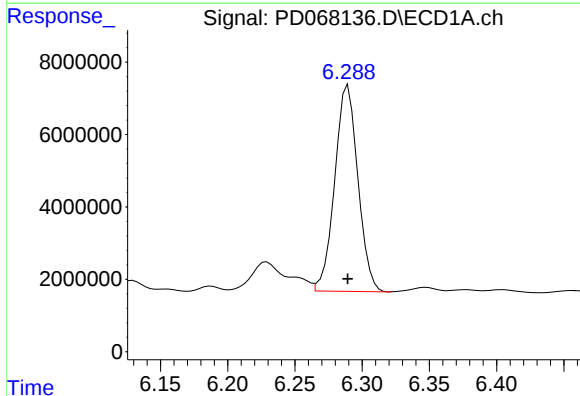


#27 Chlordane-5

R.T.: 6.290 min
Delta R.T.: 0.000 min
Response: 68042640
Conc: 976.41 ng/ml

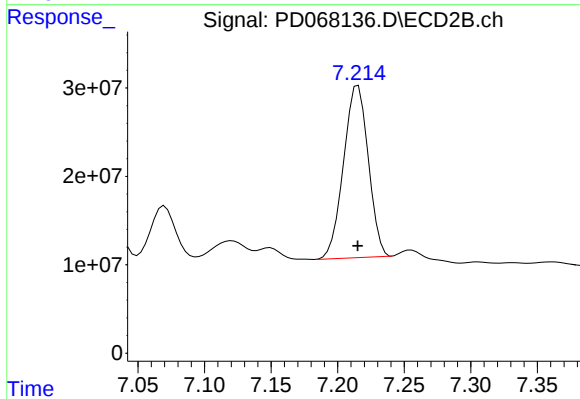

#27 Chlordane-5


R.T.: 7.215 min
Delta R.T.: 0.000 min
Response: 252573550
Conc: 939.23 ng/ml

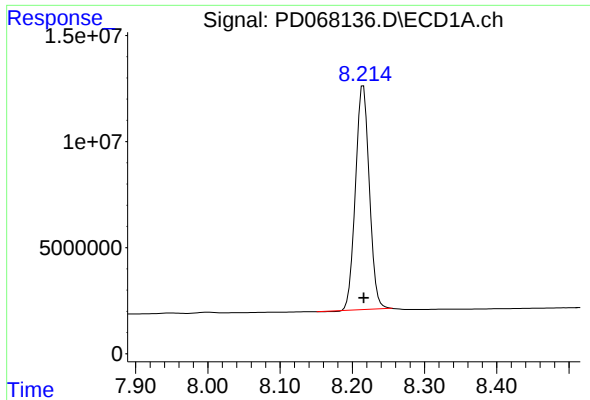

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: 0.000 min
Response: 140778218
Conc: 94.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

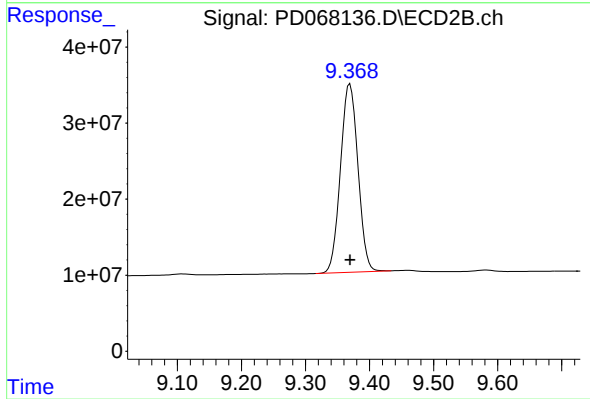

#28 Decachlorobiphenyl

R.T.: 9.369 min
Delta R.T.: 0.000 min
Response: 469508259
Conc: 92.18 ng/ml