

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022222\
 Data File : PD068130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2022 09:31
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 18:11:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 13:16:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.175	31183791	209.5E6	21.421	22.659
28)	SA Decachlor...	8.215	9.369	30278356	109.2E6	21.129	21.945
Target Compounds							
9)	A Endosulfan I	5.505	6.452	18559688	103.3E6	10.353	11.524
10)	B gamma-Chl...	5.392	6.326	20511101	113.5E6	10.313	11.566
12)	B 4,4'-DDE	5.618	6.551	36692385	194.1E6	20.143	21.481
13)	MA Dieldrin	5.749	6.710	39842071	207.2E6	20.088	21.543
19)	B Endosulfa...	6.663	7.484	29142766	133.8E6	18.536	19.581
20)	A Methoxychlor	6.927	7.797	79075364	261.3E6	101.632	96.559
21)	B Endrin ke...	7.156	7.959	35073013	149.1E6	19.629	20.737



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022222\
Data File : PD068130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2022 09:31
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 18:11:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 13:16:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

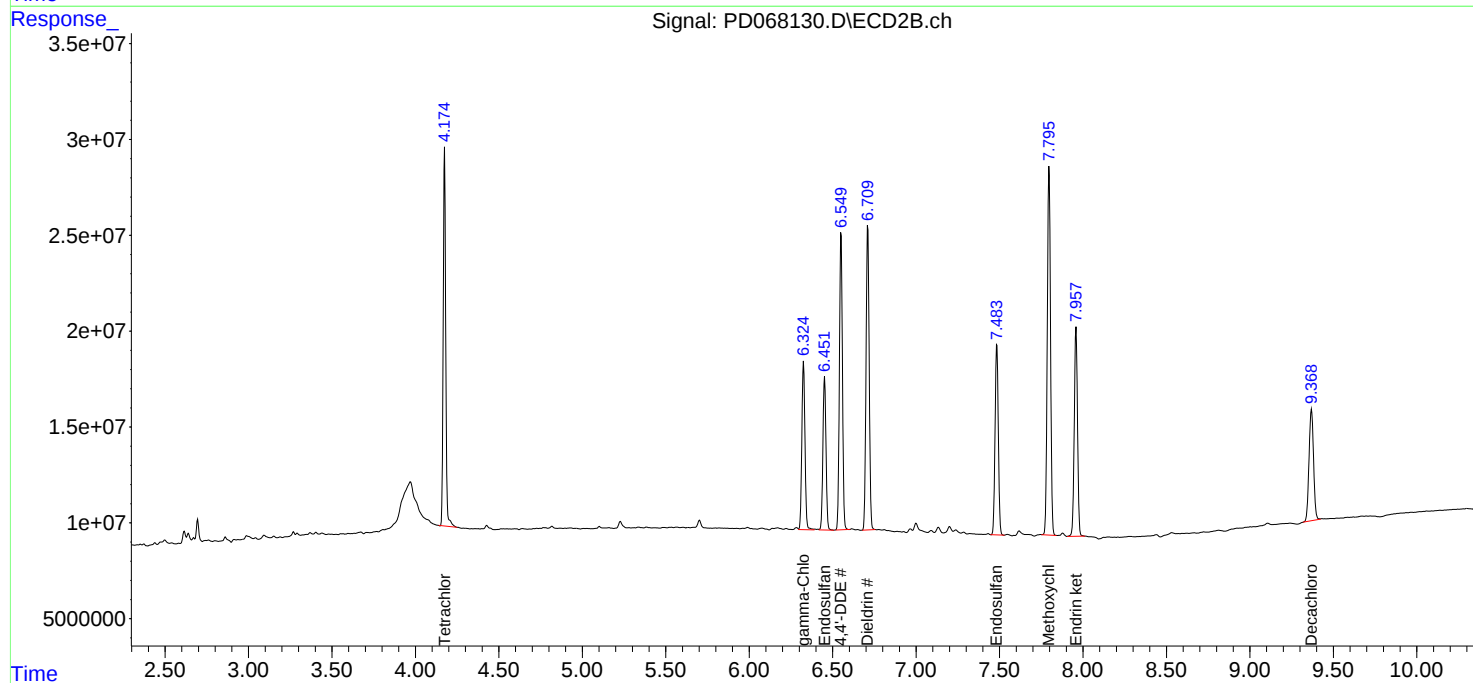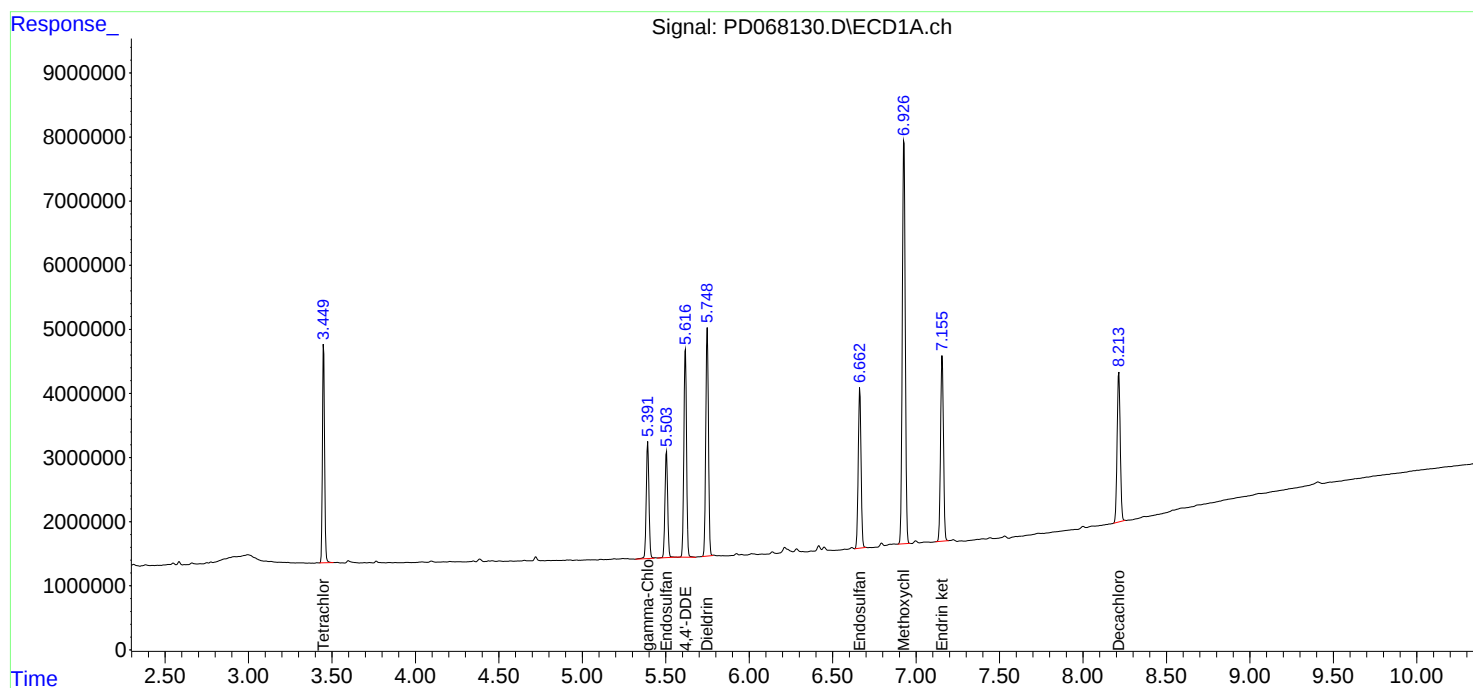


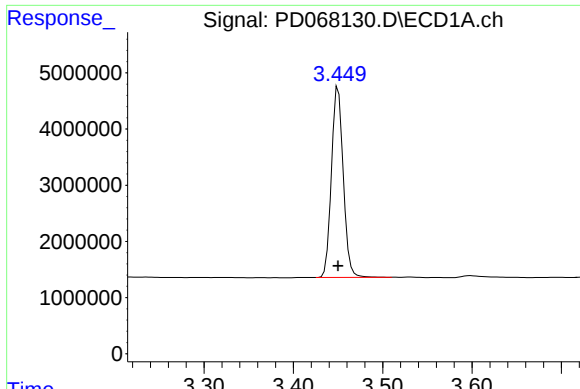

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 31183791
Conc: 21.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

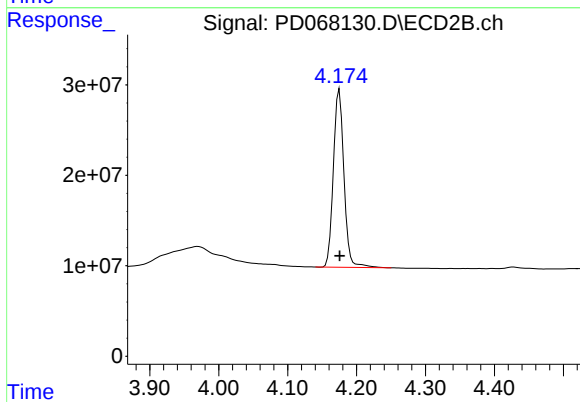


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 209540740
Conc: 22.66 ng/ml

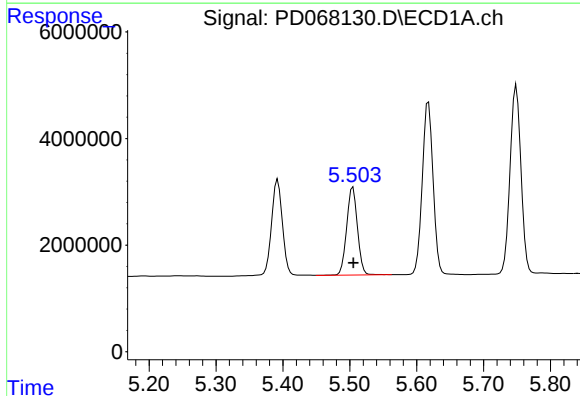


#9 Endosulfan I

R.T.: 5.505 min
Delta R.T.: 0.000 min
Response: 18559688
Conc: 10.35 ng/ml

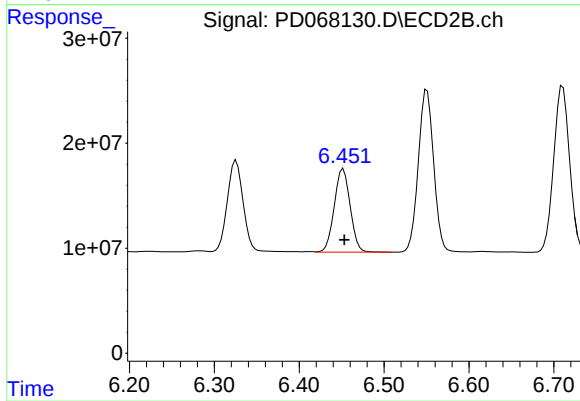

#9 Endosulfan I


R.T.: 6.452 min
Delta R.T.: -0.001 min
Response: 103322560
Conc: 11.52 ng/ml

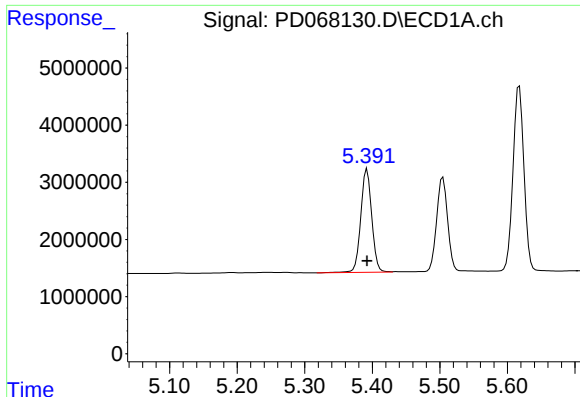

#10 gamma-Chlordane


R.T.: 5.392 min
Delta R.T.: 0.000 min
Response: 20511101
Conc: 10.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

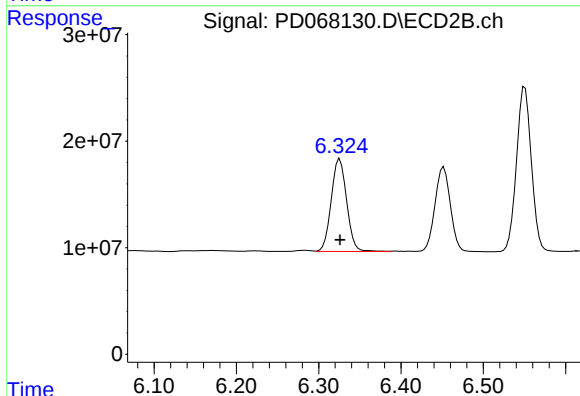


#10 gamma-Chlordane

R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 113472267
Conc: 11.57 ng/ml

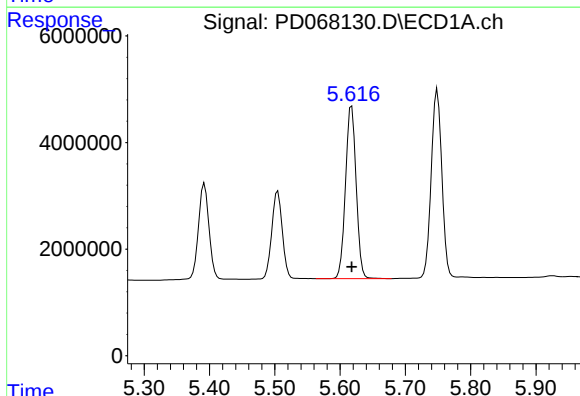


#12 4,4'-DDE

R.T.: 5.618 min
Delta R.T.: 0.000 min
Response: 36692385
Conc: 20.14 ng/ml

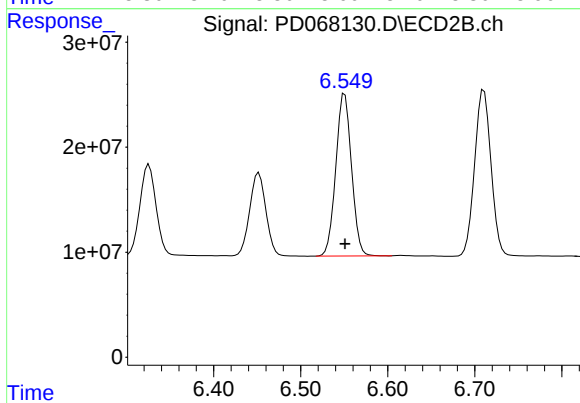

#12 4,4'-DDE


R.T.: 6.551 min
Delta R.T.: 0.000 min
Response: 194060572
Conc: 21.48 ng/ml

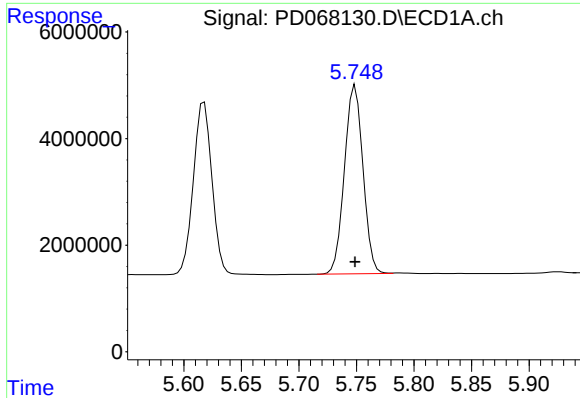

#13 Dieldrin


R.T.: 5.749 min
Delta R.T.: 0.000 min
Response: 39842071
Conc: 20.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

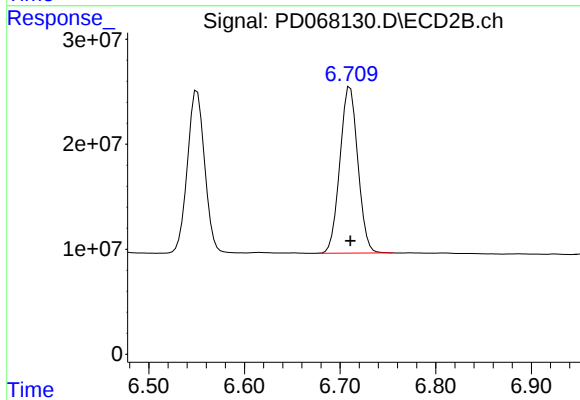


#13 Dieldrin

R.T.: 6.710 min
Delta R.T.: 0.000 min
Response: 207180462
Conc: 21.54 ng/ml

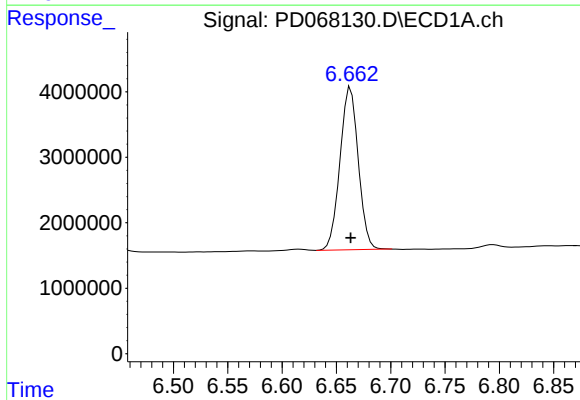


#19 Endosulfan Sulfate

R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 29142766
Conc: 18.54 ng/ml

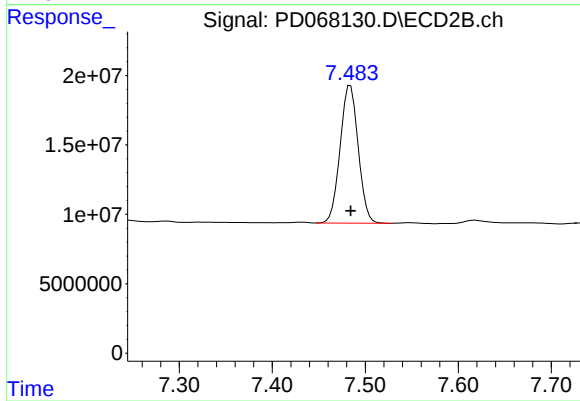

#19 Endosulfan Sulfate


R.T.: 7.484 min
Delta R.T.: 0.000 min
Response: 133802034
Conc: 19.58 ng/ml

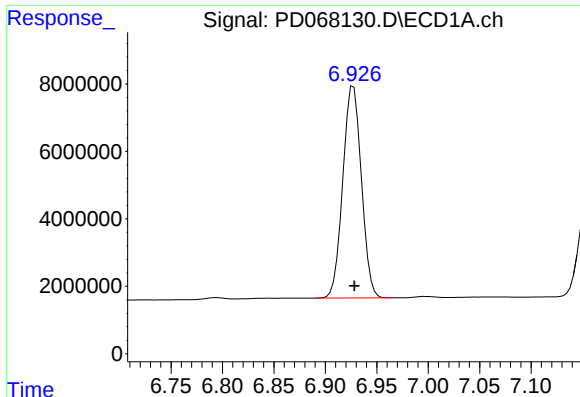

#20 Methoxychlor


R.T.: 6.927 min
Delta R.T.: 0.000 min
Response: 79075364
Conc: 101.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

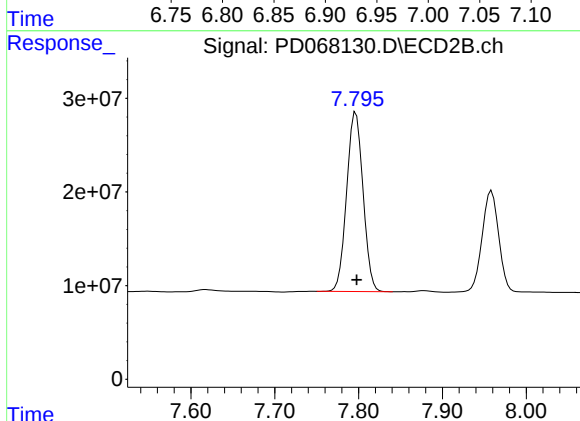


#20 Methoxychlor

R.T.: 7.797 min
Delta R.T.: 0.000 min
Response: 261329048
Conc: 96.56 ng/ml

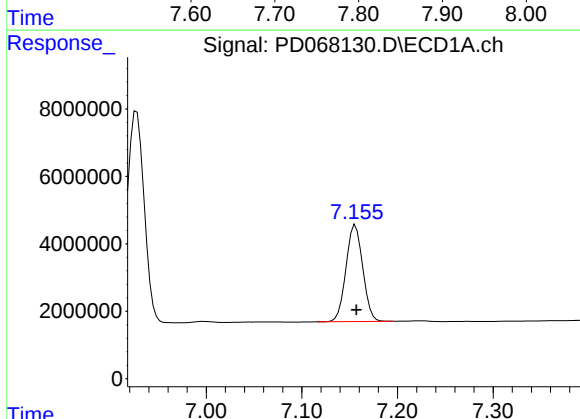


#21 Endrin ketone

R.T.: 7.156 min
Delta R.T.: 0.000 min
Response: 35073013
Conc: 19.63 ng/ml

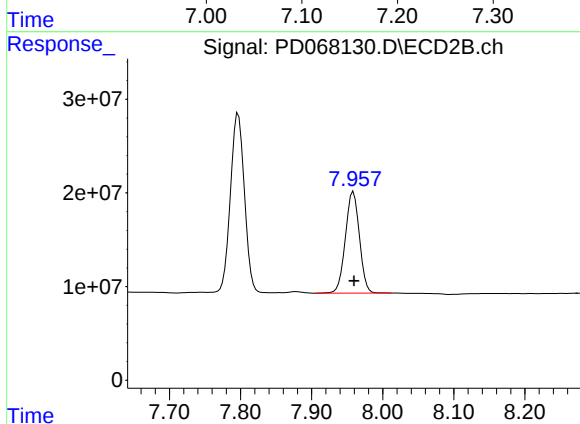

#21 Endrin ketone


R.T.: 7.959 min
Delta R.T.: 0.000 min
Response: 149054301
Conc: 20.74 ng/ml

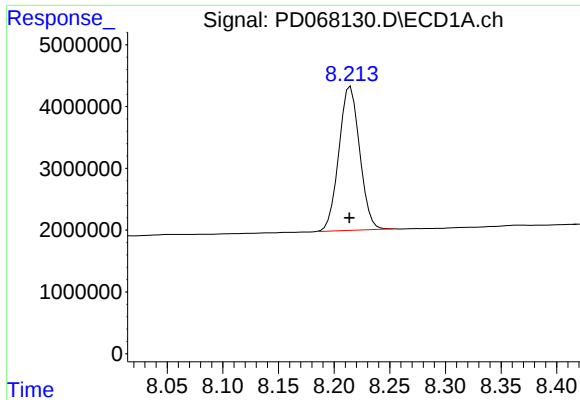

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: 0.001 min
Response: 30278356
Conc: 21.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

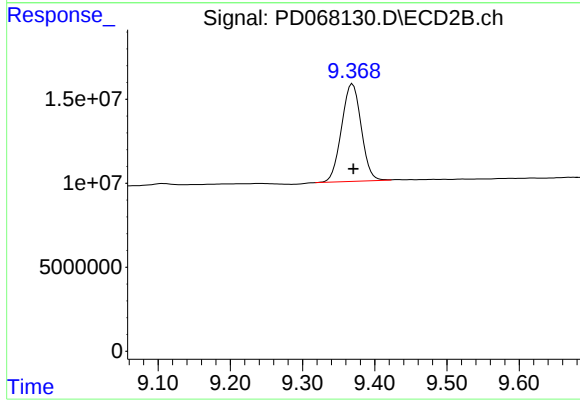

#28 Decachlorobiphenyl

R.T.: 9.369 min
Delta R.T.: 0.000 min
Response: 109247438
Conc: 21.95 ng/ml