

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022222\
 Data File : PD068137.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2022 11:16
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 13:05:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 13:00:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.175	130.7E6	674.9E6	74.541	72.967
28)	SA Decachlor...	8.216	9.369	109.1E6	371.4E6	73.296	72.921
Target Compounds							
23)	Chlordane-1	4.321	5.198	45604408	298.5E6	742.494	729.517
24)	Chlordane-2	4.824	5.671	50137873	286.2E6	709.328	715.718
25)	Chlordane-3	5.393	6.326	160.0E6	1047.1E6	742.095	735.150
26)	Chlordane-4	5.451	6.404	133.5E6	1190.4E6	736.867	733.531
27)	Chlordane-5	6.289	7.215	51281475	197.3E6	735.888	733.800



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022222\
Data File : PD068137.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2022 11:16
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 13:05:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 13:00:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

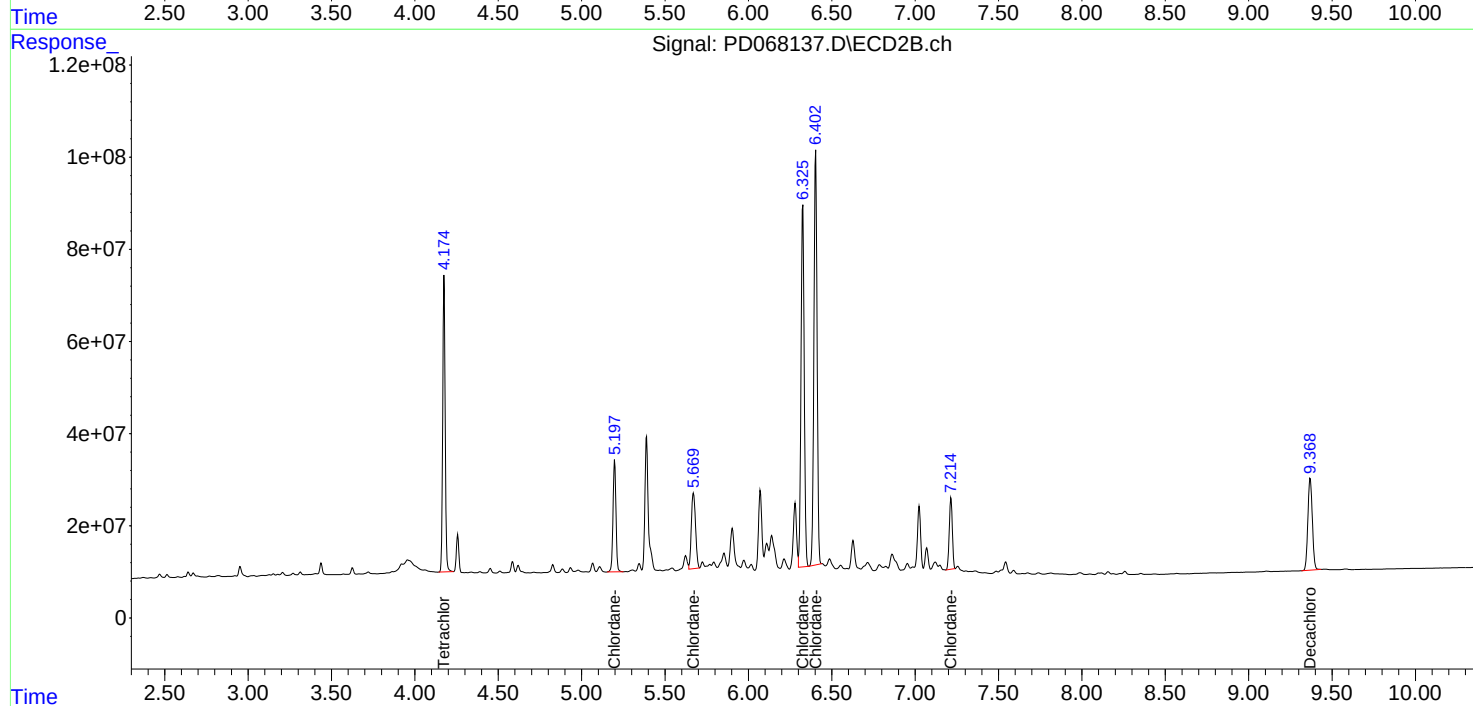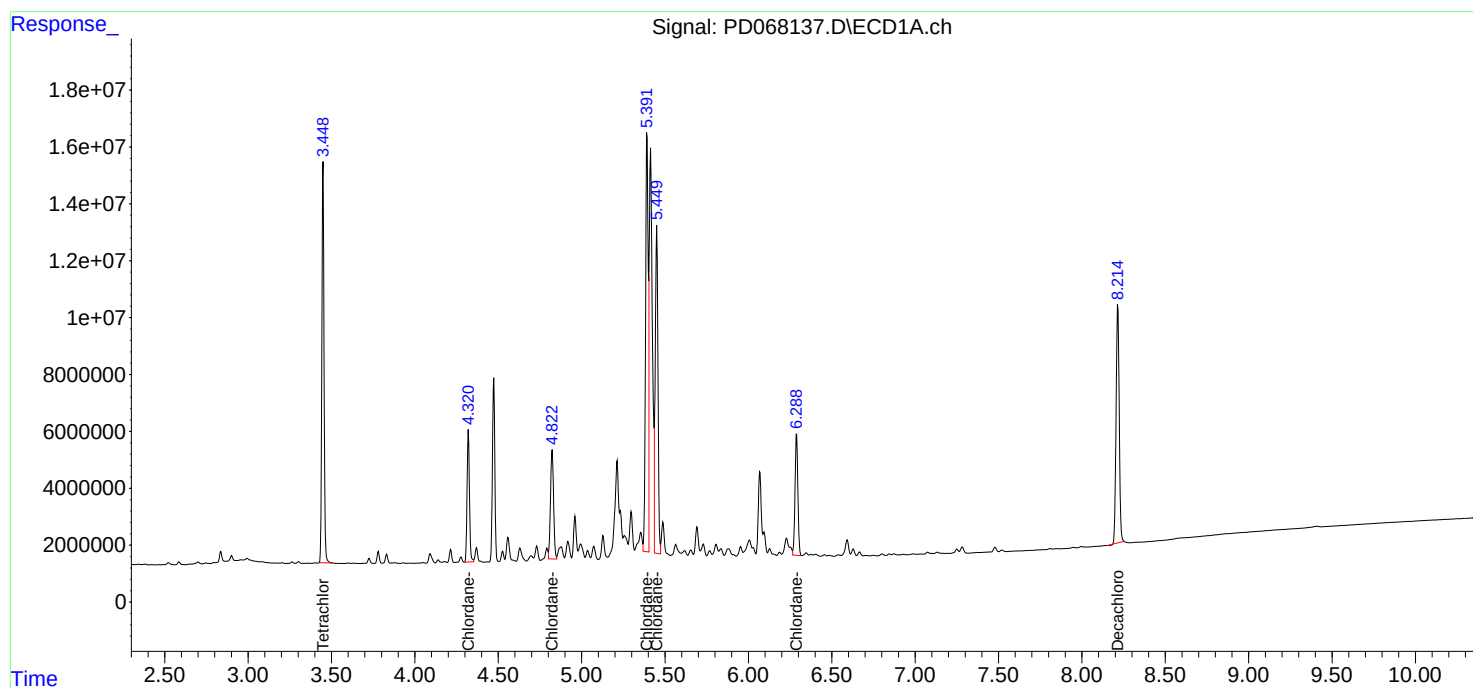


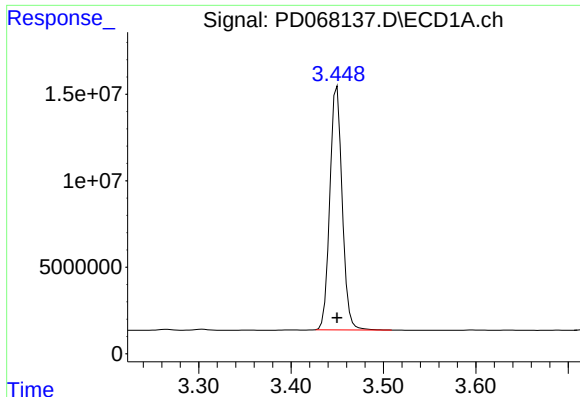

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 130656657
Conc: 74.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

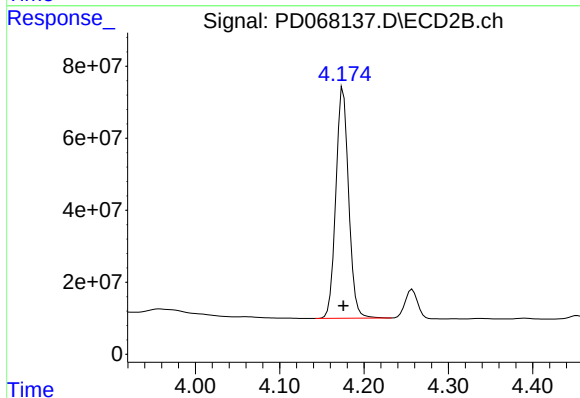


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 674935949
Conc: 72.97 ng/ml

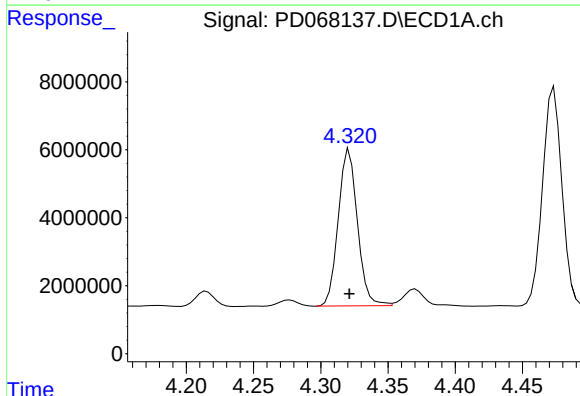


#23 Chlordane-1

R.T.: 4.321 min
Delta R.T.: 0.000 min
Response: 45604408
Conc: 742.49 ng/ml

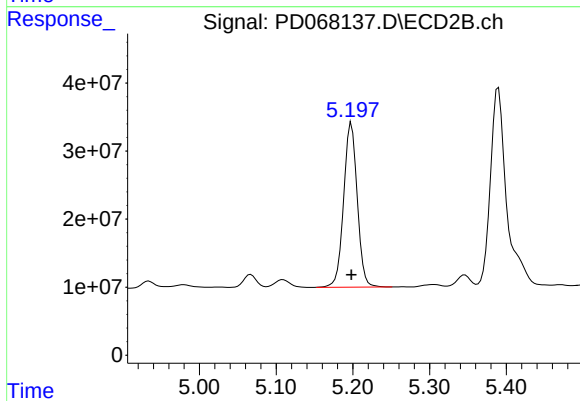

#23 Chlordane-1


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 298481904
Conc: 729.52 ng/ml

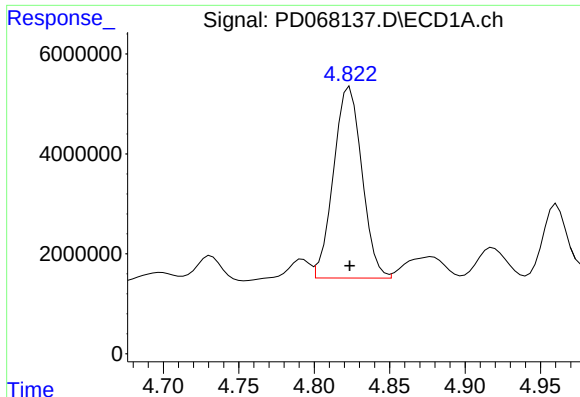

#24 Chlordane-2


R.T.: 4.824 min
Delta R.T.: 0.000 min
Response: 50137873
Conc: 709.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

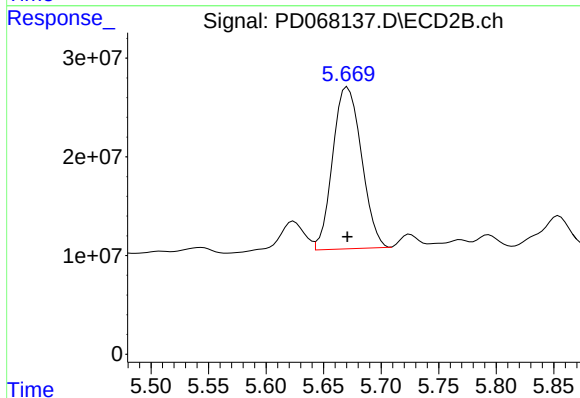


#24 Chlordane-2

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 286194308
Conc: 715.72 ng/ml

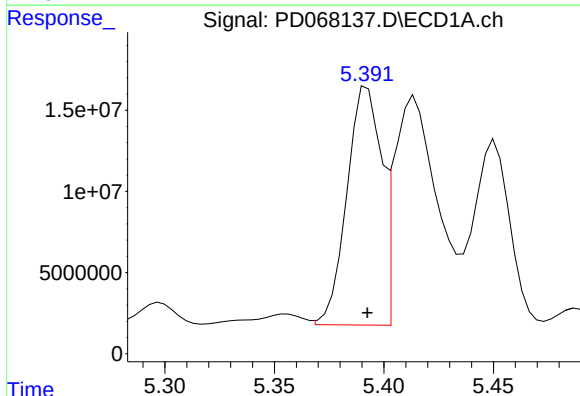


#25 Chlordane-3

R.T.: 5.393 min
Delta R.T.: 0.000 min
Response: 159971830
Conc: 742.09 ng/ml

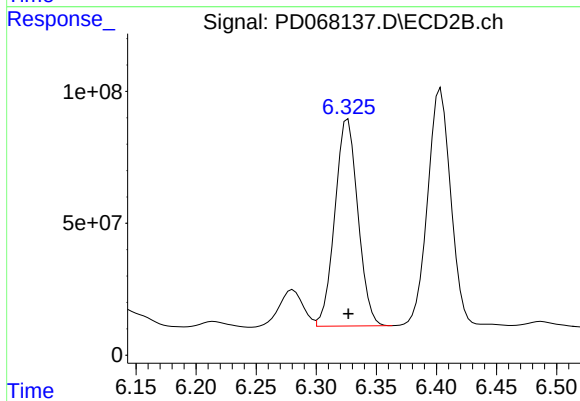

#25 Chlordane-3


R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 1047137226
Conc: 735.15 ng/ml

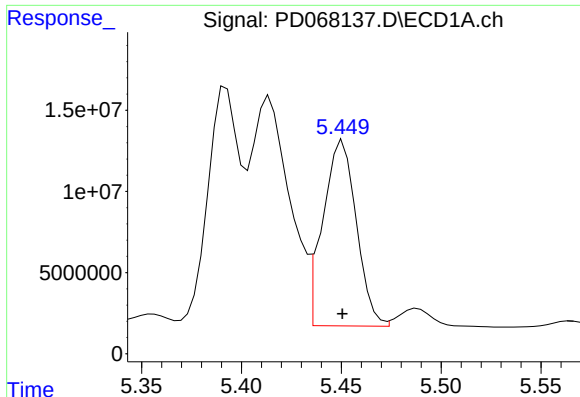

#26 Chlordane-4


R.T.: 5.451 min
Delta R.T.: 0.000 min
Response: 133519328
Conc: 736.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

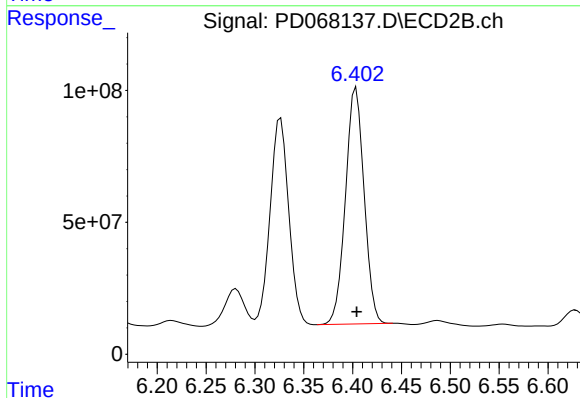


#26 Chlordane-4

R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 1190439973
Conc: 733.53 ng/ml

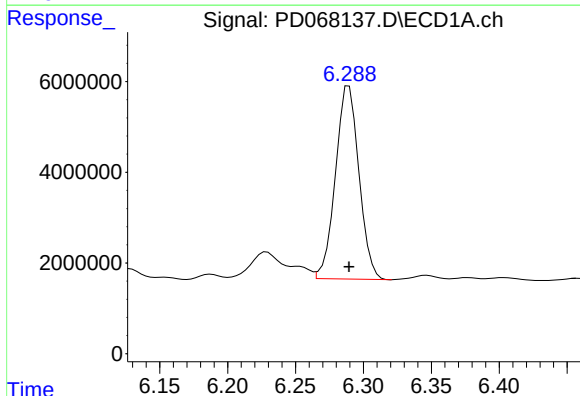


#27 Chlordane-5

R.T.: 6.289 min
Delta R.T.: 0.000 min
Response: 51281475
Conc: 735.89 ng/ml

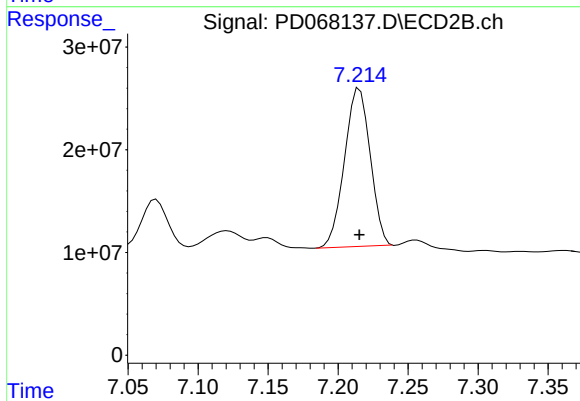

#27 Chlordane-5

R.T.: 7.215 min
Delta R.T.: 0.000 min
Response: 197329195
Conc: 733.80 ng/ml

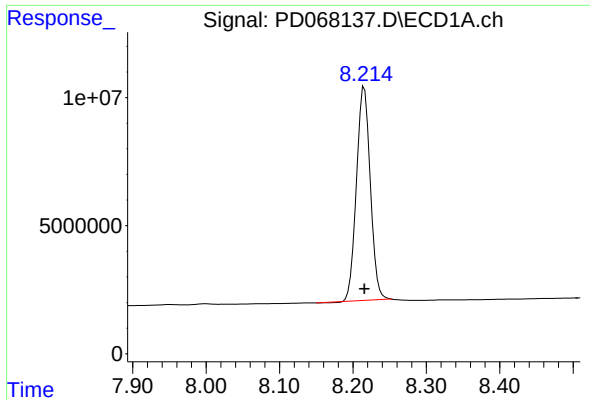

#28 Decachlorobiphenyl


R.T.: 8.216 min

Delta R.T.: 0.000 min

Response: 109140115

Conc: 73.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

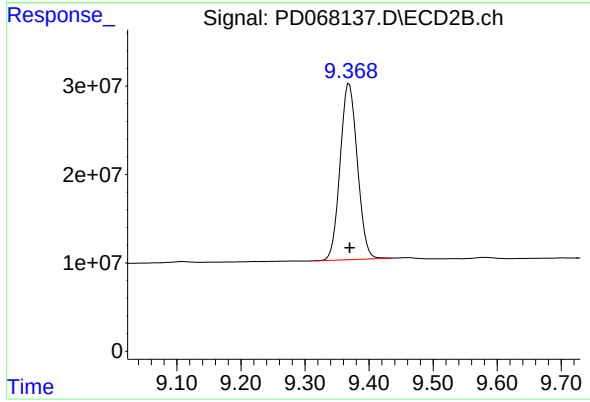

#28 Decachlorobiphenyl

R.T.: 9.369 min

Delta R.T.: 0.000 min

Response: 371417479

Conc: 72.92 ng/ml