

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022222\
 Data File : PD068139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2022 11:44
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 13:05:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 13:00:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.175	40617428	238.2E6	23.173	25.747
28)	SA Decachlor...	8.215	9.370	36904663	131.1E6	24.784	25.733
Target Compounds							
23)	Chlordane-1	4.321	5.197	14768894	105.8E6	240.455	258.554
24)	Chlordane-2	4.824	5.670	17750134	105.6E6	251.121	264.021
25)	Chlordane-3	5.392	6.326	49523698	361.5E6	229.736	253.817
26)	Chlordane-4	5.451	6.403	41731742	416.1E6	230.309	256.397
27)	Chlordane-5	6.289	7.214	15824250	67787969	227.077	252.080



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022222\
Data File : PD068139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2022 11:44
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 13:05:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 13:00:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

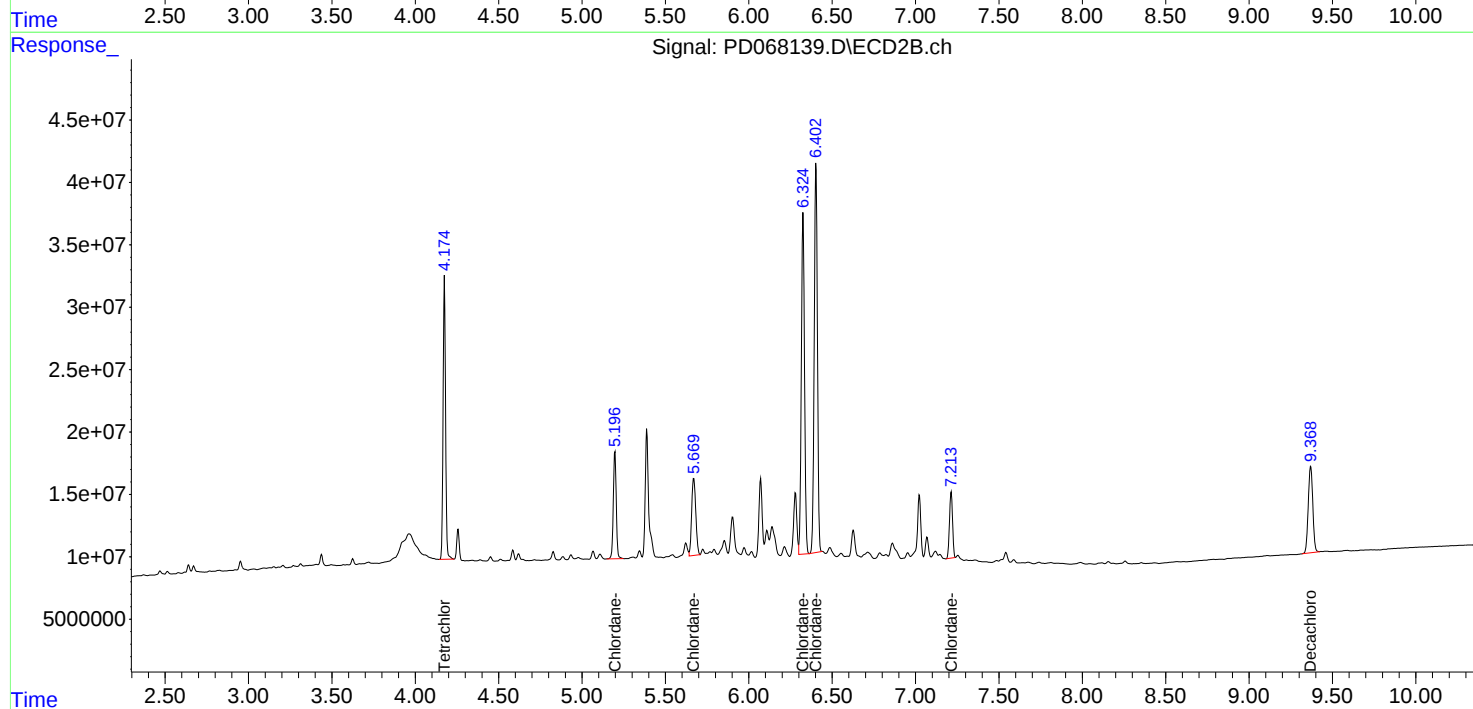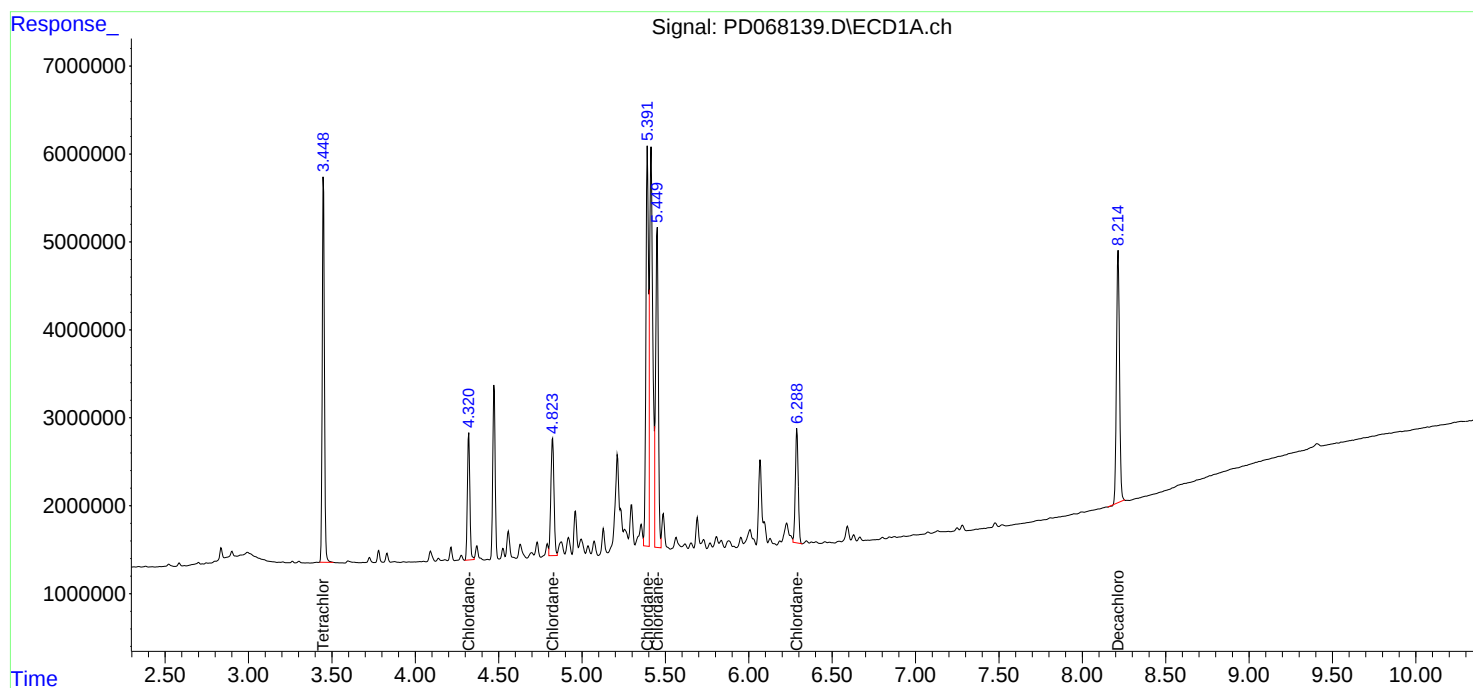


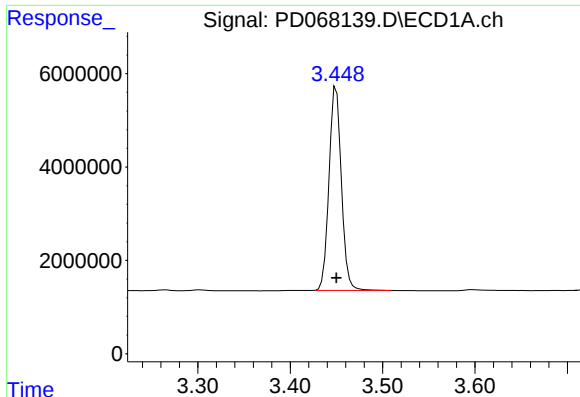

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 40617428
Conc: 23.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

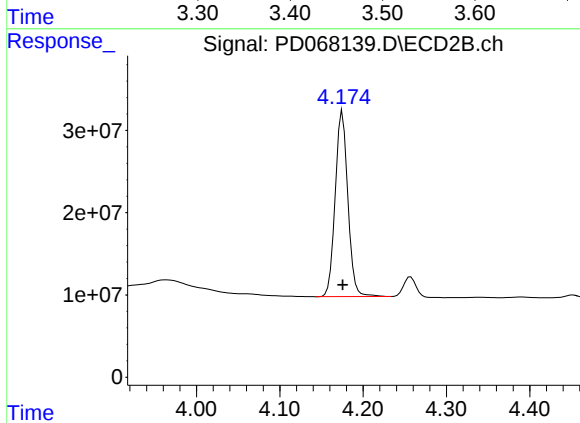


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 238155652
Conc: 25.75 ng/ml

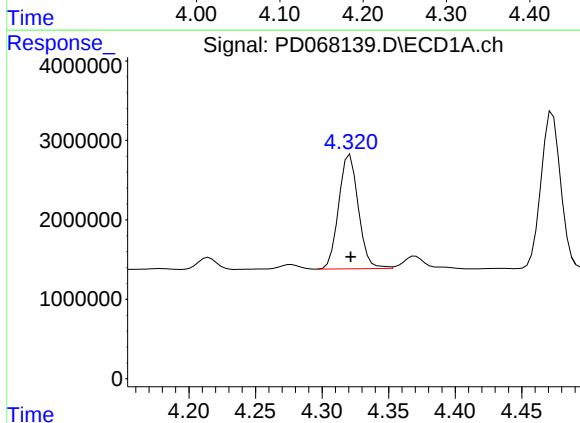


#23 Chlordane-1

R.T.: 4.321 min
Delta R.T.: 0.000 min
Response: 14768894
Conc: 240.46 ng/ml

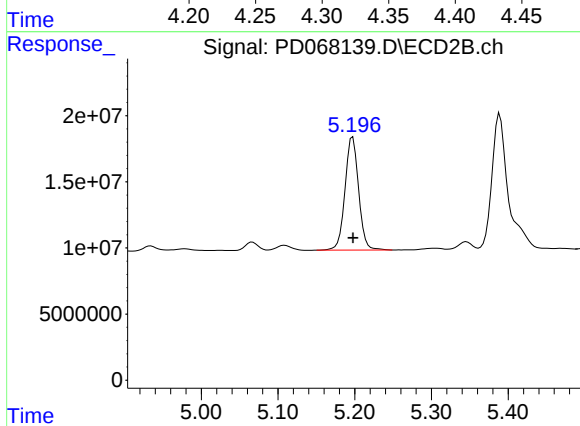

#23 Chlordane-1


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 105787417
Conc: 258.55 ng/ml

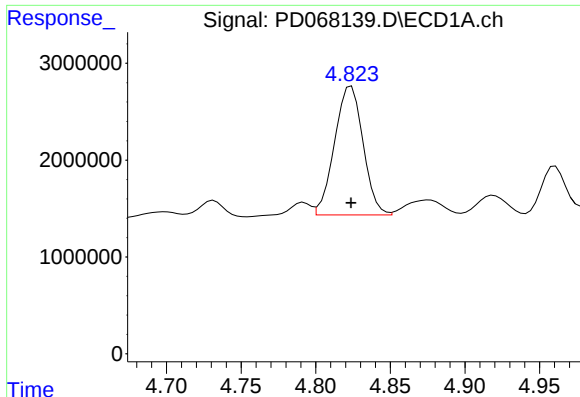

#24 Chlordane-2


R.T.: 4.824 min
Delta R.T.: 0.000 min
Response: 17750134
Conc: 251.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

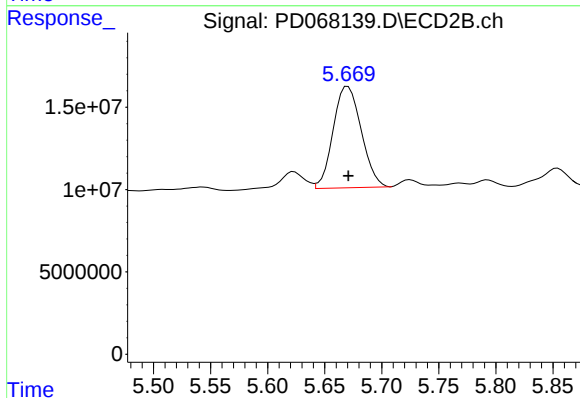


#24 Chlordane-2

R.T.: 5.670 min
Delta R.T.: 0.000 min
Response: 105574171
Conc: 264.02 ng/ml

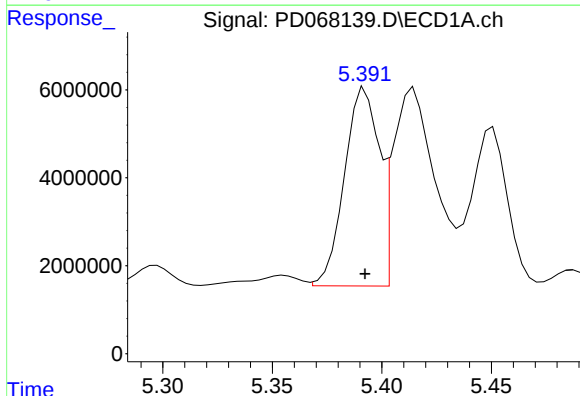


#25 Chlordane-3

R.T.: 5.392 min
Delta R.T.: 0.000 min
Response: 49523698
Conc: 229.74 ng/ml

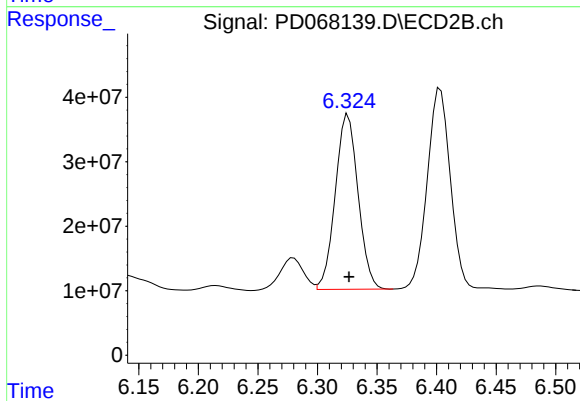

#25 Chlordane-3


R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 361533272
Conc: 253.82 ng/ml

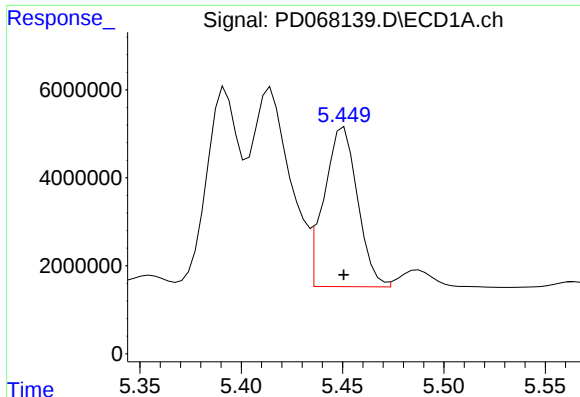

#26 Chlordane-4


R.T.: 5.451 min
Delta R.T.: 0.000 min
Response: 41731742
Conc: 230.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

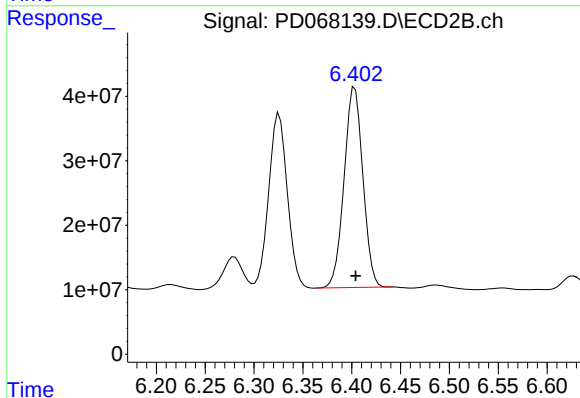


#26 Chlordane-4

R.T.: 6.403 min
Delta R.T.: -0.001 min
Response: 416103581
Conc: 256.40 ng/ml

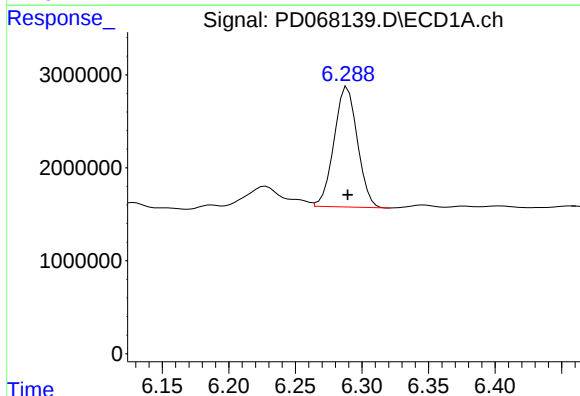


#27 Chlordane-5

R.T.: 6.289 min
Delta R.T.: 0.000 min
Response: 15824250
Conc: 227.08 ng/ml

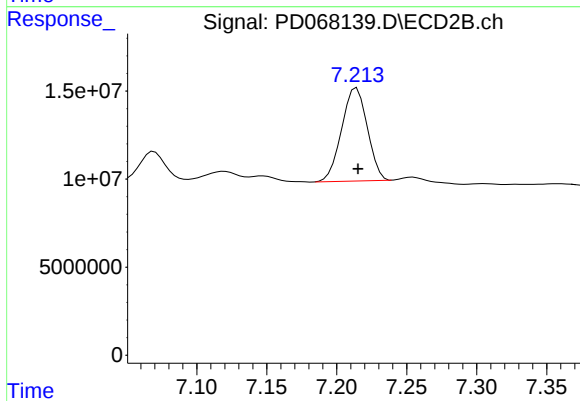

#27 Chlordane-5


R.T.: 7.214 min
Delta R.T.: 0.000 min
Response: 67787969
Conc: 252.08 ng/ml

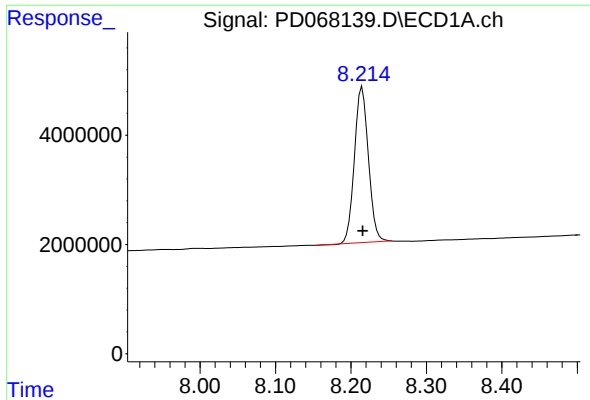

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: 0.000 min
Response: 36904663
Conc: 24.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

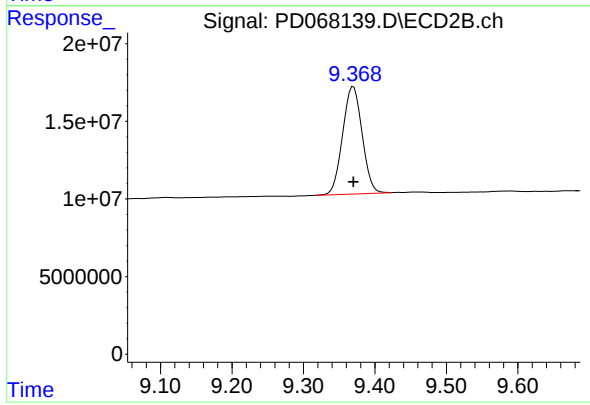

#28 Decachlorobiphenyl

R.T.: 9.370 min
Delta R.T.: 0.000 min
Response: 131067746
Conc: 25.73 ng/ml