

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022222\
 Data File : PD068147.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2022 13:36
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD022222CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 17:45:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 13:16:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	4.177	83060361	449.6E6	57.055	48.613
28)	SA Decachlor...	8.216	9.372	73143602	253.5E6	51.042	50.922
Target Compounds							
23)	Chlordane-1	4.322	5.199	29634500	201.6E6	488.361	481.649
24)	Chlordane-2	4.824	5.672	34128925	198.4E6	485.093	481.131
25)	Chlordane-3	5.394	6.328	104.8E6	716.8E6	503.168	493.841
26)	Chlordane-4	5.452	6.405	86493219	827.2E6	491.827	496.242
27)	Chlordane-5	6.290	7.217	33439168	140.3E6	506.493	522.049



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022222\
Data File : PD068147.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2022 13:36
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD022222CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 17:45:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 13:16:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

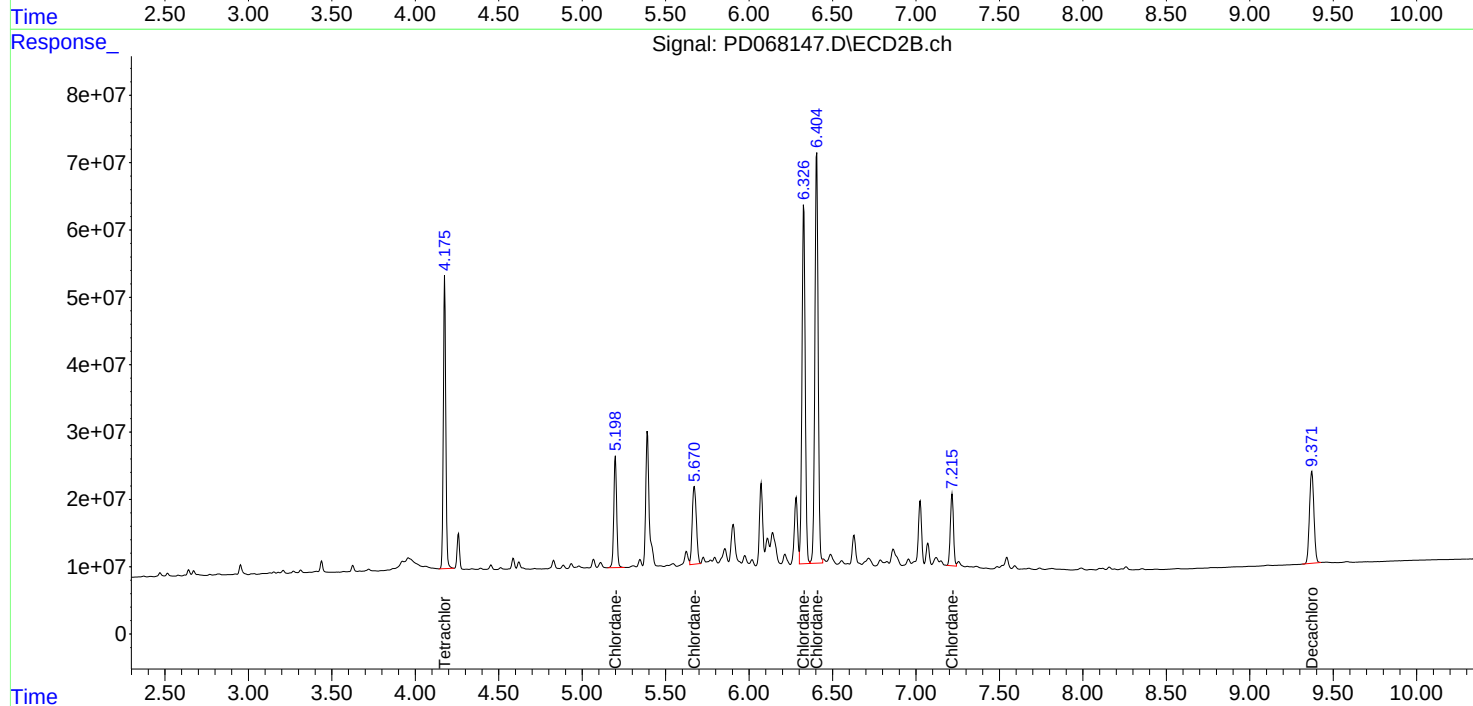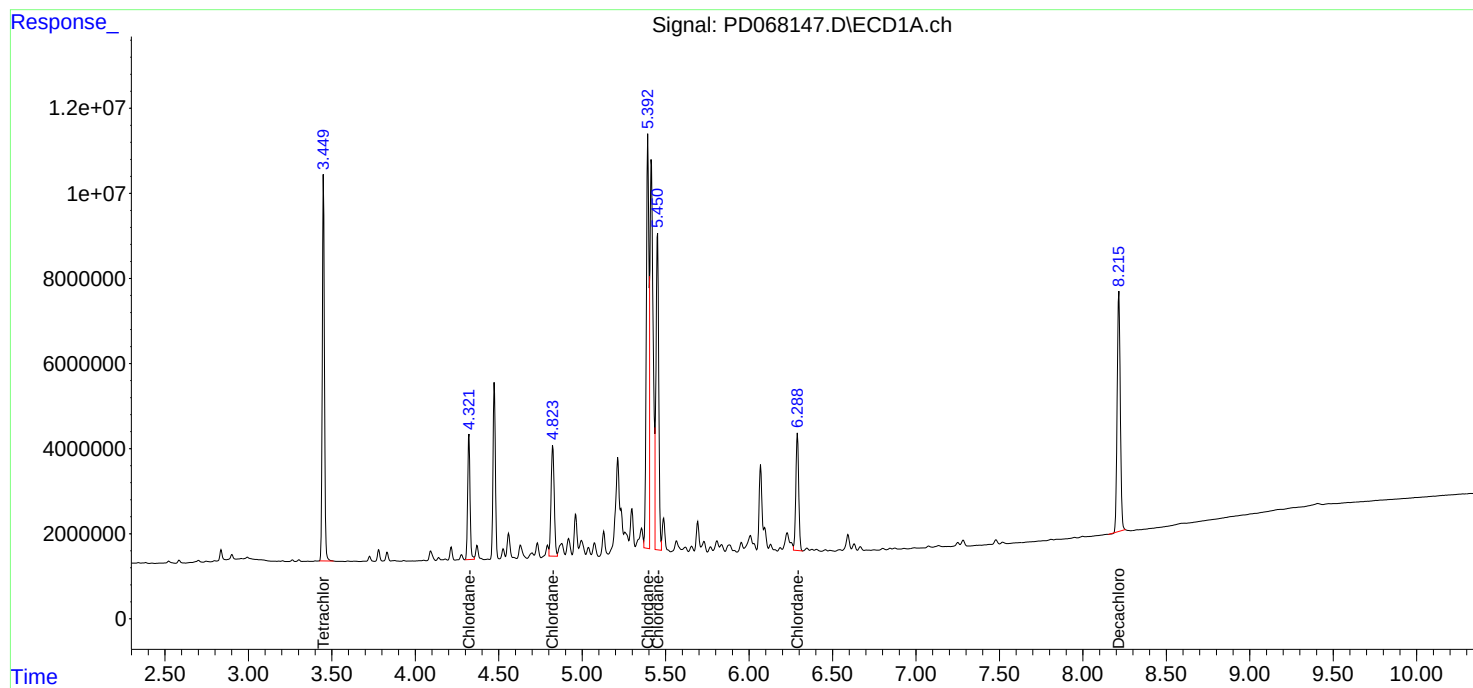


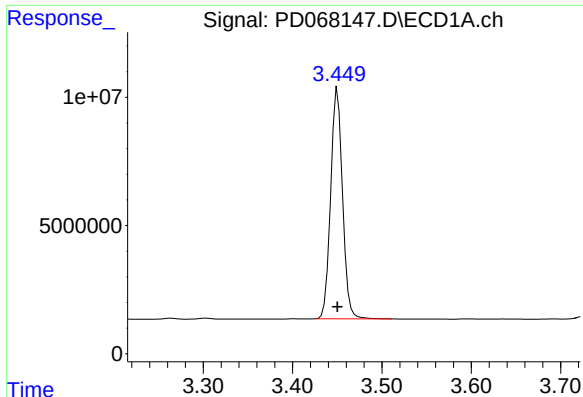

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 83060361
Conc: 57.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD022222CHLOR

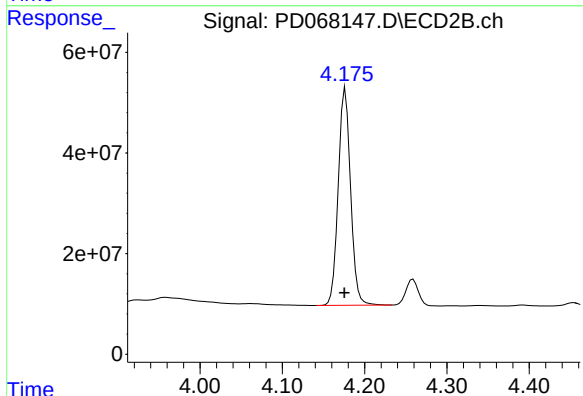


#1 Tetrachloro-m-xylene

R.T.: 4.177 min
Delta R.T.: 0.001 min
Response: 449552881
Conc: 48.61 ng/ml

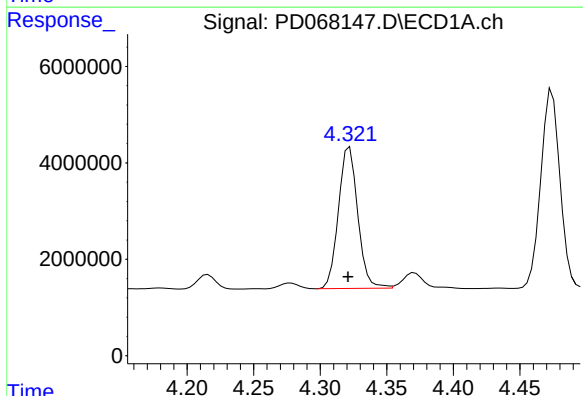


#23 Chlordane-1

R.T.: 4.322 min
Delta R.T.: 0.001 min
Response: 29634500
Conc: 488.36 ng/ml

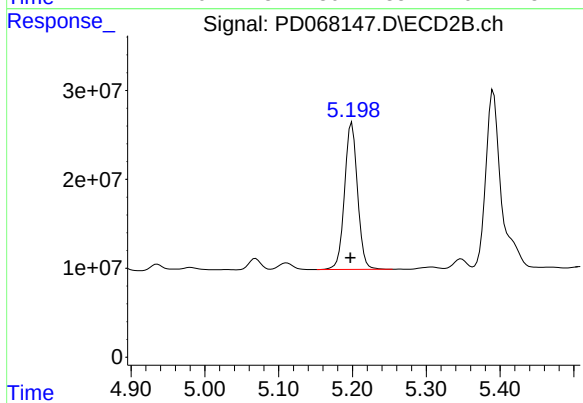

#23 Chlordane-1


R.T.: 5.199 min
Delta R.T.: 0.002 min
Response: 201634614
Conc: 481.65 ng/ml

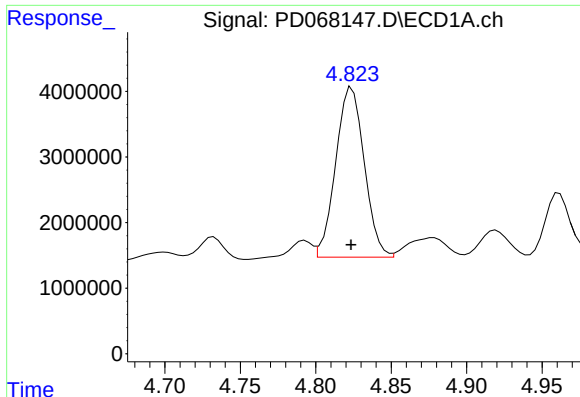

#24 Chlordane-2


R.T.: 4.824 min
Delta R.T.: 0.000 min
Response: 34128925
Conc: 485.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD022222CHLOR

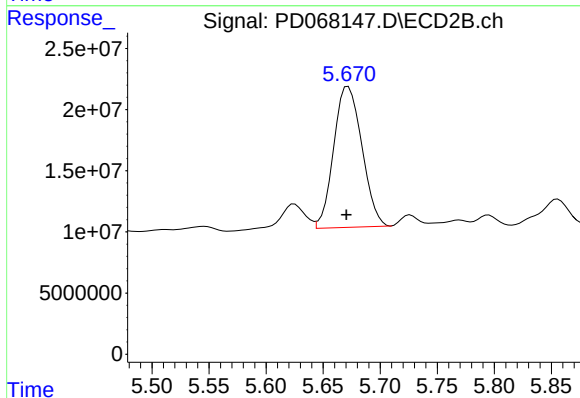


#24 Chlordane-2

R.T.: 5.672 min
Delta R.T.: 0.001 min
Response: 198397377
Conc: 481.13 ng/ml

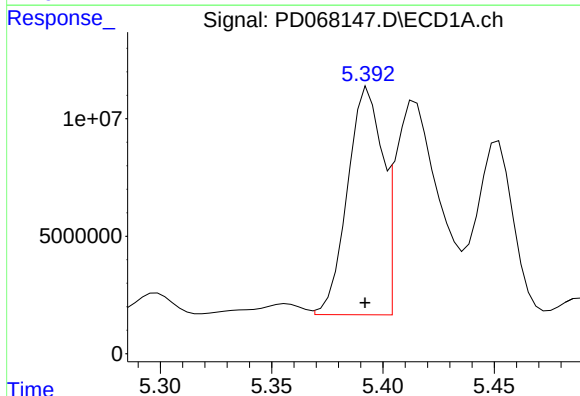


#25 Chlordane-3

R.T.: 5.394 min
Delta R.T.: 0.002 min
Response: 104847679
Conc: 503.17 ng/ml

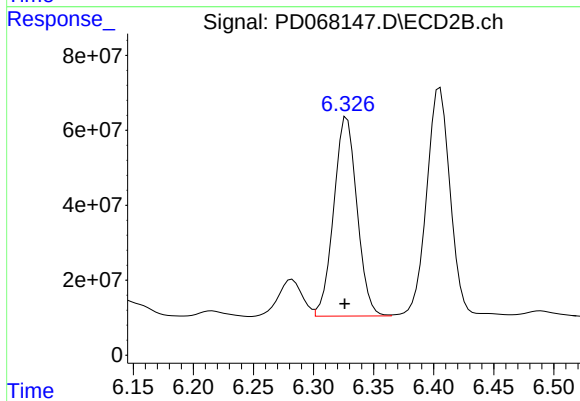

#25 Chlordane-3


R.T.: 6.328 min
Delta R.T.: 0.002 min
Response: 716825358
Conc: 493.84 ng/ml

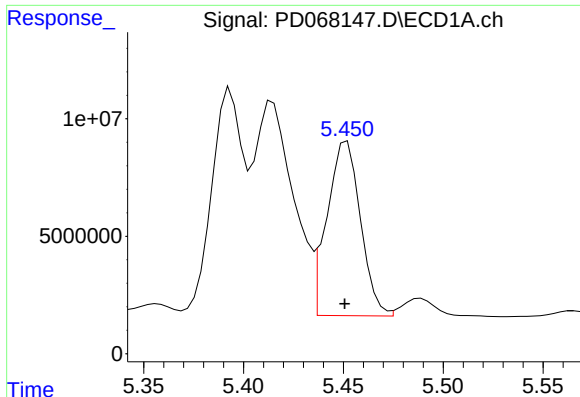

#26 Chlordane-4


R.T.: 5.452 min
Delta R.T.: 0.001 min
Response: 86493219
Conc: 491.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD022222CHLOR

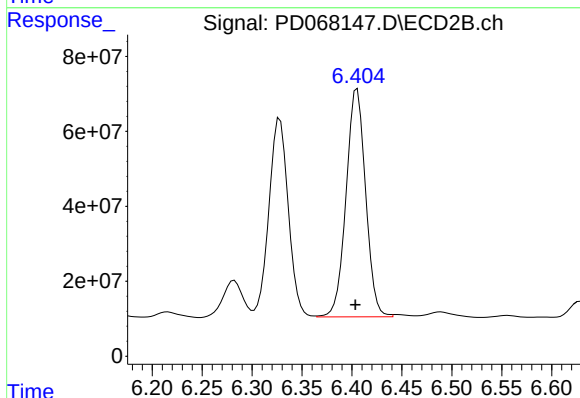


#26 Chlordane-4

R.T.: 6.405 min
Delta R.T.: 0.002 min
Response: 827184894
Conc: 496.24 ng/ml

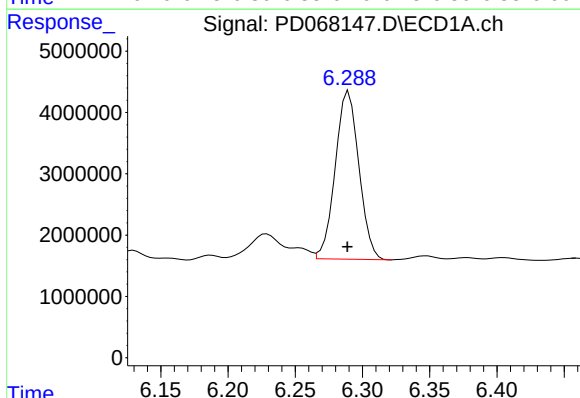


#27 Chlordane-5

R.T.: 6.290 min
Delta R.T.: 0.001 min
Response: 33439168
Conc: 506.49 ng/ml

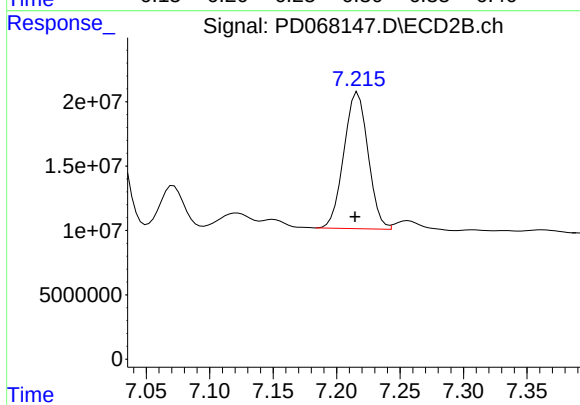

#27 Chlordane-5


R.T.: 7.217 min
Delta R.T.: 0.002 min
Response: 140348510
Conc: 522.05 ng/ml

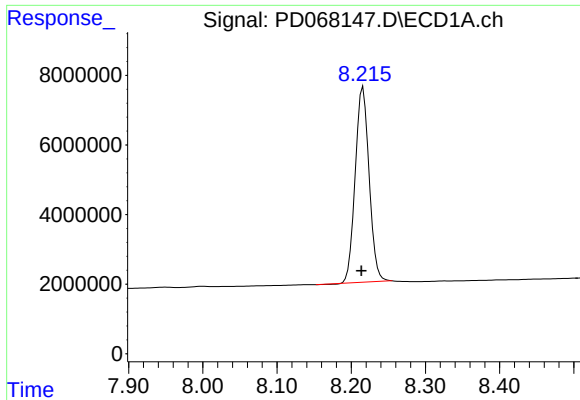

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: 0.002 min
Response: 73143602
Conc: 51.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD022222CHLOR

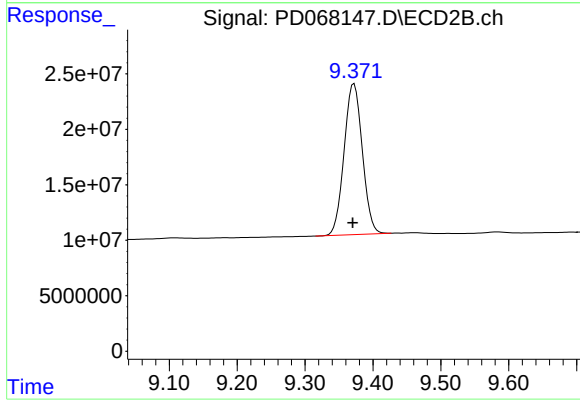

#28 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: 0.002 min
Response: 253500567
Conc: 50.92 ng/ml