

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022223\
 Data File : PD074026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2023 10:41
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 05:49:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022223CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 13 05:44:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	9.094	7.928	340266	190193	0.129	0.155
Target Compounds							
3)	MA gamma-BHC...	4.293f	0.000	91550	0	<MDL	N.D. #
5)	MB Aldrin	0.000	4.208	0	524027	N.D.	0.309
8)	B Heptachlo...	5.698	0.000	5296346	0	1.746	N.D. #
9)	A Endosulfan I	6.122	0.000	719324	0	0.243	N.D. #
12)	B 4,4'-DDE	6.273f	0.000	171055	0	<MDL	N.D. #
14)	MA Endrin	0.000	5.663	0	400826	N.D.	0.303
15)	B Endosulfa...	6.839	5.890f	655921	448355	0.225	0.327 #
17)	MA 4,4'-DDT	7.073	0.000	738986	0	0.274	N.D. #
21)	B Endrin ke...	7.697	6.811f	141121	-28760	<MDL	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022223\
Data File : PD074026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2023 10:41
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 05:49:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022223CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 13 05:44:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

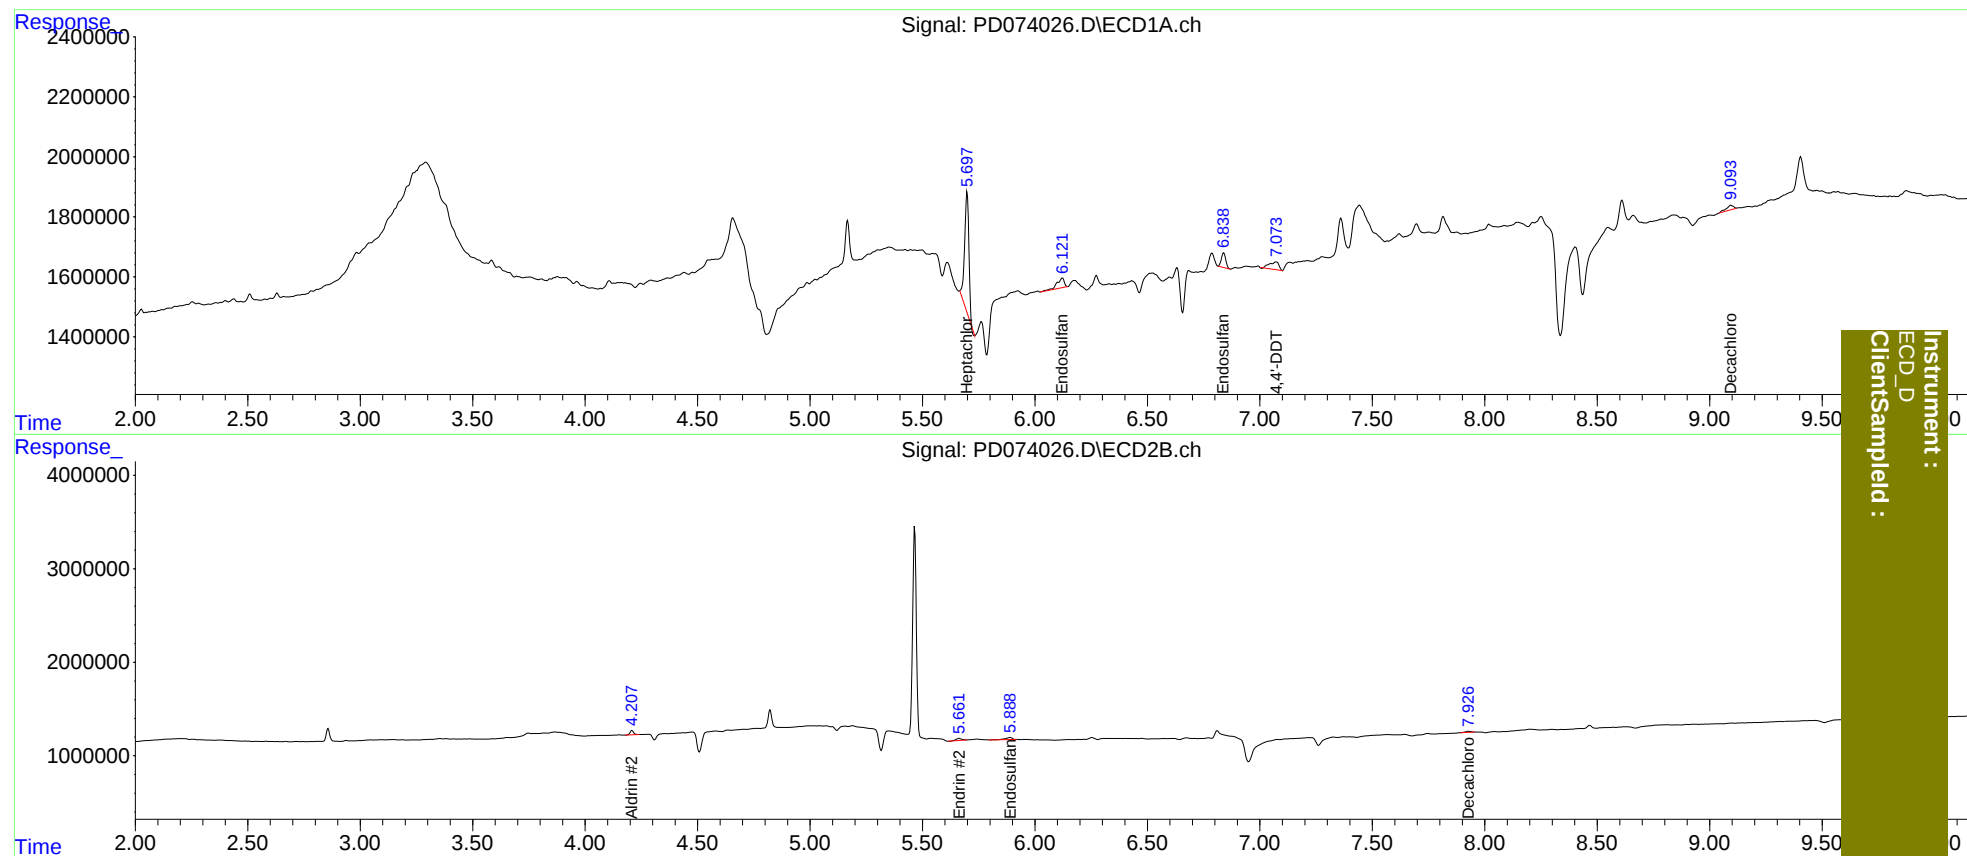


Instrument :
ECD_D
ClientSampled :
0

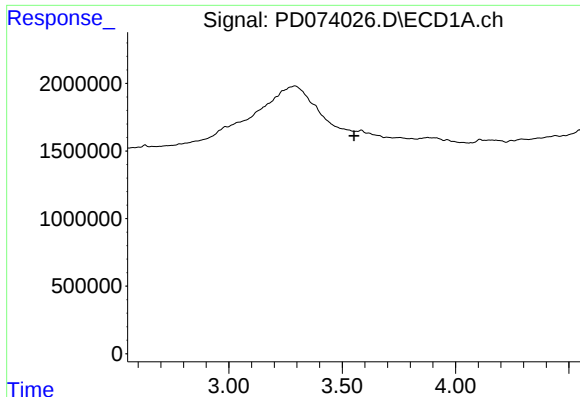

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.552 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

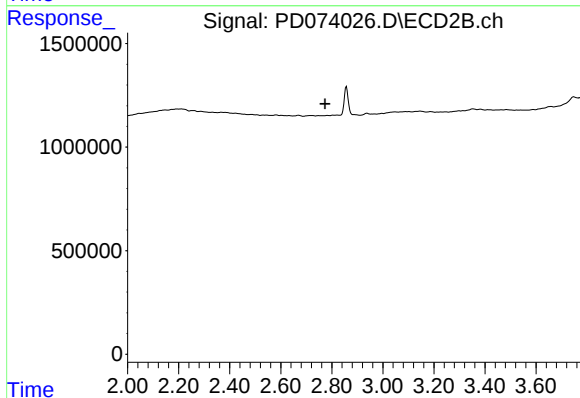


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.774 min
Response: 0
Conc: N.D.

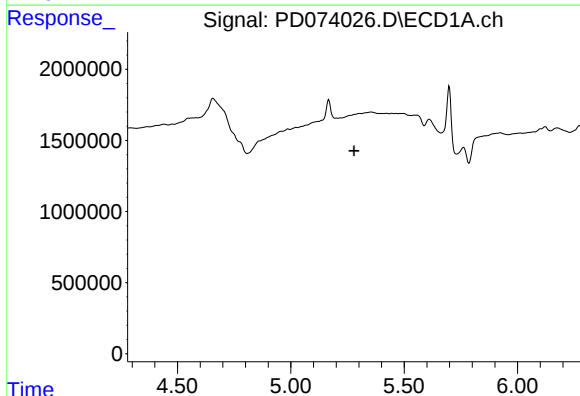


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.279 min
Response: 0
Conc: N.D.

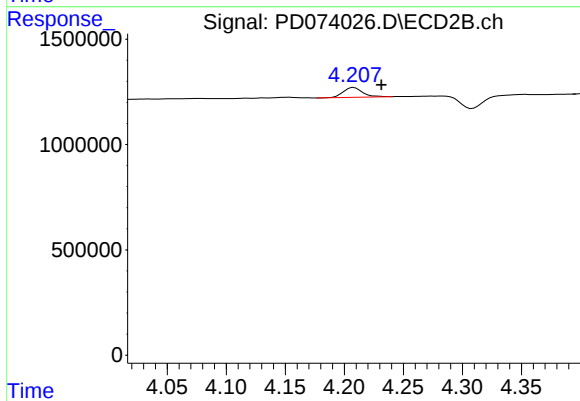

#5 Aldrin


R.T.: 4.208 min
Delta R.T.: -0.023 min
Response: 524027
Conc: 0.31 ng/ml

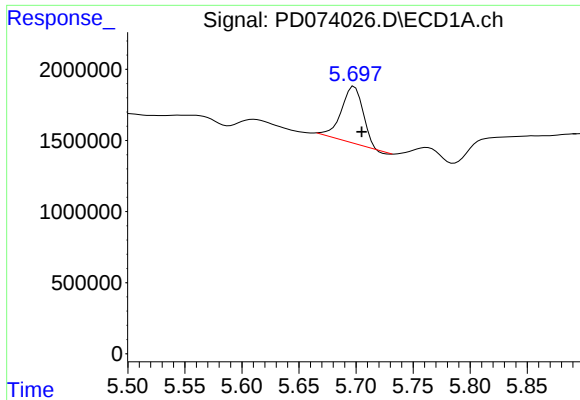

#8 Heptachlor epoxide


R.T.: 5.698 min
Delta R.T.: -0.007 min
Response: 5296346
Conc: 1.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

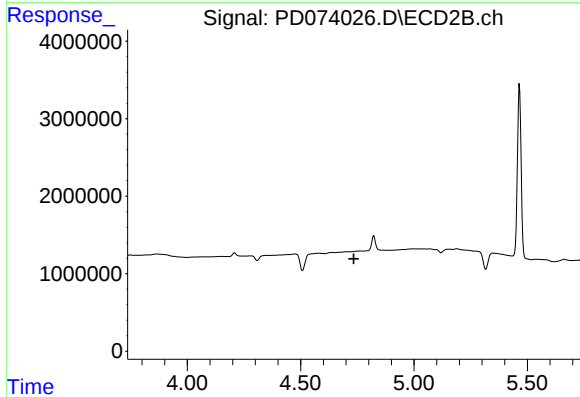


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

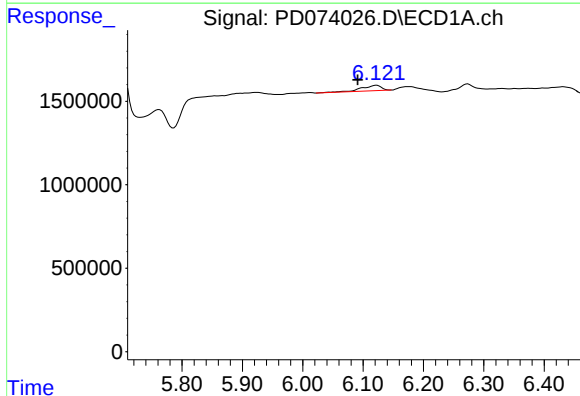


#9 Endosulfan I

R.T.: 6.122 min
Delta R.T.: 0.031 min
Response: 719324
Conc: 0.24 ng/ml

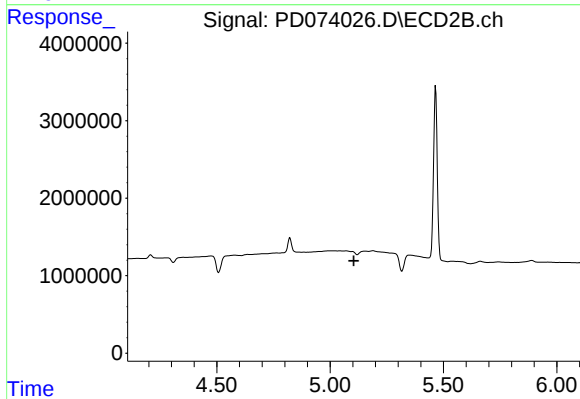

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.105 min
Response: 0
Conc: N.D.

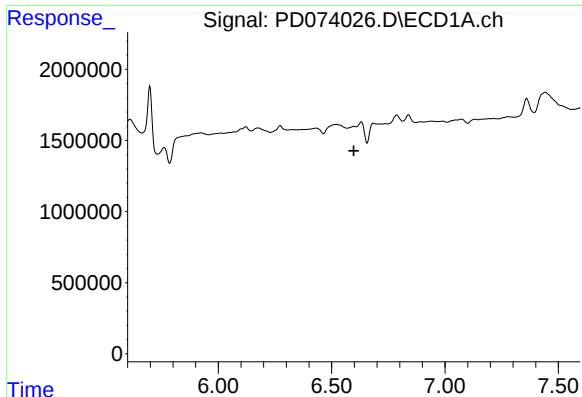

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.598 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

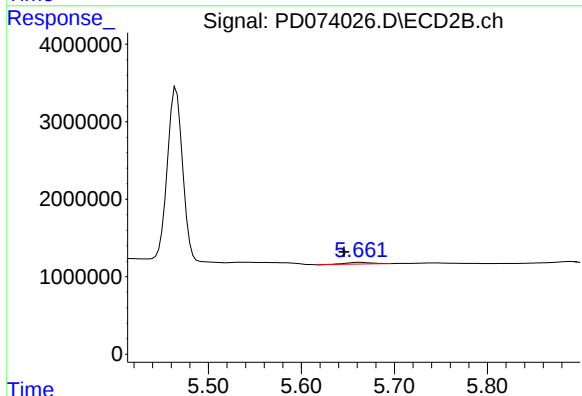


#14 Endrin

R.T.: 5.663 min
Delta R.T.: 0.017 min
Response: 400826
Conc: 0.30 ng/ml

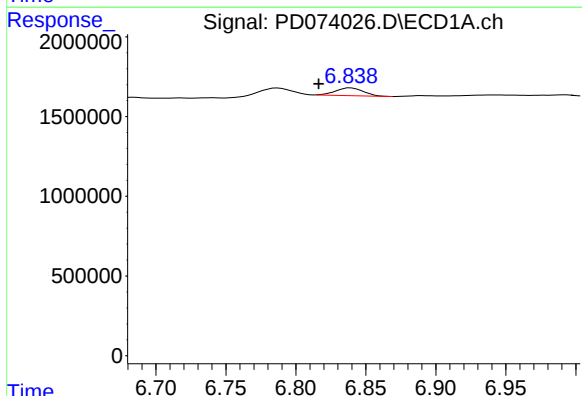


#15 Endosulfan II

R.T.: 6.839 min
Delta R.T.: 0.023 min
Response: 655921
Conc: 0.22 ng/ml

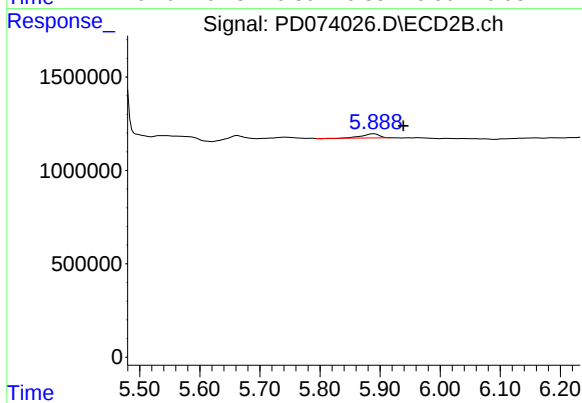

#15 Endosulfan II


R.T.: 5.890 min
Delta R.T.: -0.049 min
Response: 448355
Conc: 0.33 ng/ml

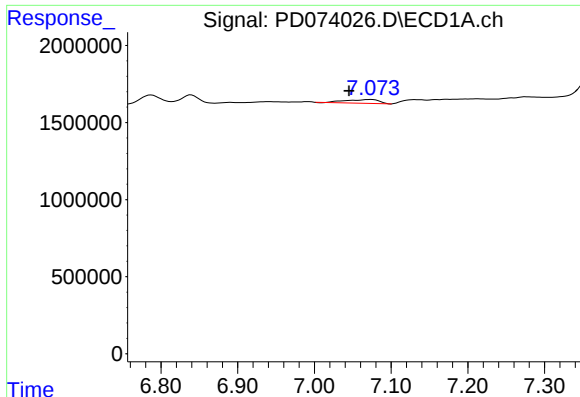

#17 4,4'-DDT


R.T.: 7.073 min
Delta R.T.: 0.027 min
Response: 738986
Conc: 0.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

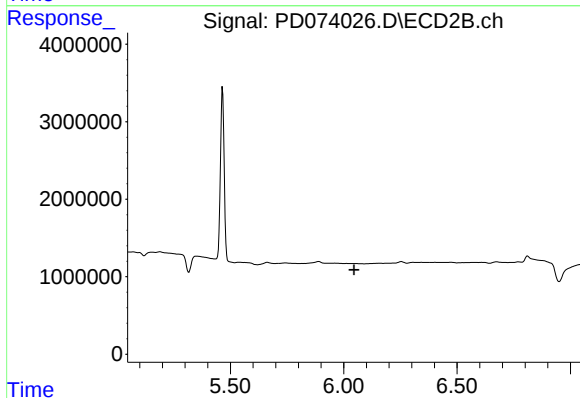


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.046 min
Response: 0
Conc: N.D.

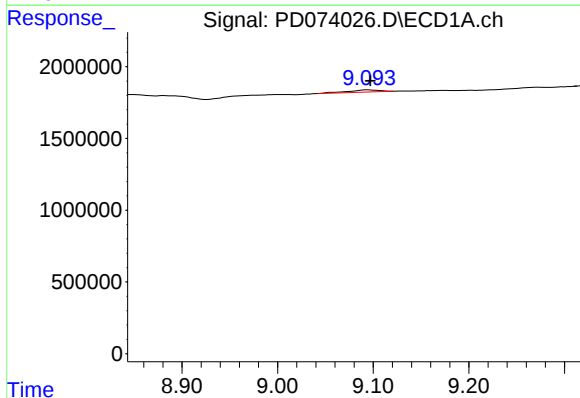

#27 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: -0.003 min
Response: 340266
Conc: 0.13 ng/ml

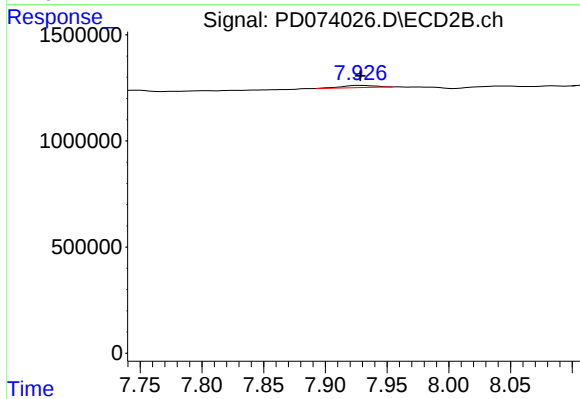

#27 Decachlorobiphenyl

R.T.: 7.928 min
Delta R.T.: 0.000 min
Response: 190193
Conc: 0.16 ng/ml