

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022223\
 Data File : PD074027.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2023 10:54
 Operator : AR\AJ
 Sample : RESC352
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC003

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 06:09:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022223CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 13 06:07:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.774	47390865	25451194	19.553	20.463
27)	SA Decachlor...	9.098	7.929	105.8E6	49134163	40.244	40.052
Target Compounds							
2)	A alpha-BHC	4.010	3.277	33378728	17318354	8.971	9.749
3)	MA gamma-BHC...	4.343	3.608	32516044	16829123	9.100	9.927
4)	MA Heptachlor	4.936	3.950	29883904	15769451	8.647	9.414
5)	MB Aldrin	5.279	4.231	31029192	16965837	8.922	10.018
6)	B beta-BHC	4.537	3.903	16086676	7918359	9.684	9.469
7)	B delta-BHC	4.786	4.135	23409700	17167597	7.993	9.683
8)	B Heptachlo...	5.705	4.734	24661560	15736183	8.131	9.909
9)	A Endosulfan I	6.093	5.105	25841634	13777379	8.719	9.552
10)	B trans-Chl...	5.962	4.985	28075525	15268503	8.949	9.841
11)	B cis-Chlor...	6.042	5.050	28306177	15282863	8.667	9.606
12)	B 4,4'-DDE	6.214	5.240	54101875	28376153	17.696	19.003
13)	MA Dieldrin	6.369	5.371	59021920	30122186	18.041	19.111
14)	MA Endrin	6.599	5.647	50095367	25537900	18.168	19.299
15)	B Endosulfa...	6.817	5.939	55628539	26205578	19.064	19.086
16)	A 4,4'-DDD	6.731	5.794	44783993	22704652	18.198	18.634
17)	MA 4,4'-DDT	7.047	6.046	51228925	24174066	18.961	18.775
18)	B Endrin al...	6.948	6.120	45809176	21848141	19.254	19.477
19)	B Endosulfa...	7.182	6.342	53425990	25287986	19.205	19.361
20)	A Methoxychlor	7.522	6.623	148.8E6	66315776	99.147	101.295
21)	B Endrin ke...	7.669	6.849	62201537	30810626	19.412	19.533

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022223\
Data File : PD074027.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2023 10:54
Operator : AR\AJ
Sample : RESC352
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 06:09:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022223CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 13 06:07:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

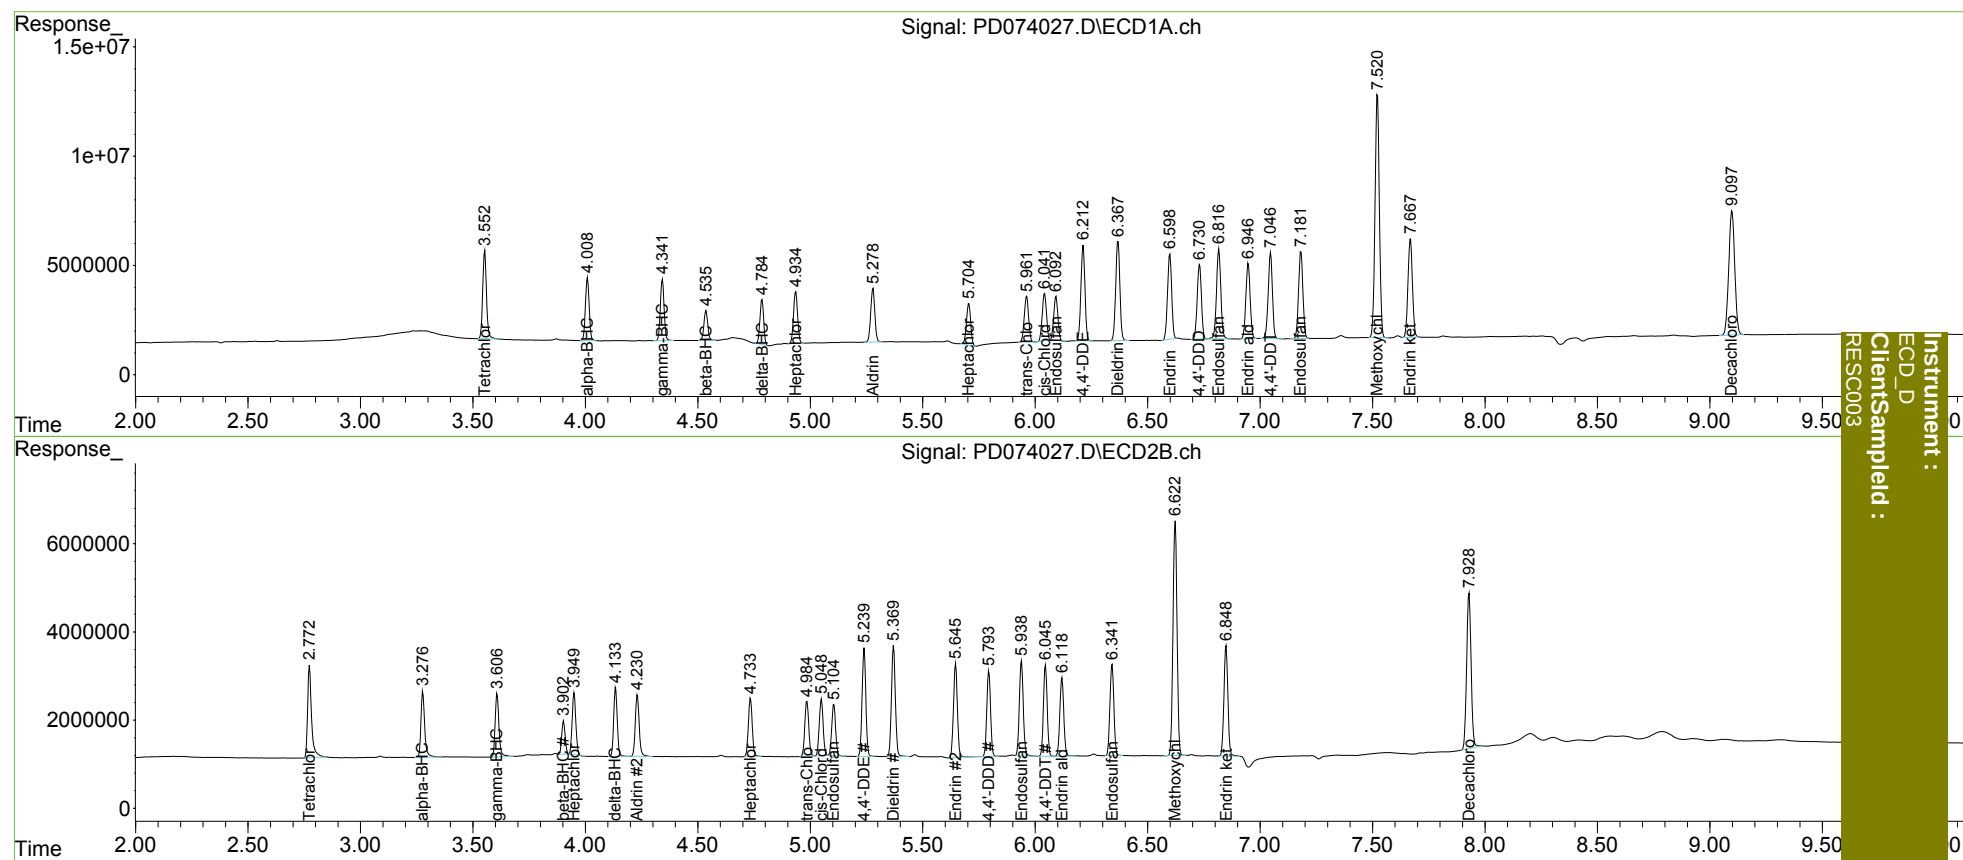

Instrument :
ECD_D
Client Sampled :
RESC003

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022223\
Data File : PD074027.D
Acq On : 22 Feb 2023 10:54
Operator : AR\AJ
Sample : RESC352
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC003

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022223CLP.M
Title : GC Extractables
Last Update : Mon Mar 13 06:07:45 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.553	4.010	100.00%
4.010	4.343	100.00%
4.343	4.537	100.00%
4.537	4.786	100.00%
4.786	4.936	100.00%
4.936	5.279	100.00%
5.279	5.705	100.00%
5.705	5.962	100.00%
5.962	6.042	100.00%
6.042	6.093	100.00%
6.093	6.214	100.00%
6.214	6.369	100.00%
6.369	6.599	100.00%
6.599	6.731	100.00%
6.731	6.817	100.00%
6.817	6.948	100.00%
6.948	7.047	100.00%
7.047	7.182	100.00%
7.182	7.522	100.00%
7.522	7.669	100.00%
7.669	9.098	100.00%

Signal #2

2.774	3.278	100.00%
3.278	3.608	100.00%
3.608	3.903	100.00%
3.903	3.950	100.00%
3.950	4.135	100.00%
4.135	4.232	100.00%
4.232	4.734	100.00%
4.734	4.985	100.00%
4.985	5.050	100.00%
5.050	5.105	100.00%
5.105	5.240	100.00%
5.240	5.371	100.00%
5.371	5.647	100.00%
5.647	5.794	100.00%
5.794	5.939	100.00%
5.939	6.046	100.00%
6.046	6.120	100.00%
6.120	6.342	100.00%
6.342	6.623	100.00%
6.623	6.849	100.00%
6.849	7.929	100.00%