

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022224\
 Data File : PD081547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2024 16:34
 Operator : AR\AJ
 Sample : P1469-02MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH9R0MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 20:43:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.794	25056634	42604005	18.328	17.378
27)	SA Decachlor...	9.108	7.928	39248047	53930013	20.343	21.740
Target Compounds							
2)	A alpha-BHC	4.021	3.295	124.6E6	203.1E6	53.372	52.812
3)	MA gamma-BHC...	4.355	3.624	113.8E6	183.1E6	49.240	50.540
4)	MA Heptachlor	4.947	3.964	124.6E6	182.1E6	50.819	51.322
5)	MB Aldrin	5.290	4.244	120.4E6	177.3E6	50.899	52.358
6)	B beta-BHC	4.549	3.919	50085993	76948759	48.196	45.540
7)	B delta-BHC	4.798	4.149	121.5E6	188.5E6	51.312	50.343
8)	B Heptachlo...	5.717	4.745	107.5E6	160.2E6	47.443	49.936
9)	A Endosulfan I	6.104	5.115	104.0E6	152.3E6	49.393	50.857
10)	B trans-Chl...	5.972	4.995	104.3E6	162.2E6	47.643	51.969
11)	B cis-Chlor...	6.052	5.059	108.0E6	161.9E6	47.962	50.526
12)	B 4,4'-DDE	6.223	5.248	213.5E6	313.4E6	99.463	105.973
13)	MA Dieldrin	6.378	5.380	224.0E6	338.3E6	100.882	102.997
14)	MA Endrin	6.609	5.654	190.6E6	302.2E6	101.582	105.166
15)	B Endosulfa...	6.828	5.947	193.5E6	295.4E6	100.243	104.659
16)	A 4,4'-DDD	6.740	5.801	167.8E6	260.4E6	101.037	103.324
17)	MA 4,4'-DDT	7.055	6.052	185.1E6	275.6E6	106.522	106.729
18)	B Endrin al...	6.957	6.126	139.1E6	209.5E6	93.144	96.698
19)	B Endosulfa...	7.192	6.348	184.7E6	274.6E6	100.881	102.342
20)	A Methoxychlor	7.530	6.626	472.6E6	662.5E6	515.189	495.853
21)	B Endrin ke...	7.678	6.854	206.2E6	318.0E6	106.635	106.054

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022224\
Data File : PD081547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2024 16:34
Operator : AR\AJ
Sample : P1469-02MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 20:43:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

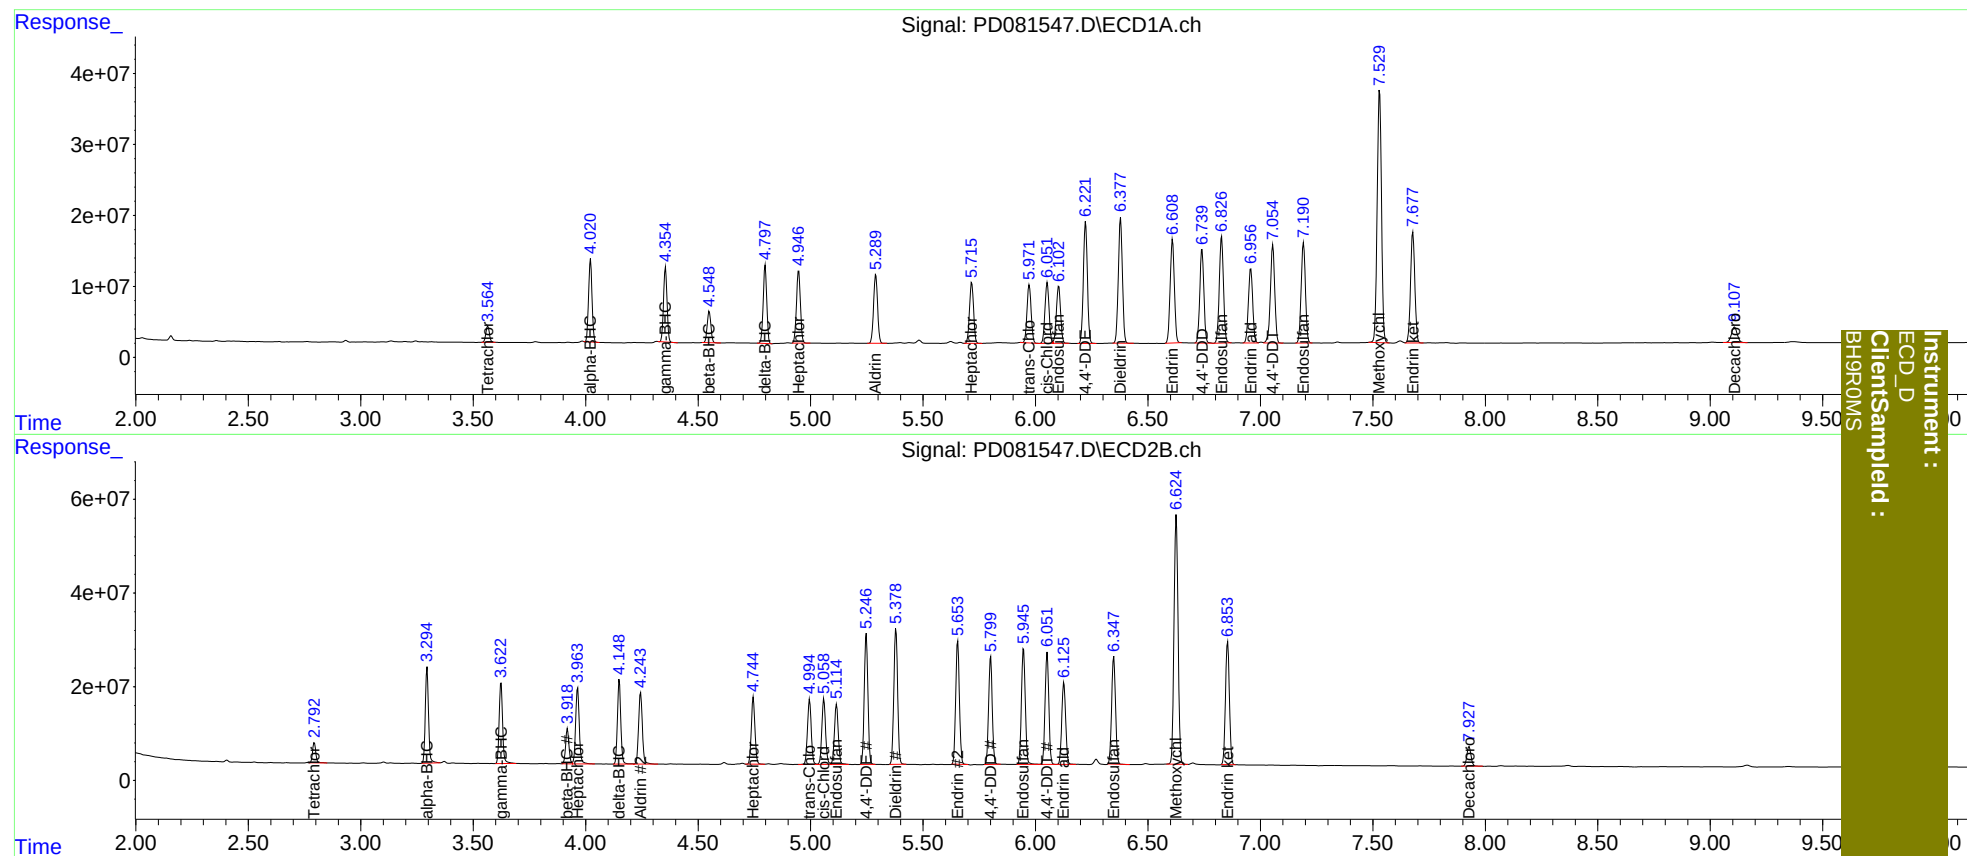

Instrument :
ECD_D
ClientSampled :
BH9R0MS