

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022319\
 Data File : PD051330.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Feb 2019 00:53
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 05:59:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022319.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 05:56:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	9.185f	0	516778	N.D.	0.027 #
Target Compounds							
3)	MA gamma-BHC...	3.935f	0.000	991809	0	0.438	N.D. #
8)	B Heptachlo...	0.000	5.928	0	42204817	N.D.	1.238 #
10)	B gamma-Chl...	0.000	6.184f	0	1119984	N.D.	0.032 #
13)	MA Dieldrin	0.000	6.549	0	345054	N.D.	0.011 #
14)	MA Endrin	0.000	6.759	0	7157518	N.D.	0.264 #
15)	B Endosulfa...	0.000	6.981	0	2410296	N.D.	0.088 #
25)	Chlordane-3	0.000	6.184f	0	1119984	N.D.	0.238 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022319\
Data File : PD051330.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2019 00:53
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 05:59:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022319.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 05:56:56 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

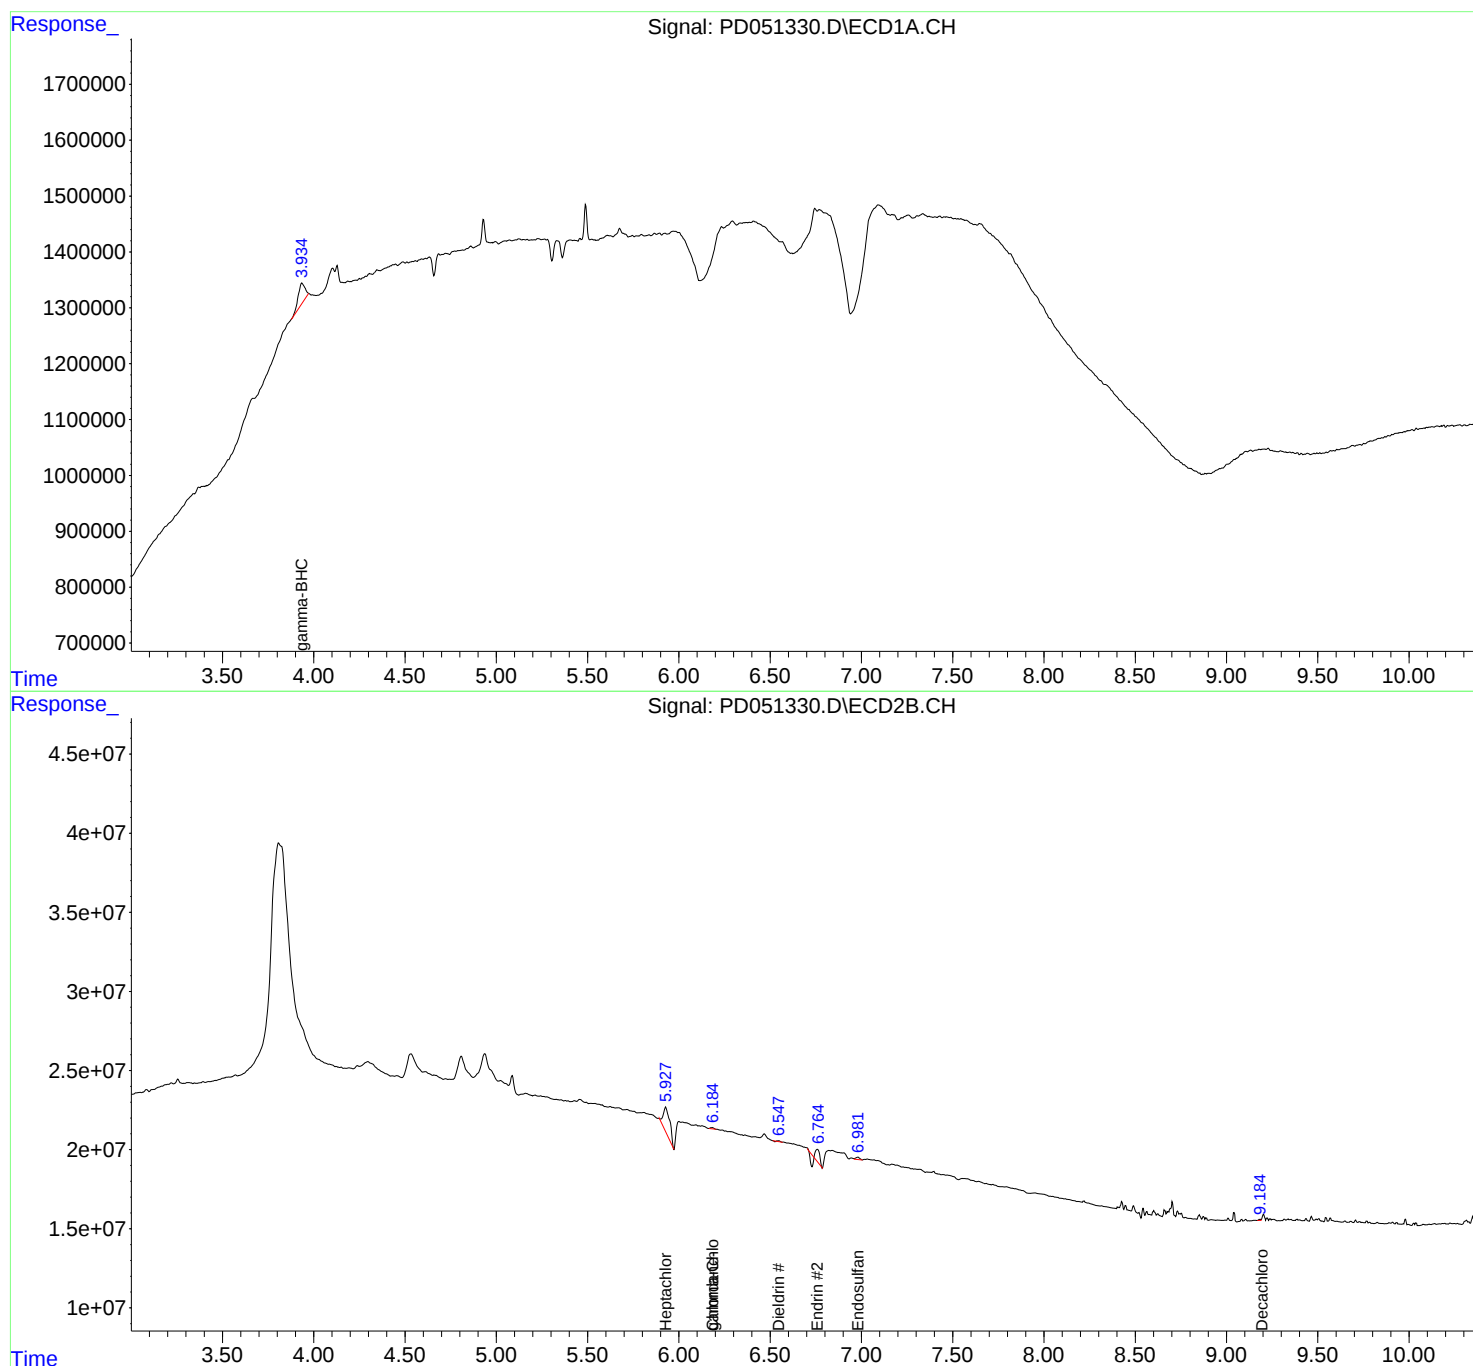


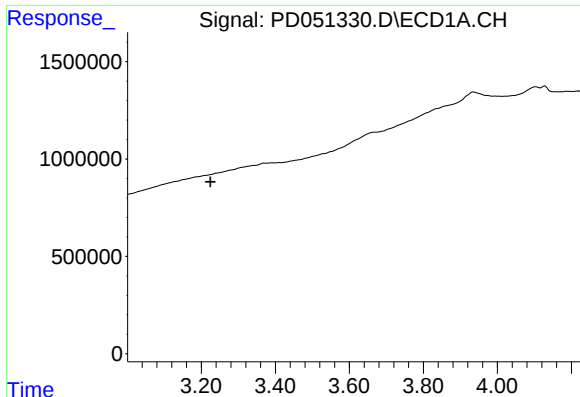

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.225 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

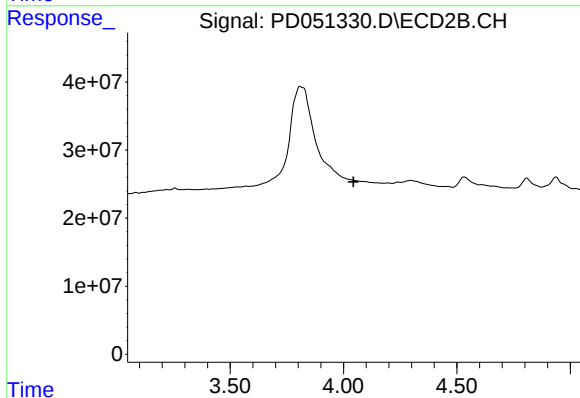


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.045 min
Response: 0
Conc: N.D.

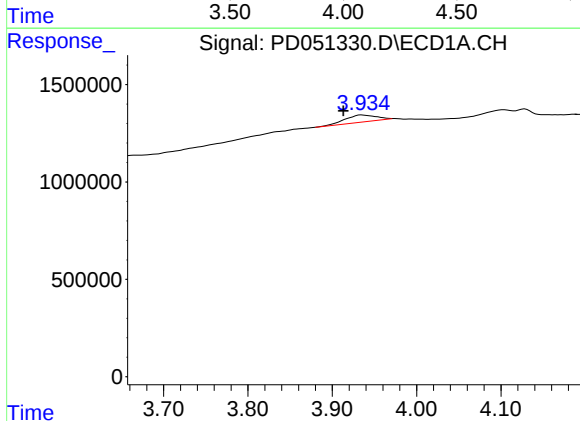


#3 gamma-BHC (Lindane)

R.T.: 3.935 min
Delta R.T.: 0.022 min
Response: 991809
Conc: 0.44 ng/ml

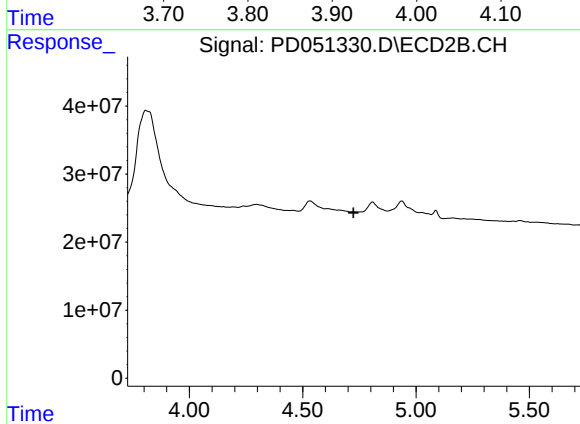

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.724 min
Response: 0
Conc: N.D.

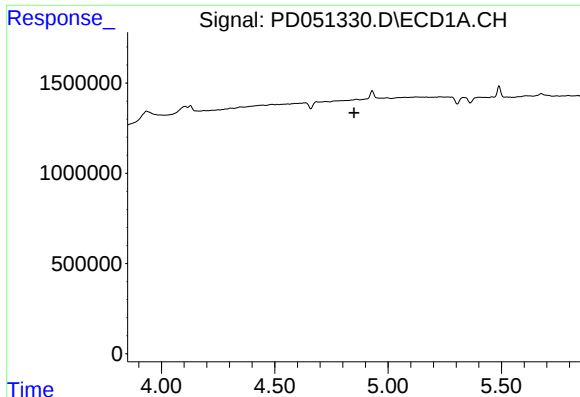

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.850 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

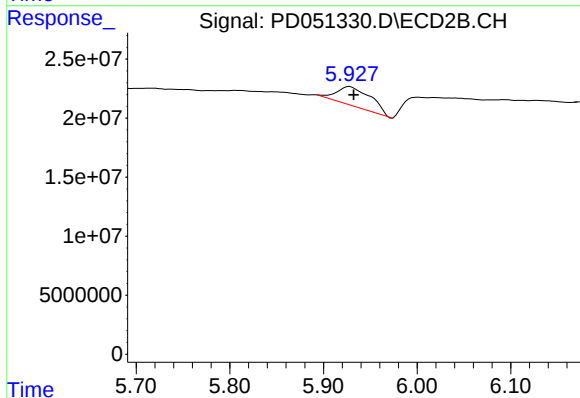


#8 Heptachlor epoxide

R.T.: 5.928 min
Delta R.T.: -0.004 min
Response: 42204817
Conc: 1.24 ng/ml

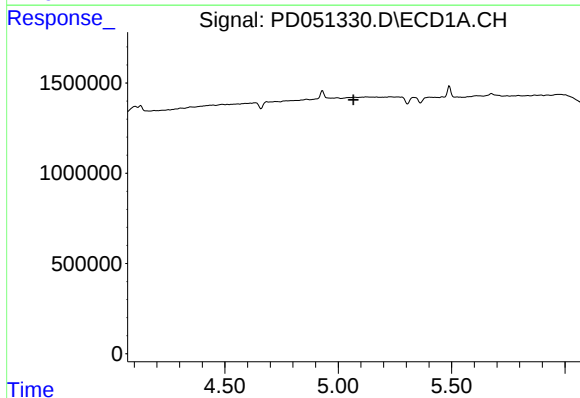


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.068 min
Response: 0
Conc: N.D.

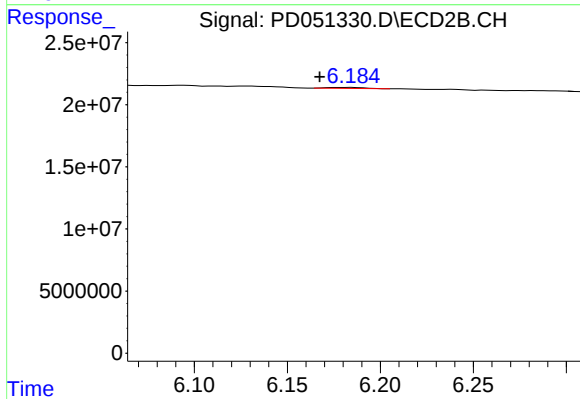

#10 gamma-Chlordane


R.T.: 6.184 min
Delta R.T.: 0.017 min
Response: 1119984
Conc: 0.03 ng/ml

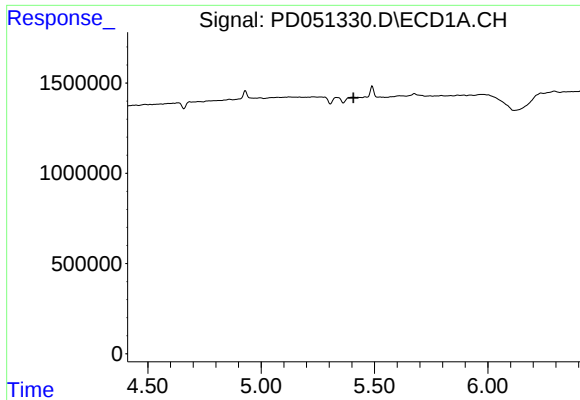

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

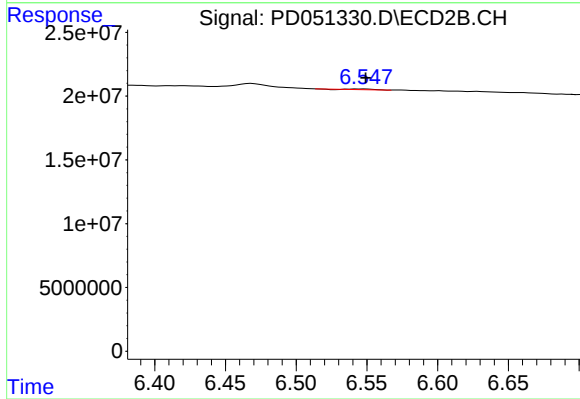


#13 Dieldrin

R.T.: 6.549 min
Delta R.T.: 0.000 min
Response: 345054
Conc: 0.01 ng/ml

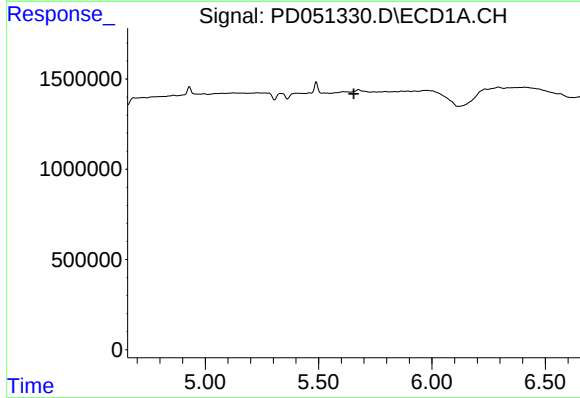


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.655 min
Response: 0
Conc: N.D.

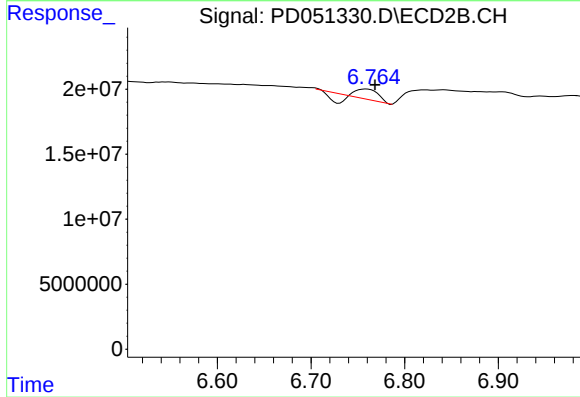

#14 Endrin


R.T.: 6.759 min
Delta R.T.: -0.009 min
Response: 7157518
Conc: 0.26 ng/ml

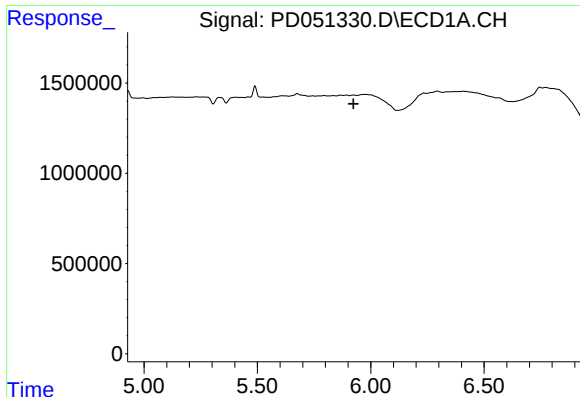

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.925 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

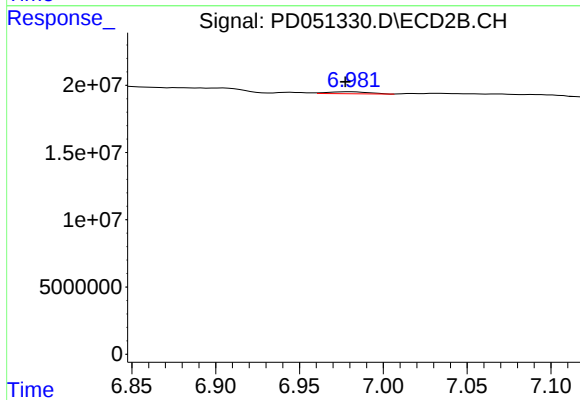


#15 Endosulfan II

R.T.: 6.981 min
Delta R.T.: 0.004 min
Response: 2410296
Conc: 0.09 ng/ml

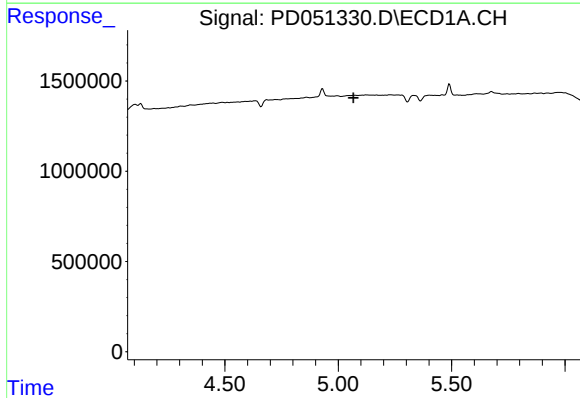


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.068 min
Response: 0
Conc: N.D.

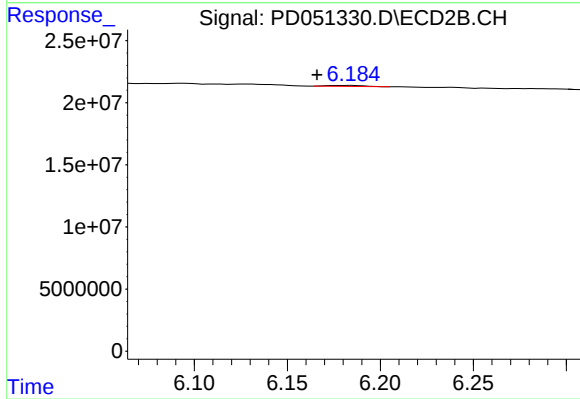

#25 Chlordane-3


R.T.: 6.184 min
Delta R.T.: 0.018 min
Response: 1119984
Conc: 0.24 ng/ml

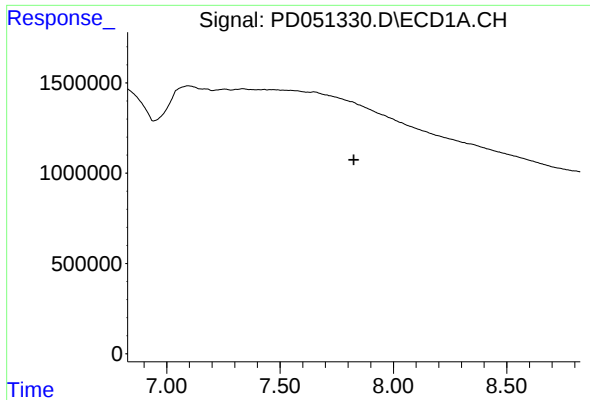

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.826 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

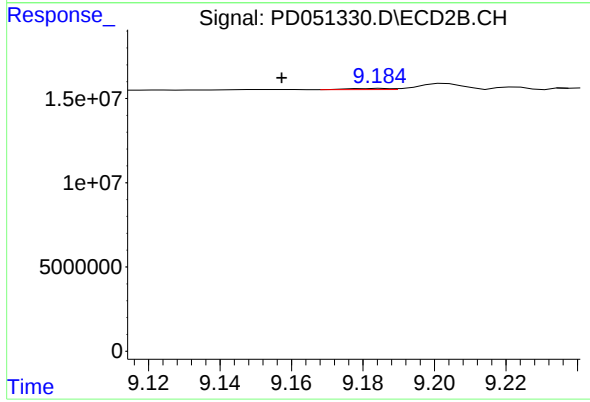

#28 Decachlorobiphenyl

R.T.: 9.185 min
Delta R.T.: 0.028 min
Response: 516778
Conc: 0.03 ng/ml