

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022319\
 Data File : PD051350.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Feb 2019 5:33
 Operator : AJ\SJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD022319CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 05:49:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022319.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 05:46:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.045	80270332	1382.3E6	52.198	45.572
28)	SA Decachlor...	7.825	9.157	52093083	876.6E6	43.013	44.770
Target Compounds							
23)	Chlordane-1	4.047	5.047	24455610	561.8E6	356.050	359.037
24)	Chlordane-2	4.527	5.517	30899673	524.6E6	371.166	360.640
25)	Chlordane-3	5.068	6.167	95673006	1946.5E6	382.781	413.501
26)	Chlordane-4	5.122	6.242	92347805	2238.3E6	382.105	414.587
27)	Chlordane-5	5.928	7.050	33154225	395.5E6	411.790	373.531



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022319\
Data File : PD051350.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2019 5:33
Operator : AJ\SJ
Sample : PCHLORICV500
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD022319CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 05:49:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022319.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 05:46:49 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

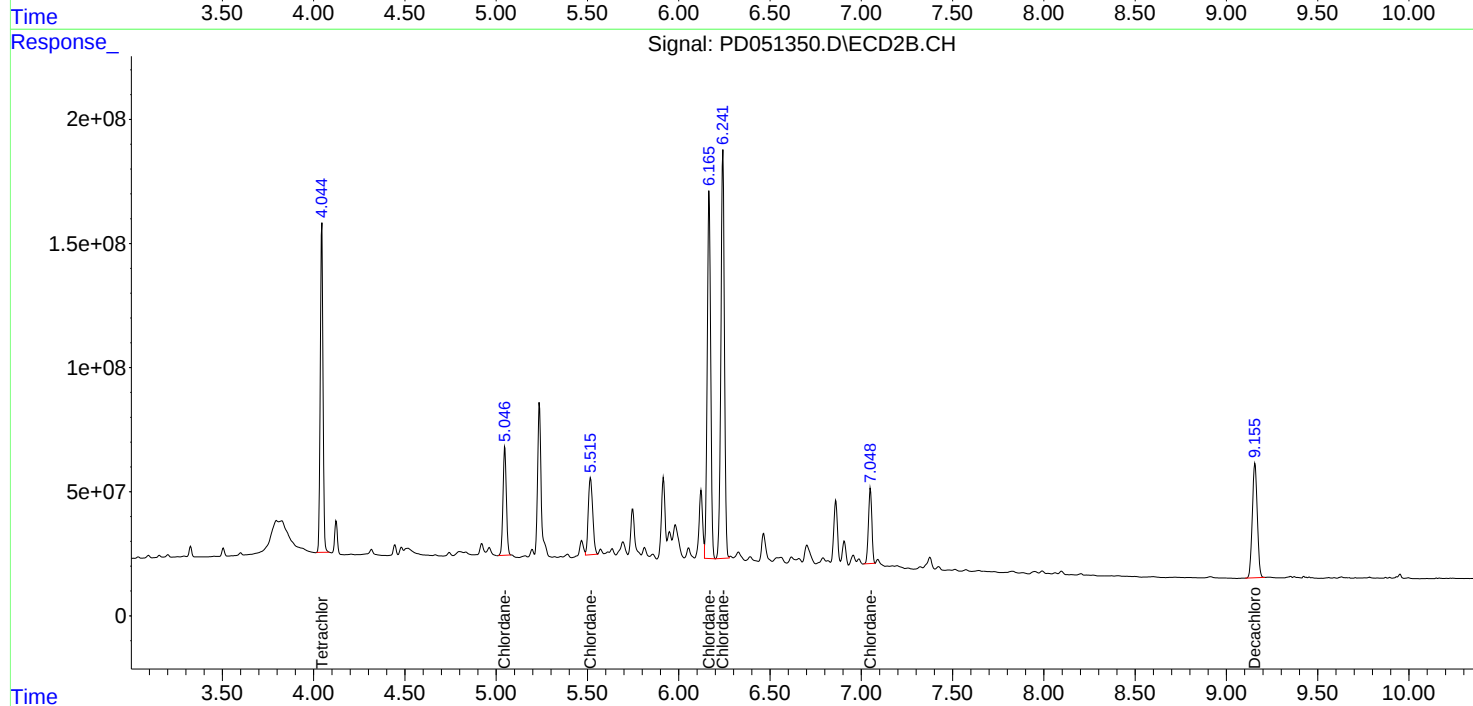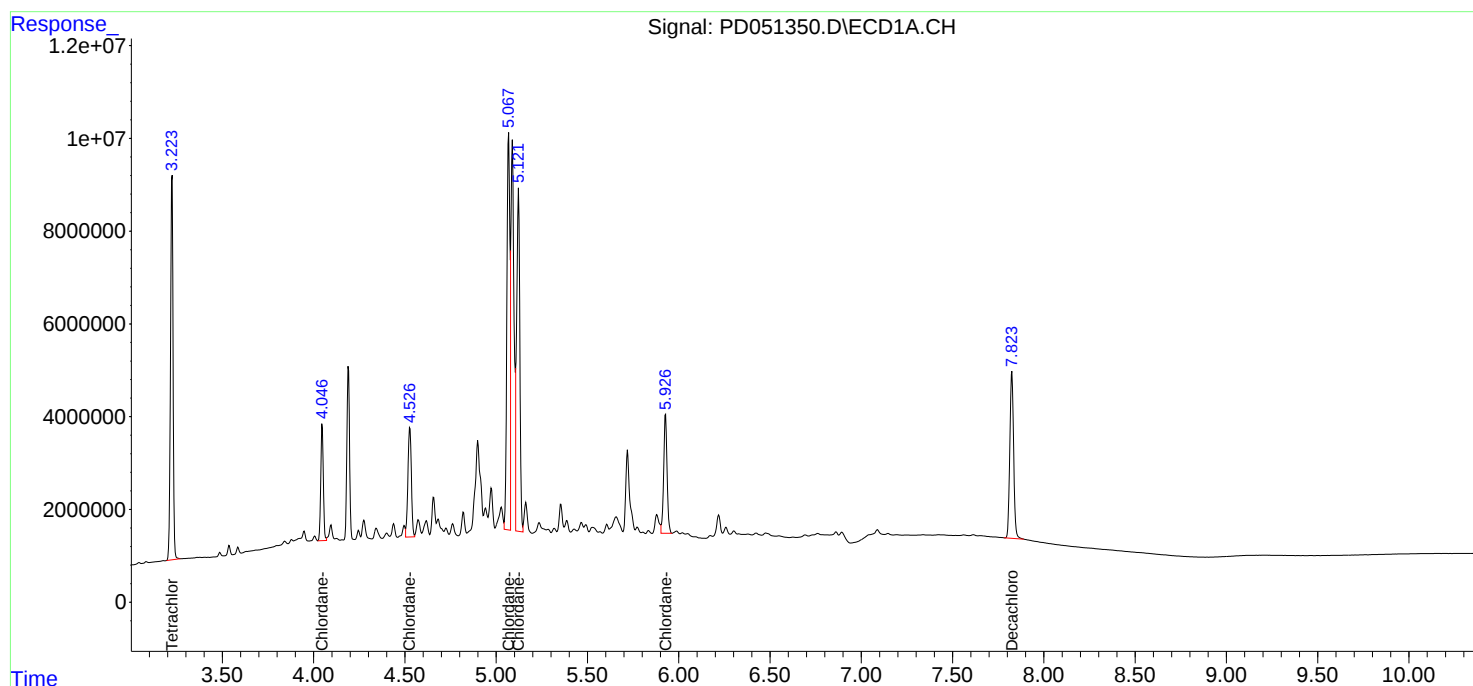


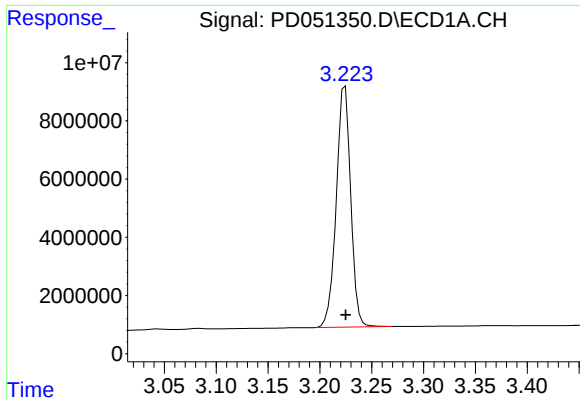

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 80270332
Conc: 52.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD022319CHLOR

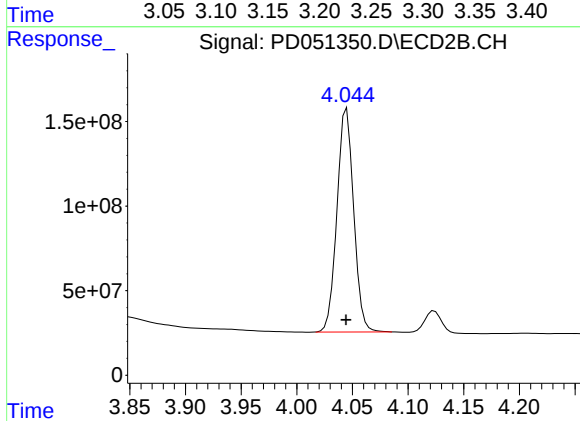


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 1382346983
Conc: 45.57 ng/ml

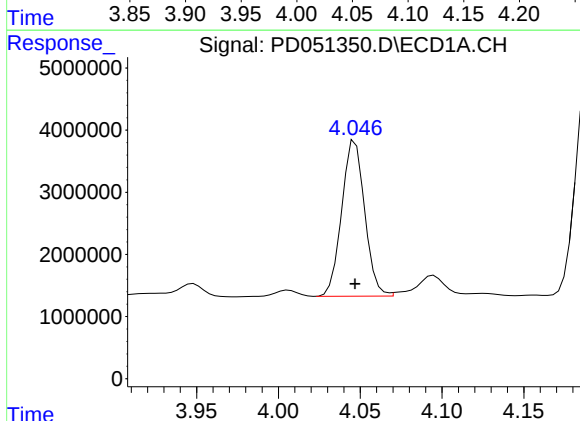


#23 Chlordane-1

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 24455610
Conc: 356.05 ng/ml

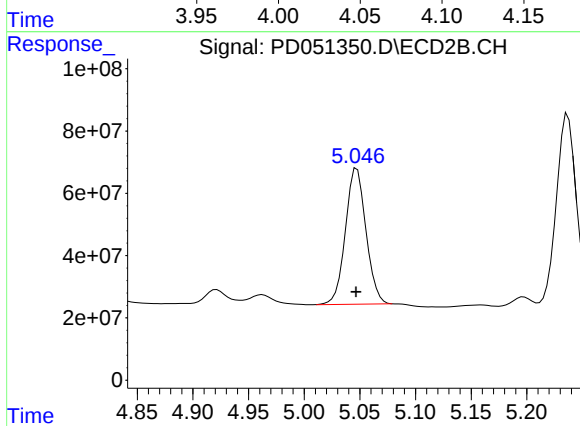

#23 Chlordane-1


R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 561794950
Conc: 359.04 ng/ml

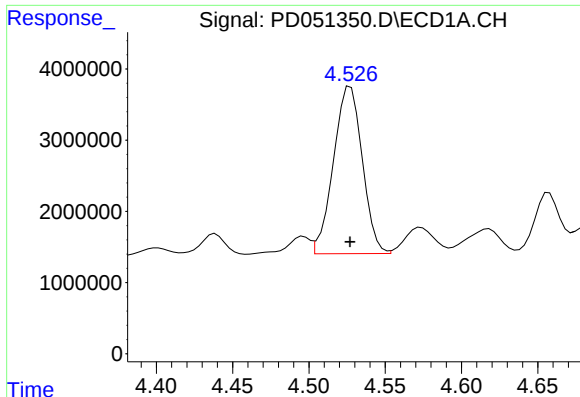

#24 Chlordane-2


R.T.: 4.527 min
Delta R.T.: 0.000 min
Response: 30899673
Conc: 371.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD022319CHLOR

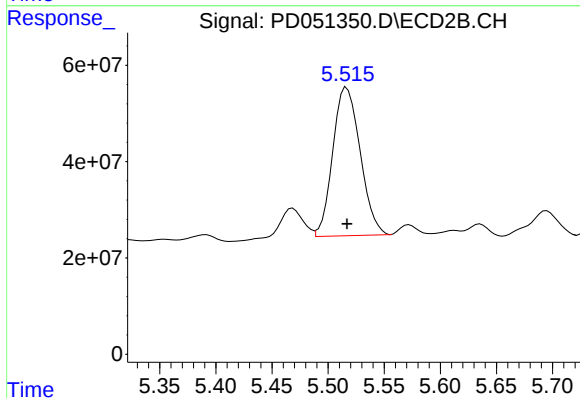


#24 Chlordane-2

R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 524585828
Conc: 360.64 ng/ml

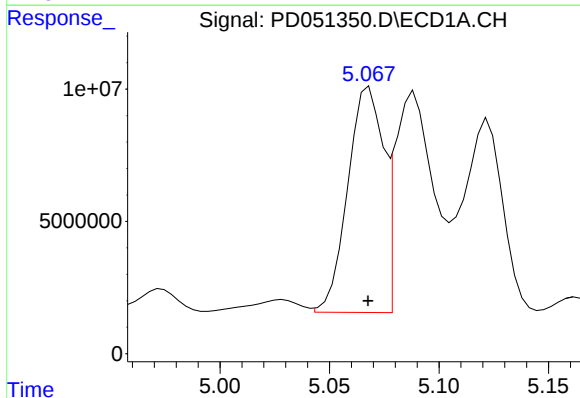


#25 Chlordane-3

R.T.: 5.068 min
Delta R.T.: 0.000 min
Response: 95673006
Conc: 382.78 ng/ml

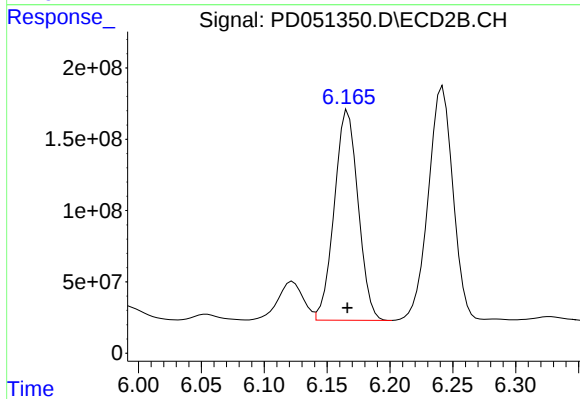

#25 Chlordane-3


R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 1946493332
Conc: 413.50 ng/ml

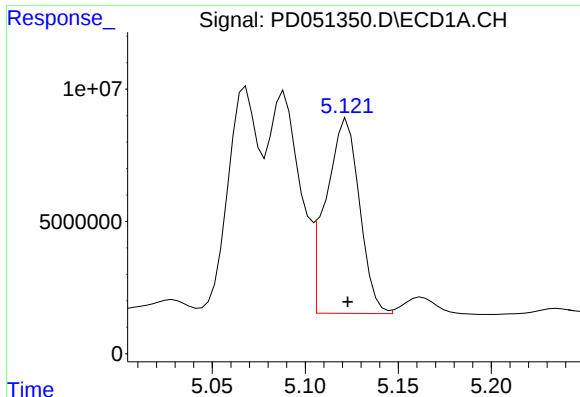

#26 Chlordane-4


R.T.: 5.122 min
Delta R.T.: 0.000 min
Response: 92347805
Conc: 382.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD022319CHLOR

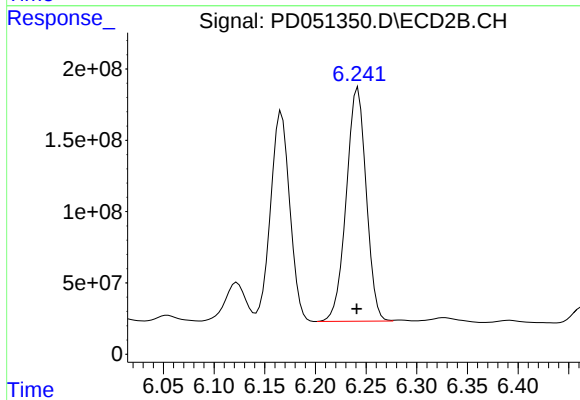


#26 Chlordane-4

R.T.: 6.242 min
Delta R.T.: 0.001 min
Response: 2238301500
Conc: 414.59 ng/ml

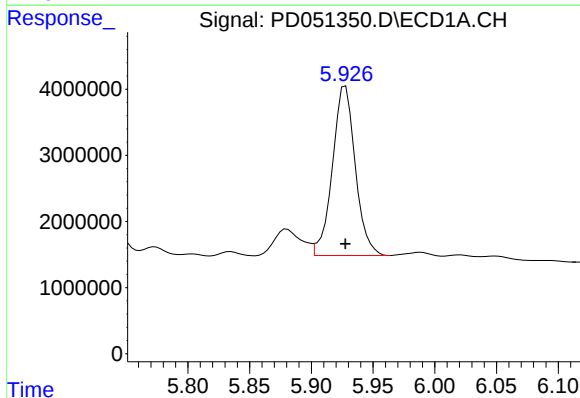


#27 Chlordane-5

R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 33154225
Conc: 411.79 ng/ml

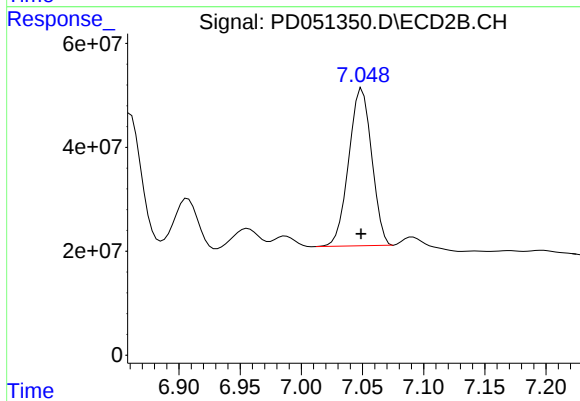

#27 Chlordane-5

R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 395528557
Conc: 373.53 ng/ml

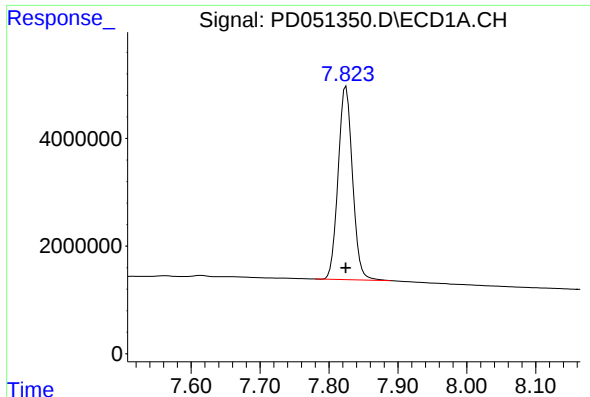

#28 Decachlorobiphenyl


R.T.: 7.825 min

Delta R.T.: 0.000 min

Response: 52093083

Conc: 43.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD022319CHLOR

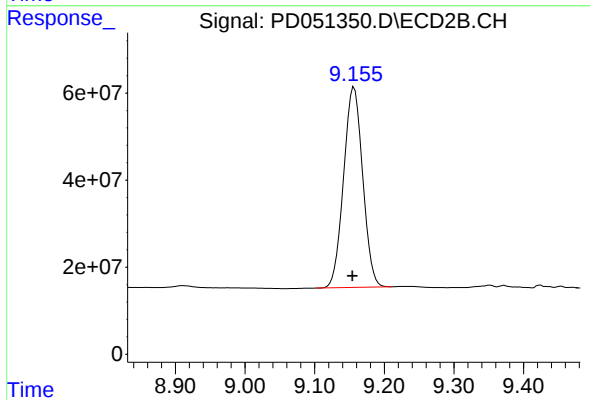

#28 Decachlorobiphenyl

R.T.: 9.157 min

Delta R.T.: 0.002 min

Response: 876632177

Conc: 44.77 ng/ml