

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022319\
 Data File : PD051340.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Feb 2019 3:13
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 05:39:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022319.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 05:38:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.225	4.045	117.2E6	2088.6E6	75.044	70.884
28)	SA Decachlor...	7.825	9.156	84470718	1303.8E6	72.687	69.878
Target Compounds							
23)	Chlordane-1	4.047	5.048	52071640	1086.7E6	748.938	709.069
24)	Chlordane-2	4.527	5.518	59946937	974.3E6	726.126	691.214
25)	Chlordane-3	5.068	6.167	195.2E6	3251.8E6	759.214	711.896
26)	Chlordane-4	5.123	6.242	186.2E6	3699.7E6	756.895	711.054
27)	Chlordane-5	5.928	7.050	60798766	742.7E6	743.946	712.240



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022319\
Data File : PD051340.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2019 3:13
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 05:39:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022319.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 05:38:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

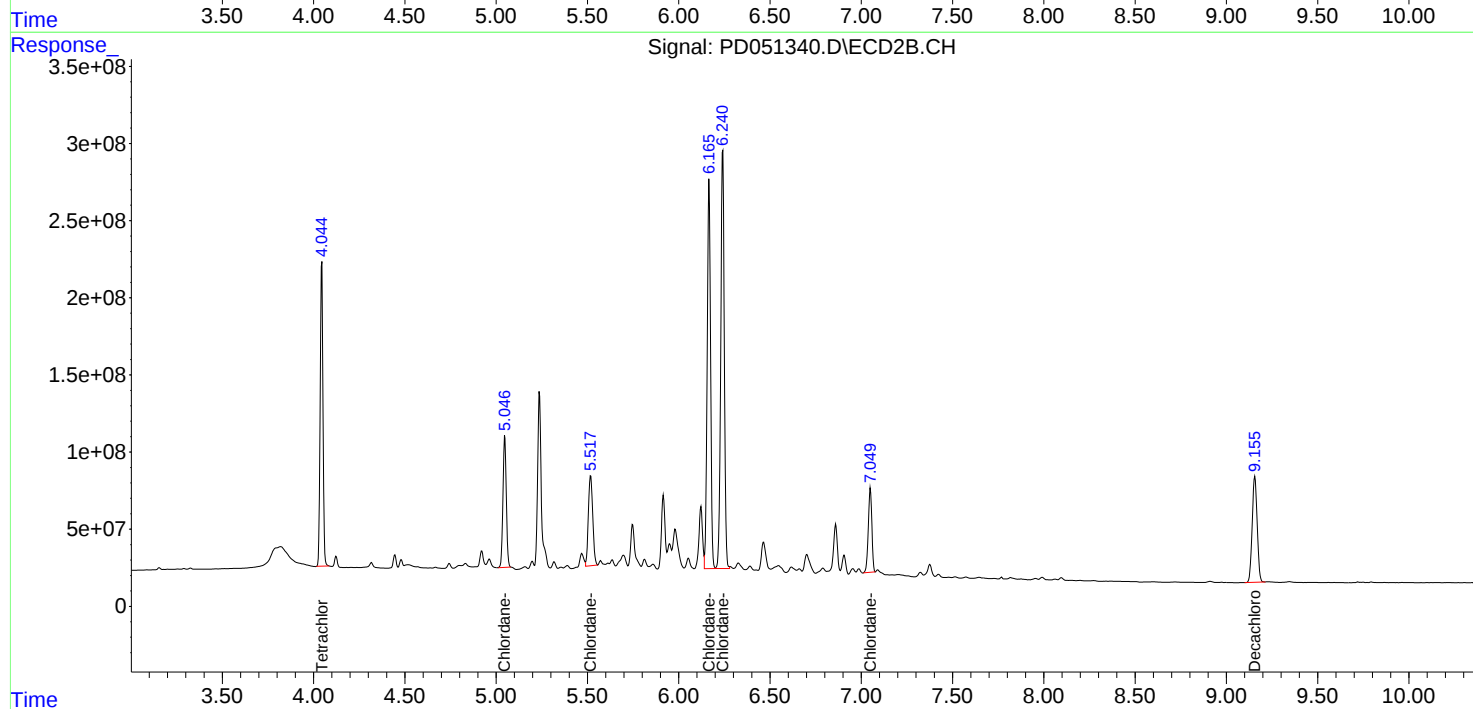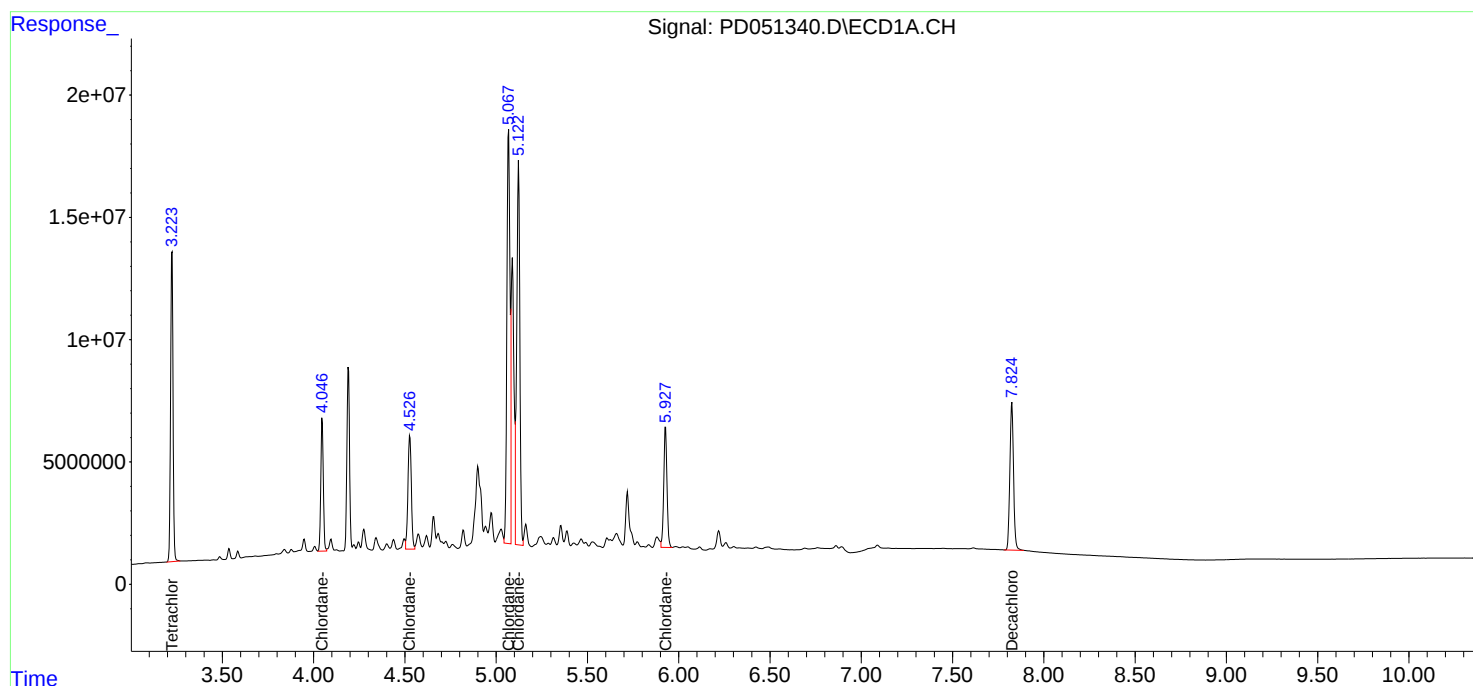


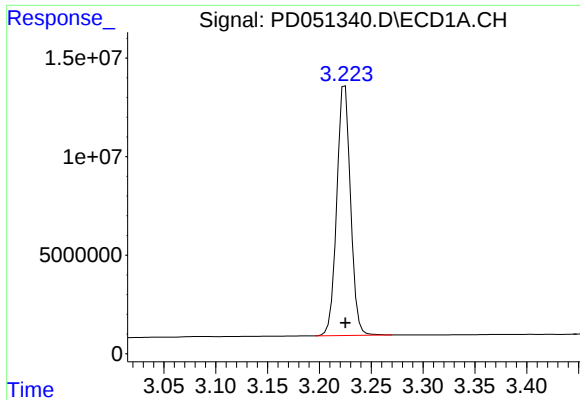

#1 Tetrachloro-m-xylene


R.T.: 3.225 min
Delta R.T.: 0.000 min
Response: 117155459
Conc: 75.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

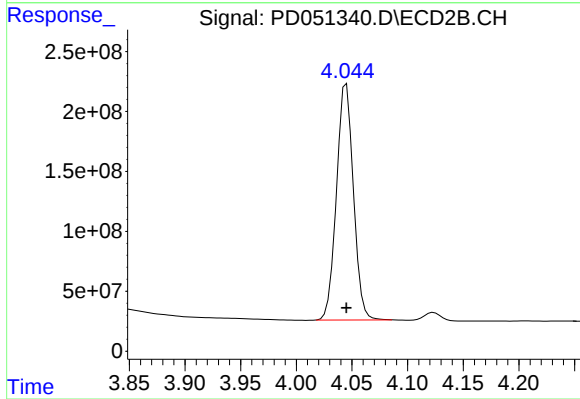


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 2088567678
Conc: 70.88 ng/ml

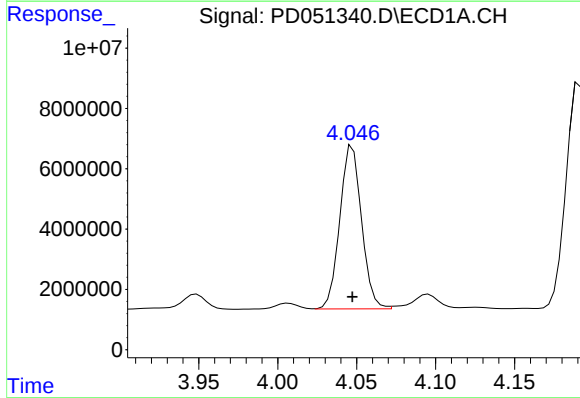


#23 Chlordane-1

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 52071640
Conc: 748.94 ng/ml

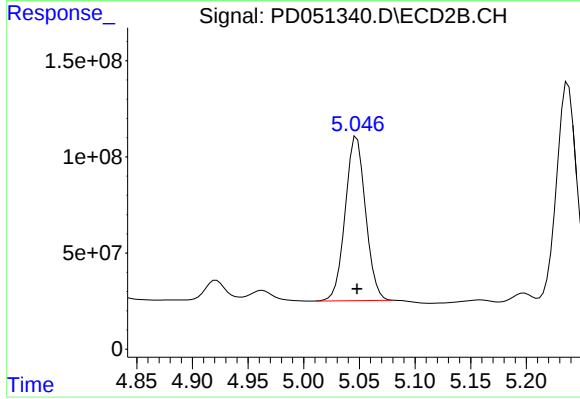

#23 Chlordane-1


R.T.: 5.048 min
Delta R.T.: 0.000 min
Response: 1086671329
Conc: 709.07 ng/ml

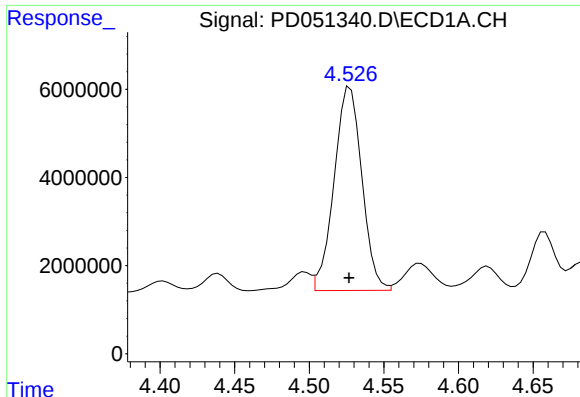

#24 Chlordane-2


R.T.: 4.527 min
Delta R.T.: 0.000 min
Response: 59946937
Conc: 726.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

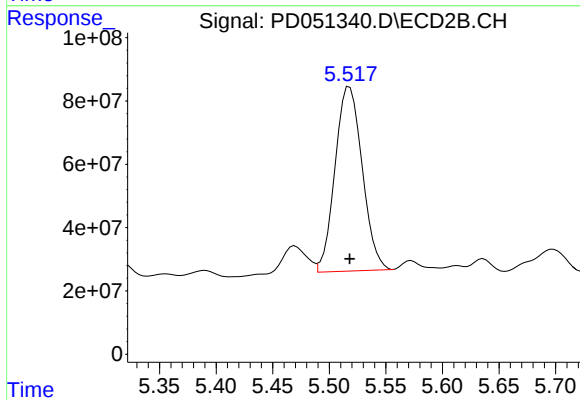


#24 Chlordane-2

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 974281571
Conc: 691.21 ng/ml

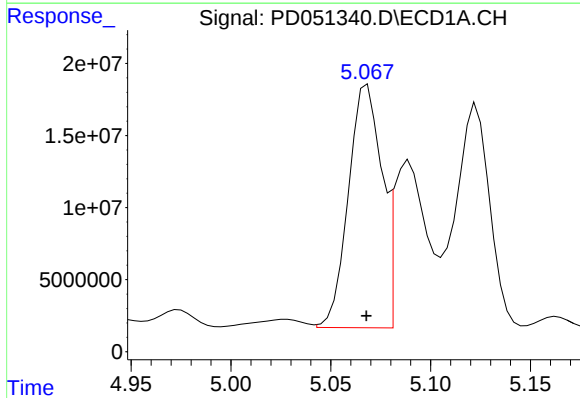


#25 Chlordane-3

R.T.: 5.068 min
Delta R.T.: 0.000 min
Response: 195184876
Conc: 759.21 ng/ml

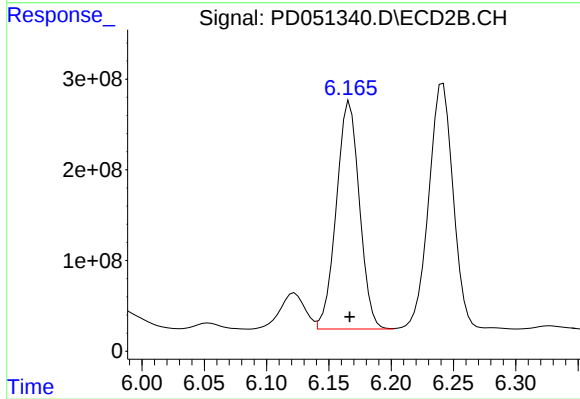

#25 Chlordane-3


R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 3251768612
Conc: 711.90 ng/ml

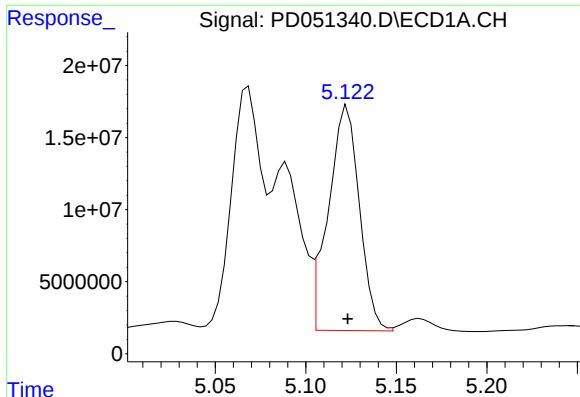

#26 Chlordane-4


R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 186178717
Conc: 756.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

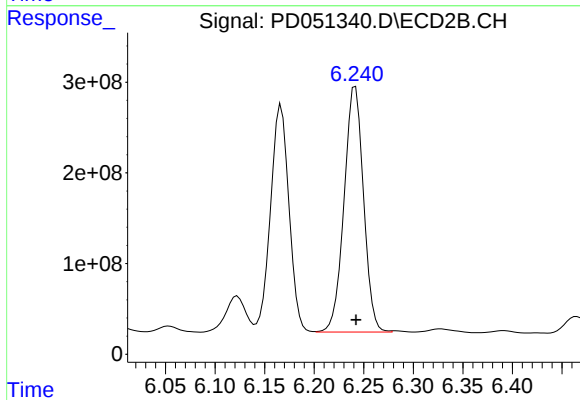


#26 Chlordane-4

R.T.: 6.242 min
Delta R.T.: 0.000 min
Response: 3699702649
Conc: 711.05 ng/ml

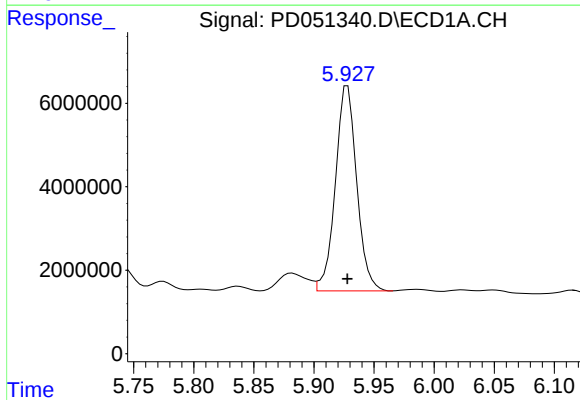


#27 Chlordane-5

R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 60798766
Conc: 743.95 ng/ml

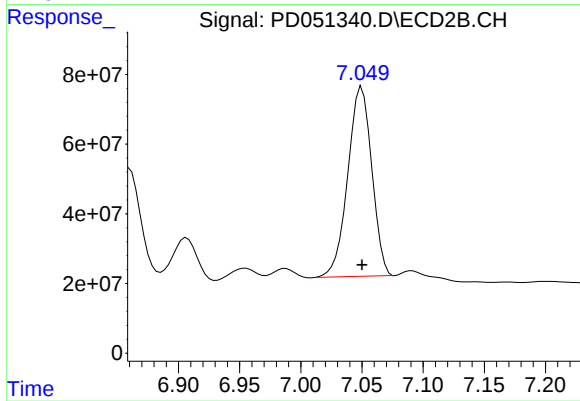

#27 Chlordane-5


R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 742724417
Conc: 712.24 ng/ml

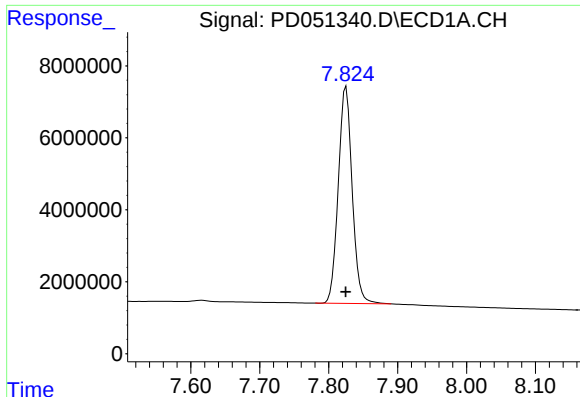

#28 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 84470718
Conc: 72.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

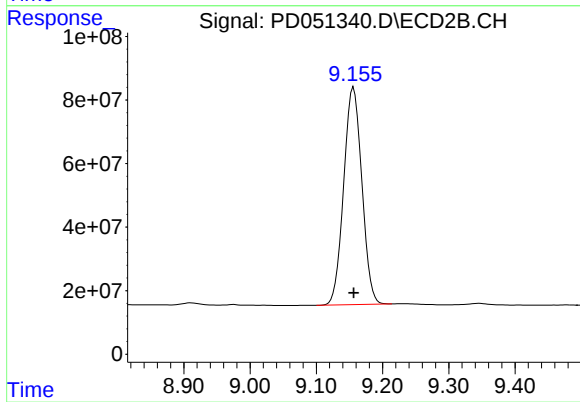

#28 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 1303779258
Conc: 69.88 ng/ml