

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022319\
 Data File : PD051341.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Feb 2019 3:27
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 05:39:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022319.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 05:38:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.225	4.045	78057544	1473.2E6	50.000	50.000
28)	SA Decachlor...	7.825	9.157	58105448	932.9E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.047	5.048	34763632	766.3E6	500.000	500.000
24)	Chlordane-2	4.527	5.518	41278584	704.8E6	500.000	500.000
25)	Chlordane-3	5.068	6.167	128.5E6	2283.9E6	500.000	500.000
26)	Chlordane-4	5.123	6.242	123.0E6	2601.6E6	500.000	500.000
27)	Chlordane-5	5.928	7.050	40862330	521.4E6	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022319\
Data File : PD051341.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2019 3:27
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 05:39:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022319.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 05:38:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

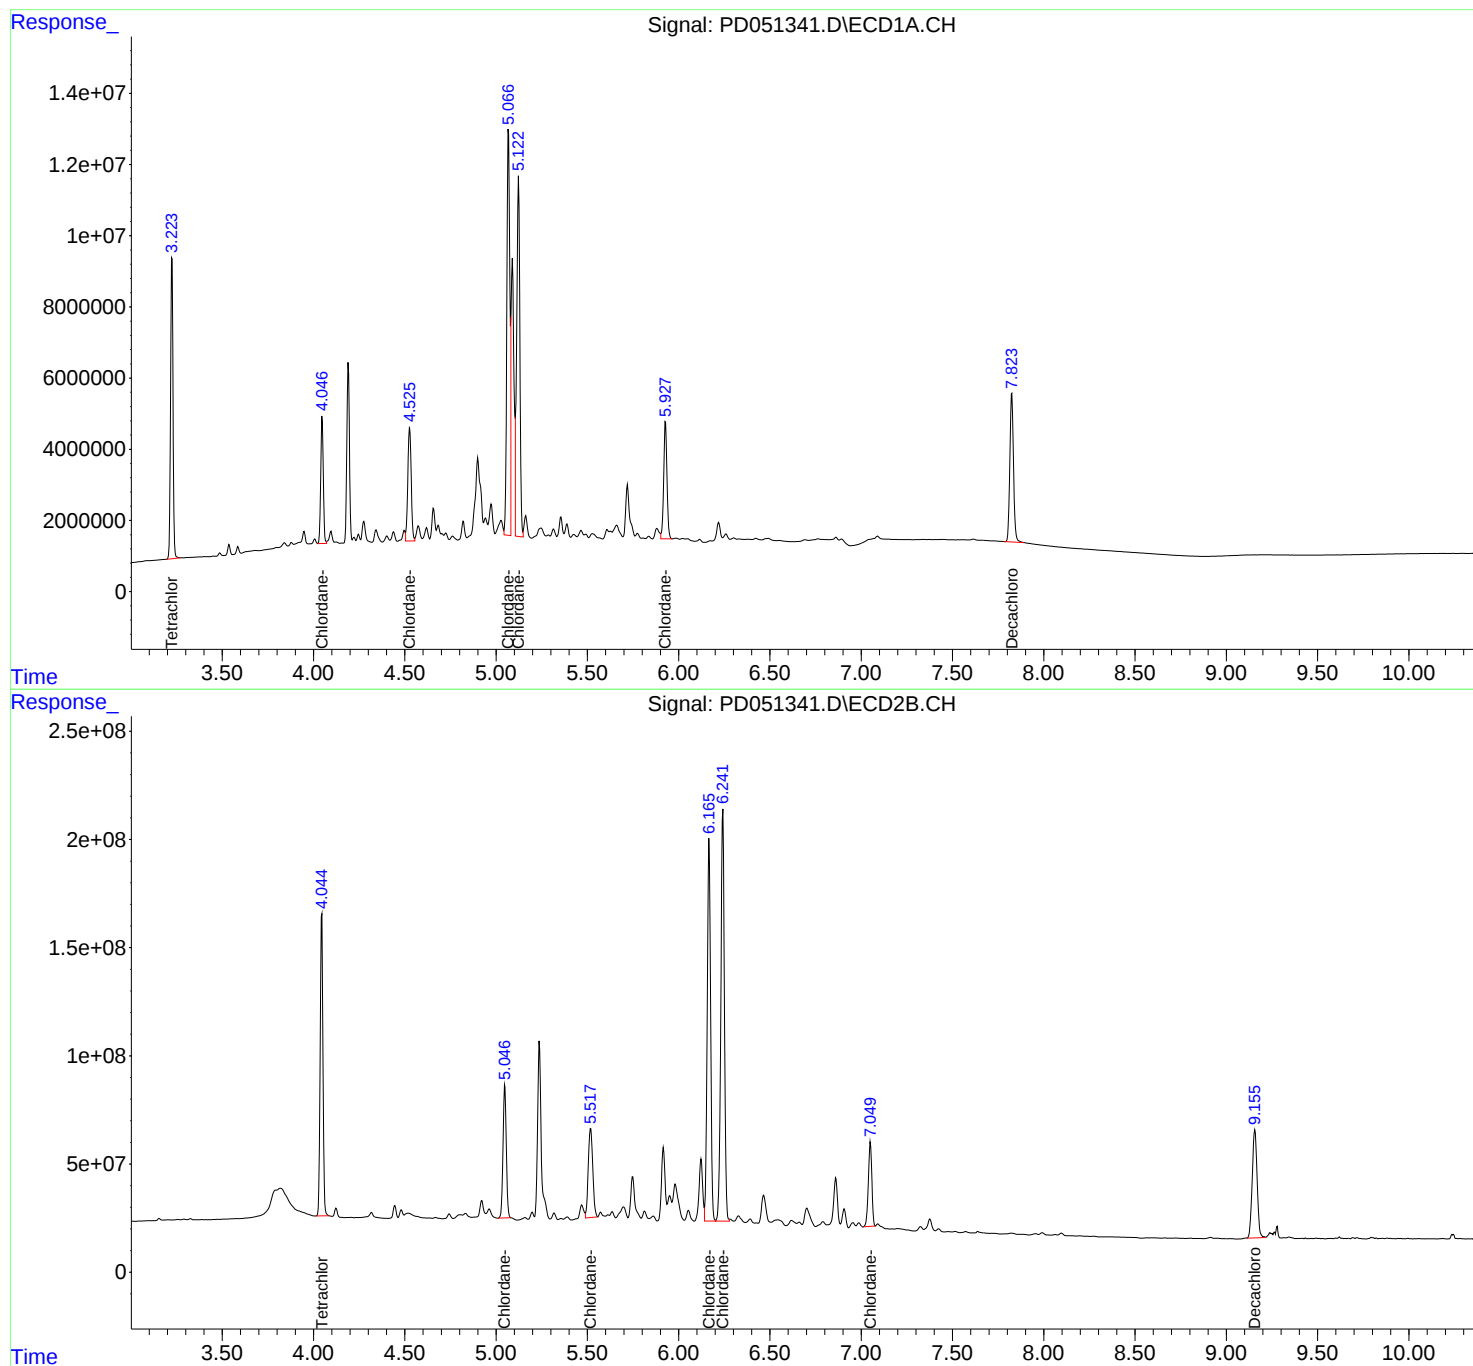


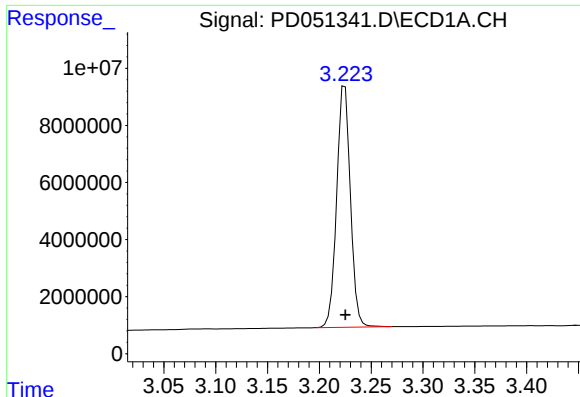

#1 Tetrachloro-m-xylene


R.T.: 3.225 min
Delta R.T.: 0.000 min
Response: 78057544
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

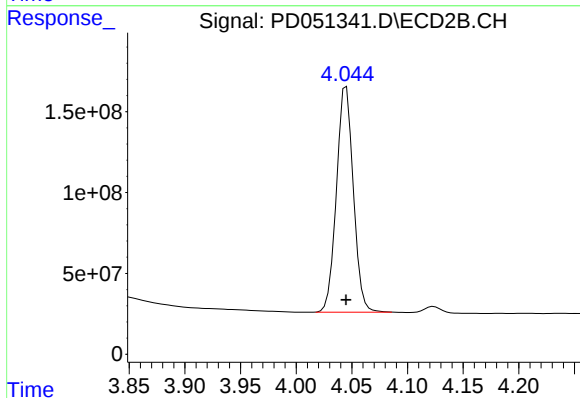


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 1473232331
Conc: 50.00 ng/ml

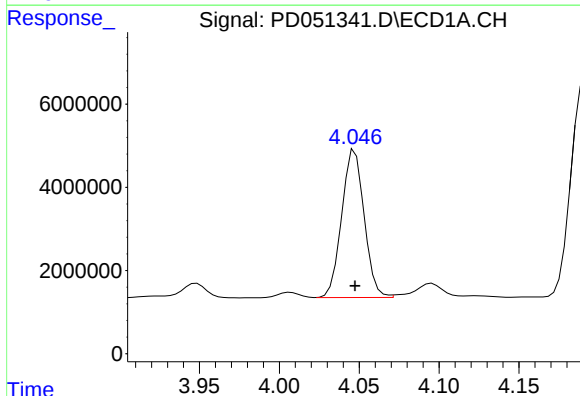


#23 Chlordane-1

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 34763632
Conc: 500.00 ng/ml

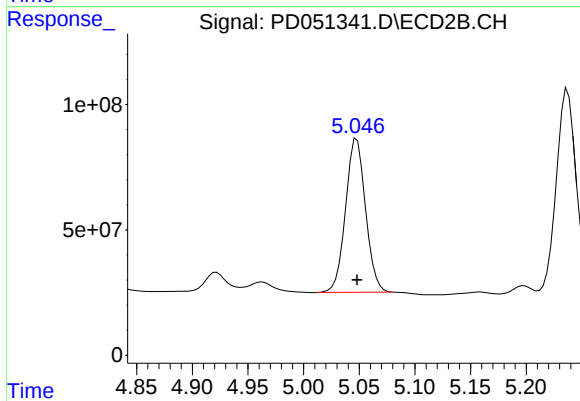

#23 Chlordane-1


R.T.: 5.048 min
Delta R.T.: 0.000 min
Response: 766265834
Conc: 500.00 ng/ml

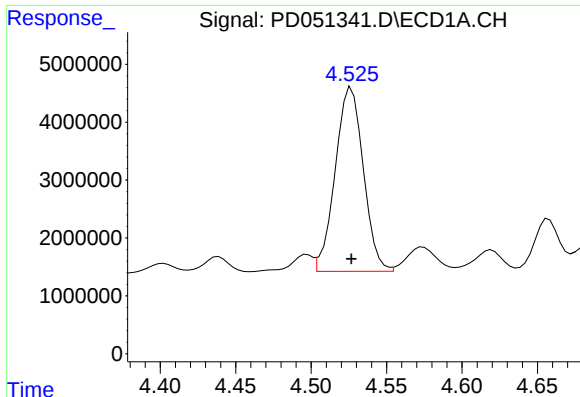

#24 Chlordane-2


R.T.: 4.527 min
Delta R.T.: 0.000 min
Response: 41278584
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

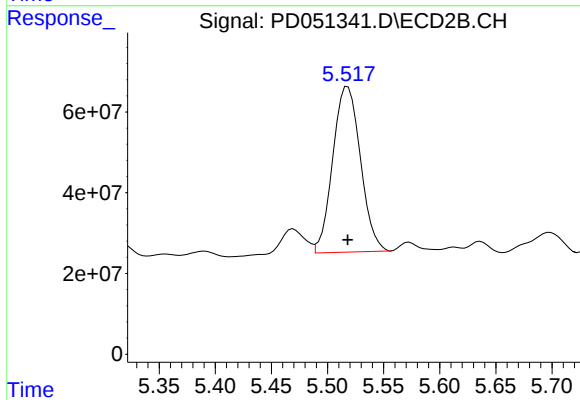


#24 Chlordane-2

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 704761146
Conc: 500.00 ng/ml

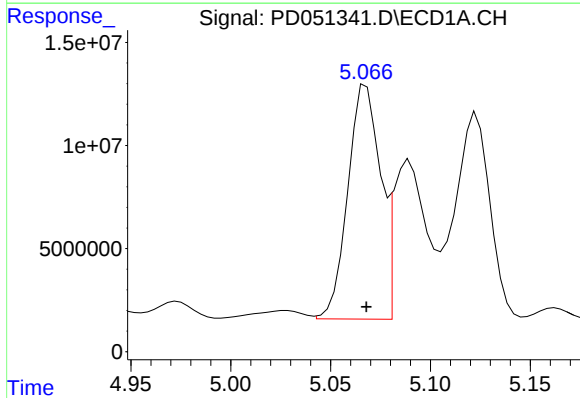


#25 Chlordane-3

R.T.: 5.068 min
Delta R.T.: 0.000 min
Response: 128544098
Conc: 500.00 ng/ml

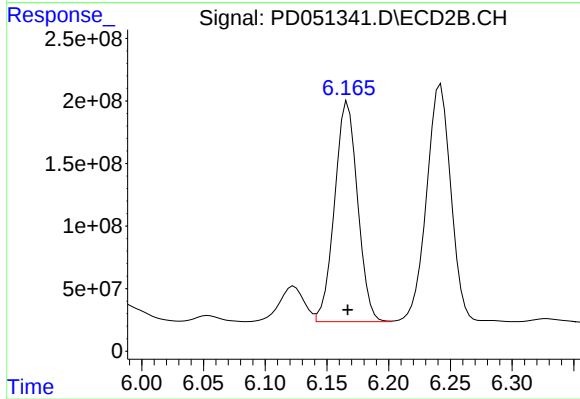

#25 Chlordane-3


R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 2283880017
Conc: 500.00 ng/ml

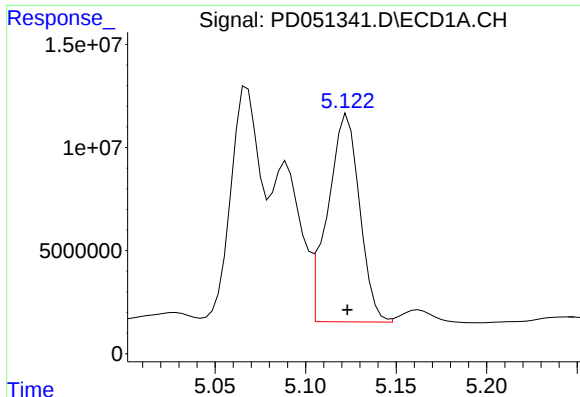

#26 Chlordane-4


R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 122988427
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

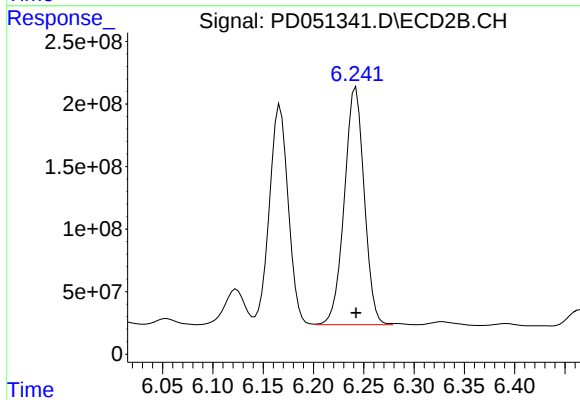


#26 Chlordane-4

R.T.: 6.242 min
Delta R.T.: 0.000 min
Response: 2601562585
Conc: 500.00 ng/ml

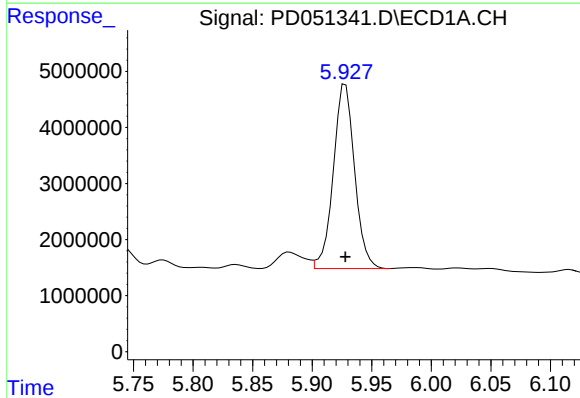


#27 Chlordane-5

R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 40862330
Conc: 500.00 ng/ml

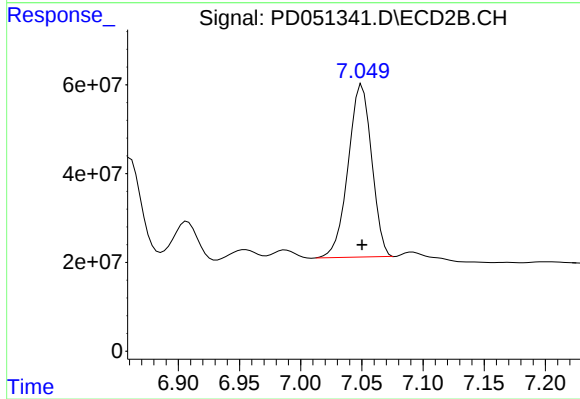

#27 Chlordane-5


R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 521400582
Conc: 500.00 ng/ml

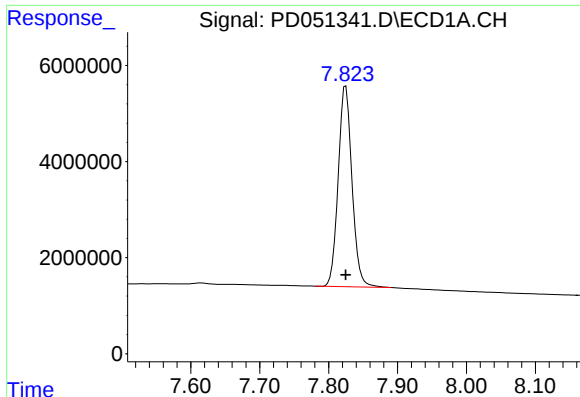

#28 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 58105448
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

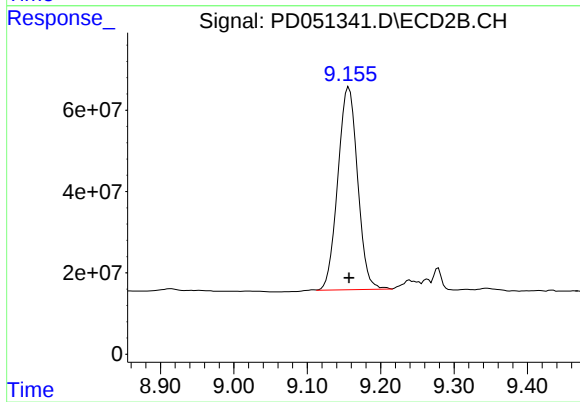

#28 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: 0.000 min
Response: 932894795
Conc: 50.00 ng/ml