

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022319\
 Data File : PD051342.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Feb 2019 3:41
 Operator : AJ\SJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 05:39:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022319.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 05:38:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.225	4.045	36578535	754.9E6	23.430	25.621
28)	SA Decachlor...	7.826	9.158	30223619	502.0E6	26.008	26.904
Target Compounds							
23)	Chlordane-1	4.047	5.048	16514835	394.7E6	237.530	257.548
24)	Chlordane-2	4.526	5.518	20357034	369.2E6	246.581	261.918
25)	Chlordane-3	5.068	6.168	58429005	1171.7E6	227.272	256.519
26)	Chlordane-4	5.123	6.242	56988148	1349.3E6	231.681	259.316
27)	Chlordane-5	5.928	7.050	19448789	268.0E6	237.979	256.999



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022319\
Data File : PD051342.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2019 3:41
Operator : AJ\SJ
Sample : PCHLORICC250
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 05:39:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022319.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 05:38:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

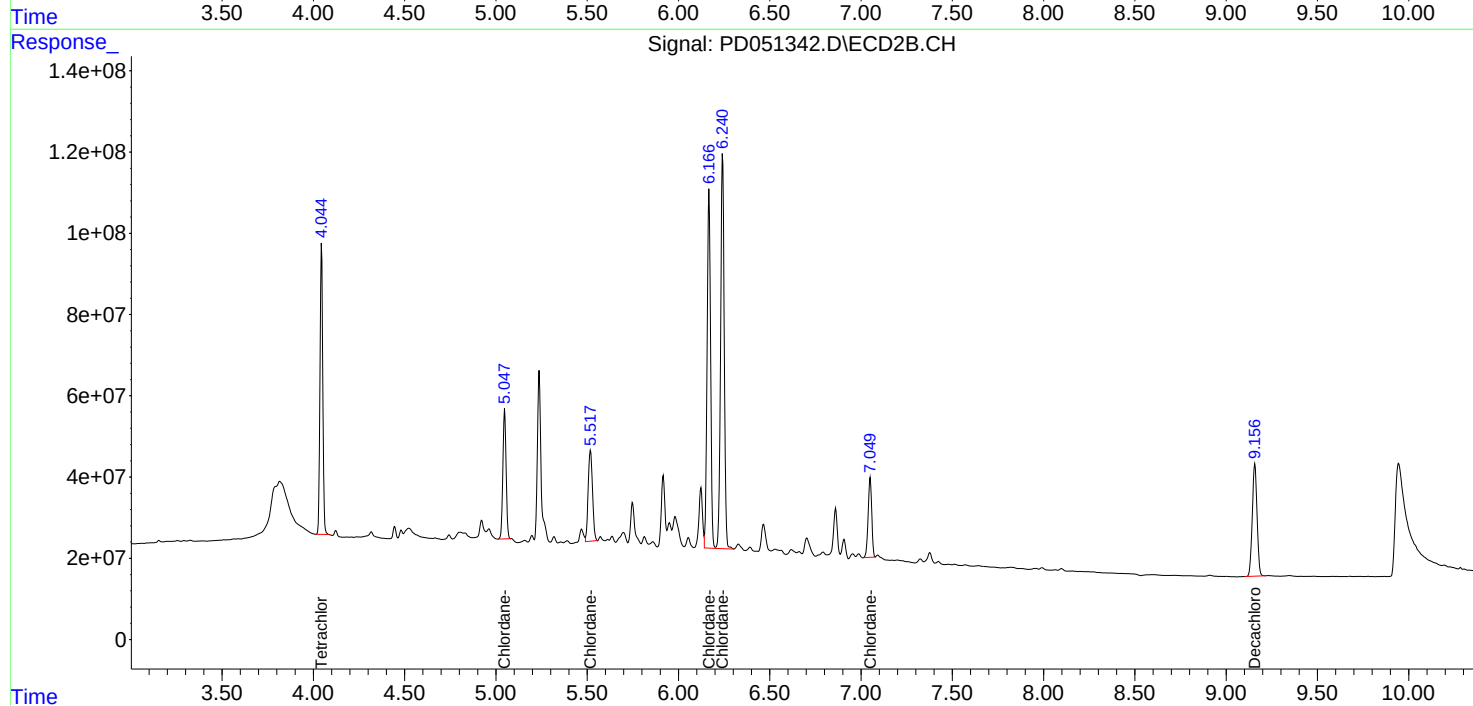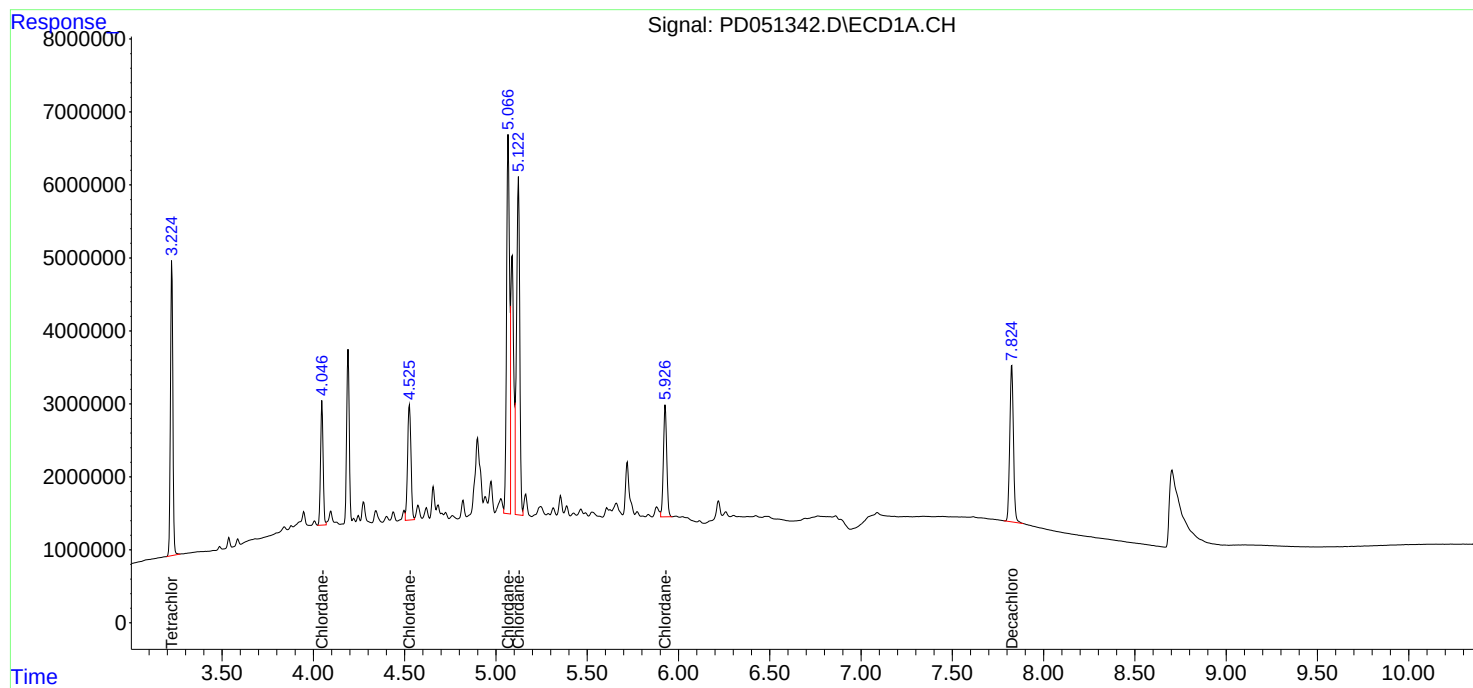


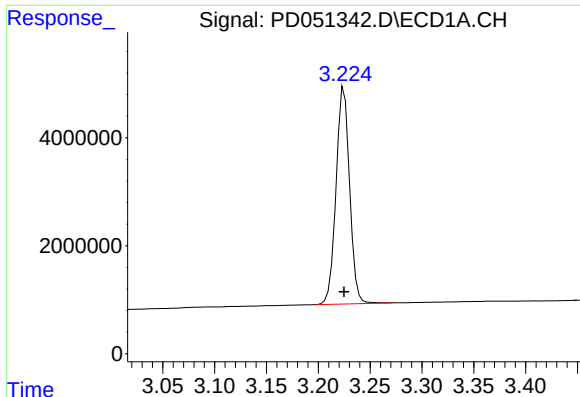

#1 Tetrachloro-m-xylene


R.T.: 3.225 min
Delta R.T.: 0.000 min
Response: 36578535
Conc: 23.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

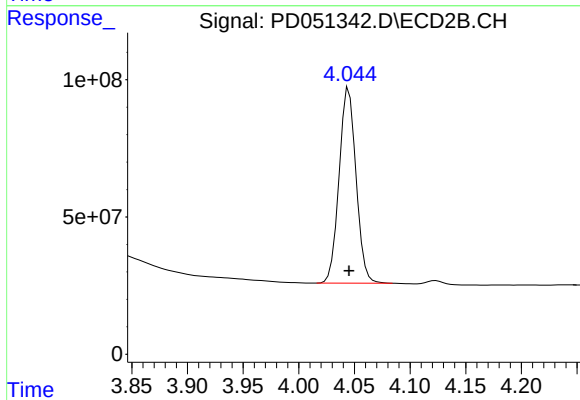


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 754915289
Conc: 25.62 ng/ml

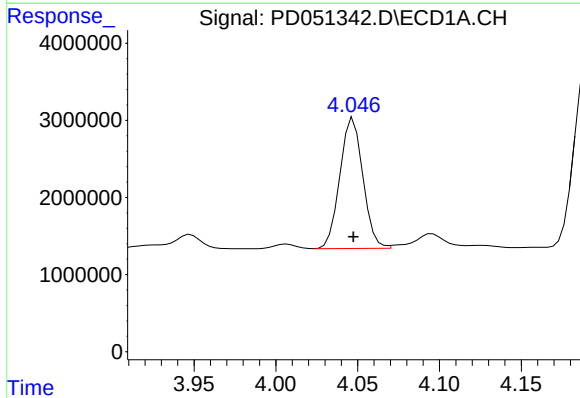


#23 Chlordane-1

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 16514835
Conc: 237.53 ng/ml

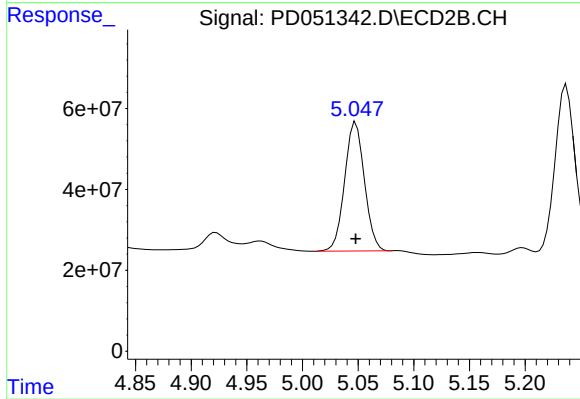

#23 Chlordane-1


R.T.: 5.048 min
Delta R.T.: 0.000 min
Response: 394700654
Conc: 257.55 ng/ml

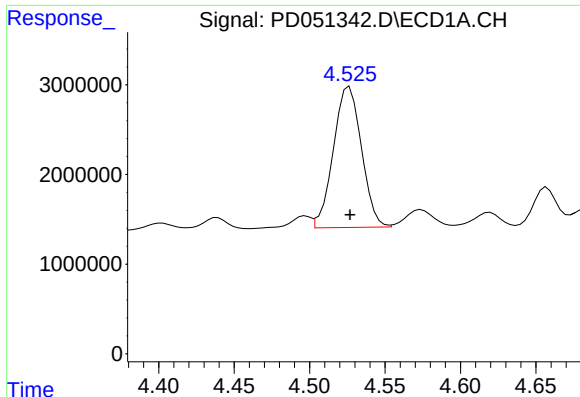

#24 Chlordane-2


R.T.: 4.526 min
Delta R.T.: 0.000 min
Response: 20357034
Conc: 246.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

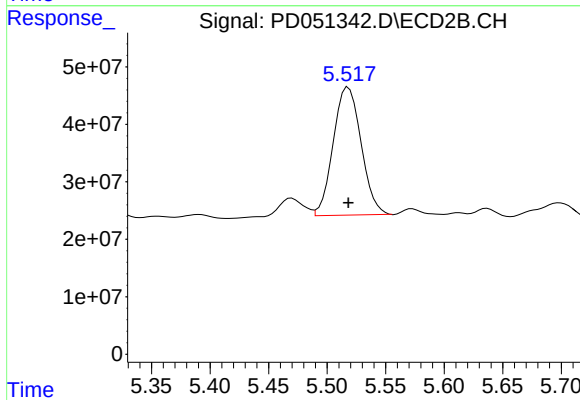


#24 Chlordane-2

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 369179051
Conc: 261.92 ng/ml

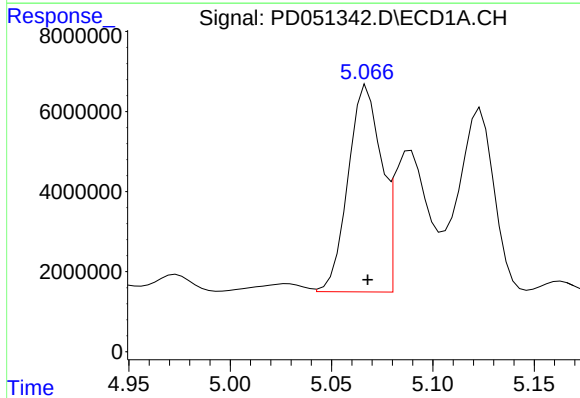


#25 Chlordane-3

R.T.: 5.068 min
Delta R.T.: 0.000 min
Response: 58429005
Conc: 227.27 ng/ml

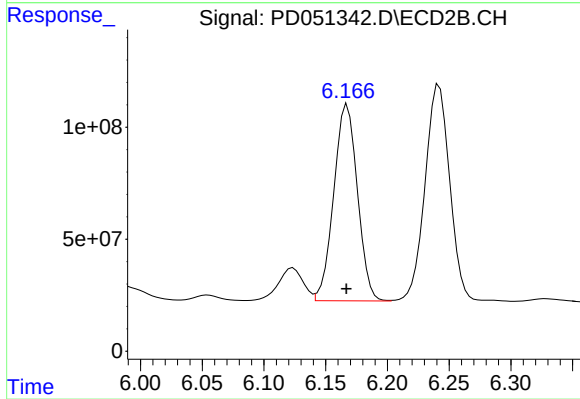

#25 Chlordane-3


R.T.: 6.168 min
Delta R.T.: 0.000 min
Response: 1171715340
Conc: 256.52 ng/ml

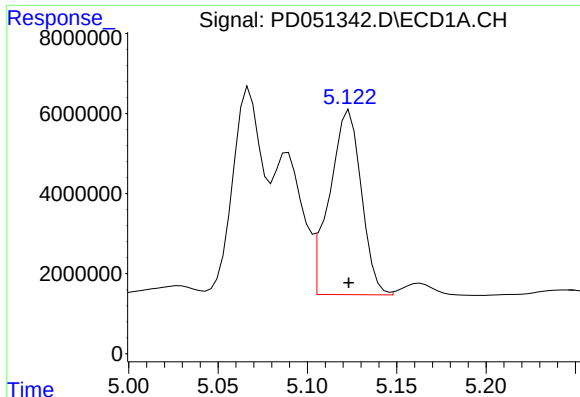

#26 Chlordane-4


R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 56988148
Conc: 231.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

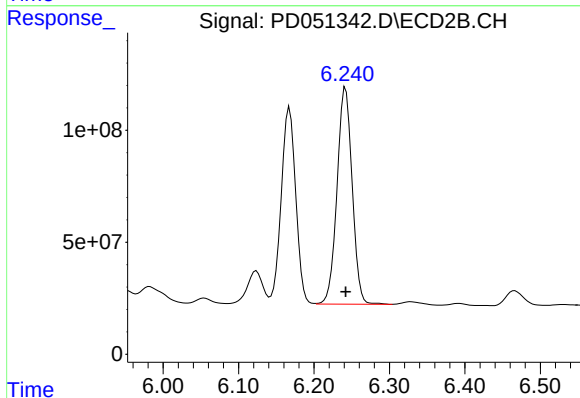


#26 Chlordane-4

R.T.: 6.242 min
Delta R.T.: 0.000 min
Response: 1349251484
Conc: 259.32 ng/ml

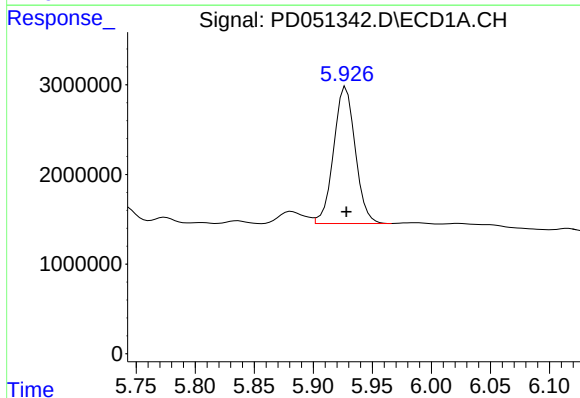


#27 Chlordane-5

R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 19448789
Conc: 237.98 ng/ml

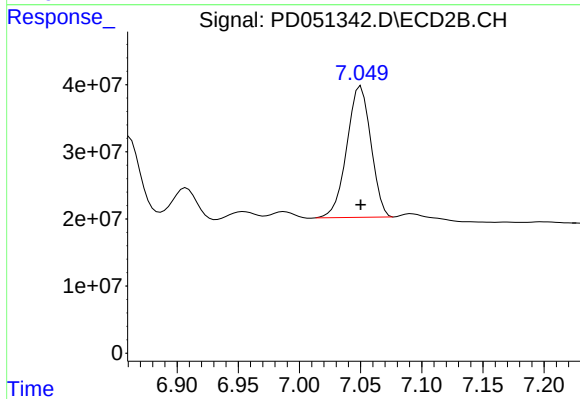

#27 Chlordane-5


R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 267998916
Conc: 257.00 ng/ml

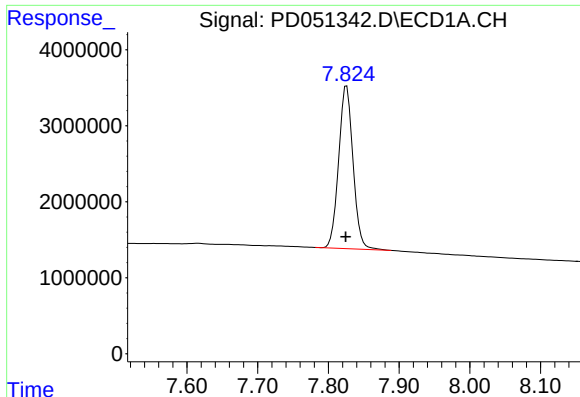

#28 Decachlorobiphenyl

R.T.: 7.826 min
Delta R.T.: 0.000 min
Response: 30223619
Conc: 26.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

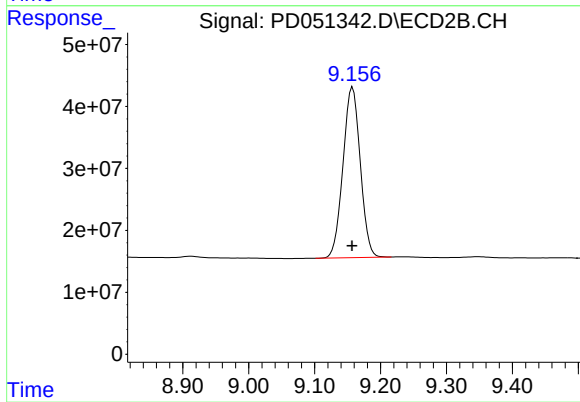

#28 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.000 min
Response: 501981239
Conc: 26.90 ng/ml