

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022324\
 Data File : PD081591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2024 14:27
 Operator : AR\AJ
 Sample : P1501-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E10A4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 22:03:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.793	29582342	54379217	21.638	22.181
27)	SA Decachlor...	9.108	7.927	47445512	66504152	24.591	26.809
Target Compounds							
3)	MA gamma-BHC...	0.000	3.614	0	270999	N.D.	<MDL
4)	MA Heptachlor	0.000	3.925f	0	545258	N.D.	0.154
6)	B beta-BHC	0.000	3.925	0	545258	N.D.	0.323
14)	MA Endrin	0.000	5.672	0	231972	N.D.	<MDL
15)	B Endosulfa...	0.000	5.891f	0	551621	N.D.	0.195
18)	B Endrin al...	0.000	6.161	0	227422	N.D.	0.105

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022324\
Data File : PD081591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 14:27
Operator : AR\AJ
Sample : P1501-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 22:03:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

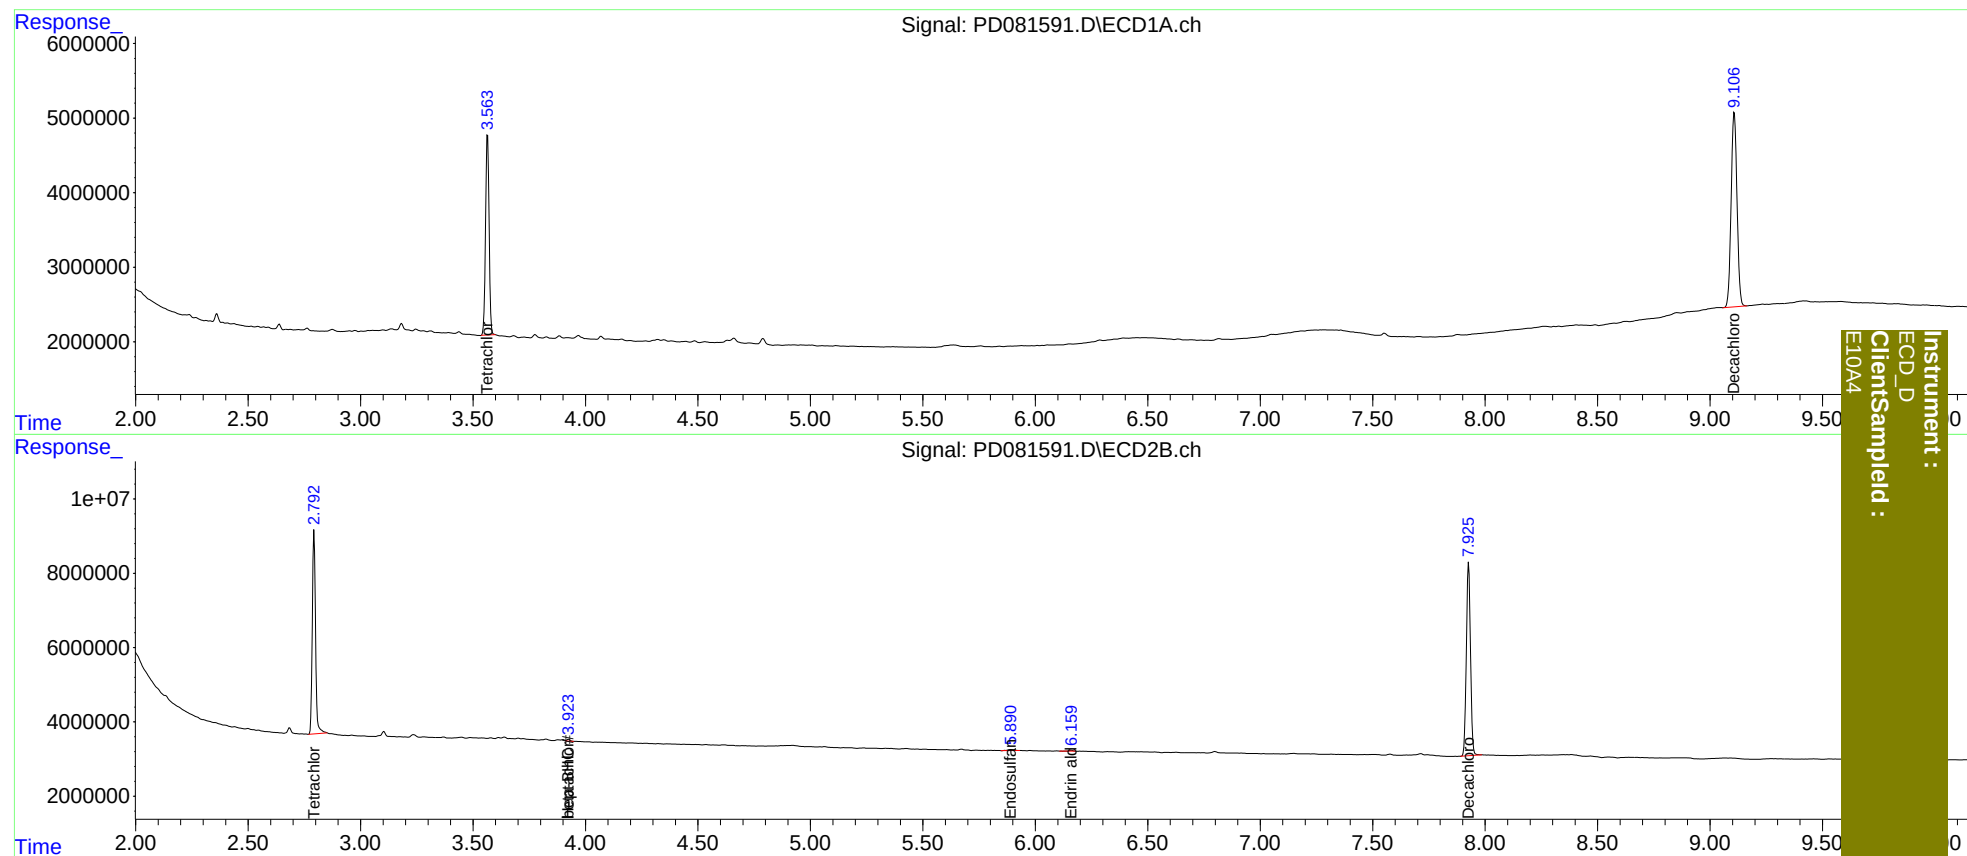


Instrument :
ECD_D
ClientSampled :
E10A4

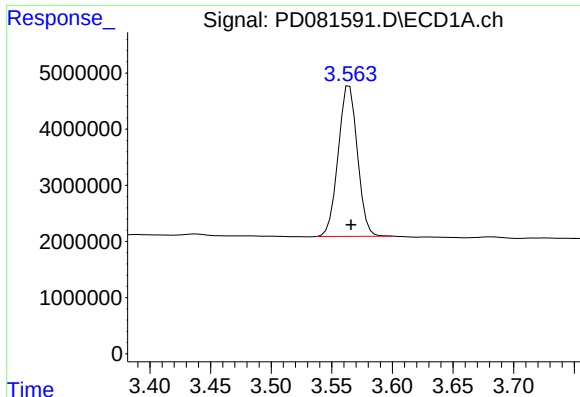

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: -0.001 min
Response: 29582342
Conc: 21.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
E10A4

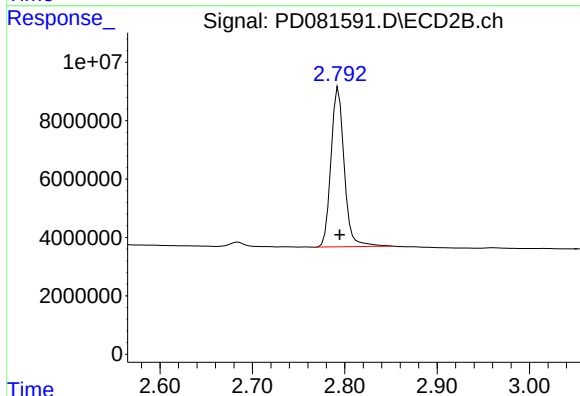


#1 Tetrachloro-m-xylene

R.T.: 2.793 min
Delta R.T.: -0.001 min
Response: 54379217
Conc: 22.18 ng/ml

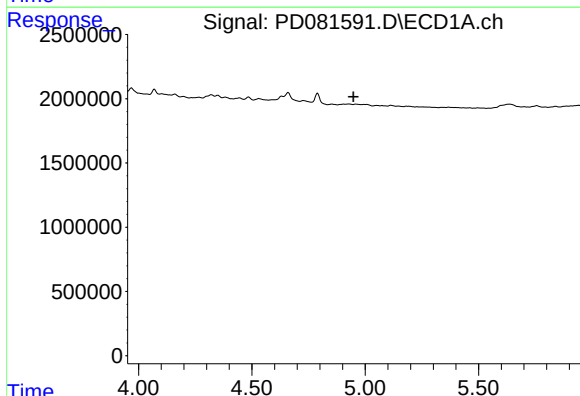


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.949 min
Response: 0
Conc: N.D.

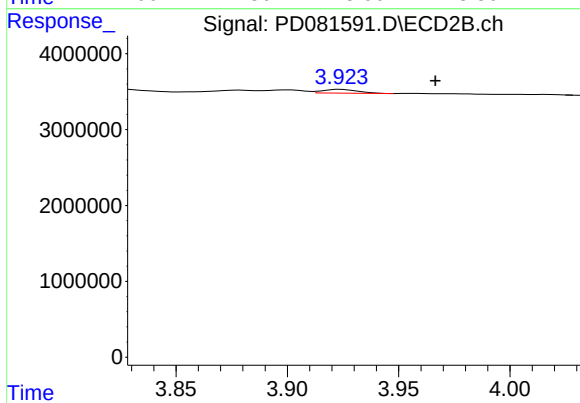

#4 Heptachlor


R.T.: 3.925 min
Delta R.T.: -0.042 min
Response: 545258
Conc: 0.15 ng/ml

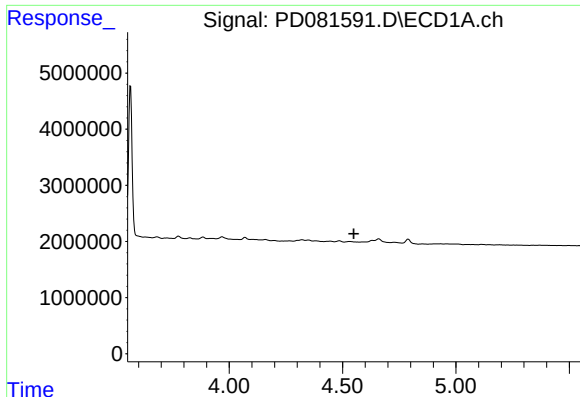

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
E10A4

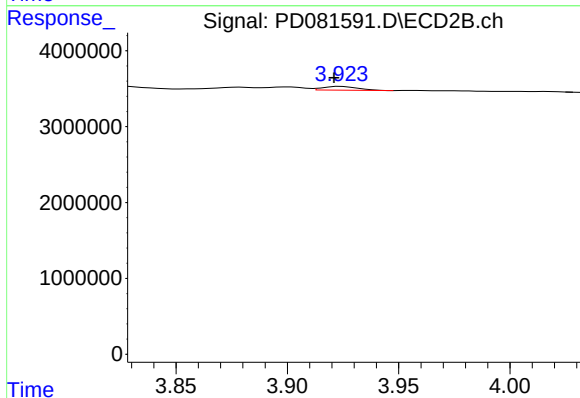


#6 beta-BHC

R.T.: 3.925 min
Delta R.T.: 0.004 min
Response: 545258
Conc: 0.32 ng/ml

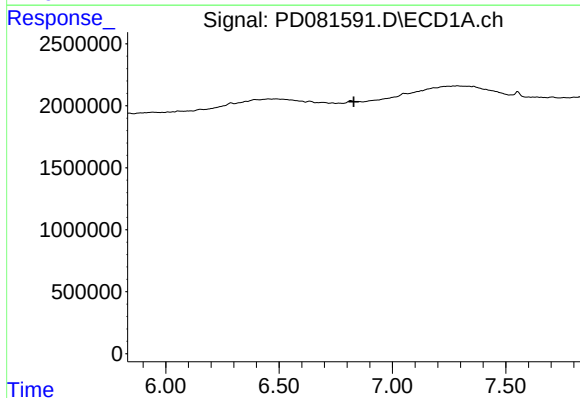


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.829 min
Response: 0
Conc: N.D.

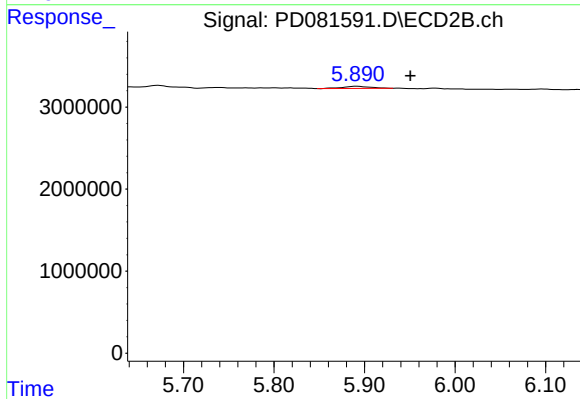

#15 Endosulfan II


R.T.: 5.891 min
Delta R.T.: -0.059 min
Response: 551621
Conc: 0.20 ng/ml

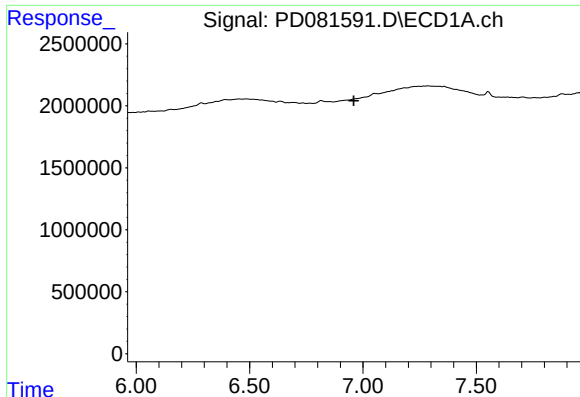

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
E10A4

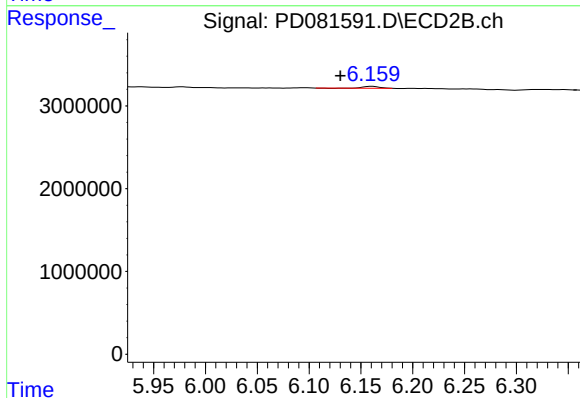


#18 Endrin aldehyde

R.T.: 6.161 min
Delta R.T.: 0.031 min
Response: 227422
Conc: 0.10 ng/ml

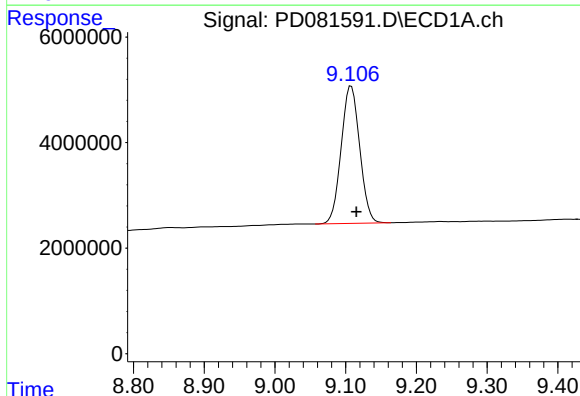

#27 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: -0.007 min
Response: 47445512
Conc: 24.59 ng/ml

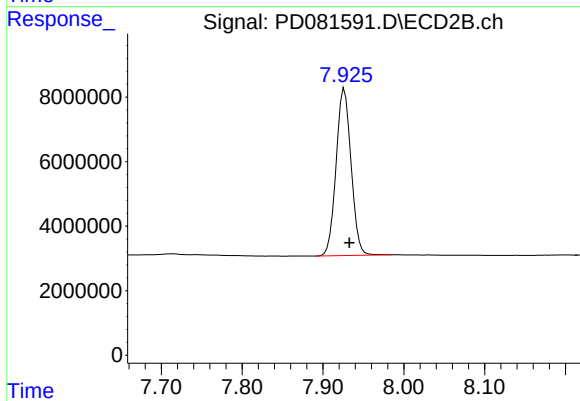

#27 Decachlorobiphenyl

R.T.: 7.927 min
Delta R.T.: -0.006 min
Response: 66504152
Conc: 26.81 ng/ml