

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022324\
 Data File : PD081592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2024 14:40
 Operator : AR\AJ
 Sample : P1469-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH9X6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 22:03:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.793	18788169	33594460	13.743	13.703
2)	SA Decachlor...	9.107	7.928	27471817	39269847	14.239	15.830
Target Compounds							
3)	MA gamma-BHC...	0.000	3.641	0	193765	N.D.	<MDL
4)	MA Heptachlor	0.000	3.930f	0	177374	N.D.	<MDL
5)	MB Aldrin	0.000	4.249	0	70695	N.D.	<MDL
6)	B beta-BHC	0.000	3.930	0	177374	N.D.	0.105
7)	B delta-BHC	4.789	0.000	1825279	0	0.771	N.D. #
9)	A Endosulfan I	0.000	5.163f	0	358196	N.D.	0.120
10)	B trans-Chl...	0.000	4.929f	0	885594	N.D.	0.284
14)	MA Endrin	0.000	5.671	0	1137193	N.D.	0.396
15)	B Endosulfa...	0.000	5.975	0	111768	N.D.	<MDL
17)	MA 4,4'-DDT	0.000	6.058	0	457055	N.D.	0.177
19)	B Endosulfa...	0.000	6.288f	0	411722	N.D.	0.153
20)	A Methoxychlor	0.000	6.667f	0	509513	N.D.	0.381
21)	B Endrin ke...	0.000	6.819f	0	82645	N.D.	<MDL
24)	Toxaphene-3	0.000	6.667f	0	509513	N.D.	8.705
25)	Toxaphene-4	0.000	6.730	0	237363	N.D.	2.983


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022324\
Data File : PD081592.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 14:40
Operator : AR\AJ
Sample : P1469-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 22:03:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

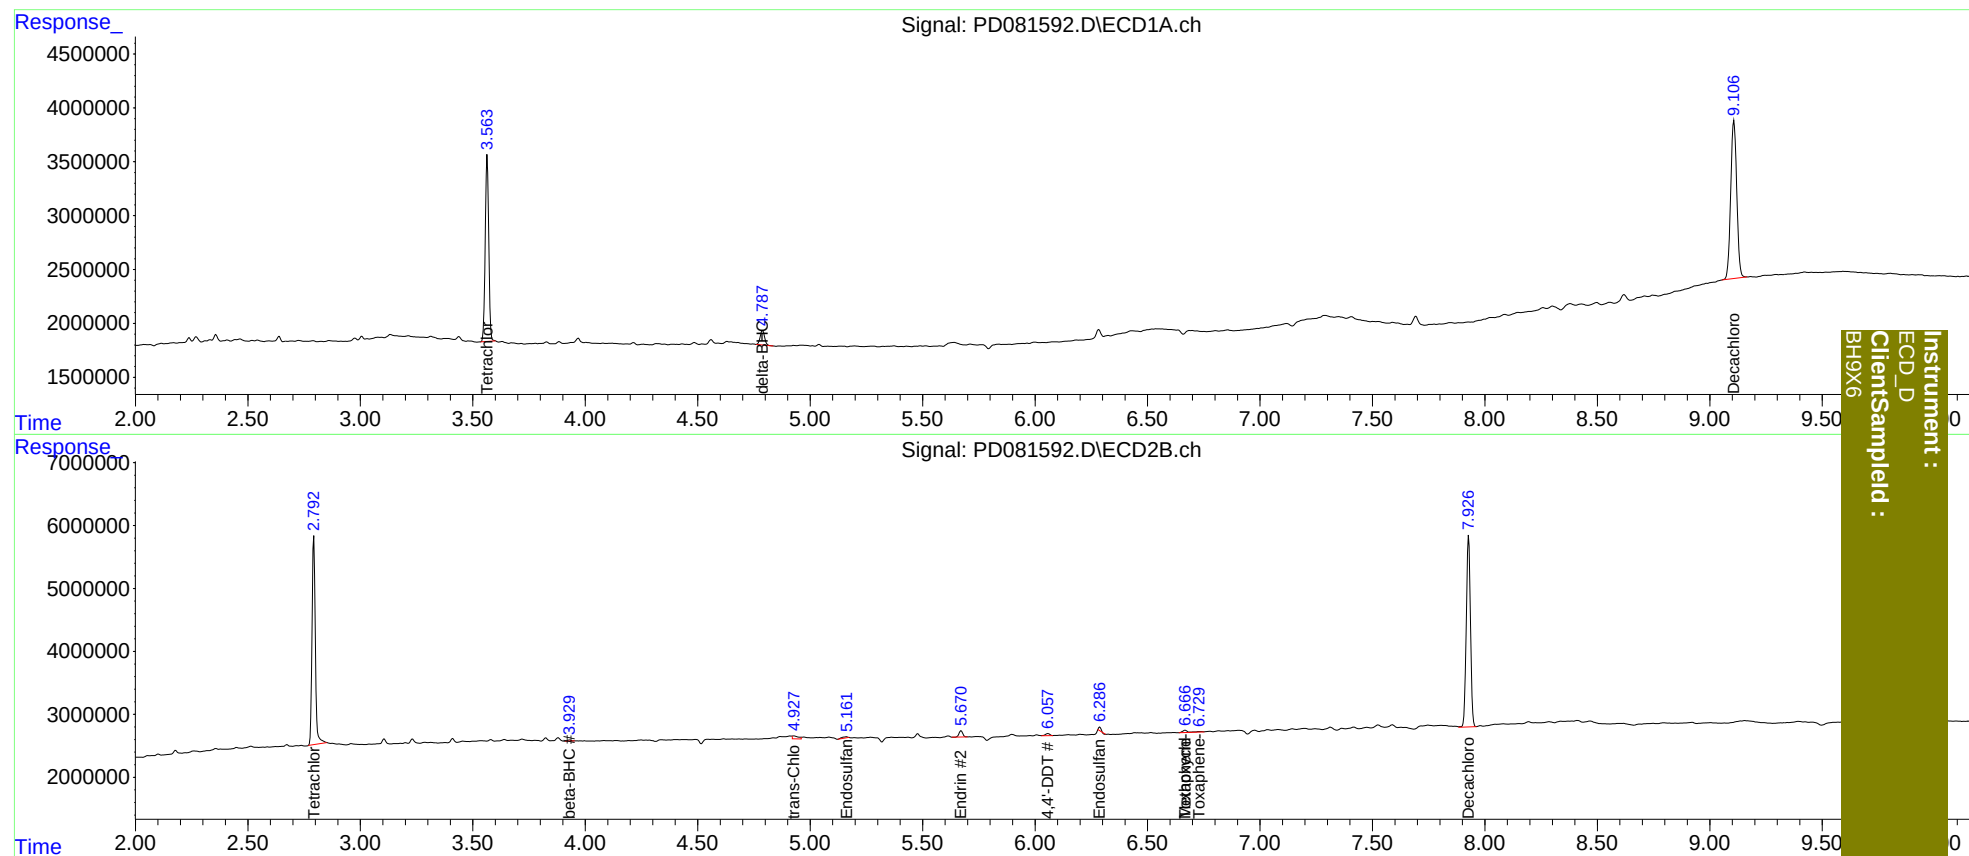


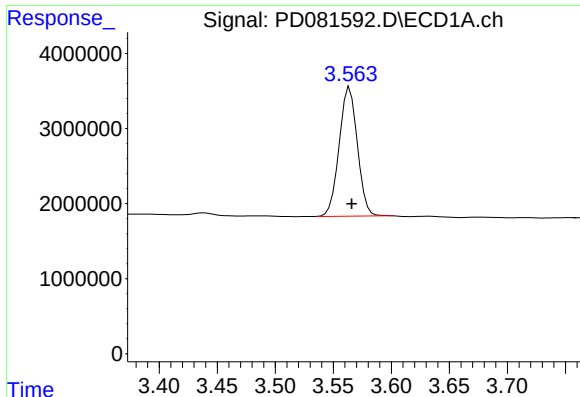

#1 Tetrachloro-m-xylene


R.T.: 3.564 min
Delta R.T.: -0.002 min
Response: 18788169
Conc: 13.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
BH9X6

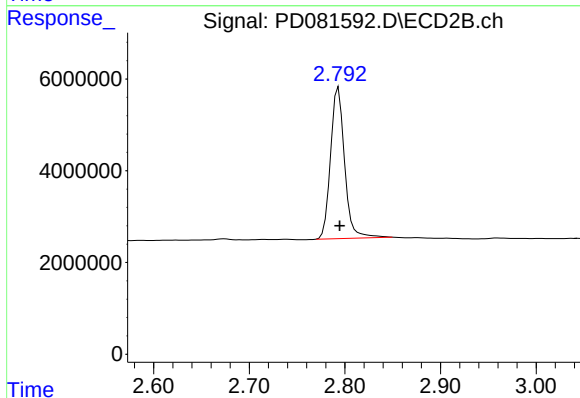


#1 Tetrachloro-m-xylene

R.T.: 2.793 min
Delta R.T.: -0.001 min
Response: 33594460
Conc: 13.70 ng/ml

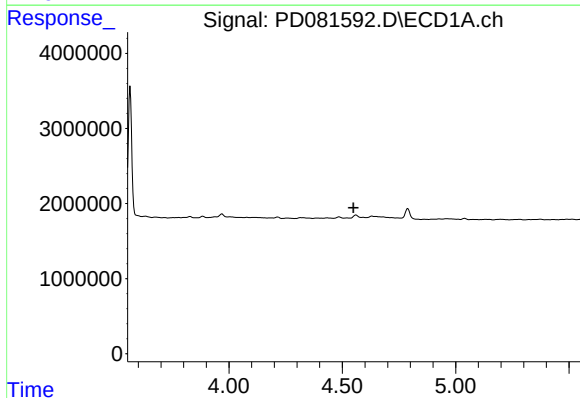


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.550 min
Response: 0
Conc: N.D.

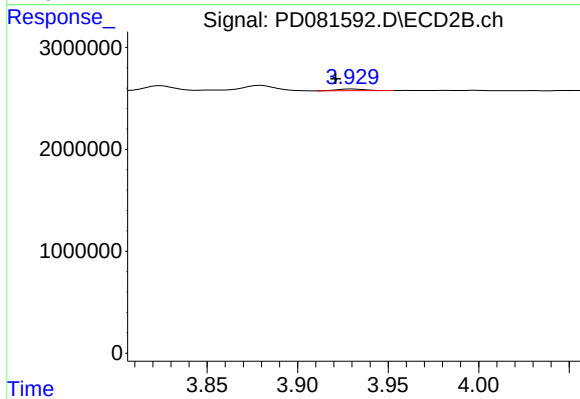

#6 beta-BHC


R.T.: 3.930 min
Delta R.T.: 0.009 min
Response: 177374
Conc: 0.10 ng/ml

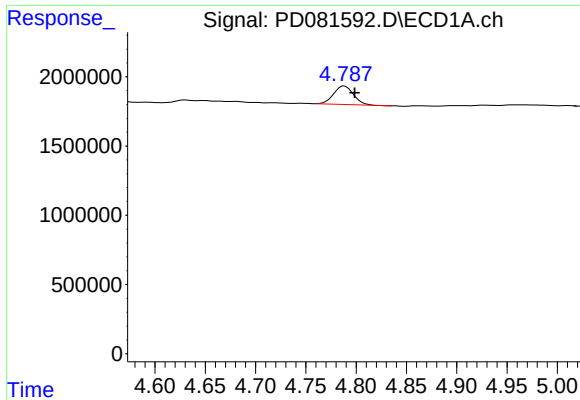

#7 delta-BHC


R.T.: 4.789 min
Delta R.T.: -0.010 min
Response: 1825279
Conc: 0.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
BH9X6

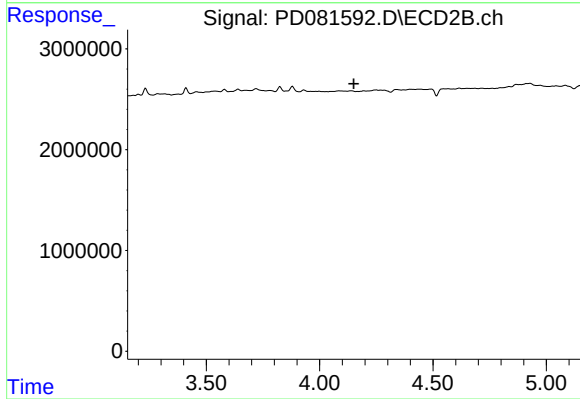


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.151 min
Response: 0
Conc: N.D.

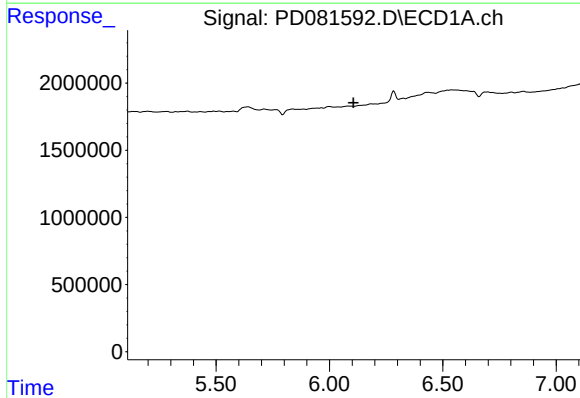


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.106 min
Response: 0
Conc: N.D.

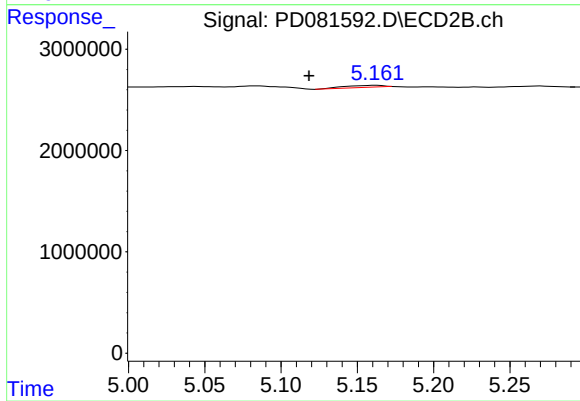

#9 Endosulfan I


R.T.: 5.163 min
Delta R.T.: 0.044 min
Response: 358196
Conc: 0.12 ng/ml

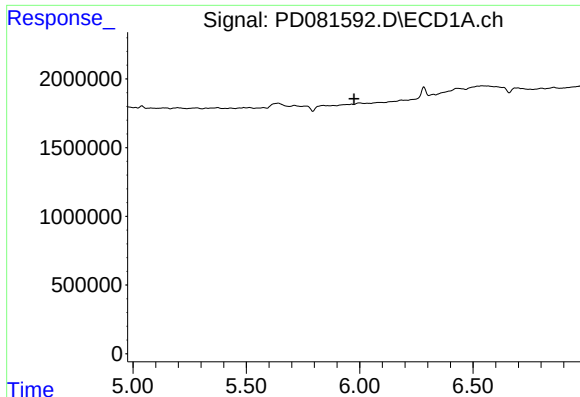

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BH9X6

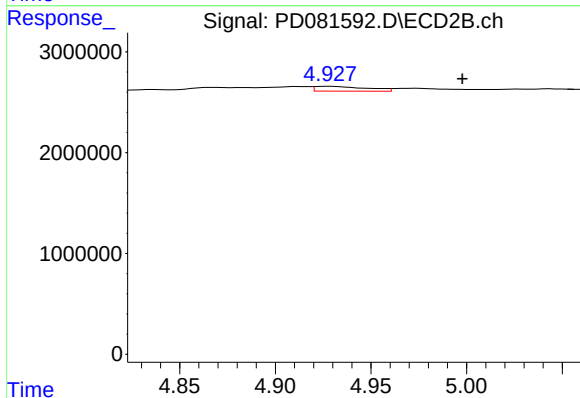


#10 trans-Chlordane

R.T.: 4.929 min
Delta R.T.: -0.069 min
Response: 885594
Conc: 0.28 ng/ml

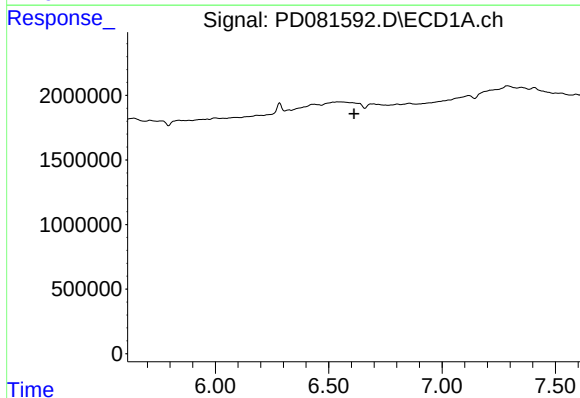


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

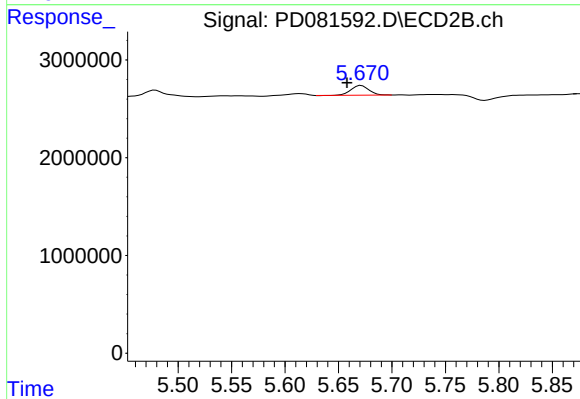

#14 Endrin


R.T.: 5.671 min
Delta R.T.: 0.013 min
Response: 1137193
Conc: 0.40 ng/ml

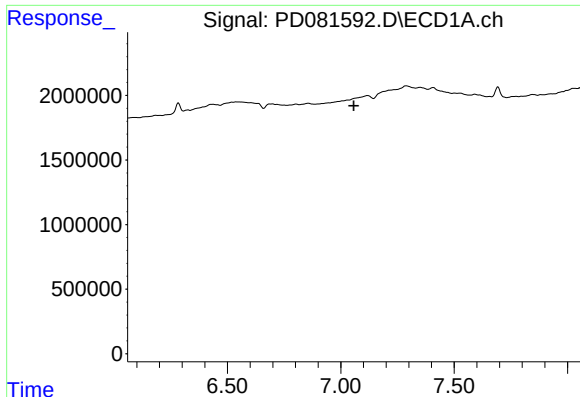

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.058 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BH9X6

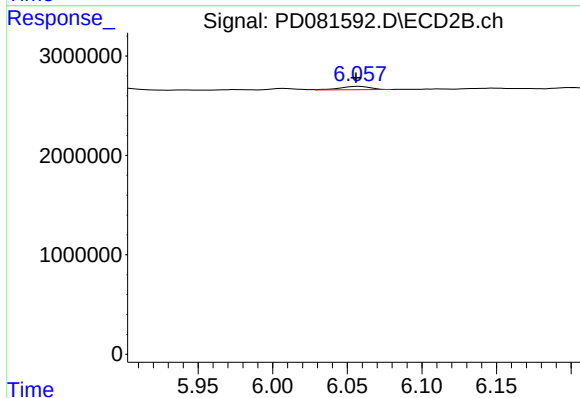


#17 4,4'-DDT

R.T.: 6.058 min
Delta R.T.: 0.002 min
Response: 457055
Conc: 0.18 ng/ml

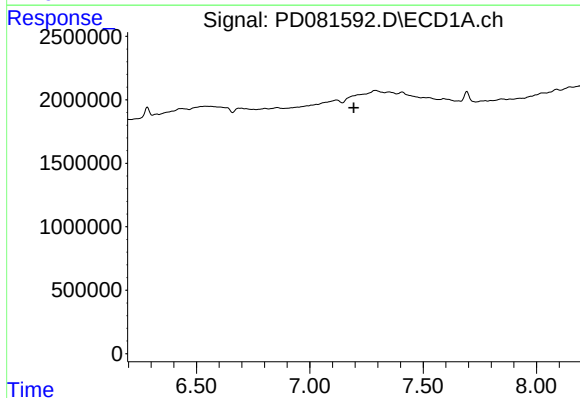


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.195 min
Response: 0
Conc: N.D.

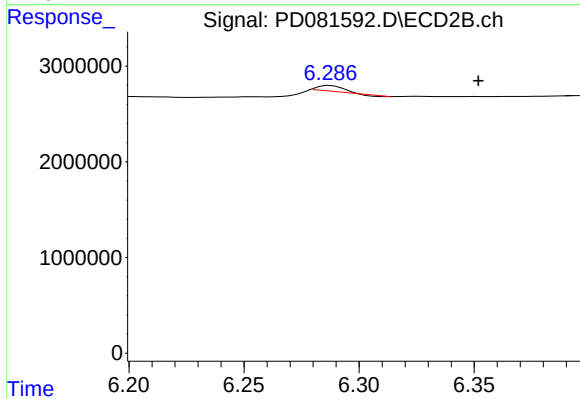

#19 Endosulfan Sulfate


R.T.: 6.288 min
Delta R.T.: -0.064 min
Response: 411722
Conc: 0.15 ng/ml

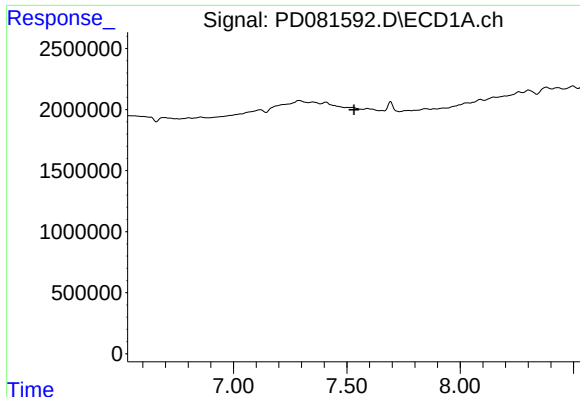

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.532 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BH9X6

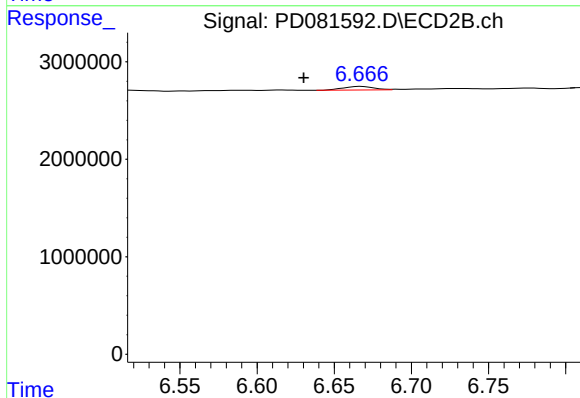


#20 Methoxychlor

R.T.: 6.667 min
Delta R.T.: 0.037 min
Response: 509513
Conc: 0.38 ng/ml

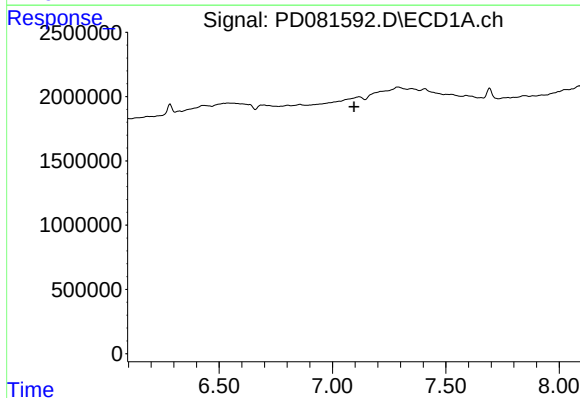


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T.: 7.096 min
Response: 0
Conc: N.D.

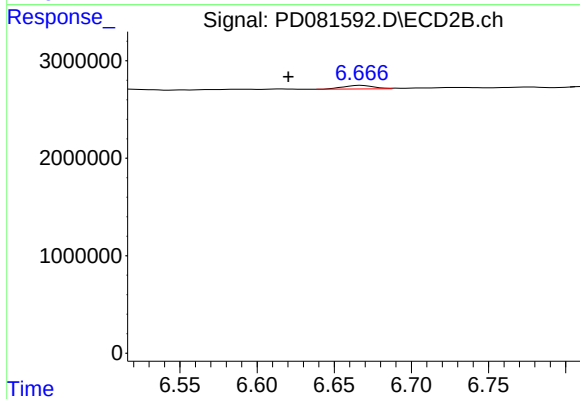

#24 Toxaphene-3


R.T.: 6.667 min
Delta R.T.: 0.047 min
Response: 509513
Conc: 8.70 ng/ml

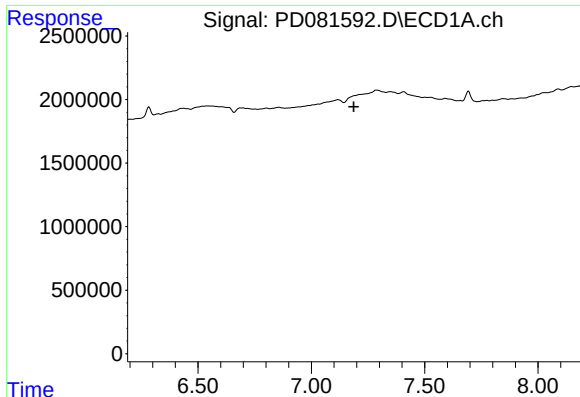

#25 Toxaphene-4


R.T.: 0.000 min
Exp R.T.: 7.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BH9X6

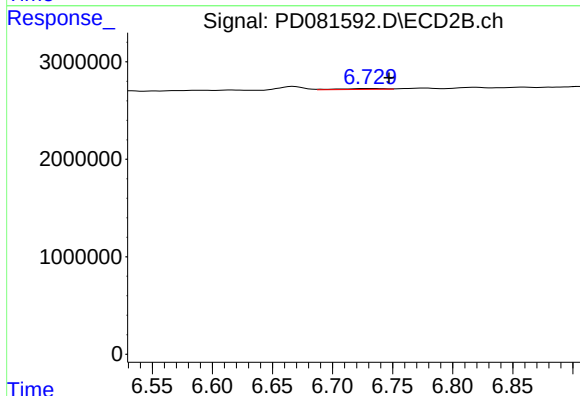


#25 Toxaphene-4

R.T.: 6.730 min
Delta R.T.: -0.016 min
Response: 237363
Conc: 2.98 ng/ml

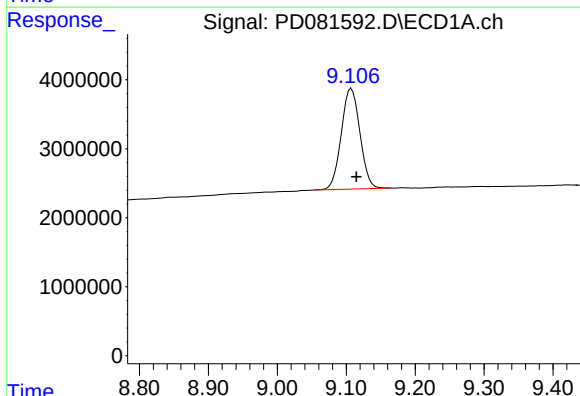

#27 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: -0.007 min
Response: 27471817
Conc: 14.24 ng/ml

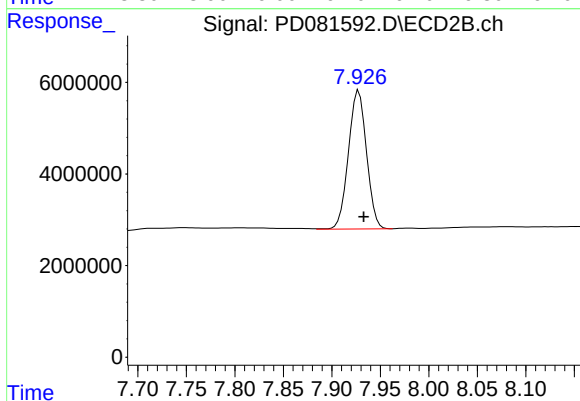

#27 Decachlorobiphenyl

R.T.: 7.928 min
Delta R.T.: -0.005 min
Response: 39269847
Conc: 15.83 ng/ml