

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD022324\  
 Data File : PD081576.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 21 Feb 2024 11:06  
 Operator : AR\AJ  
 Sample : P1501-03MS  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 E10A0MS

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 21 22:00:18 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD021224CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Feb 12 17:06:05 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|----------|---------|---------|
| -----                       |                 |       |       |          |          |         |         |
| System Monitoring Compounds |                 |       |       |          |          |         |         |
| 1)                          | SA Tetrachlo... | 3.565 | 2.794 | 29562851 | 54448690 | 21.624  | 22.210  |
| 2)                          | SA Decachlor... | 9.107 | 7.927 | 44548729 | 63170548 | 23.090  | 25.465  |
| Target Compounds            |                 |       |       |          |          |         |         |
| 2)                          | A alpha-BHC     | 4.021 | 3.294 | 125.6E6  | 210.3E6  | 53.777  | 54.684  |
| 3)                          | MA gamma-BHC... | 4.354 | 3.623 | 117.0E6  | 188.7E6  | 50.653  | 52.094  |
| 4)                          | MA Heptachlor   | 4.947 | 3.964 | 124.0E6  | 181.1E6  | 50.542  | 51.062  |
| 5)                          | MB Aldrin       | 5.290 | 4.244 | 120.3E6  | 177.6E6  | 50.871  | 52.434  |
| 6)                          | B beta-BHC      | 4.548 | 3.918 | 51198154 | 81117429 | 49.266  | 48.007  |
| 7)                          | B delta-BHC     | 4.798 | 4.149 | 125.3E6  | 195.5E6  | 52.910  | 52.216  |
| 8)                          | B Heptachlo...  | 5.716 | 4.745 | 111.0E6  | 167.3E6  | 49.014  | 52.141  |
| 9)                          | A Endosulfan I  | 6.102 | 5.115 | 103.8E6  | 157.6E6  | 49.276  | 52.634  |
| 10)                         | B trans-Chl...  | 5.972 | 4.995 | 106.6E6  | 165.1E6  | 48.690  | 52.918  |
| 11)                         | B cis-Chlor...  | 6.051 | 5.059 | 107.7E6  | 165.5E6  | 47.828  | 51.663  |
| 12)                         | B 4,4'-DDE      | 6.222 | 5.247 | 208.5E6  | 320.1E6  | 97.112  | 108.252 |
| 13)                         | MA Dieldrin     | 6.377 | 5.379 | 241.7E6  | 347.9E6  | 108.847 | 105.919 |
| 14)                         | MA Endrin       | 6.608 | 5.654 | 193.4E6  | 295.7E6  | 103.066 | 102.911 |
| 15)                         | B Endosulfa...  | 6.826 | 5.946 | 204.0E6  | 303.1E6  | 105.684 | 107.386 |
| 16)                         | A 4,4'-DDD      | 6.739 | 5.800 | 179.5E6  | 273.0E6  | 108.076 | 108.326 |
| 17)                         | MA 4,4'-DDT     | 7.054 | 6.052 | 183.0E6  | 274.1E6  | 105.319 | 106.136 |
| 18)                         | B Endrin al...  | 6.956 | 6.126 | 145.6E6  | 217.8E6  | 97.456  | 100.516 |
| 19)                         | B Endosulfa...  | 7.190 | 6.348 | 183.5E6  | 281.2E6  | 100.252 | 104.828 |
| 20)                         | A Methoxychlor  | 7.528 | 6.626 | 449.8E6  | 644.1E6  | 490.318 | 482.076 |
| 21)                         | B Endrin ke...  | 7.677 | 6.854 | 211.6E6  | 327.3E6  | 109.404 | 109.136 |
| -----                       |                 |       |       |          |          |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD022324\  
Data File : PD081576.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 21 Feb 2024 11:06  
Operator : AR\AJ  
Sample : P1501-03MS  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 21 22:00:18 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD021224CLP.M  
Quant Title : GC Extractables  
QLast Update : Mon Feb 12 17:06:05 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

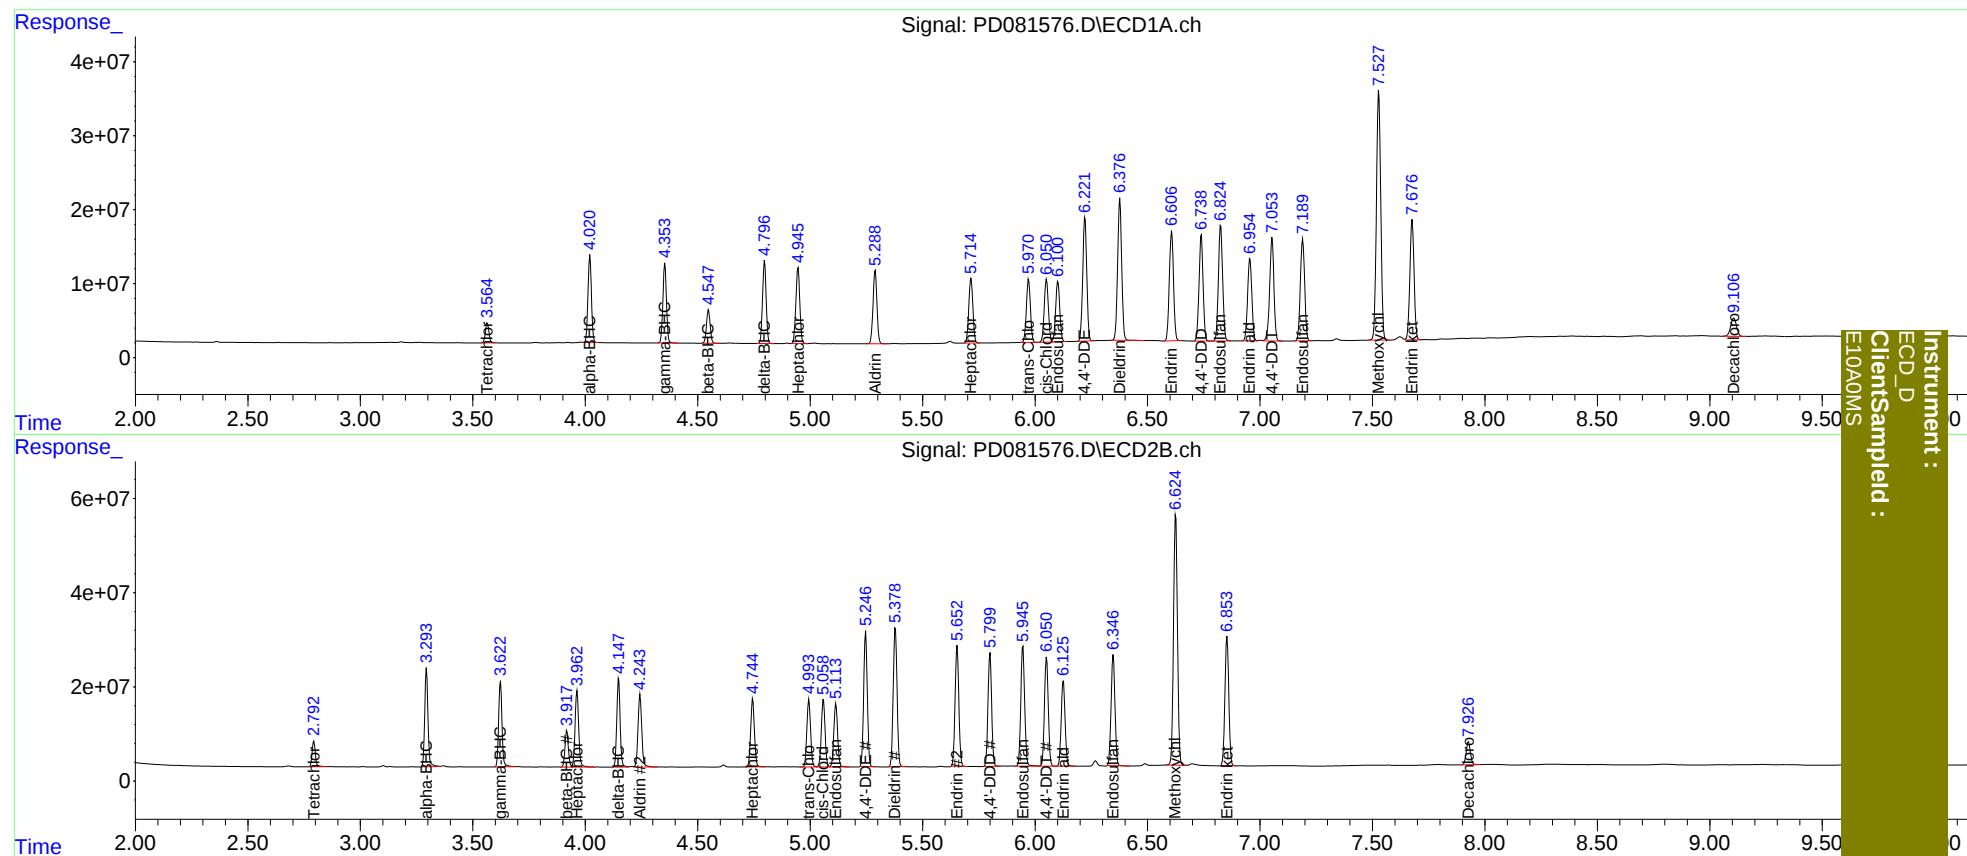

Instrument :  
ECD\_D  
ClientSampled :  
E10A0MS