

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022324\
 Data File : PD081576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2024 11:06
 Operator : AR\AJ
 Sample : P1501-03MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E10A0MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 22:00:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.794	29562851	54448690	21.624	22.210
2)	SA Decachlor...	9.107	7.927	44548729	63170548	23.090	25.465
Target Compounds							
2)	A alpha-BHC	4.021	3.294	125.6E6	210.3E6	53.777	54.684
3)	MA gamma-BHC...	4.354	3.623	117.0E6	188.7E6	50.653	52.094
4)	MA Heptachlor	4.947	3.964	124.0E6	181.1E6	50.542	51.062
5)	MB Aldrin	5.290	4.244	120.3E6	177.6E6	50.871	52.434
6)	B beta-BHC	4.548	3.918	51198154	81117429	49.266	48.007
7)	B delta-BHC	4.798	4.149	125.3E6	195.5E6	52.910	52.216
8)	B Heptachlo...	5.716	4.745	111.0E6	167.3E6	49.014	52.141
9)	A Endosulfan I	6.102	5.115	103.8E6	157.6E6	49.276	52.634
10)	B trans-Chl...	5.972	4.995	106.6E6	165.1E6	48.690	52.918
11)	B cis-Chlor...	6.051	5.059	107.7E6	165.5E6	47.828	51.663
12)	B 4,4'-DDE	6.222	5.247	208.5E6	320.1E6	97.112	108.252
13)	MA Dieldrin	6.377	5.379	241.7E6	347.9E6	108.847	105.919
14)	MA Endrin	6.608	5.654	193.4E6	295.7E6	103.066	102.911
15)	B Endosulfa...	6.826	5.946	204.0E6	303.1E6	105.684	107.386
16)	A 4,4'-DDD	6.739	5.800	179.5E6	273.0E6	108.076	108.326
17)	MA 4,4'-DDT	7.054	6.052	183.0E6	274.1E6	105.319	106.136
18)	B Endrin al...	6.956	6.126	145.6E6	217.8E6	97.456	100.516
19)	B Endosulfa...	7.190	6.348	183.5E6	281.2E6	100.252	104.828
20)	A Methoxychlor	7.528	6.626	449.8E6	644.1E6	490.318	482.076
21)	B Endrin ke...	7.677	6.854	211.6E6	327.3E6	109.404	109.136

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022324\
Data File : PD081576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 11:06
Operator : AR\AJ
Sample : P1501-03MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 22:00:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

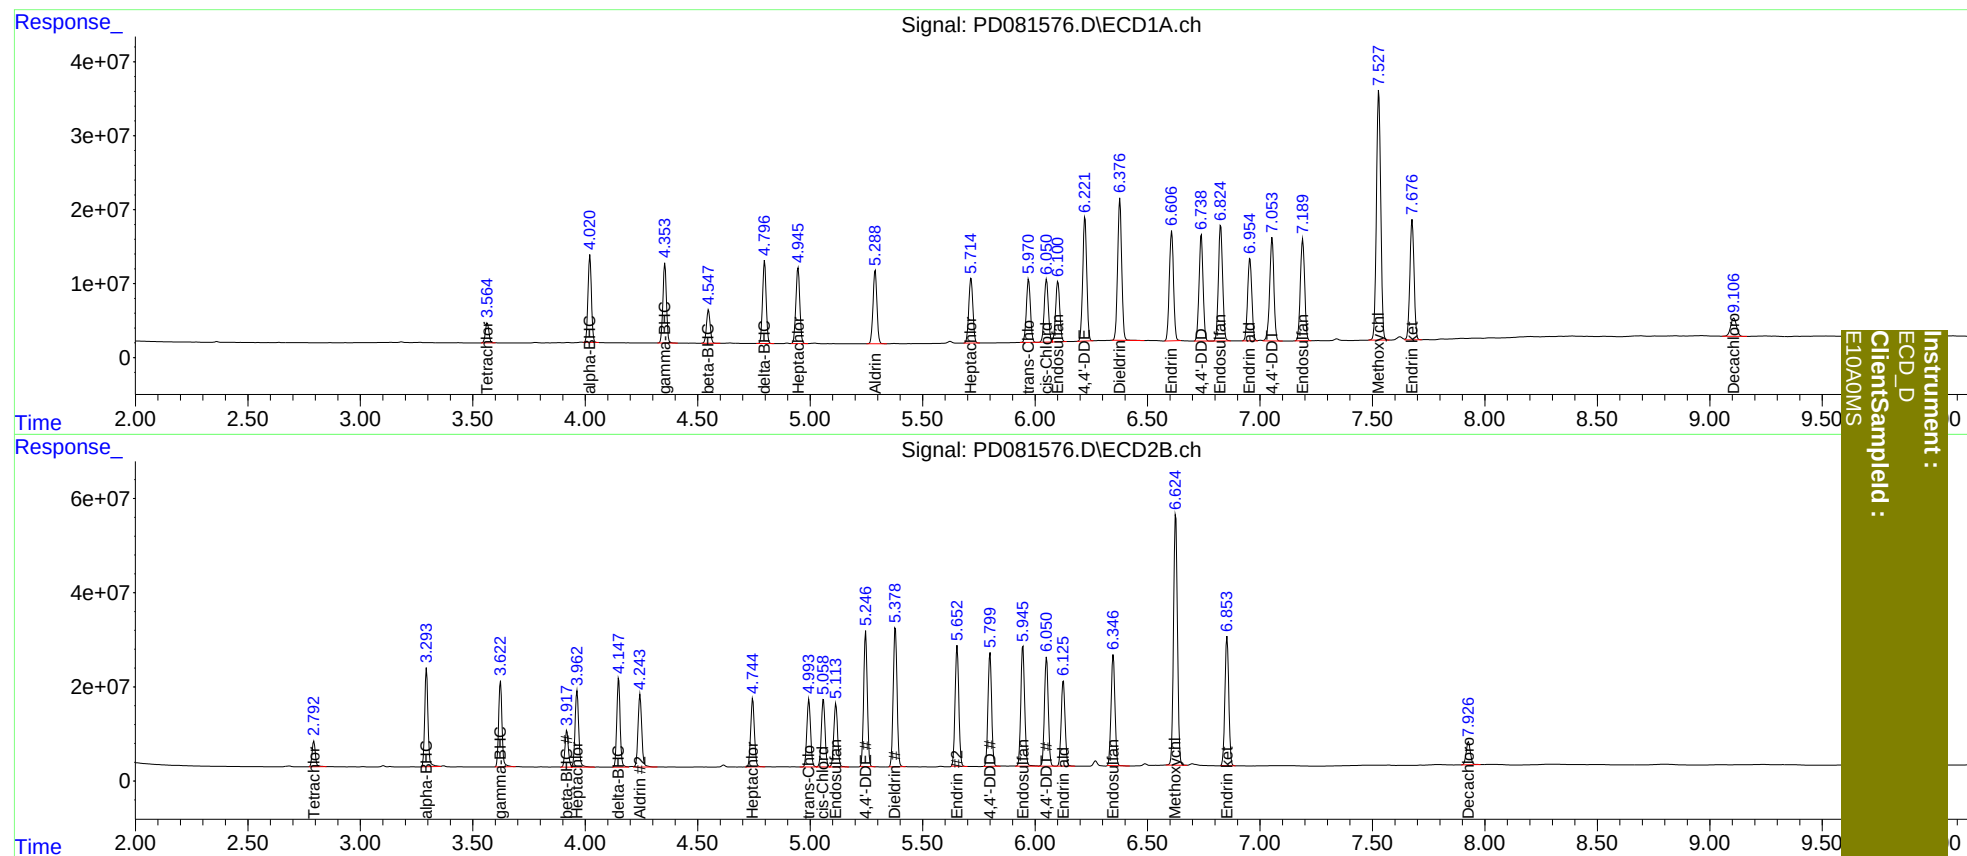

Instrument :
ECD_D
ClientSampled :
E10A0MS