

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022422\
 Data File : PD068175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2022 14:53
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/25/2022
 Supervised By :Ankita Jodhani 02/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 06:50:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 13:55:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.457	4.175	75679133	470.6E6	52.551	52.212
7) SA Decachlor...	8.224	9.374	71392222	256.4E6	50.755	52.424
Target Compounds						
2) Toxaphene-1	5.720	6.195	6289331	13476855	490.257	537.956
3) Toxaphene-2	5.937	6.799	9970893	52392734	543.629	514.063
4) Toxaphene-3	6.323	7.479	16046747	64516822	531.678	534.447
5) Toxaphene-4	6.570	7.618	16510409	22877099	529.564	503.904
6) Toxaphene-5	7.056	7.891	16570160	43381811	529.087m	538.231

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022422\
Data File : PD068175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2022 14:53
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 06:50:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 13:55:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

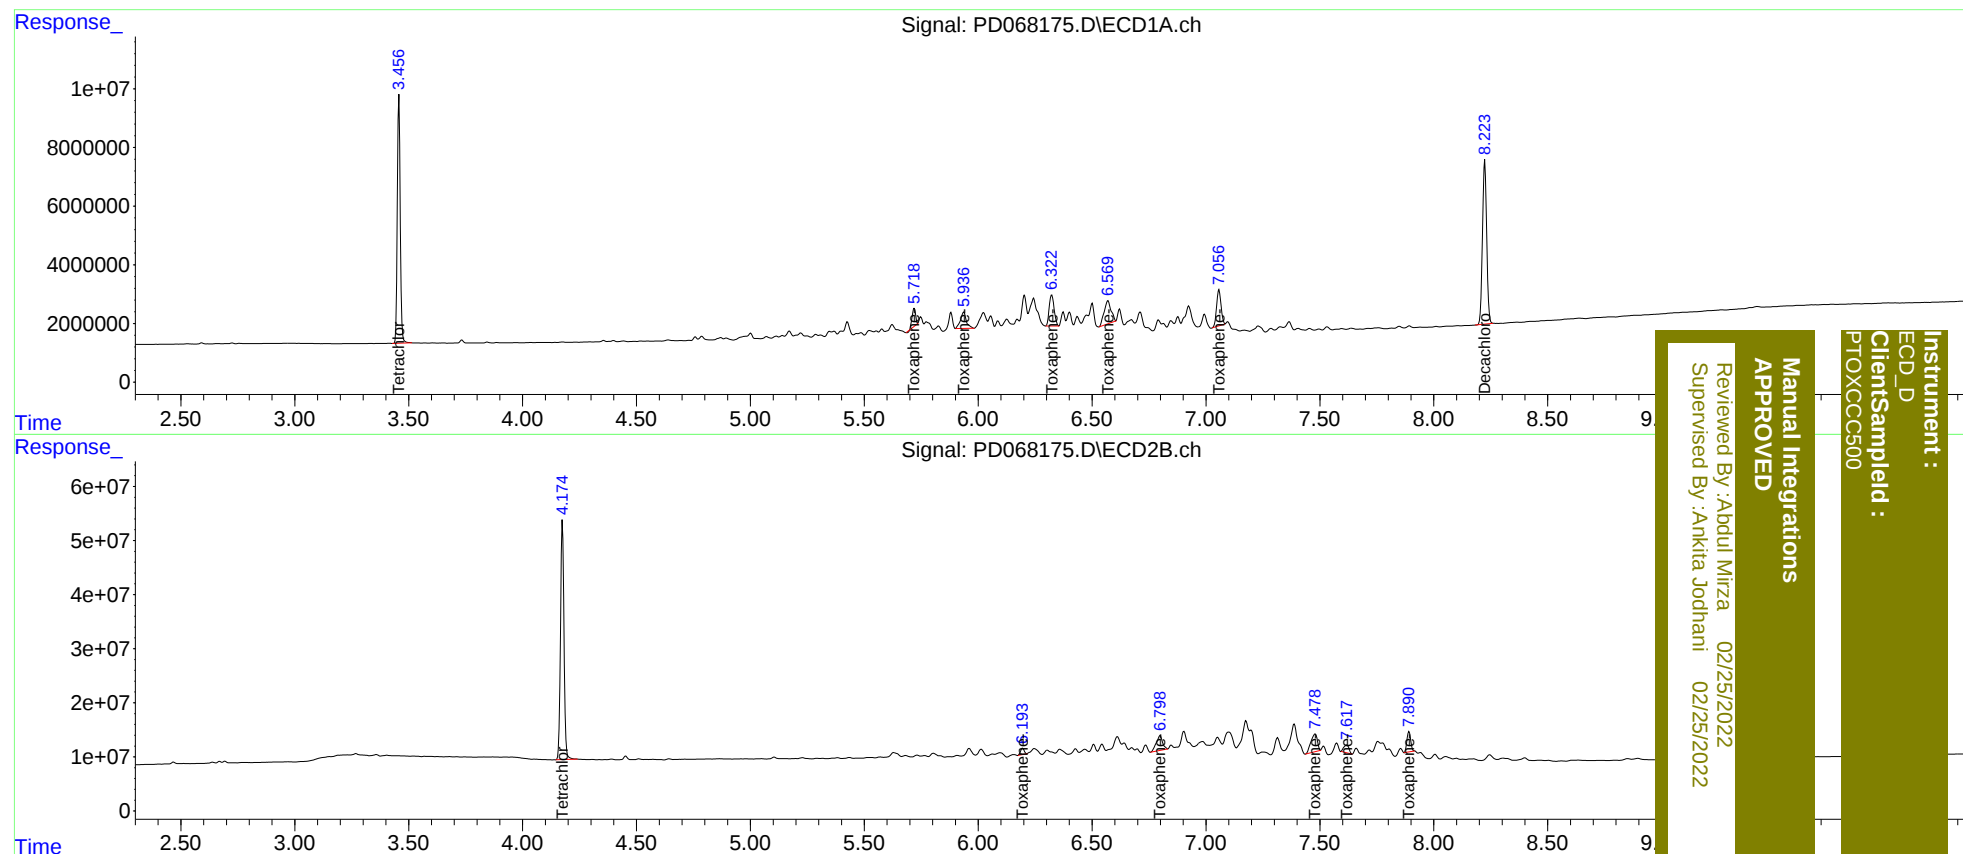

Reviewed By: Abdul Mirza 02/25/2022
Supervised By: Ankita Jodhani 02/25/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
PTOXCCC500