

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022422\
 Data File : PD068174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2022 14:16
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 01:04:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 13:16:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.176	85541474	451.7E6	58.759	48.846
28)	SA Decachlor...	8.224	9.374	68671871	247.0E6	47.922	49.615
Target Compounds							
23)	Chlordane-1	4.330	5.198	29345255	201.0E6	483.594	480.061
24)	Chlordane-2	4.833	5.672	34833164	195.3E6	495.103	473.549
25)	Chlordane-3	5.402	6.328	105.5E6	700.8E6	506.489	482.825
26)	Chlordane-4	5.460	6.405	88611753	811.3E6	503.874	486.734
27)	Chlordane-5	6.299	7.217	33195253	139.1E6	502.798	517.554



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022422\
Data File : PD068174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2022 14:16
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 01:04:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 13:16:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

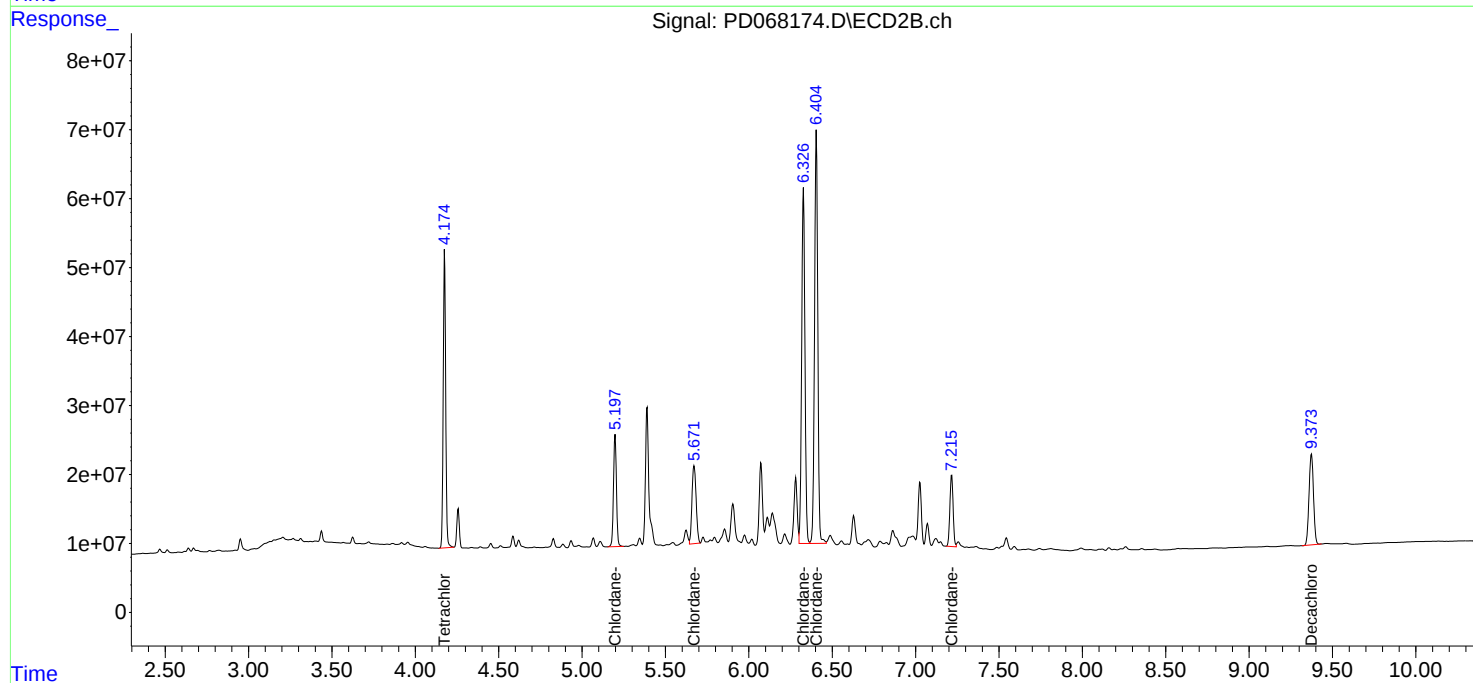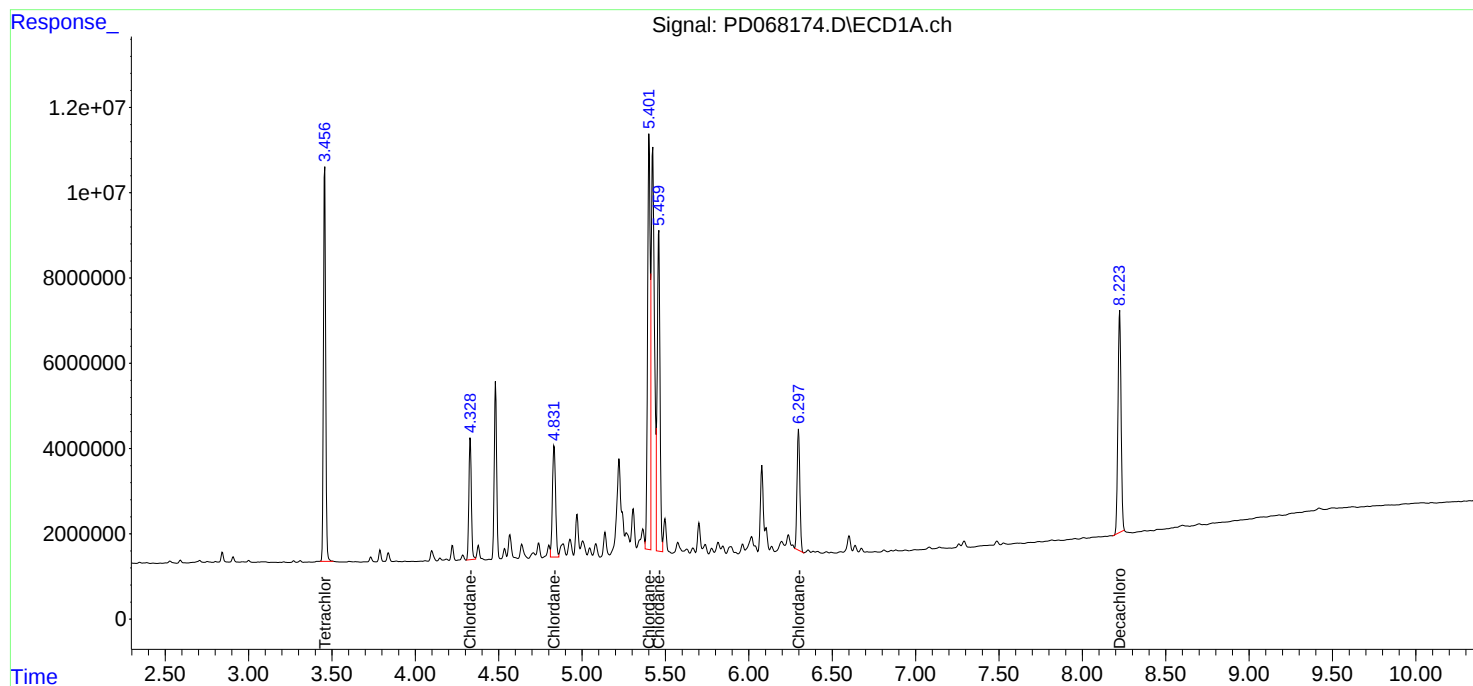


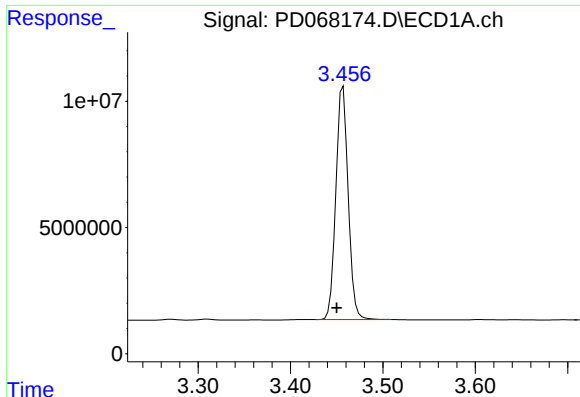

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.007 min
Response: 85541474
Conc: 58.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

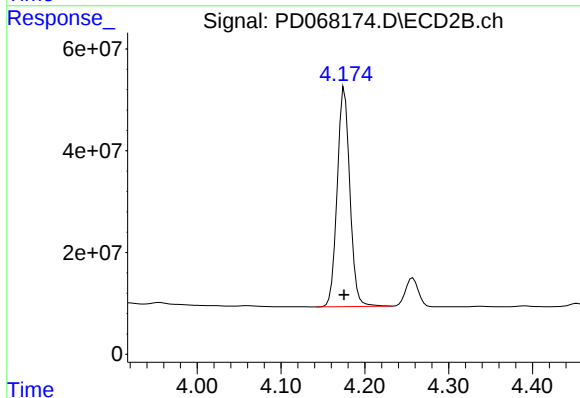


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 451706640
Conc: 48.85 ng/ml

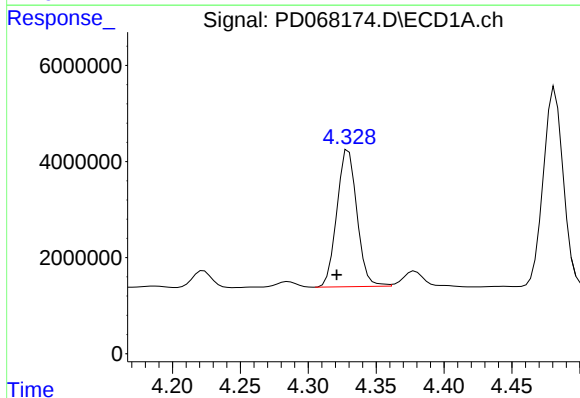


#23 Chlordane-1

R.T.: 4.330 min
Delta R.T.: 0.009 min
Response: 29345255
Conc: 483.59 ng/ml

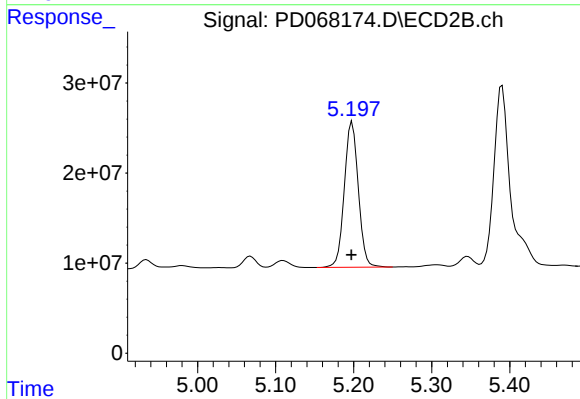

#23 Chlordane-1


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 200970079
Conc: 480.06 ng/ml

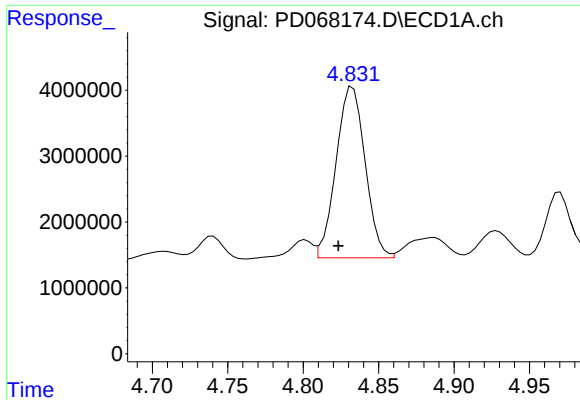

#24 Chlordane-2


R.T.: 4.833 min
Delta R.T.: 0.009 min
Response: 34833164
Conc: 495.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

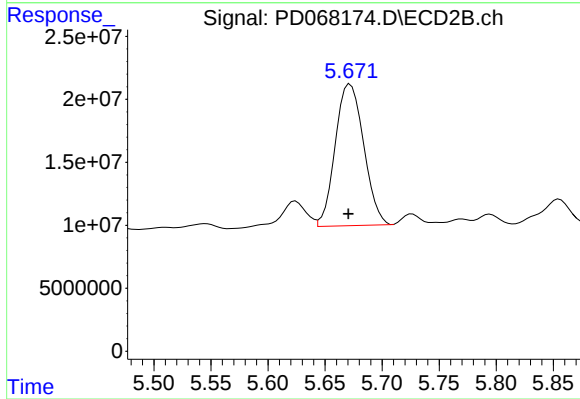


#24 Chlordane-2

R.T.: 5.672 min
Delta R.T.: 0.002 min
Response: 195270615
Conc: 473.55 ng/ml

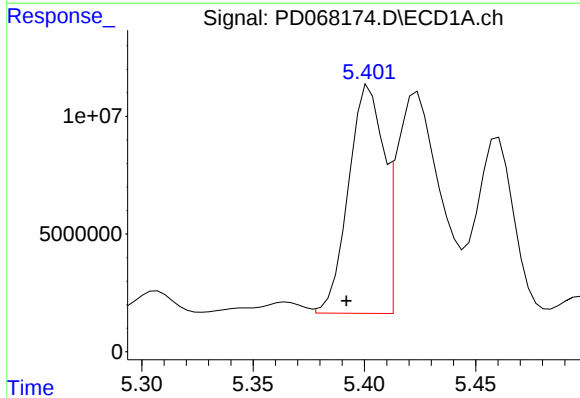


#25 Chlordane-3

R.T.: 5.402 min
Delta R.T.: 0.011 min
Response: 105539573
Conc: 506.49 ng/ml

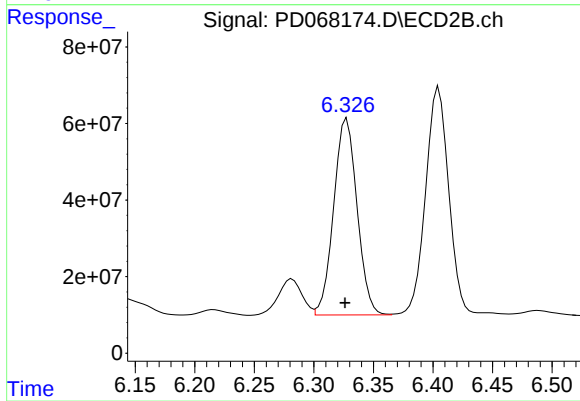

#25 Chlordane-3


R.T.: 6.328 min
Delta R.T.: 0.002 min
Response: 700834504
Conc: 482.82 ng/ml

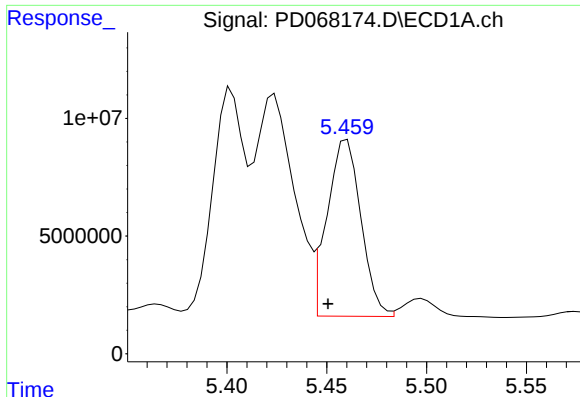

#26 Chlordane-4


R.T.: 5.460 min
Delta R.T.: 0.010 min
Response: 88611753
Conc: 503.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

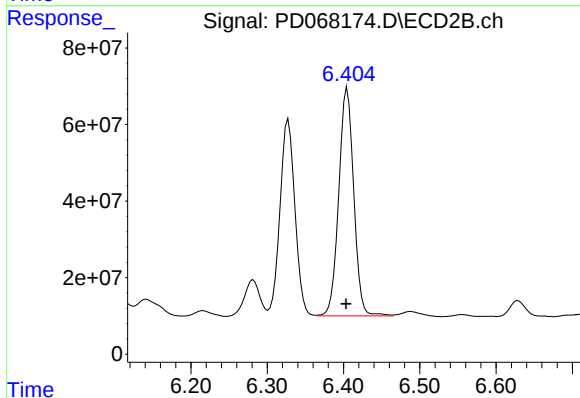


#26 Chlordane-4

R.T.: 6.405 min
Delta R.T.: 0.002 min
Response: 811335918
Conc: 486.73 ng/ml

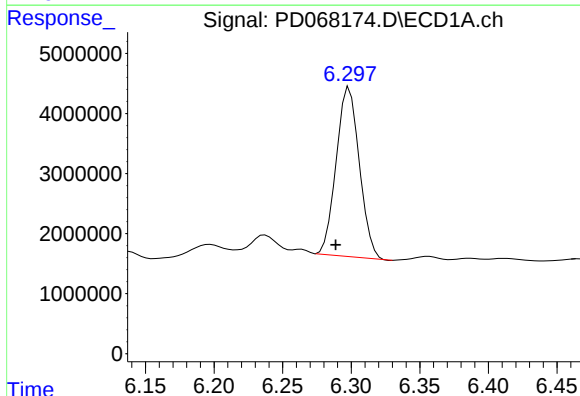


#27 Chlordane-5

R.T.: 6.299 min
Delta R.T.: 0.010 min
Response: 33195253
Conc: 502.80 ng/ml

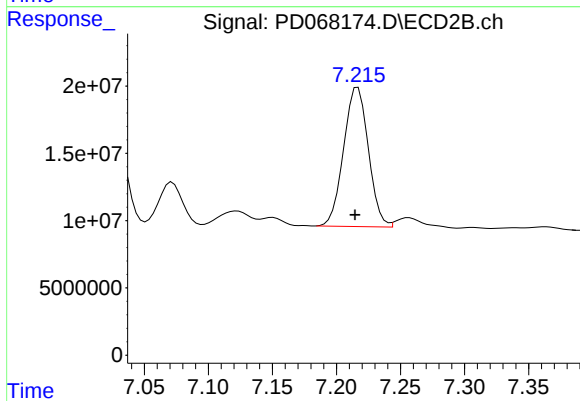

#27 Chlordane-5


R.T.: 7.217 min
Delta R.T.: 0.002 min
Response: 139139903
Conc: 517.55 ng/ml

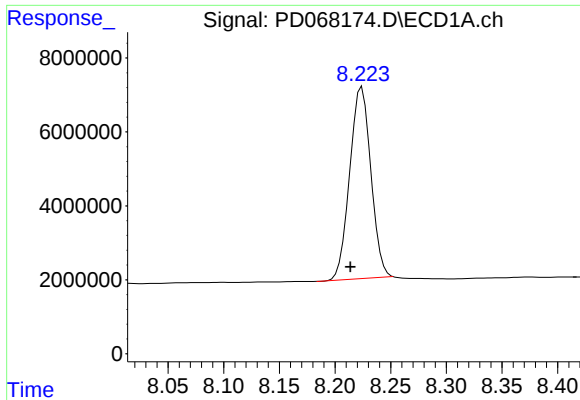

#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: 0.010 min
Response: 68671871
Conc: 47.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

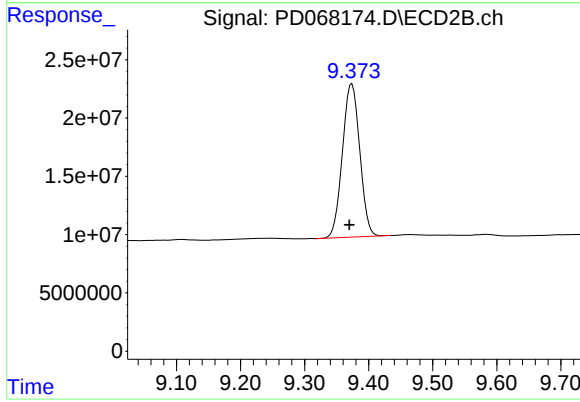

#28 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: 0.004 min
Response: 246996860
Conc: 49.62 ng/ml